

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100118\
 Data File : VV008008.D
 Acq On : 01 Oct 2018 21:26
 Operator : SY/MD
 Sample : J5159-12
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAC98

Quant Time: Oct 02 05:04:13 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 02 04:17:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	83418	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	78280	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	37124	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	22788	5.09	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.80%
7) Chloroethane-d5	1.59	69	20038	5.19	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.80%
11) 1,1-Dichloroethene-d2	2.13	63	35371	3.50	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.00%
20) 2-Butanone-d5	3.97	46	64790	48.17	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.34%
24) Chloroform-d	4.41	84	49939	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.00%
26) 1,2-Dichloroethane-d4	5.09	65	27967	4.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.80%
32) Benzene-d6	5.10	84	99384	5.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.40%
36) 1,2-Dichloropropane-d6	6.13	67	31128	5.25	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.00%
41) Toluene-d8	7.36	98	90493	4.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.20%
43) trans-1,3-Dichloropropene-	7.67	79	10350	4.54	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.80%
46) 2-Hexanone-d5	8.14	63	47167	46.84	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.68%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	21508	4.70	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	37932	5.28	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.60%


Target Compounds					Ovalue
47) Tetrachloroethene	8.02	164	38302	6.440 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100118\
Data File : VV008008.D
Acq On : 01 Oct 2018 21:26
Operator : SY/MD
Sample : J5159-12
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAC98

Quant Time: Oct 02 05:04:13 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 02 04:17:24 2018
Response via : Initial Calibration

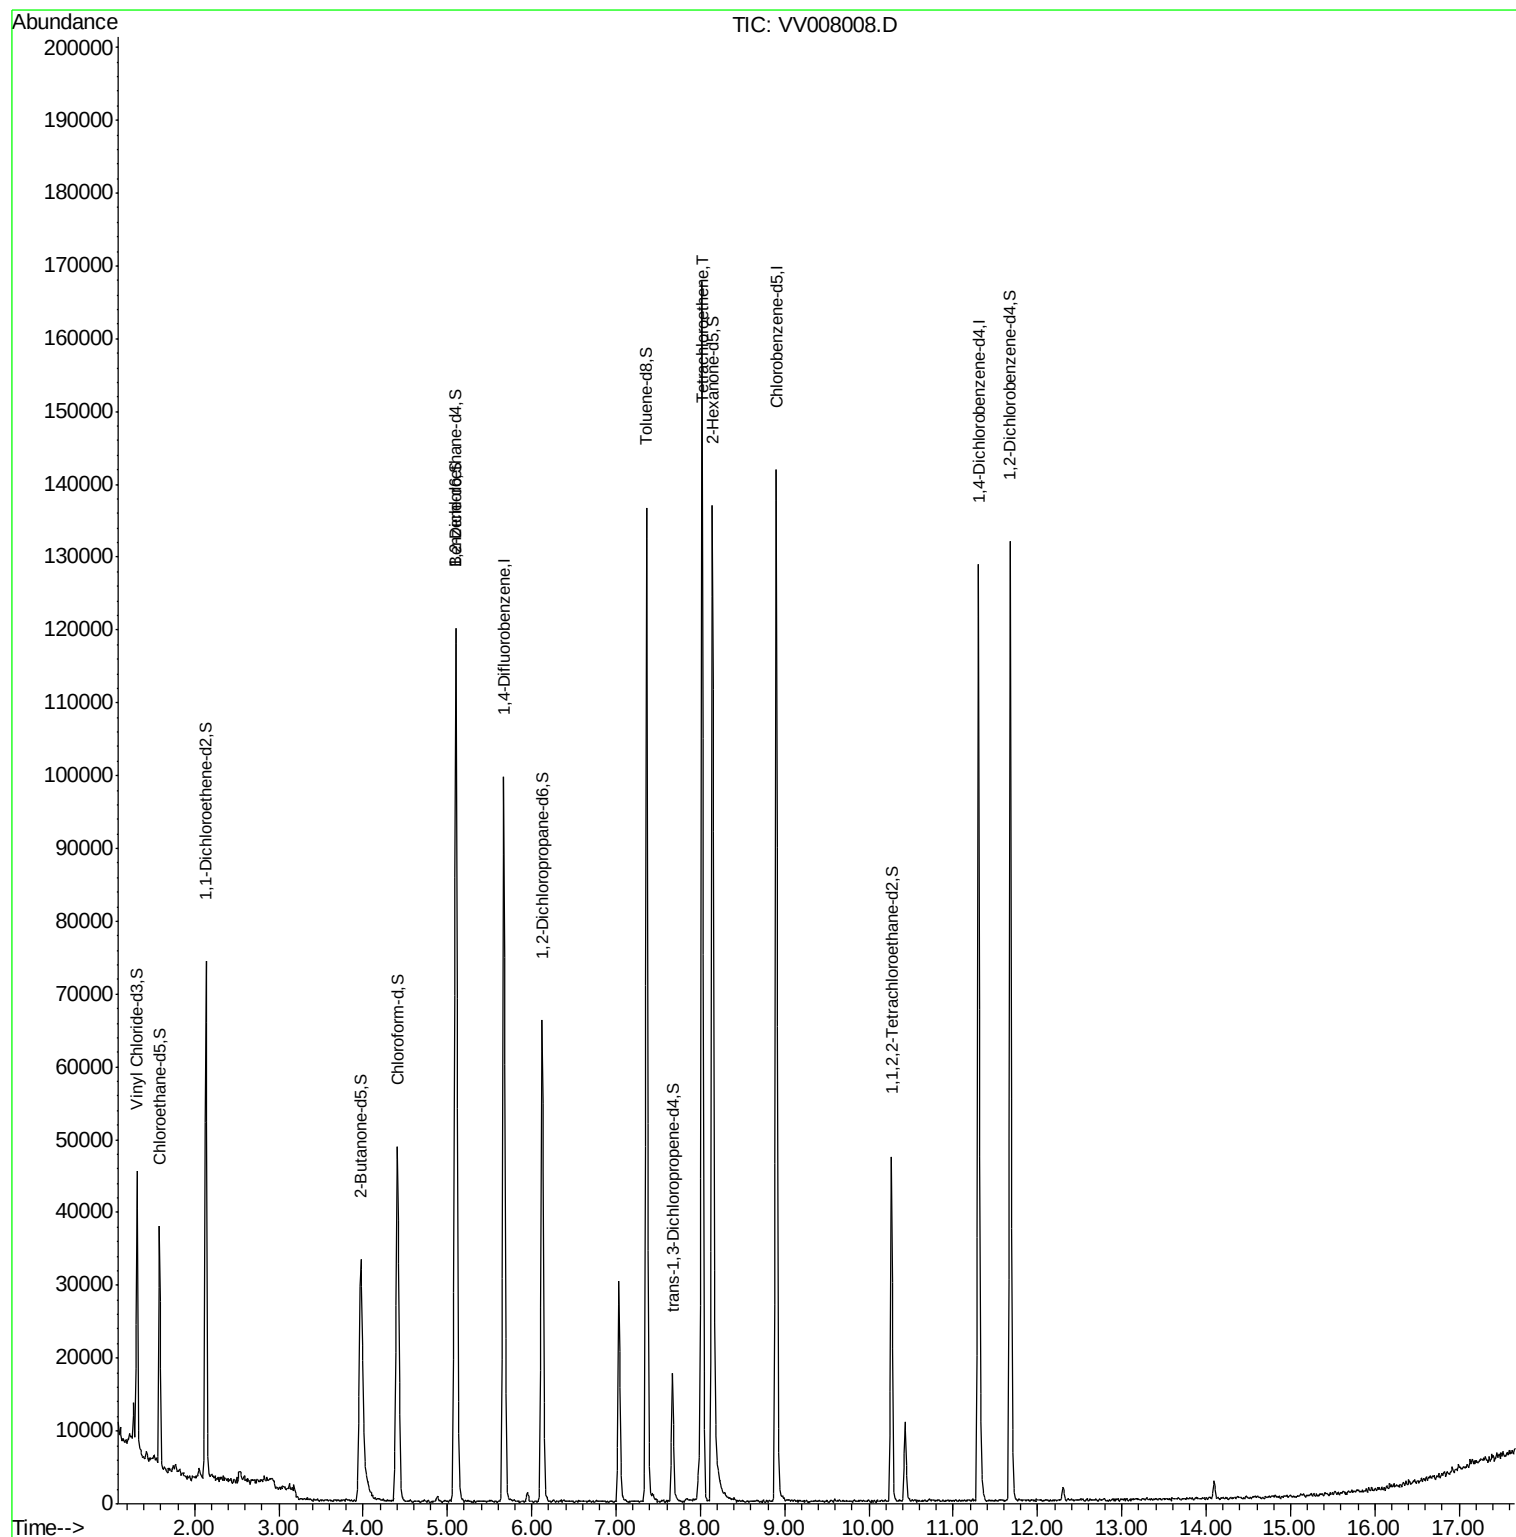


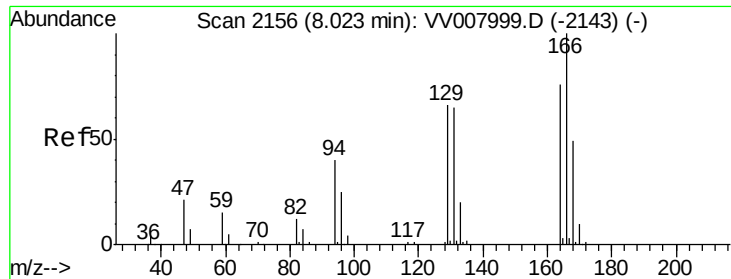

#47
Tetrachloroethene
Concen: 6.440 ug/L
RT: 8.02 min Scan# 2156
Delta R.T. -0.00 min
Lab File: VV008008.D
Acq: 01 Oct 2018 21:26

Instrument :
MSVOA_V
ClientSampleId :
GAC98

Tot Ion:	164	Resp:	38302
Ion	Ratio	Lower	Upper
164	100		
129	89.6	59.2	110.0
131	87.6	57.1	106.1
166	133.0	88.6	164.6

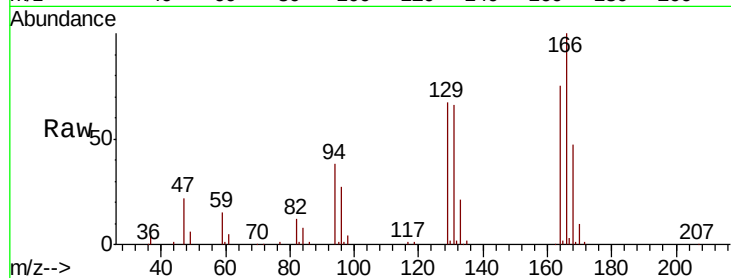

Abundance Ion 163.90 (163.60 to 164.60): V
Ion 128.95 (128.65 to 129.65): V
Ion 130.95 (130.65 to 131.65): V
Ion 165.90 (165.60 to 166.60): V

