


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100118\
Data File : VV007988.D
Acq On : 01 Oct 2018 09:20
Operator : SY/MD
Sample : BFB78
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB78

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Oct 02 04:17:24 2018

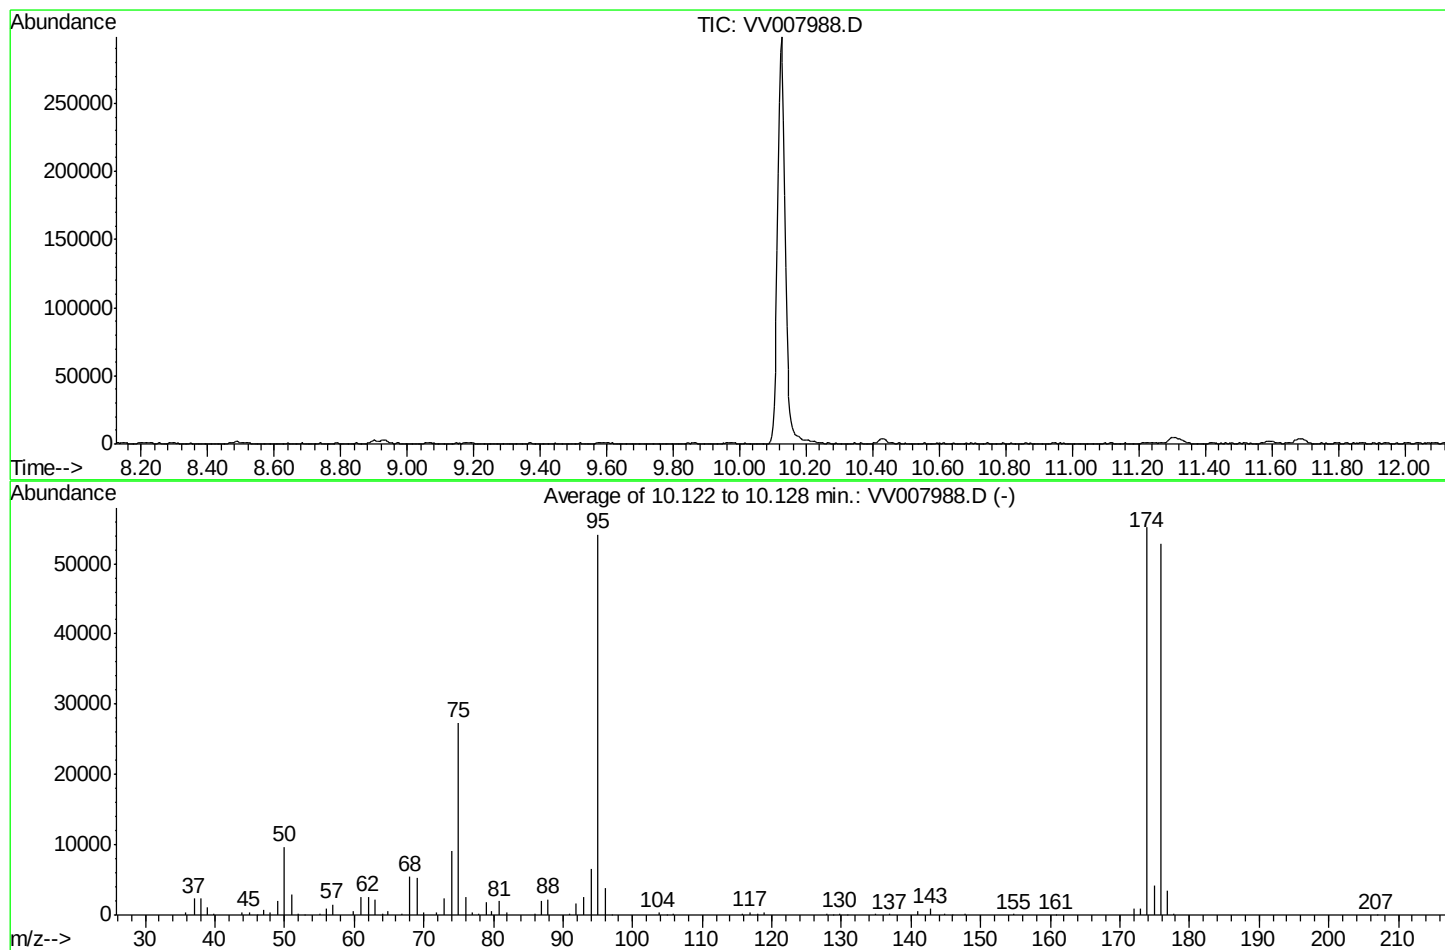

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	9712	PASS
75	95	30	80	50.5	27370	PASS
95	95	100	100	100.0	54162	PASS
96	95	5	9	7.0	3780	PASS
173	174	0.00	2	1.5	845	PASS
174	95	50	120	101.9	55170	PASS
175	174	5	9	7.7	4244	PASS
176	174	95	101	95.9	52882	PASS
177	176	5	9	6.5	3455	PASS

m/z	Abundance
43.80	311.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78

m/z	Abundance
35.80	442.0
37.00	2501.0
38.00	2350.0
39.00	1068.0
39.90	163.0
43.90	696.0
44.90	416.0
46.00	123.0
47.00	761.0
47.90	366.0
49.00	2107.0
50.00	10031.0
51.00	2842.0
52.00	121.0
52.80	122.0
55.00	292.0
55.90	915.0
56.90	1479.0
59.90	475.0
61.00	2560.0
62.00	2642.0
63.00	2142.0
64.00	246.0
64.90	562.0
66.80	150.0
68.00	5336.0
69.00	5308.0
70.00	397.0
71.90	378.0
73.00	2374.0
74.00	9207.0
75.00	27560.0
76.00	2515.0
76.90	391.0
77.90	240.0
78.90	1861.0
79.80	587.0
80.90	2001.0
81.80	397.0
86.00	165.0
86.90	2091.0
87.90	2218.0
90.80	240.0
91.90	1706.0
93.00	2562.0
94.00	6437.0
95.00	54344.0
96.00	4011.0
97.00	113.0
103.80	282.0
104.90	101.0
105.80	250.0
115.80	217.0
116.90	460.0
117.90	256.0
118.80	319.0
127.80	205.0
128.70	117.0
129.80	216.0
130.80	102.0
134.90	108.0
137.00	116.0
140.90	641.0
142.80	850.0
144.70	157.0
147.80	169.0
154.80	116.0
172.00	811.0
172.90	825.0
173.90	53608.0
174.90	4165.0
175.90	51736.0
176.90	3417.0
177.80	128.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78

m/z	Abundance
35.90	465.0
37.00	2364.0
38.00	2388.0
38.90	1043.0
39.80	151.0
43.90	695.0
44.90	406.0
46.10	122.0
46.90	720.0
48.00	402.0
48.90	2139.0
50.00	10076.0
51.00	3011.0
51.90	131.0
52.80	116.0
55.00	239.0
56.00	965.0
56.90	1541.0
59.90	513.0
61.00	2586.0
62.00	2738.0
63.00	2130.0
64.00	273.0
64.90	576.0
66.90	157.0
68.00	5620.0
69.00	5405.0
70.00	399.0
71.90	325.0
73.00	2469.0
74.00	9291.0
75.00	28368.0
76.00	2545.0
76.90	448.0
77.90	239.0
78.90	1861.0
79.80	606.0
80.90	1992.0
81.80	403.0
86.00	186.0
86.90	2185.0
87.90	2337.0
90.90	252.0
91.90	1741.0
93.00	2642.0
94.00	6749.0
95.00	55904.0
96.00	3881.0
96.90	112.0
103.80	314.0
104.90	110.0
105.90	287.0
115.70	205.0
116.90	488.0
117.90	266.0
118.80	302.0
127.80	189.0
128.80	121.0
129.70	227.0
134.90	116.0
136.90	119.0
140.90	654.0
142.80	905.0
144.80	157.0
145.90	110.0
147.80	164.0
154.80	139.0
160.90	105.0
171.90	851.0
173.00	856.0
173.90	57144.0
174.90	4371.0
175.90	54800.0
176.90	3577.0
177.80	143.0
206.90	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78

m/z	Abundance
35.90	430.0
37.00	2096.0
38.00	2156.0
38.90	966.0
39.80	131.0
43.90	657.0
44.90	391.0
46.90	562.0
47.90	369.0
48.90	2052.0
50.00	9030.0
51.00	2988.0
51.90	130.0
55.00	178.0
56.00	909.0
56.90	1452.0
59.90	482.0
60.90	2374.0
62.00	2512.0
63.00	2056.0
64.00	284.0
64.90	508.0
67.00	175.0
68.00	5307.0
69.00	5121.0
70.00	397.0
71.90	289.0
73.00	2322.0
74.00	8576.0
75.00	26184.0
76.00	2366.0
76.90	436.0
77.90	195.0
78.90	1697.0
79.80	552.0
80.90	1836.0
81.90	414.0
86.00	159.0
86.90	2024.0
87.90	2262.0
90.90	248.0
91.90	1602.0
93.00	2440.0
94.00	6512.0
95.00	52240.0
96.00	3450.0
103.80	293.0
105.90	295.0
115.80	180.0
116.90	427.0
117.90	247.0
118.80	293.0
127.90	173.0
129.80	198.0
134.80	108.0
136.90	119.0
140.90	618.0
142.80	820.0
144.80	156.0
145.90	104.0
147.70	140.0
154.80	158.0
171.90	891.0
173.00	856.0
173.90	54760.0
174.90	4198.0
175.90	52112.0
176.90	3371.0
177.80	132.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78