

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100120\
 Data File : VV018588.D
 Acq On : 01 Oct 2020 13:50
 Operator : SY/MD
 Sample : L4144-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM3

Quant Time: Oct 02 03:50:43 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 01 23:37:24 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	308360	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	300185	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	157554	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	66685	36.87	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	73.74%
7) Chloroethane-d5	1.58	69	69164	46.25	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	92.50%
11) 1,1-Dichloroethene-d2	2.12	63	116103	31.51	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	63.02%
21) 2-Butanone-d5	3.92	46	139786	103.62	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	103.62%
24) Chloroform-d	4.38	84	174415	44.60	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.20%
26) 1,2-Dichloroethane-d4	5.06	65	119326	48.07	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.14%
32) Benzene-d6	5.07	84	336392	44.24	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.48%
36) 1,2-Dichloropropane-d6	6.09	67	109496	47.66	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.32%
41) Toluene-d8	7.34	98	304288	42.54	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.08%
43) trans-1,3-Dichloropropene-	7.64	79	54241	43.70	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.40%
47) 2-Hexanone-d5	8.11	63	73255	83.95	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	83.95%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	135083	44.35	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.70%
64) 1,2-Dichlorobenzene-d4	11.65	152	149947	49.49	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.98%


Target Compounds					Ovalue
13) Acetone	2.20	43	11998	10.295 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100120\
Data File : VV018588.D
Acq On : 01 Oct 2020 13:50
Operator : SY/MD
Sample : L4144-08
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM3

Quant Time: Oct 02 03:50:43 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 01 23:37:24 2020
Response via : Initial Calibration

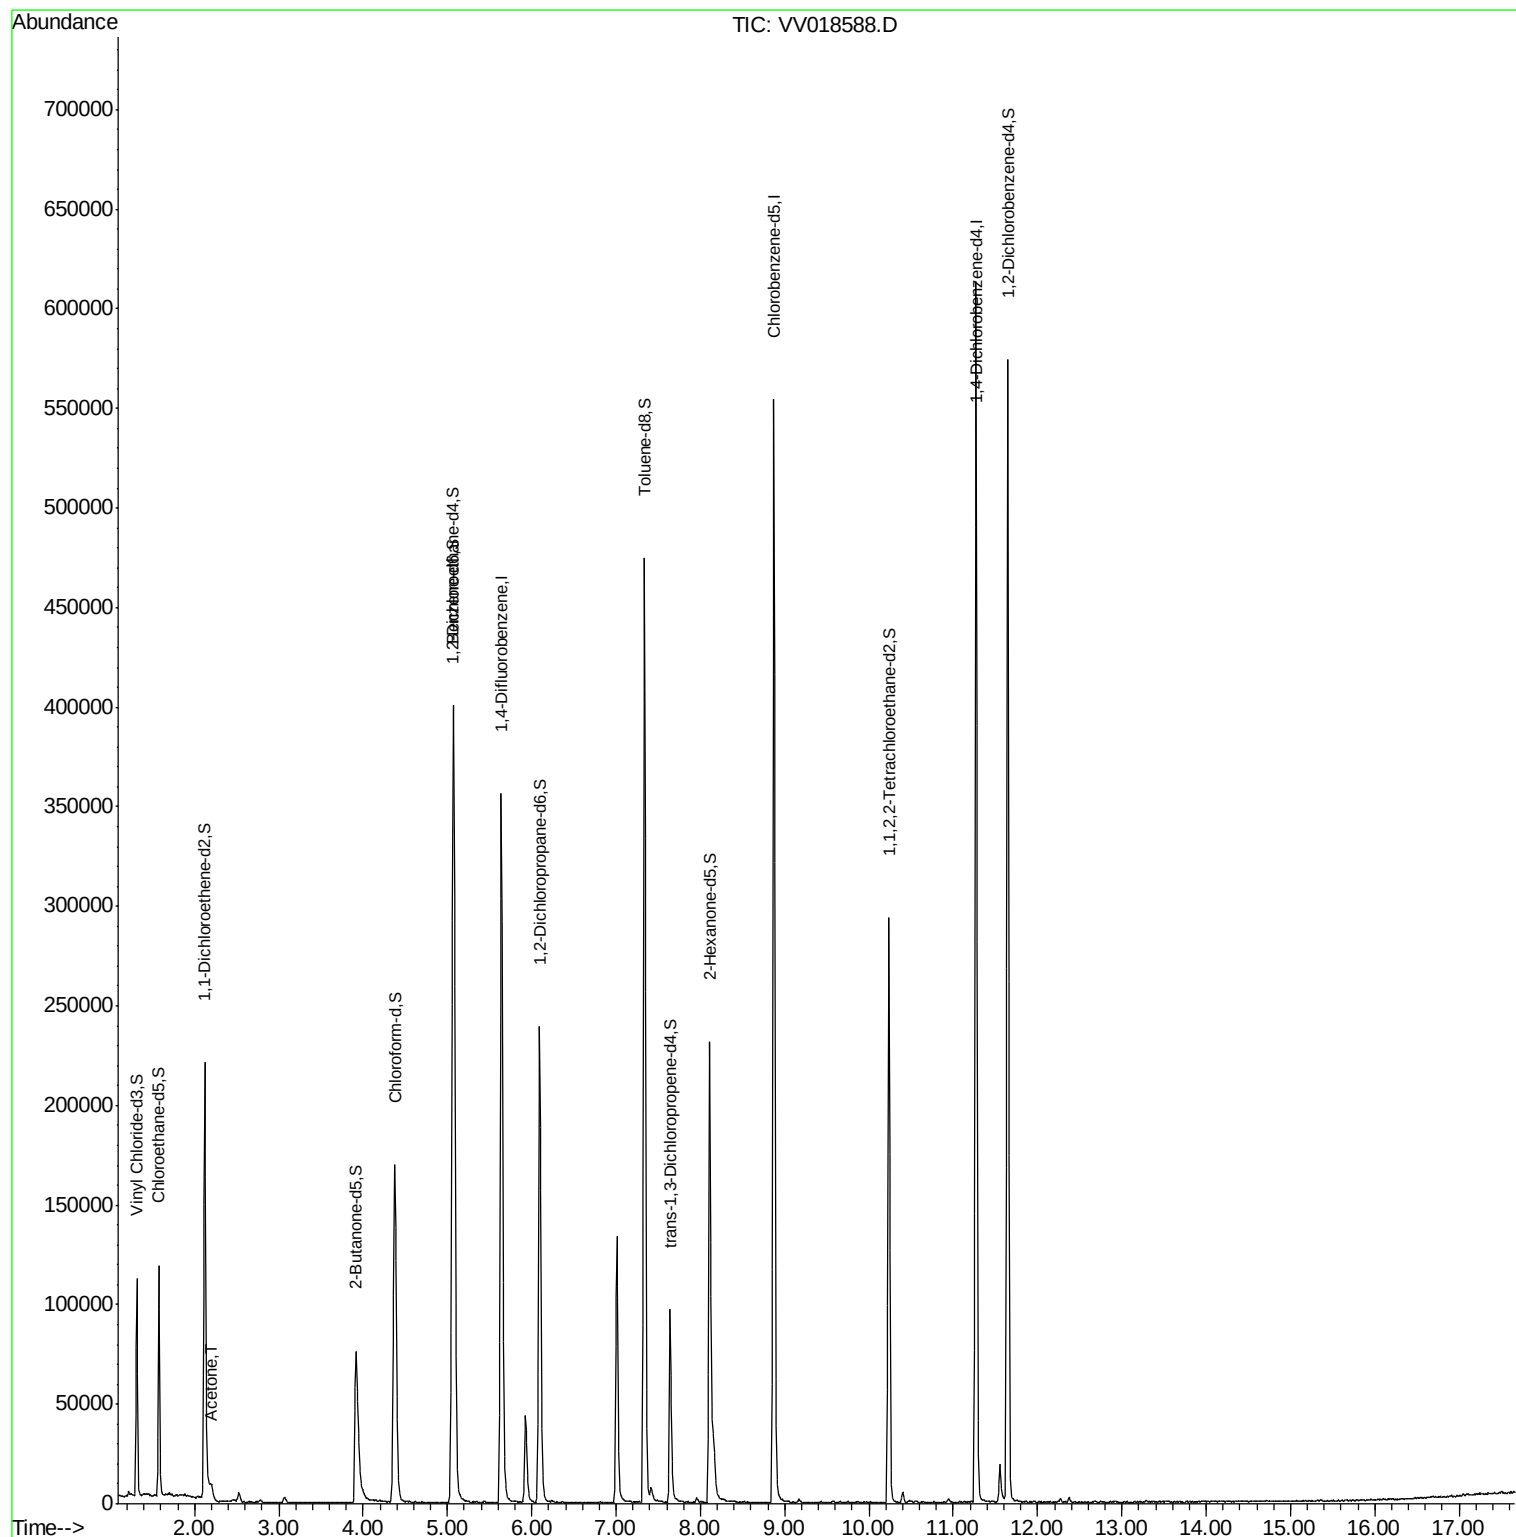

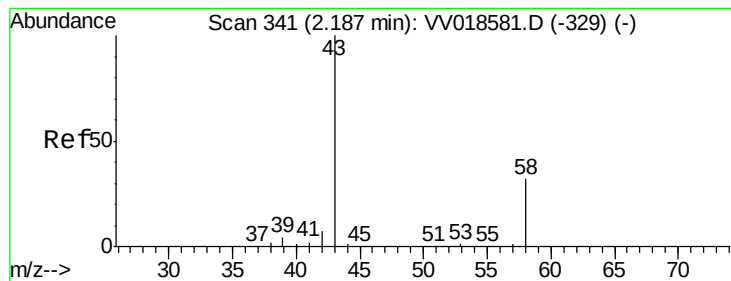

#13
 Acetone
 Concen: 10.295 ug/L
 RT: 2.20 min Scan# 345
 Delta R.T. 0.01 min
 Lab File: VV018588.D
 Acq: 01 Oct 2020 13:50

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM3

Tot Ion: 43 Resp: 11998
 Ion Ratio Lower Upper
 43 100
 58 33.0 0.0 64.0

