

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100120\
 Data File : VV018594.D
 Acq On : 01 Oct 2020 17:13
 Operator : SY/MD
 Sample : VIBLK71
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK71

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	81	rVB	153991	153659	14.15%	1.787%
2	1.579	144	152	164	rBV	143879	164708	15.17%	1.916%
3	2.119	310	320	348	rVB	293897	451579	41.59%	5.252%
4	2.373	394	399	405	rBV3	505	549	0.05%	0.006%
5	2.496	432	437	439	rBV	458	348	0.03%	0.004%
6	2.525	440	446	456	rVB5	2064	3204	0.30%	0.037%
7	2.849	544	547	550	rBV	349	291	0.03%	0.003%
8	2.891	557	560	562	rBV	297	209	0.02%	0.002%
9	3.004	594	595	600	rVB3	287	181	0.02%	0.002%
10	3.251	669	672	674	rBV	288	205	0.02%	0.002%
11	3.360	704	706	708	rVB	199	80	0.01%	0.001%
12	3.377	708	711	714	rBV2	253	183	0.02%	0.002%
13	3.396	715	717	720	rVB	370	143	0.01%	0.002%
14	3.412	720	722	724	rBV	191	66	0.01%	0.001%
15	3.454	733	735	739	rBV	291	227	0.02%	0.003%
16	3.496	745	748	749	rBV	227	123	0.01%	0.001%
17	3.631	787	790	792	rBV	222	162	0.01%	0.002%
18	3.682	803	806	810	rBV2	162	116	0.01%	0.001%
19	3.714	810	816	820	rVB	256	264	0.02%	0.003%
20	3.914	868	878	910	rBV2	60297	186351	17.16%	2.167%
21	4.373	1004	1021	1046	rBV	173543	432720	39.85%	5.033%
22	4.631	1098	1101	1104	rBV3	369	241	0.02%	0.003%
23	4.676	1113	1115	1118	rBV2	271	114	0.01%	0.001%
24	4.846	1166	1168	1172	rVB2	210	114	0.01%	0.001%
25	4.904	1182	1186	1189	rBV2	284	242	0.02%	0.003%
26	4.965	1203	1205	1208	rBV2	389	163	0.02%	0.002%
27	5.068	1220	1237	1265	rBV2	423704	1085914	100.00%	12.630%
28	5.331	1316	1319	1322	rBV2	325	244	0.02%	0.003%
29	5.415	1342	1345	1346	rBV2	368	230	0.02%	0.003%
30	5.463	1356	1360	1362	rBV	377	251	0.02%	0.003%
31	5.515	1373	1376	1378	rVB2	218	90	0.01%	0.001%
32	5.582	1395	1397	1402	rBV2	168	111	0.01%	0.001%
33	5.637	1402	1414	1438	rBV	352989	711533	65.52%	8.276%
34	5.926	1492	1504	1520	rBV2	31984	64833	5.97%	0.754%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100120\
 Data File : VV018594.D
 Acq On : 01 Oct 2020 17:13
 Operator : SY/MD
 Sample : VIBLK71
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK71

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

35	6.023	1532	1534	1538	rBV3	289	189	0.02%	0.002%
36	6.090	1541	1555	1581	rBV	238557	487073	44.85%	5.665%
37	6.277	1612	1613	1617	rVB	390	183	0.02%	0.002%
38	6.312	1623	1624	1629	rBV2	167	105	0.01%	0.001%
39	6.335	1629	1631	1632	rBV2	321	113	0.01%	0.001%
40	6.492	1678	1680	1681	rBV2	303	153	0.01%	0.002%
41	6.553	1697	1699	1701	rBV	197	64	0.01%	0.001%
42	6.630	1721	1723	1725	rBV	259	112	0.01%	0.001%
43	6.798	1772	1775	1778	rVB	223	152	0.01%	0.002%
44	6.814	1778	1780	1781	rBV	177	60	0.01%	0.001%
45	6.849	1789	1791	1793	rBV2	188	91	0.01%	0.001%
46	6.894	1803	1805	1809	rVB2	217	111	0.01%	0.001%
47	7.007	1829	1840	1858	rBV	136929	246374	22.69%	2.866%
48	7.225	1904	1908	1912	rBV3	743	768	0.07%	0.009%
49	7.335	1930	1942	1967	rBV	520566	891960	82.14%	10.375%
50	7.640	2027	2037	2063	rBV	99270	171673	15.81%	1.997%
51	7.888	2112	2114	2115	rBV	234	75	0.01%	0.001%
52	7.997	2138	2148	2164	rVB2	23391	40855	3.76%	0.475%
53	8.106	2173	2182	2216	rBV2	195996	402615	37.08%	4.683%
54	8.637	2345	2347	2348	rBV	241	100	0.01%	0.001%
55	8.753	2379	2383	2386	rBV2	269	273	0.03%	0.003%
56	8.872	2408	2420	2445	rBV	556628	893028	82.24%	10.387%
57	9.592	2641	2644	2646	rBV	309	183	0.02%	0.002%
58	10.238	2833	2845	2868	rVV	272015	424095	39.05%	4.933%
59	10.331	2871	2874	2877	rBV2	413	292	0.03%	0.003%
60	10.679	2979	2982	2985	rBV	228	165	0.02%	0.002%
61	10.698	2985	2988	2991	rBV	261	227	0.02%	0.003%
62	11.183	3136	3139	3140	rBV	397	171	0.02%	0.002%
63	11.270	3154	3166	3188	rBV	594170	906593	83.49%	10.545%
64	11.482	3229	3232	3233	rBV	299	188	0.02%	0.002%
65	11.646	3271	3283	3305	rBV	554244	868733	80.00%	10.104%
66	11.814	3330	3335	3340	rBV3	552	673	0.06%	0.008%
67	11.887	3354	3358	3361	rBV3	571	427	0.04%	0.005%
68	12.360	3502	3505	3507	rBV	364	235	0.02%	0.003%


Sum of corrected areas: 8597557

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100120\
Data File : VV018594.D
Acq On : 01 Oct 2020 17:13
Operator : SY/MD
Sample : VIBLK71
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VIBLK71

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

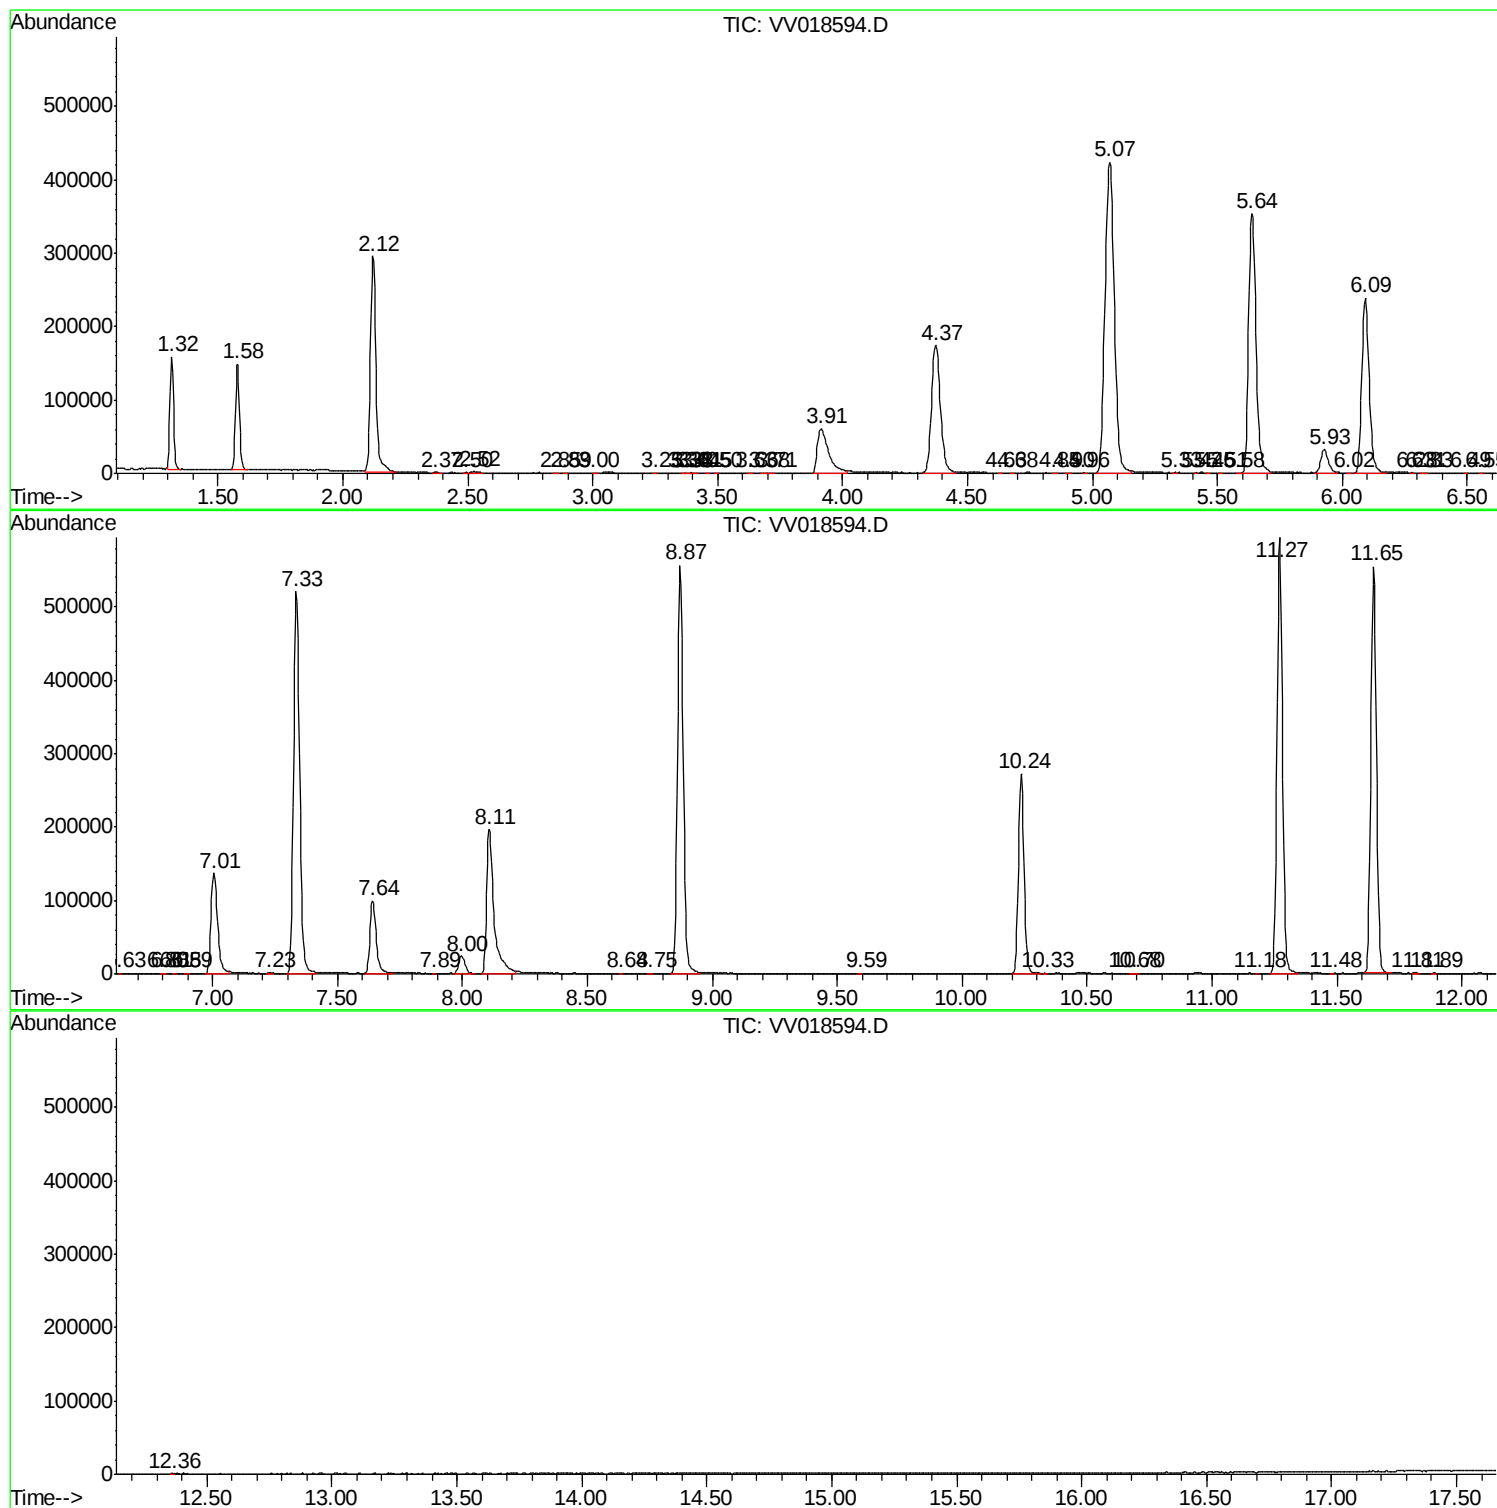

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100120\
Data File : VV018594.D
Acq On : 01 Oct 2020 17:13
Operator : SY/MD
Sample : VIBLK71
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK71










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.93	4.56 ug/L	64833	1,4-Difluorobenzene	5.64

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Propanoic acid, 2,2,3-trichloro-...	190	C4H5Cl3O2	004749-35-3	37
2		Dihydro-4,5-dichloro-2(3H)furanone	154	C4H4Cl2O2	114434-99-0	25
3		Ethylene, 1,2-dichloro-, (Z)-	96	C2H2Cl2	000156-59-2	25
4		Ethane, 1,1,1,2-tetrachloro-	166	C2H2Cl4	000630-20-6	25
5		Carbamic acid, acetylthio-, O-me...	133	C4H7NO2S	016696-87-0	10

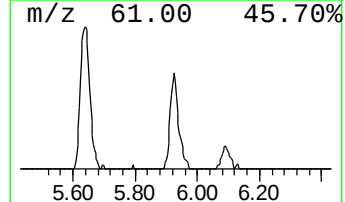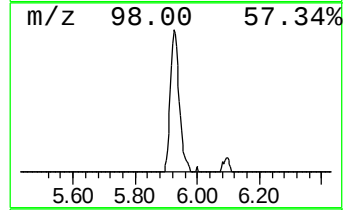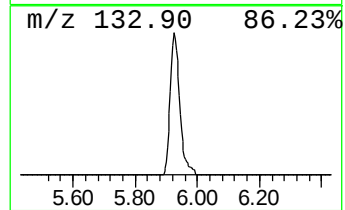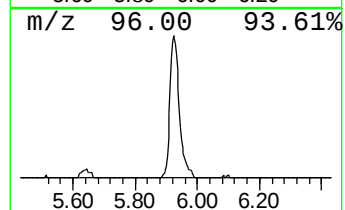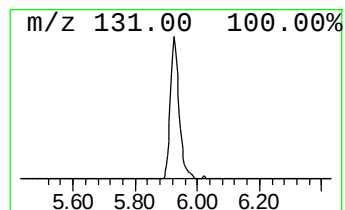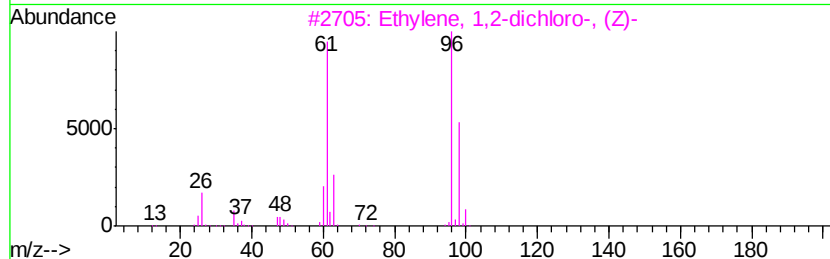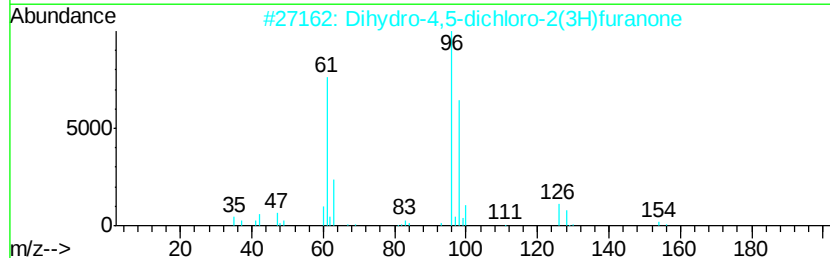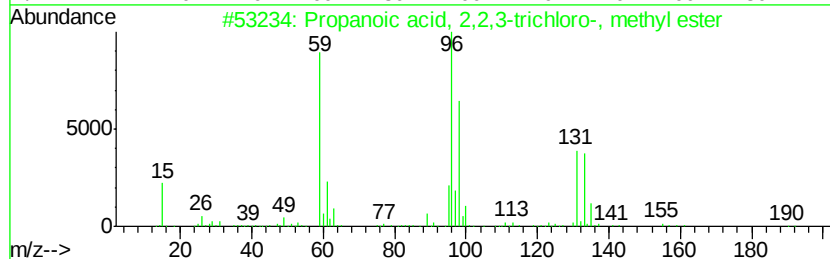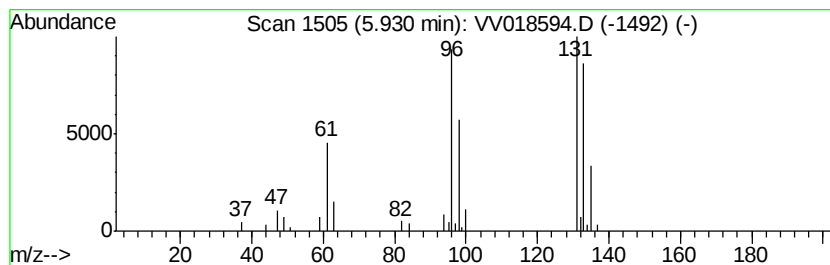

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV100120\
Data File : VV018594.D
Acq On : 01 Oct 2020 17:13
Operator : SY/MD
Sample : VIBLK71
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK71

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	5.93	4.6	ug/L	64833	1	5.64	711533	50.0