

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100120\
 Data File : VV018600.D
 Acq On : 01 Oct 2020 20:00
 Operator : SY/MD
 Sample : L4237-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AB7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	81	rBV	151364	149962	3.84%	1.265%
2	1.579	145	152	164	rVB	136606	151031	3.86%	1.274%
3	2.122	311	321	352	rVB	276764	426366	10.91%	3.597%
4	2.672	490	492	493	rBV	231	110	0.00%	0.001%
5	2.778	521	525	526	rBV	450	324	0.01%	0.003%
6	2.843	542	545	547	rVB2	469	211	0.01%	0.002%
7	2.891	554	560	564	rBV2	310	333	0.01%	0.003%
8	3.167	643	646	652	rVB2	202	137	0.00%	0.001%
9	3.196	652	655	656	rBV	213	97	0.00%	0.001%
10	3.315	690	692	694	rBV	189	76	0.00%	0.001%
11	3.511	750	753	757	rBV2	265	284	0.01%	0.002%
12	3.595	777	779	783	rVB2	162	98	0.00%	0.001%
13	3.917	868	879	917	rBV	60070	192031	4.91%	1.620%
14	4.376	1006	1022	1054	rVB	163798	405766	10.38%	3.423%
15	4.518	1064	1066	1069	rVB2	541	314	0.01%	0.003%
16	4.540	1069	1073	1079	rVB3	524	568	0.01%	0.005%
17	4.582	1084	1086	1088	rVB2	406	165	0.00%	0.001%
18	4.605	1091	1093	1097	rVB3	324	218	0.01%	0.002%
19	4.646	1105	1106	1108	rBV3	254	140	0.00%	0.001%
20	4.756	1136	1140	1142	rBV2	93	58	0.00%	0.000%
21	4.804	1153	1155	1157	rVB	182	53	0.00%	0.000%
22	4.852	1168	1170	1179	rVB2	443	325	0.01%	0.003%
23	4.971	1204	1207	1210	rBV2	260	157	0.00%	0.001%
24	4.994	1212	1214	1217	rVB	342	154	0.00%	0.001%
25	5.074	1221	1239	1273	rBV2	398518	1032518	26.42%	8.711%
26	5.444	1352	1354	1355	rBV2	286	127	0.00%	0.001%
27	5.508	1370	1374	1377	rBV2	229	178	0.00%	0.002%
28	5.531	1377	1381	1384	rVB3	315	232	0.01%	0.002%
29	5.547	1384	1386	1389	rBV2	238	131	0.00%	0.001%
30	5.640	1402	1415	1444	rBV	323085	649812	16.63%	5.482%
31	5.936	1492	1507	1538	rBV	2013212	3908157	100.00%	32.972%
32	6.093	1545	1556	1578	rVB	227825	454839	11.64%	3.837%
33	6.277	1612	1613	1614	rBV	295	112	0.00%	0.001%
34	6.341	1628	1633	1634	rBV	438	286	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100120\
 Data File : VV018600.D
 Acq On : 01 Oct 2020 20:00
 Operator : SY/MD
 Sample : L4237-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AB7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

35	6.357	1634	1638	1642	rVB3	492	342	0.01%	0.003%
36	6.405	1652	1653	1658	rVB2	429	253	0.01%	0.002%
37	6.675	1733	1737	1738	rBV2	306	185	0.00%	0.002%
38	6.727	1751	1753	1755	rVB2	225	95	0.00%	0.001%
39	6.743	1755	1758	1759	rBV	107	53	0.00%	0.000%
40	6.942	1817	1820	1822	rBV	313	177	0.00%	0.001%
41	7.006	1829	1840	1860	rBV	129065	233404	5.97%	1.969%
42	7.241	1911	1913	1917	rBV3	368	292	0.01%	0.002%
43	7.338	1930	1943	1967	rBV	489323	829261	21.22%	6.996%
44	7.643	2028	2038	2069	rBV	92024	163073	4.17%	1.376%
45	7.907	2118	2120	2123	rBV2	182	100	0.00%	0.001%
46	8.003	2140	2150	2164	rVB4	13327	23310	0.60%	0.197%
47	8.109	2173	2183	2215	rBV2	189344	378193	9.68%	3.191%
48	8.402	2273	2274	2278	rBV2	302	167	0.00%	0.001%
49	8.524	2310	2312	2313	rBV	235	65	0.00%	0.001%
50	8.575	2323	2328	2329	rBV	288	177	0.00%	0.001%
51	8.608	2336	2338	2339	rBV	220	48	0.00%	0.000%
52	8.665	2354	2356	2357	rBV	201	62	0.00%	0.001%
53	8.810	2399	2401	2402	rBV	180	76	0.00%	0.001%
54	8.874	2408	2421	2446	rBV	504285	812543	20.79%	6.855%
55	9.116	2493	2496	2499	rBV	273	133	0.00%	0.001%
56	9.161	2507	2510	2511	rBV	421	193	0.00%	0.002%
57	9.325	2559	2561	2564	rVB2	156	46	0.00%	0.000%
58	9.350	2564	2569	2574	rVB2	359	400	0.01%	0.003%
59	9.379	2574	2578	2580	rBV	250	218	0.01%	0.002%
60	9.653	2661	2663	2664	rBV	177	51	0.00%	0.000%
61	9.685	2670	2673	2675	rBV2	334	221	0.01%	0.002%
62	9.733	2685	2688	2692	rBV	413	270	0.01%	0.002%
63	9.797	2705	2708	2709	rBV2	226	122	0.00%	0.001%
64	9.926	2744	2748	2756	rBV2	402	477	0.01%	0.004%
65	10.029	2778	2780	2782	rBV	188	110	0.00%	0.001%
66	10.074	2791	2794	2798	rBV2	253	189	0.00%	0.002%
67	10.238	2833	2845	2865	rBV	256834	404213	10.34%	3.410%
68	10.611	2959	2961	2963	rBV	291	85	0.00%	0.001%
69	10.746	3000	3003	3007	rVB2	300	164	0.00%	0.001%
70	10.765	3007	3009	3010	rBV	171	72	0.00%	0.001%
71	10.833	3027	3030	3032	rBV	253	139	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100120\
Data File : VV018600.D
Acq On : 01 Oct 2020 20:00
Operator : SY/MD
Sample : L4237-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AB7

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Title : VOC Analysis

72	11.209	3145	3147	3152	rVB3	520	338	0.01%	0.003%
73	11.270	3155	3166	3192	rBV	537242	813882	20.83%	6.866%
74	11.559	3248	3256	3262	rBV5	3744	5917	0.15%	0.050%
75	11.646	3271	3283	3308	rBV	512145	807247	20.66%	6.810%
76	12.546	3561	3563	3564	rBV	210	73	0.00%	0.001%
77	12.755	3624	3628	3631	rBV	300	273	0.01%	0.002%
78	12.903	3669	3674	3676	rBV2	335	279	0.01%	0.002%
79	12.977	3692	3697	3702	rBV2	476	542	0.01%	0.005%
80	13.771	3942	3944	3945	rBV	449	151	0.00%	0.001%


Sum of corrected areas: 11853051

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100120\
Data File : VV018600.D
Acq On : 01 Oct 2020 20:00
Operator : SY/MD
Sample : L4237-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AB7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

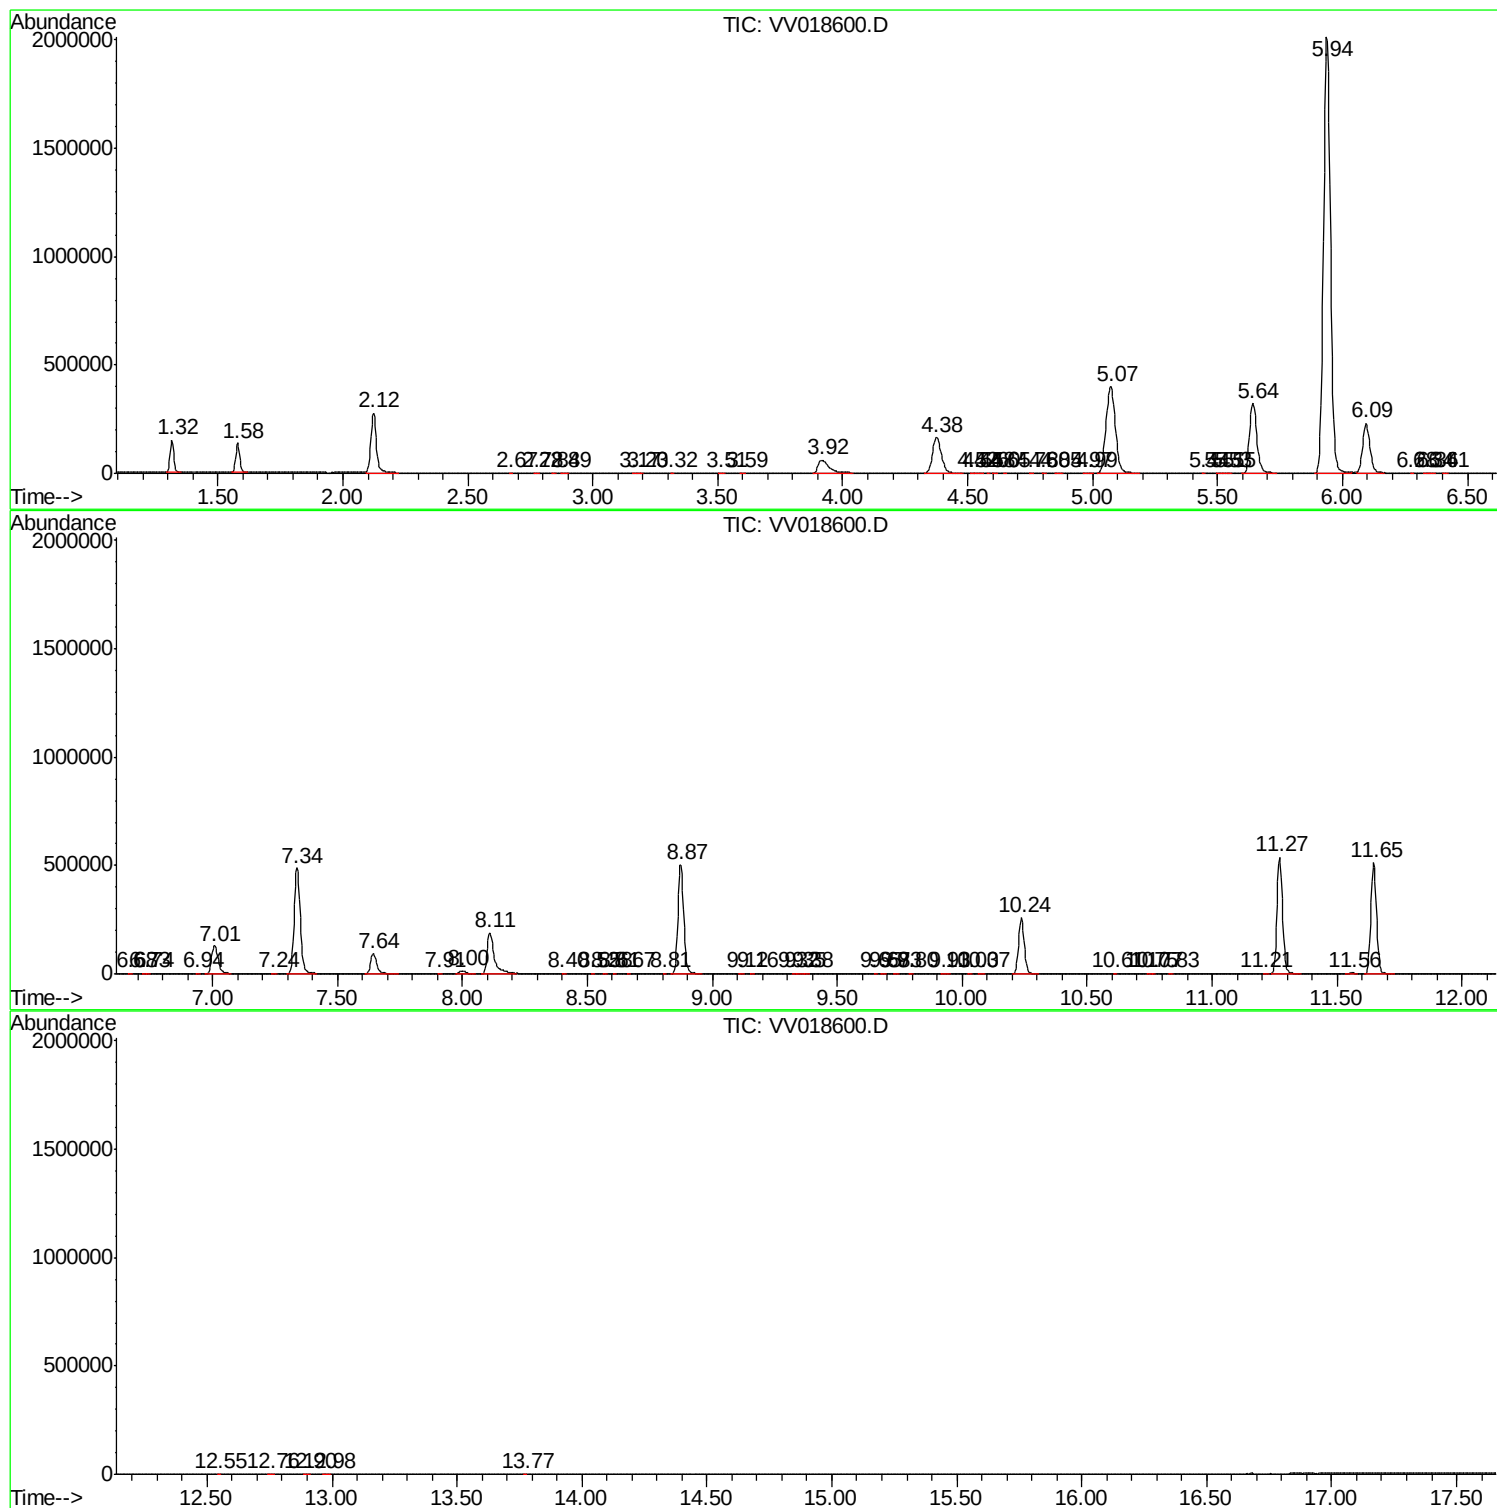

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV100120\
Data File : VV018600.D
Acq On : 01 Oct 2020 20:00
Operator : SY/MD
Sample : L4237-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AB7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV100120\
Data File : VV018600.D
Acq On : 01 Oct 2020 20:00
Operator : SY/MD
Sample : L4237-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AB7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc