

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100120\
 Data File : VV018603.D
 Acq On : 01 Oct 2020 21:11
 Operator : SY/MD
 Sample : L4237-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	82	rVB	171842	165590	1.49%	0.845%
2	1.579	144	152	166	rVB	143464	159796	1.44%	0.815%
3	2.122	310	321	349	rVB	282292	428592	3.86%	2.187%
4	2.347	385	391	397	rBV5	647	826	0.01%	0.004%
5	2.637	476	481	482	rBV2	428	325	0.00%	0.002%
6	2.782	519	526	540	rVB5	3286	5039	0.05%	0.026%
7	3.058	607	612	616	rBV4	1453	1620	0.01%	0.008%
8	3.273	673	679	681	rVB	231	209	0.00%	0.001%
9	3.351	699	703	707	rBV2	230	256	0.00%	0.001%
10	3.476	733	742	745	rBV3	366	424	0.00%	0.002%
11	3.630	784	790	792	rVB2	288	208	0.00%	0.001%
12	3.859	857	861	867	rVB	354	319	0.00%	0.002%
13	3.926	868	882	914	rBV2	72979	257435	2.32%	1.314%
14	4.138	946	948	951	rVB3	430	228	0.00%	0.001%
15	4.376	1005	1022	1053	rBV	169645	422374	3.80%	2.155%
16	4.572	1080	1083	1085	rBV	321	215	0.00%	0.001%
17	4.589	1085	1088	1092	rVB2	405	285	0.00%	0.001%
18	4.640	1102	1104	1109	rVB	409	275	0.00%	0.001%
19	4.916	1186	1190	1194	rBV2	227	226	0.00%	0.001%
20	5.071	1219	1238	1270	rBV2	405505	1048386	9.44%	5.350%
21	5.392	1335	1338	1340	rBV2	411	228	0.00%	0.001%
22	5.408	1340	1343	1348	rVB3	381	381	0.00%	0.002%
23	5.508	1372	1374	1379	rBV2	427	386	0.00%	0.002%
24	5.643	1401	1416	1441	rBV	354087	701802	6.32%	3.581%
25	5.939	1492	1508	1541	rBV	5763419	11103174	100.00%	56.658%
26	6.093	1545	1556	1585	rVV	238387	497135	4.48%	2.537%
27	6.206	1589	1591	1595	rVB3	996	632	0.01%	0.003%
28	6.318	1620	1626	1631	rBV7	669	853	0.01%	0.004%
29	6.415	1652	1656	1658	rBV	387	243	0.00%	0.001%
30	6.476	1671	1675	1678	rVV2	248	211	0.00%	0.001%
31	6.569	1698	1704	1707	rBV2	425	462	0.00%	0.002%
32	6.611	1714	1717	1723	rBV2	169	220	0.00%	0.001%
33	6.875	1797	1799	1805	rBV	289	242	0.00%	0.001%
34	7.010	1829	1841	1860	rBV	129478	237089	2.14%	1.210%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100120\
 Data File : VV018603.D
 Acq On : 01 Oct 2020 21:11
 Operator : SY/MD
 Sample : L4237-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

35	7.132	1875	1879	1881	rBV2	453	292	0.00%	0.001%
36	7.203	1900	1901	1905	rBV	366	234	0.00%	0.001%
37	7.231	1907	1910	1912	rBV2	468	281	0.00%	0.001%
38	7.267	1918	1921	1926	rBV4	435	342	0.00%	0.002%
39	7.338	1931	1943	1968	rBV	502225	854520	7.70%	4.361%
40	7.643	2027	2038	2055	rBV	96320	164133	1.48%	0.838%
41	7.797	2083	2086	2089	rBV	437	253	0.00%	0.001%
42	7.817	2090	2092	2095	rVV2	395	250	0.00%	0.001%
43	7.910	2116	2121	2124	rBV2	459	557	0.01%	0.003%
44	8.003	2141	2150	2160	rVB3	7779	13036	0.12%	0.067%
45	8.109	2173	2183	2218	rBV2	207991	417746	3.76%	2.132%
46	8.495	2300	2303	2310	rVB4	294	292	0.00%	0.001%
47	8.553	2317	2321	2324	rBV	387	365	0.00%	0.002%
48	8.624	2337	2343	2345	rBV2	419	338	0.00%	0.002%
49	8.791	2391	2395	2397	rVB2	392	225	0.00%	0.001%
50	8.875	2409	2421	2447	rBV	557616	910635	8.20%	4.647%
51	9.045	2471	2474	2477	rBV3	350	275	0.00%	0.001%
52	9.064	2478	2480	2486	rVB2	573	396	0.00%	0.002%
53	9.161	2507	2510	2511	rBV2	431	241	0.00%	0.001%
54	9.209	2522	2525	2529	rBV2	403	292	0.00%	0.001%
55	9.328	2559	2562	2563	rBV	459	220	0.00%	0.001%
56	9.424	2588	2592	2595	rBV2	366	205	0.00%	0.001%
57	9.601	2643	2647	2649	rVB2	327	234	0.00%	0.001%
58	9.717	2680	2683	2687	rVB2	269	202	0.00%	0.001%
59	9.739	2687	2690	2694	rBV3	270	267	0.00%	0.001%
60	9.907	2739	2742	2744	rBV	348	228	0.00%	0.001%
61	9.974	2758	2763	2765	rBV	254	257	0.00%	0.001%
62	10.083	2792	2797	2800	rBV3	393	290	0.00%	0.001%
63	10.148	2813	2817	2818	rBV	399	244	0.00%	0.001%
64	10.238	2833	2845	2863	rBV	310580	465517	4.19%	2.375%
65	10.354	2878	2881	2885	rVV2	422	245	0.00%	0.001%
66	10.376	2885	2888	2891	rVV2	438	245	0.00%	0.001%
67	10.405	2891	2897	2904	rVB3	726	1121	0.01%	0.006%
68	10.698	2985	2988	2991	rVV3	345	247	0.00%	0.001%
69	10.897	3045	3050	3054	rBV2	298	313	0.00%	0.002%
70	10.929	3059	3060	3062	rBV2	382	208	0.00%	0.001%
71	11.032	3088	3092	3097	rVV2	424	427	0.00%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100120\
 Data File : VV018603.D
 Acq On : 01 Oct 2020 21:11
 Operator : SY/MD
 Sample : L4237-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

72	11.054	3097	3099	3103	rVV2	311	229	0.00%	0.001%
73	11.080	3104	3107	3110	rVV2	403	245	0.00%	0.001%
74	11.270	3154	3166	3189	rVV	573488	878091	7.91%	4.481%
75	11.360	3192	3194	3198	rVV2	504	343	0.00%	0.002%
76	11.563	3248	3257	3270	rBV5	2782	5202	0.05%	0.027%
77	11.646	3271	3283	3301	rVV	537894	835898	7.53%	4.265%
78	11.723	3305	3307	3313	rVB5	561	428	0.00%	0.002%
79	11.784	3323	3326	3332	rVB2	468	342	0.00%	0.002%
80	11.842	3342	3344	3348	rVB3	392	202	0.00%	0.001%
81	11.961	3378	3381	3383	rBV	378	249	0.00%	0.001%
82	12.341	3493	3499	3502	rBV2	294	313	0.00%	0.002%
83	12.363	3503	3506	3509	rVV2	356	245	0.00%	0.001%
84	12.379	3509	3511	3515	rVB2	321	207	0.00%	0.001%
85	12.514	3549	3553	3559	rVB3	231	245	0.00%	0.001%
86	12.717	3614	3616	3619	rVB	479	240	0.00%	0.001%
87	12.733	3619	3621	3624	rBV	311	231	0.00%	0.001%
88	12.833	3648	3652	3654	rBV	289	233	0.00%	0.001%
89	12.868	3659	3663	3664	rBV2	322	219	0.00%	0.001%
90	13.328	3803	3806	3812	rVB2	339	281	0.00%	0.001%
91	13.514	3861	3864	3867	rVB	442	270	0.00%	0.001%
92	13.546	3870	3874	3875	rBV2	348	206	0.00%	0.001%
93	13.852	3966	3969	3972	rBV	297	239	0.00%	0.001%
94	14.083	4038	4041	4044	rVB3	512	325	0.00%	0.002%
95	14.392	4136	4137	4142	rBV2	310	266	0.00%	0.001%
96	14.585	4195	4197	4203	rBV2	297	246	0.00%	0.001%
97	14.826	4269	4272	4275	rBV2	304	214	0.00%	0.001%
98	15.363	4436	4439	4441	rBV3	411	256	0.00%	0.001%
99	15.807	4575	4577	4581	rVB2	471	252	0.00%	0.001%
100	15.993	4633	4635	4638	rBV	388	243	0.00%	0.001%


Sum of corrected areas: 19596819

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100120\
Data File : VV018603.D
Acq On : 01 Oct 2020 21:11
Operator : SY/MD
Sample : L4237-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

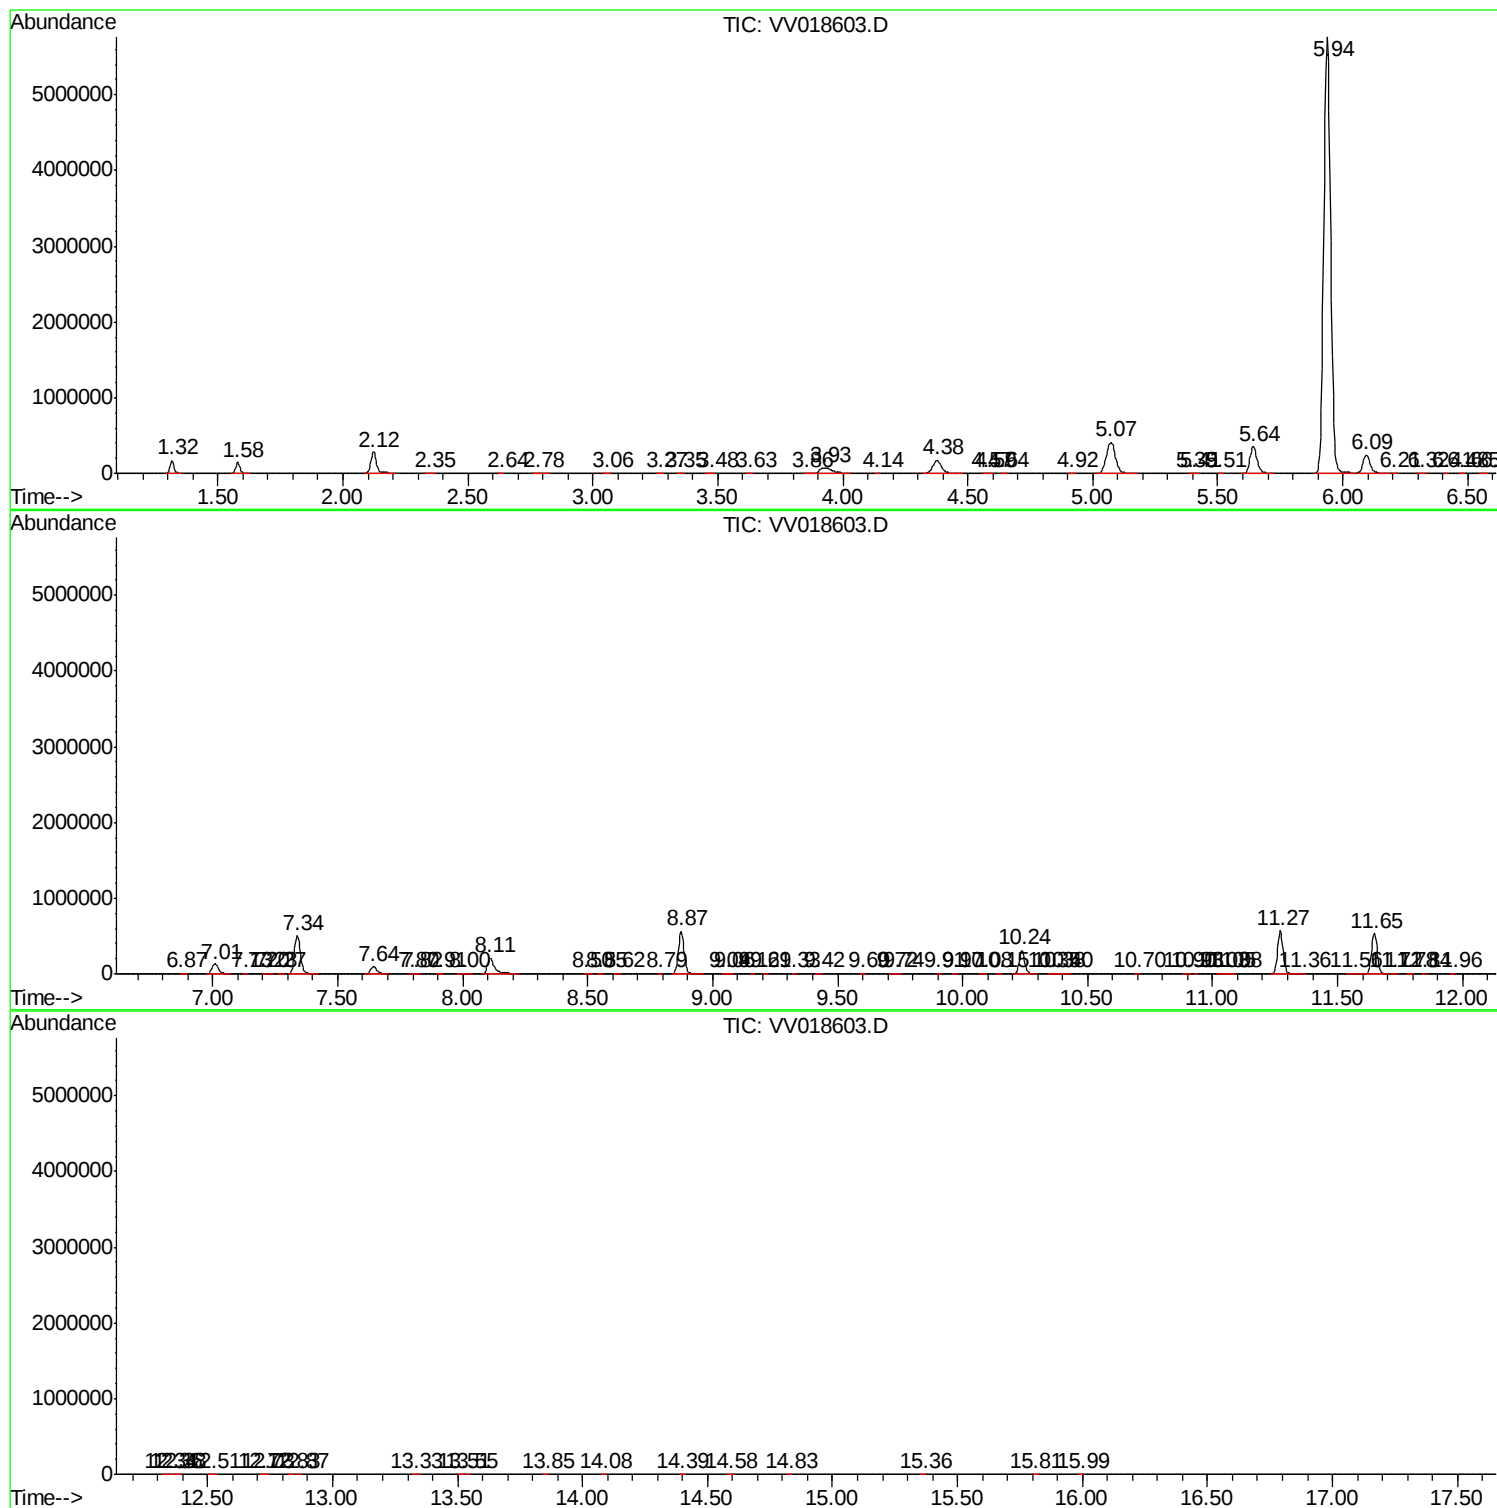

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV100120\
Data File : VV018603.D
Acq On : 01 Oct 2020 21:11
Operator : SY/MD
Sample : L4237-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV100120\
Data File : VV018603.D
Acq On : 01 Oct 2020 21:11
Operator : SY/MD
Sample : L4237-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc