

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100120\
 Data File : VV018604.D
 Acq On : 01 Oct 2020 21:34
 Operator : SY/MD
 Sample : L4237-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB	155587	150856	2.11%	0.964%
2	1.576	145	151	166	rVB	135287	155602	2.18%	0.994%
3	2.122	311	321	354	rVB	283670	445984	6.24%	2.850%
4	2.302	374	377	381	rBV3	592	413	0.01%	0.003%
5	2.682	493	495	496	rBV	184	75	0.00%	0.000%
6	2.788	519	528	540	rBV10	3707	6734	0.09%	0.043%
7	2.836	541	543	544	rBV	163	43	0.00%	0.000%
8	2.894	558	561	565	rBV2	184	168	0.00%	0.001%
9	2.958	578	581	583	rBV2	325	157	0.00%	0.001%
10	3.036	602	605	606	rBV2	300	153	0.00%	0.001%
11	3.064	608	614	624	rVB6	1318	2281	0.03%	0.015%
12	3.126	632	633	634	rBV	234	67	0.00%	0.000%
13	3.164	643	645	651	rBV3	154	145	0.00%	0.001%
14	3.251	669	672	676	rBV	244	212	0.00%	0.001%
15	3.306	687	689	690	rBV	177	63	0.00%	0.000%
16	3.335	696	698	701	rVB2	173	65	0.00%	0.000%
17	3.457	735	736	738	rBV	132	44	0.00%	0.000%
18	3.663	793	800	808	rBV3	484	812	0.01%	0.005%
19	3.769	831	833	834	rBV3	147	73	0.00%	0.000%
20	3.833	851	853	858	rVB	252	124	0.00%	0.001%
21	3.917	868	879	915	rBV2	67923	224329	3.14%	1.434%
22	4.376	1005	1022	1051	rBV2	171831	424390	5.93%	2.712%
23	4.624	1091	1099	1101	rBV2	653	538	0.01%	0.003%
24	4.759	1138	1141	1145	rVB2	536	311	0.00%	0.002%
25	4.785	1145	1149	1151	rBV2	321	250	0.00%	0.002%
26	4.846	1166	1168	1170	rBV2	253	151	0.00%	0.001%
27	4.881	1177	1179	1183	rVB2	230	142	0.00%	0.001%
28	4.904	1183	1186	1188	rBV2	161	115	0.00%	0.001%
29	4.971	1205	1207	1208	rBV	145	38	0.00%	0.000%
30	5.071	1221	1238	1275	rBV2	409052	1061351	14.84%	6.783%
31	5.412	1342	1344	1346	rVB2	286	93	0.00%	0.001%
32	5.566	1389	1392	1397	rVB	467	412	0.01%	0.003%
33	5.640	1398	1415	1441	rBV	343508	683554	9.56%	4.368%
34	5.936	1491	1507	1543	rBV	3687234	7151241	100.00%	45.700%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100120\
 Data File : VV018604.D
 Acq On : 01 Oct 2020 21:34
 Operator : SY/MD
 Sample : L4237-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

35	6.093	1545	1556	1573	rVB	236951	471239	6.59%	3.011%
36	6.466	1669	1672	1675	rVB	342	231	0.00%	0.001%
37	6.492	1675	1680	1683	rBV	245	248	0.00%	0.002%
38	6.527	1689	1691	1694	rBV	262	118	0.00%	0.001%
39	6.572	1702	1705	1709	rBV3	336	272	0.00%	0.002%
40	6.592	1709	1711	1714	rVB2	318	161	0.00%	0.001%
41	6.617	1716	1719	1721	rBV	151	90	0.00%	0.001%
42	6.730	1750	1754	1757	rVB2	281	216	0.00%	0.001%
43	6.749	1757	1760	1763	rBV2	316	287	0.00%	0.002%
44	6.820	1777	1782	1787	rBV3	331	406	0.01%	0.003%
45	6.907	1804	1809	1811	rBV2	300	291	0.00%	0.002%
46	7.006	1830	1840	1863	rBV	137483	250718	3.51%	1.602%
47	7.190	1892	1897	1899	rBV2	629	494	0.01%	0.003%
48	7.232	1908	1910	1912	rBV2	342	195	0.00%	0.001%
49	7.257	1916	1918	1919	rBV2	439	200	0.00%	0.001%
50	7.338	1931	1943	1968	rBV	537354	919514	12.86%	5.876%
51	7.643	2027	2038	2064	rBV	100214	176509	2.47%	1.128%
52	7.952	2128	2134	2137	rBV2	855	865	0.01%	0.006%
53	8.000	2140	2149	2160	rVV4	8802	15115	0.21%	0.097%
54	8.039	2160	2161	2165	rVB2	465	194	0.00%	0.001%
55	8.109	2173	2183	2217	rBV2	220220	447421	6.26%	2.859%
56	8.595	2332	2334	2335	rBV	381	146	0.00%	0.001%
57	8.823	2403	2405	2407	rBV	225	87	0.00%	0.001%
58	8.871	2408	2420	2454	rBV	559698	900229	12.59%	5.753%
59	9.077	2481	2484	2485	rBV2	161	91	0.00%	0.001%
60	9.267	2541	2543	2549	rVB2	328	211	0.00%	0.001%
61	9.293	2549	2551	2554	rBV2	287	144	0.00%	0.001%
62	9.466	2602	2605	2610	rBV3	199	180	0.00%	0.001%
63	9.572	2632	2638	2642	rBV3	684	755	0.01%	0.005%
64	9.688	2672	2674	2680	rBV	167	124	0.00%	0.001%
65	9.833	2716	2719	2722	rBV	296	207	0.00%	0.001%
66	9.891	2731	2737	2742	rBV2	371	381	0.01%	0.002%
67	9.958	2753	2758	2765	rVB3	590	754	0.01%	0.005%
68	9.997	2765	2770	2773	rBV	192	231	0.00%	0.001%
69	10.090	2793	2799	2804	rBV3	402	458	0.01%	0.003%
70	10.238	2833	2845	2865	rBV	271556	430385	6.02%	2.750%
71	10.334	2872	2875	2882	rVB4	430	408	0.01%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100120\
 Data File : VV018604.D
 Acq On : 01 Oct 2020 21:34
 Operator : SY/MD
 Sample : L4237-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

72	10.463	2910	2915	2916	rBV2	377	294	0.00%	0.002%
73	10.566	2940	2947	2956	rVB3	1051	1295	0.02%	0.008%
74	10.768	3006	3010	3012	rVB	368	250	0.00%	0.002%
75	10.868	3038	3041	3043	rVB	244	128	0.00%	0.001%
76	10.884	3043	3046	3050	rBV2	208	152	0.00%	0.001%
77	11.038	3090	3094	3098	rVB2	343	323	0.00%	0.002%
78	11.270	3154	3166	3189	rBV	568004	863013	12.07%	5.515%
79	11.563	3251	3257	3258	rBV4	987	913	0.01%	0.006%
80	11.646	3270	3283	3303	rBV	543605	848759	11.87%	5.424%
81	11.788	3324	3327	3329	rBV2	473	358	0.01%	0.002%
82	11.948	3375	3377	3378	rBV2	242	82	0.00%	0.001%
83	12.083	3416	3419	3422	rBV	380	216	0.00%	0.001%
84	12.193	3448	3453	3455	rBV	304	289	0.00%	0.002%
85	12.235	3464	3466	3468	rBV	290	166	0.00%	0.001%
86	12.418	3520	3523	3524	rBV	332	204	0.00%	0.001%
87	12.582	3571	3574	3576	rBV3	372	234	0.00%	0.001%
88	12.675	3600	3603	3607	rVB3	479	283	0.00%	0.002%
89	12.768	3630	3632	3634	rBV	315	171	0.00%	0.001%
90	13.083	3728	3730	3733	rVB2	246	95	0.00%	0.001%
91	13.357	3813	3815	3818	rBV2	395	205	0.00%	0.001%
92	14.222	4082	4084	4087	rBV	382	219	0.00%	0.001%


Sum of corrected areas: 15648210

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100120\
Data File : VV018604.D
Acq On : 01 Oct 2020 21:34
Operator : SY/MD
Sample : L4237-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

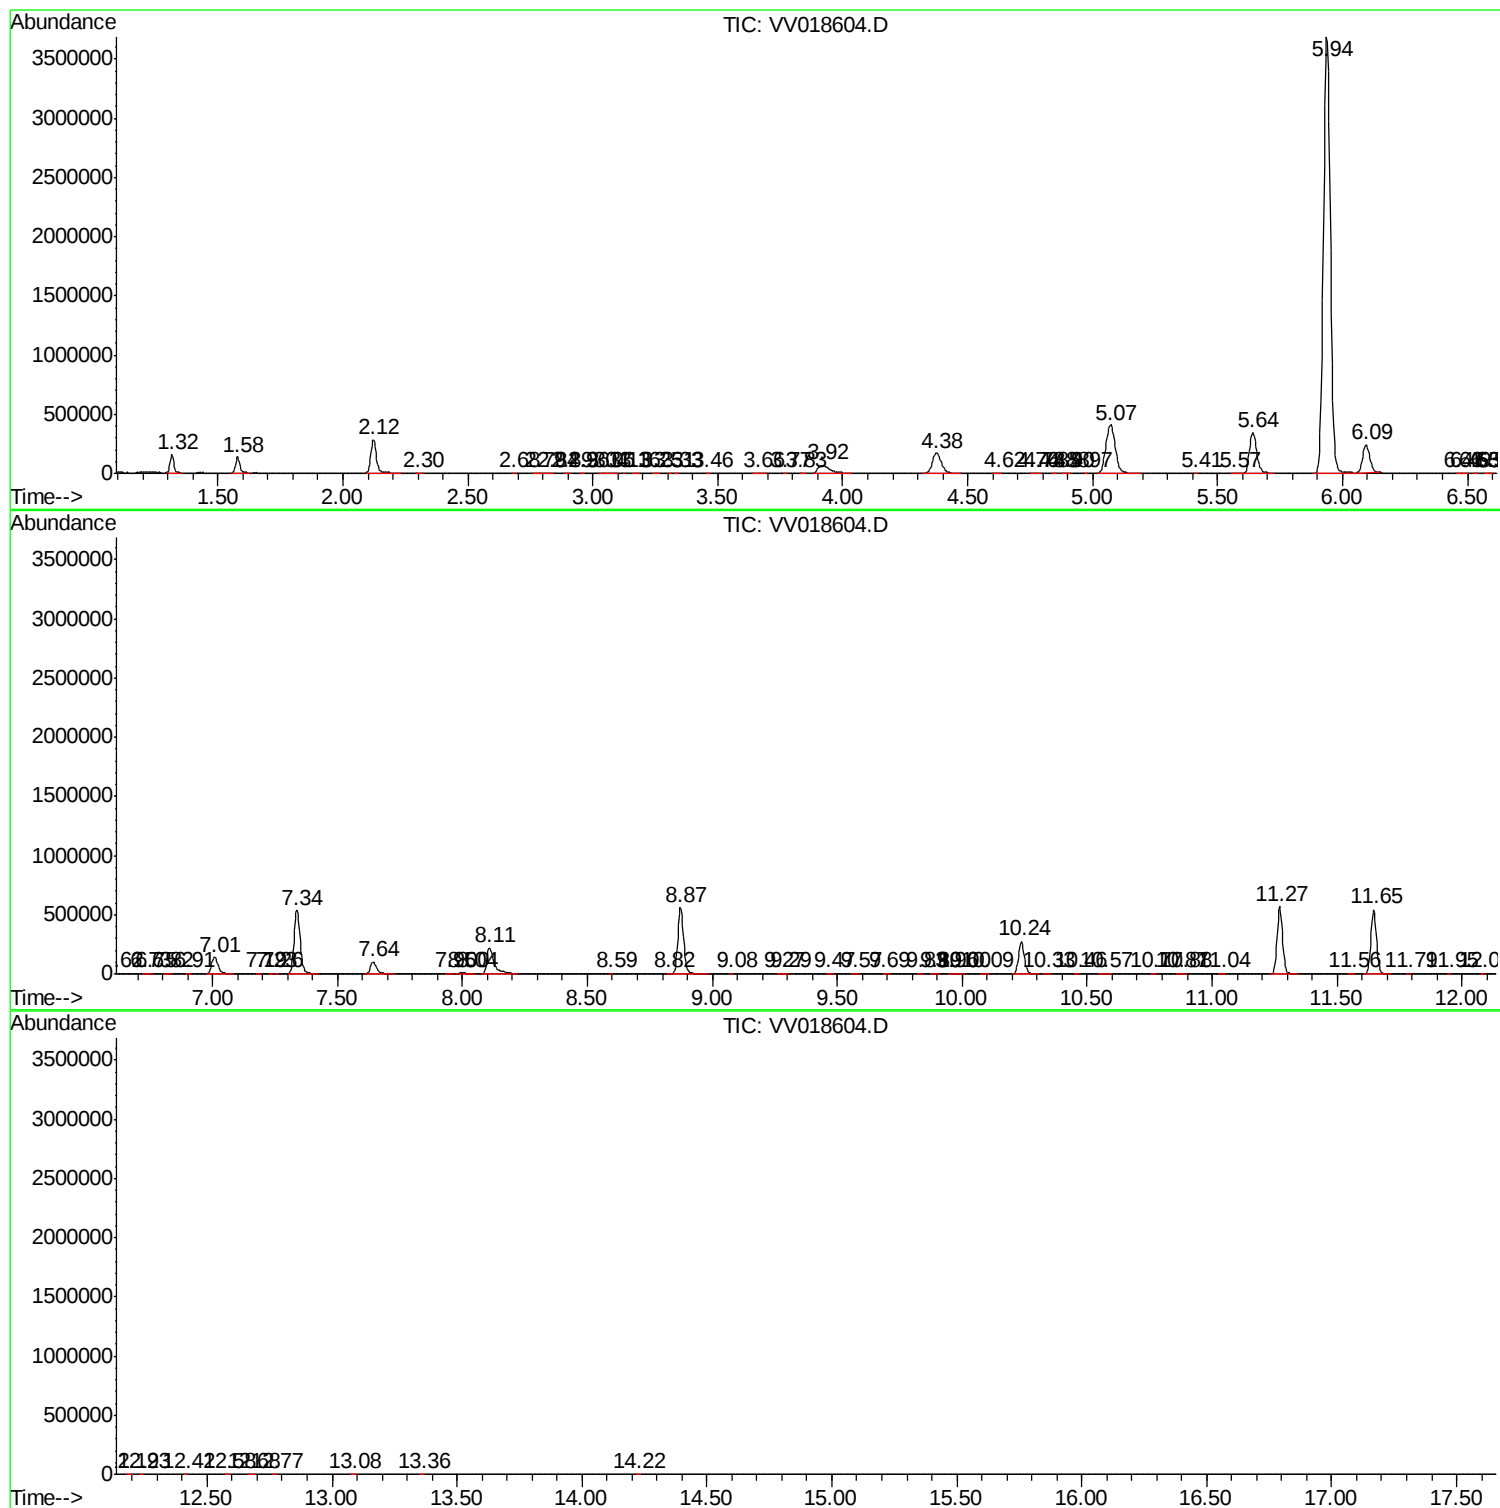

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV100120\
Data File : VV018604.D
Acq On : 01 Oct 2020 21:34
Operator : SY/MD
Sample : L4237-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV100120\
Data File : VV018604.D
Acq On : 01 Oct 2020 21:34
Operator : SY/MD
Sample : L4237-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc