

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100120\
 Data File : VV018606.D
 Acq On : 01 Oct 2020 22:21
 Operator : SY/MD
 Sample : L4237-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	76	rBV	145167	161488	15.87%	1.998%
2	1.579	147	152	162	rVB	129062	142977	14.05%	1.769%
3	2.122	313	321	348	rVB	276989	426209	41.88%	5.274%
4	2.891	558	560	564	rVB2	362	243	0.02%	0.003%
5	3.058	607	612	613	rBV2	1350	1093	0.11%	0.014%
6	3.171	645	647	650	rBV	197	126	0.01%	0.002%
7	3.241	667	669	672	rVB2	165	70	0.01%	0.001%
8	3.425	724	726	729	rBV2	140	100	0.01%	0.001%
9	3.466	735	739	741	rBV2	273	201	0.02%	0.002%
10	3.569	769	771	773	rBV2	249	124	0.01%	0.002%
11	3.634	788	791	793	rBV2	158	92	0.01%	0.001%
12	3.752	824	828	830	rBV	283	247	0.02%	0.003%
13	3.791	837	840	844	rVB	341	236	0.02%	0.003%
14	3.810	844	846	847	rBV	165	53	0.01%	0.001%
15	3.916	867	879	917	rBV	66798	217626	21.38%	2.693%
16	4.180	958	961	968	rVB3	567	536	0.05%	0.007%
17	4.376	1006	1022	1045	rBV	165630	403380	39.64%	4.991%
18	4.547	1072	1075	1076	rBV	362	248	0.02%	0.003%
19	4.572	1081	1083	1085	rBV2	401	189	0.02%	0.002%
20	4.711	1120	1126	1133	rBV4	652	625	0.06%	0.008%
21	4.769	1141	1144	1148	rBV3	285	250	0.02%	0.003%
22	4.794	1148	1152	1157	rVB3	254	239	0.02%	0.003%
23	4.846	1166	1168	1171	rBV2	276	126	0.01%	0.002%
24	4.916	1186	1190	1194	rBV2	390	274	0.03%	0.003%
25	4.978	1207	1209	1213	rVB	274	125	0.01%	0.002%
26	5.071	1220	1238	1260	rBV2	398170	1017732	100.00%	12.593%
27	5.351	1323	1325	1327	rBV2	300	110	0.01%	0.001%
28	5.415	1342	1345	1349	rVB2	236	167	0.02%	0.002%
29	5.434	1349	1351	1352	rBV2	297	110	0.01%	0.001%
30	5.543	1381	1385	1388	rBV2	273	168	0.02%	0.002%
31	5.598	1399	1402	1403	rBV	349	184	0.02%	0.002%
32	5.640	1403	1415	1439	rVV	341145	677537	66.57%	8.383%
33	5.932	1495	1506	1524	rBV7	19389	43268	4.25%	0.535%
34	6.093	1543	1556	1584	rBV	226662	461402	45.34%	5.709%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100120\
 Data File : VV018606.D
 Acq On : 01 Oct 2020 22:21
 Operator : SY/MD
 Sample : L4237-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

35	6.347	1633	1635	1641	rBV3	455	333	0.03%	0.004%
36	6.421	1654	1658	1663	rVB	5902	3280	0.32%	0.041%
37	6.479	1673	1676	1677	rBV	238	135	0.01%	0.002%
38	6.540	1692	1695	1698	rBV	301	199	0.02%	0.002%
39	6.563	1698	1702	1707	rVV2	254	275	0.03%	0.003%
40	6.707	1745	1747	1751	rVV2	356	195	0.02%	0.002%
41	6.727	1751	1753	1756	rVB2	393	210	0.02%	0.003%
42	6.772	1766	1767	1768	rBV2	140	43	0.00%	0.001%
43	6.826	1781	1784	1788	rBV	191	144	0.01%	0.002%
44	7.006	1829	1840	1863	rBV	120266	219711	21.59%	2.719%
45	7.219	1903	1906	1907	rBV	329	192	0.02%	0.002%
46	7.251	1914	1916	1919	rVB2	283	139	0.01%	0.002%
47	7.270	1919	1922	1923	rBV2	320	128	0.01%	0.002%
48	7.296	1927	1930	1931	rBV	370	203	0.02%	0.003%
49	7.338	1931	1943	1965	rBV	479487	814075	79.99%	10.073%
50	7.643	2028	2038	2053	rBV	82099	141688	13.92%	1.753%
51	7.820	2090	2093	2094	rBV2	404	187	0.02%	0.002%
52	7.923	2123	2125	2127	rBV	169	97	0.01%	0.001%
53	7.945	2128	2132	2133	rBV	745	524	0.05%	0.006%
54	8.109	2172	2183	2224	rBV2	197672	409758	40.26%	5.070%
55	8.405	2272	2275	2276	rBV2	433	227	0.02%	0.003%
56	8.646	2348	2350	2353	rBV	338	186	0.02%	0.002%
57	8.662	2353	2355	2361	rVB2	369	206	0.02%	0.003%
58	8.746	2378	2381	2383	rBV	168	86	0.01%	0.001%
59	8.871	2408	2420	2441	rBV	522910	844601	82.99%	10.450%
60	9.157	2506	2509	2511	rBV2	1165	825	0.08%	0.010%
61	9.289	2546	2550	2552	rVB	430	232	0.02%	0.003%
62	9.309	2552	2556	2557	rBV2	251	165	0.02%	0.002%
63	9.566	2633	2636	2638	rBV3	351	288	0.03%	0.004%
64	9.595	2644	2645	2647	rVB2	506	128	0.01%	0.002%
65	9.682	2671	2672	2676	rVB	234	81	0.01%	0.001%
66	10.058	2787	2789	2793	rBV2	295	217	0.02%	0.003%
67	10.138	2811	2814	2816	rVB2	386	223	0.02%	0.003%
68	10.238	2829	2845	2863	rBV	286985	447658	43.99%	5.539%
69	10.402	2891	2896	2907	rVB6	1842	2402	0.24%	0.030%
70	10.608	2958	2960	2965	rBV2	263	185	0.02%	0.002%
71	10.717	2987	2994	2998	rBV2	425	569	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100120\
Data File : VV018606.D
Acq On : 01 Oct 2020 22:21
Operator : SY/MD
Sample : L4237-08
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC3

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Title : VOC Analysis

72	10.939	3054	3063	3072	rBV3	1478	2340	0.23%	0.029%
73	11.183	3135	3139	3142	rBV2	329	276	0.03%	0.003%
74	11.270	3154	3166	3191	rBV	550035	835860	82.13%	10.342%
75	11.559	3251	3256	3258	rBV3	1435	1254	0.12%	0.016%
76	11.646	3271	3283	3301	rBV	512909	794609	78.08%	9.832%
77	11.977	3383	3386	3388	rBV	308	175	0.02%	0.002%
78	13.530	3866	3869	3870	rBV2	279	136	0.01%	0.002%


Sum of corrected areas: 8082000

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100120\
Data File : VV018606.D
Acq On : 01 Oct 2020 22:21
Operator : SY/MD
Sample : L4237-08
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

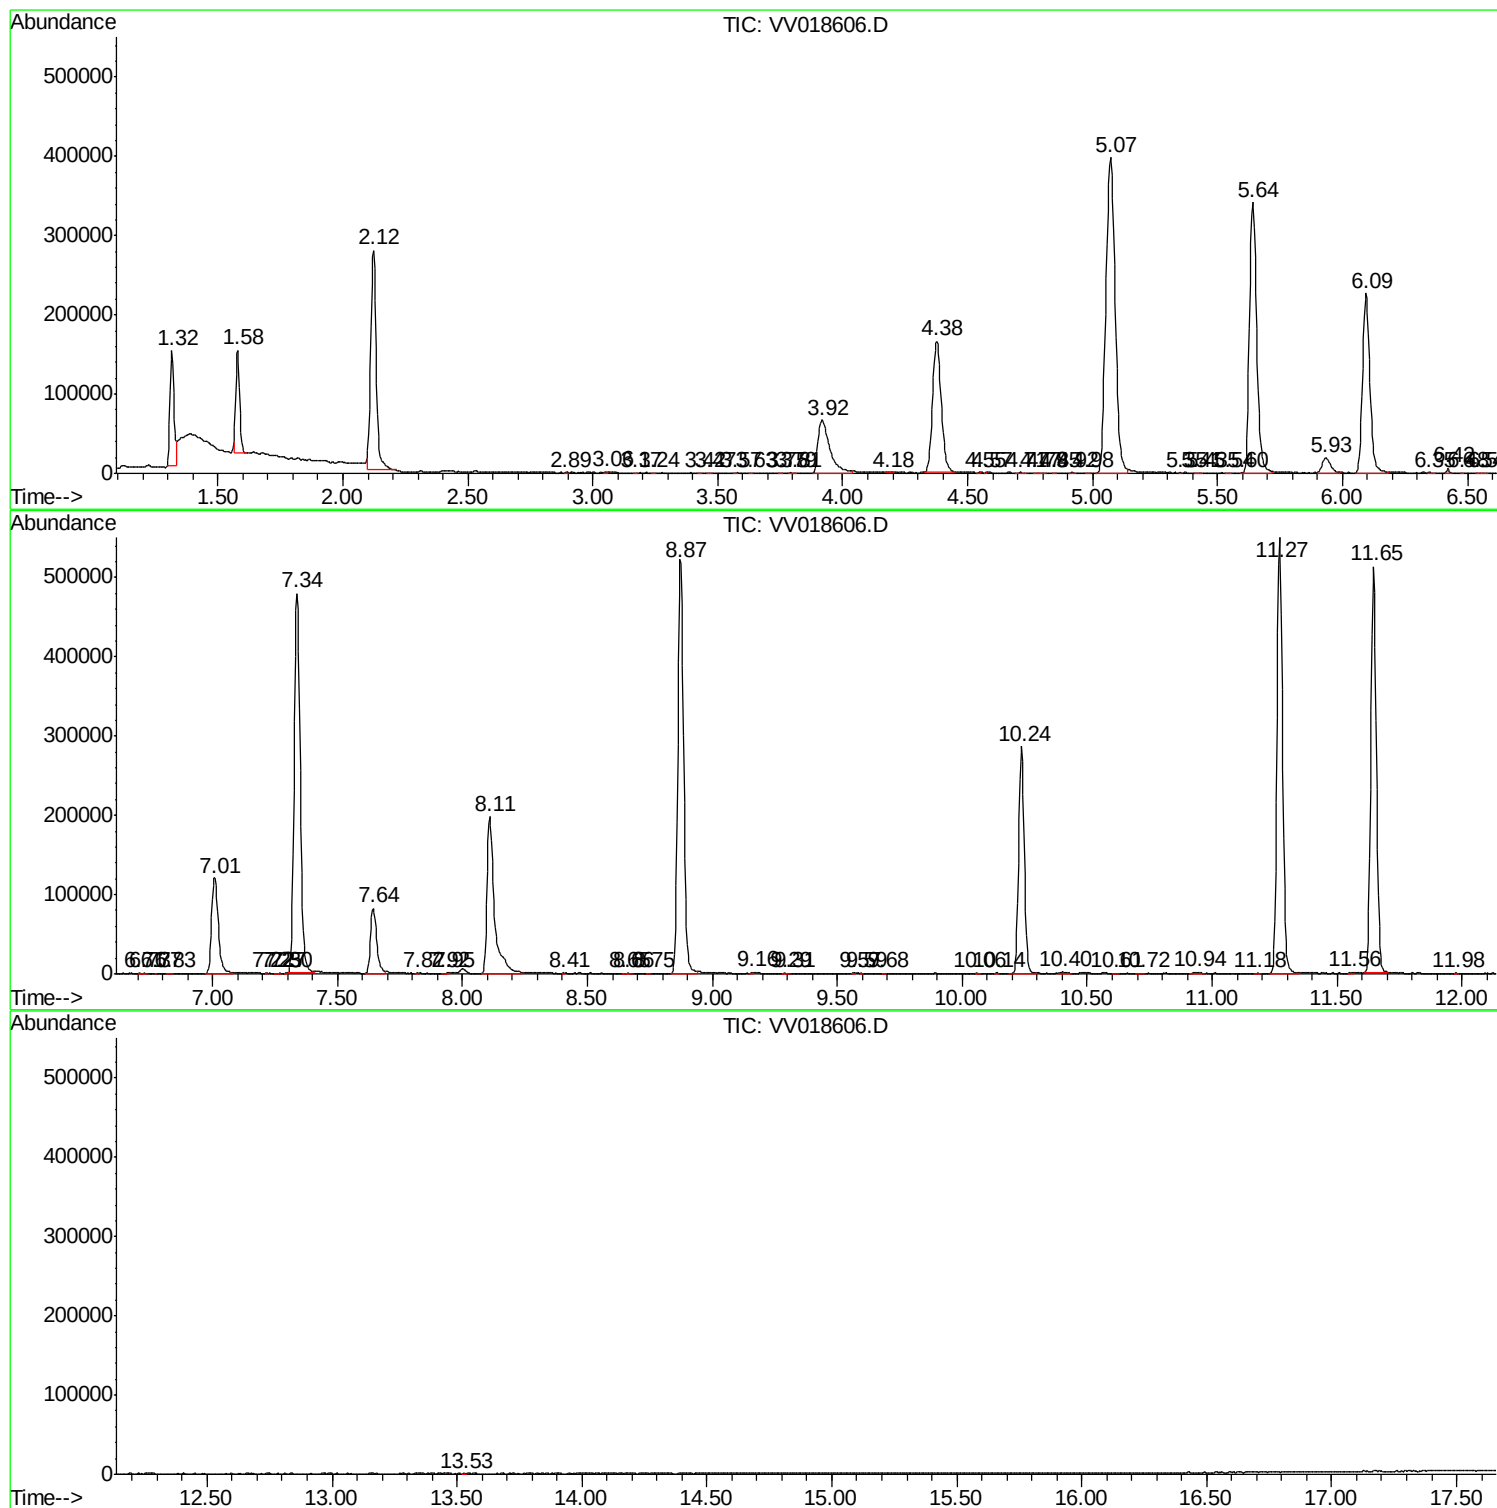

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV100120\
Data File : VV018606.D
Acq On : 01 Oct 2020 22:21
Operator : SY/MD
Sample : L4237-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV100120\
Data File : VV018606.D
Acq On : 01 Oct 2020 22:21
Operator : SY/MD
Sample : L4237-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc