

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100120\
 Data File : VV018609.D
 Acq On : 01 Oct 2020 23:32
 Operator : SY/MD
 Sample : L4237-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	82	rVB	142503	138089	11.17%	1.477%
2	1.579	145	152	166	rVB	130236	149335	12.08%	1.597%
3	2.123	312	321	361	rVB	273139	435036	35.19%	4.653%
4	2.779	520	525	527	rBV2	1189	1019	0.08%	0.011%
5	2.827	538	540	542	rBV3	273	151	0.01%	0.002%
6	3.061	608	613	614	rBV2	931	737	0.06%	0.008%
7	3.107	625	627	630	rVB	175	82	0.01%	0.001%
8	3.126	631	633	636	rVB2	225	90	0.01%	0.001%
9	3.299	683	687	690	rBV2	284	263	0.02%	0.003%
10	3.367	705	708	709	rBV2	120	64	0.01%	0.001%
11	3.422	720	725	728	rBV2	345	257	0.02%	0.003%
12	3.518	753	755	757	rVB	142	53	0.00%	0.001%
13	3.573	768	772	778	rBV2	379	430	0.03%	0.005%
14	3.605	778	782	784	rBV2	227	194	0.02%	0.002%
15	3.688	807	808	811	rBV	167	108	0.01%	0.001%
16	3.730	819	821	822	rBV	188	80	0.01%	0.001%
17	3.775	832	835	840	rBV2	283	276	0.02%	0.003%
18	3.920	869	880	924	rBV2	62227	213028	17.23%	2.278%
19	4.377	1006	1022	1045	rBV	164115	401942	32.52%	4.299%
20	4.611	1093	1095	1097	rBV	222	85	0.01%	0.001%
21	4.631	1097	1101	1105	rBV3	384	342	0.03%	0.004%
22	4.650	1105	1107	1109	rBV	198	92	0.01%	0.001%
23	4.733	1129	1133	1138	rBV3	379	279	0.02%	0.003%
24	4.778	1144	1147	1149	rBV	253	168	0.01%	0.002%
25	4.817	1156	1159	1164	rBV2	190	168	0.01%	0.002%
26	4.917	1188	1190	1192	rBV	123	37	0.00%	0.000%
27	5.071	1221	1238	1262	rBV2	399747	1016499	82.24%	10.872%
28	5.338	1317	1321	1325	rBV3	300	300	0.02%	0.003%
29	5.367	1328	1330	1337	rVB2	268	145	0.01%	0.002%
30	5.428	1348	1349	1350	rBV	196	58	0.00%	0.001%
31	5.534	1380	1382	1385	rBV2	220	111	0.01%	0.001%
32	5.640	1399	1415	1444	rBV	340916	677046	54.77%	7.242%
33	5.936	1493	1507	1529	rBV	631644	1236078	100.00%	13.221%
34	6.094	1544	1556	1580	rVB	223581	445476	36.04%	4.765%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100120\
 Data File : VV018609.D
 Acq On : 01 Oct 2020 23:32
 Operator : SY/MD
 Sample : L4237-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

35	6.290	1615	1617	1619	rBV2	247	127	0.01%	0.001%
36	6.319	1624	1626	1628	rVB	416	197	0.02%	0.002%
37	6.331	1628	1630	1633	rBV2	391	127	0.01%	0.001%
38	6.409	1652	1654	1655	rBV	273	108	0.01%	0.001%
39	6.444	1663	1665	1668	rBV	283	111	0.01%	0.001%
40	6.508	1682	1685	1687	rBV	177	107	0.01%	0.001%
41	6.544	1693	1696	1698	rVB	196	111	0.01%	0.001%
42	6.708	1743	1747	1748	rBV2	460	220	0.02%	0.002%
43	6.775	1766	1768	1772	rVB2	236	132	0.01%	0.001%
44	6.798	1773	1775	1778	rVB2	269	151	0.01%	0.002%
45	6.913	1806	1811	1814	rVB2	352	258	0.02%	0.003%
46	6.933	1814	1817	1818	rBV	198	112	0.01%	0.001%
47	7.007	1830	1840	1861	rBV	121312	223215	18.06%	2.387%
48	7.177	1890	1893	1898	rBV4	339	299	0.02%	0.003%
49	7.196	1898	1899	1903	rVB	327	140	0.01%	0.001%
50	7.222	1903	1907	1910	rBV2	438	348	0.03%	0.004%
51	7.338	1931	1943	1968	rBV	472192	813998	65.85%	8.706%
52	7.643	2028	2038	2065	rBV	87004	154893	12.53%	1.657%
53	7.910	2119	2121	2123	rBV	269	142	0.01%	0.002%
54	7.939	2127	2130	2131	rBV2	368	184	0.01%	0.002%
55	8.000	2142	2149	2159	rVB3	4801	7962	0.64%	0.085%
56	8.110	2172	2183	2225	rBV2	201453	404630	32.73%	4.328%
57	8.370	2262	2264	2267	rBV3	362	184	0.01%	0.002%
58	8.595	2332	2334	2337	rBV2	285	193	0.02%	0.002%
59	8.753	2382	2383	2388	rVB2	420	212	0.02%	0.002%
60	8.798	2394	2397	2400	rVB	421	232	0.02%	0.002%
61	8.814	2400	2402	2404	rBV	250	107	0.01%	0.001%
62	8.827	2404	2406	2407	rBV	206	70	0.01%	0.001%
63	8.872	2409	2420	2449	rBV	559890	897011	72.57%	9.594%
64	9.183	2515	2517	2519	rBV	342	172	0.01%	0.002%
65	9.572	2636	2638	2641	rVB	603	232	0.02%	0.002%
66	9.788	2704	2705	2707	rBV	245	105	0.01%	0.001%
67	9.852	2722	2725	2730	rBV2	370	252	0.02%	0.003%
68	9.907	2741	2742	2743	rBV2	196	51	0.00%	0.001%
69	9.917	2743	2745	2746	rBV2	255	104	0.01%	0.001%
70	10.238	2833	2845	2865	rBV	309670	476450	38.55%	5.096%
71	10.560	2943	2945	2950	rBV3	502	382	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100120\
 Data File : VV018609.D
 Acq On : 01 Oct 2020 23:32
 Operator : SY/MD
 Sample : L4237-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

72	10.772	3008	3011	3014	rBV2	394	306	0.02%	0.003%
73	11.174	3134	3136	3137	rBV2	230	87	0.01%	0.001%
74	11.270	3155	3166	3189	rBV	548186	846868	68.51%	9.058%
75	11.556	3250	3255	3256	rBV2	1716	1302	0.11%	0.014%
76	11.646	3271	3283	3301	rBV	509980	796717	64.46%	8.521%
77	11.804	3330	3332	3335	rBV	316	184	0.01%	0.002%
78	11.842	3343	3344	3347	rBV	315	129	0.01%	0.001%
79	12.003	3392	3394	3399	rBV	286	217	0.02%	0.002%
80	12.408	3517	3520	3521	rBV	175	119	0.01%	0.001%
81	12.746	3623	3625	3629	rBV	372	226	0.02%	0.002%
82	13.579	3881	3884	3891	rVB3	451	450	0.04%	0.005%
83	13.662	3908	3910	3912	rBV	313	141	0.01%	0.002%
84	13.675	3912	3914	3919	rVV	433	263	0.02%	0.003%
85	13.720	3926	3928	3930	rBV	306	130	0.01%	0.001%
86	13.778	3944	3946	3948	rBV	359	149	0.01%	0.002%
87	14.067	4034	4036	4039	rVB2	420	192	0.02%	0.002%
88	14.141	4056	4059	4062	rBV	550	303	0.02%	0.003%
89	14.251	4090	4093	4095	rBV2	404	268	0.02%	0.003%


Sum of corrected areas: 9349498

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100120\
Data File : VV018609.D
Acq On : 01 Oct 2020 23:32
Operator : SY/MD
Sample : L4237-11
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

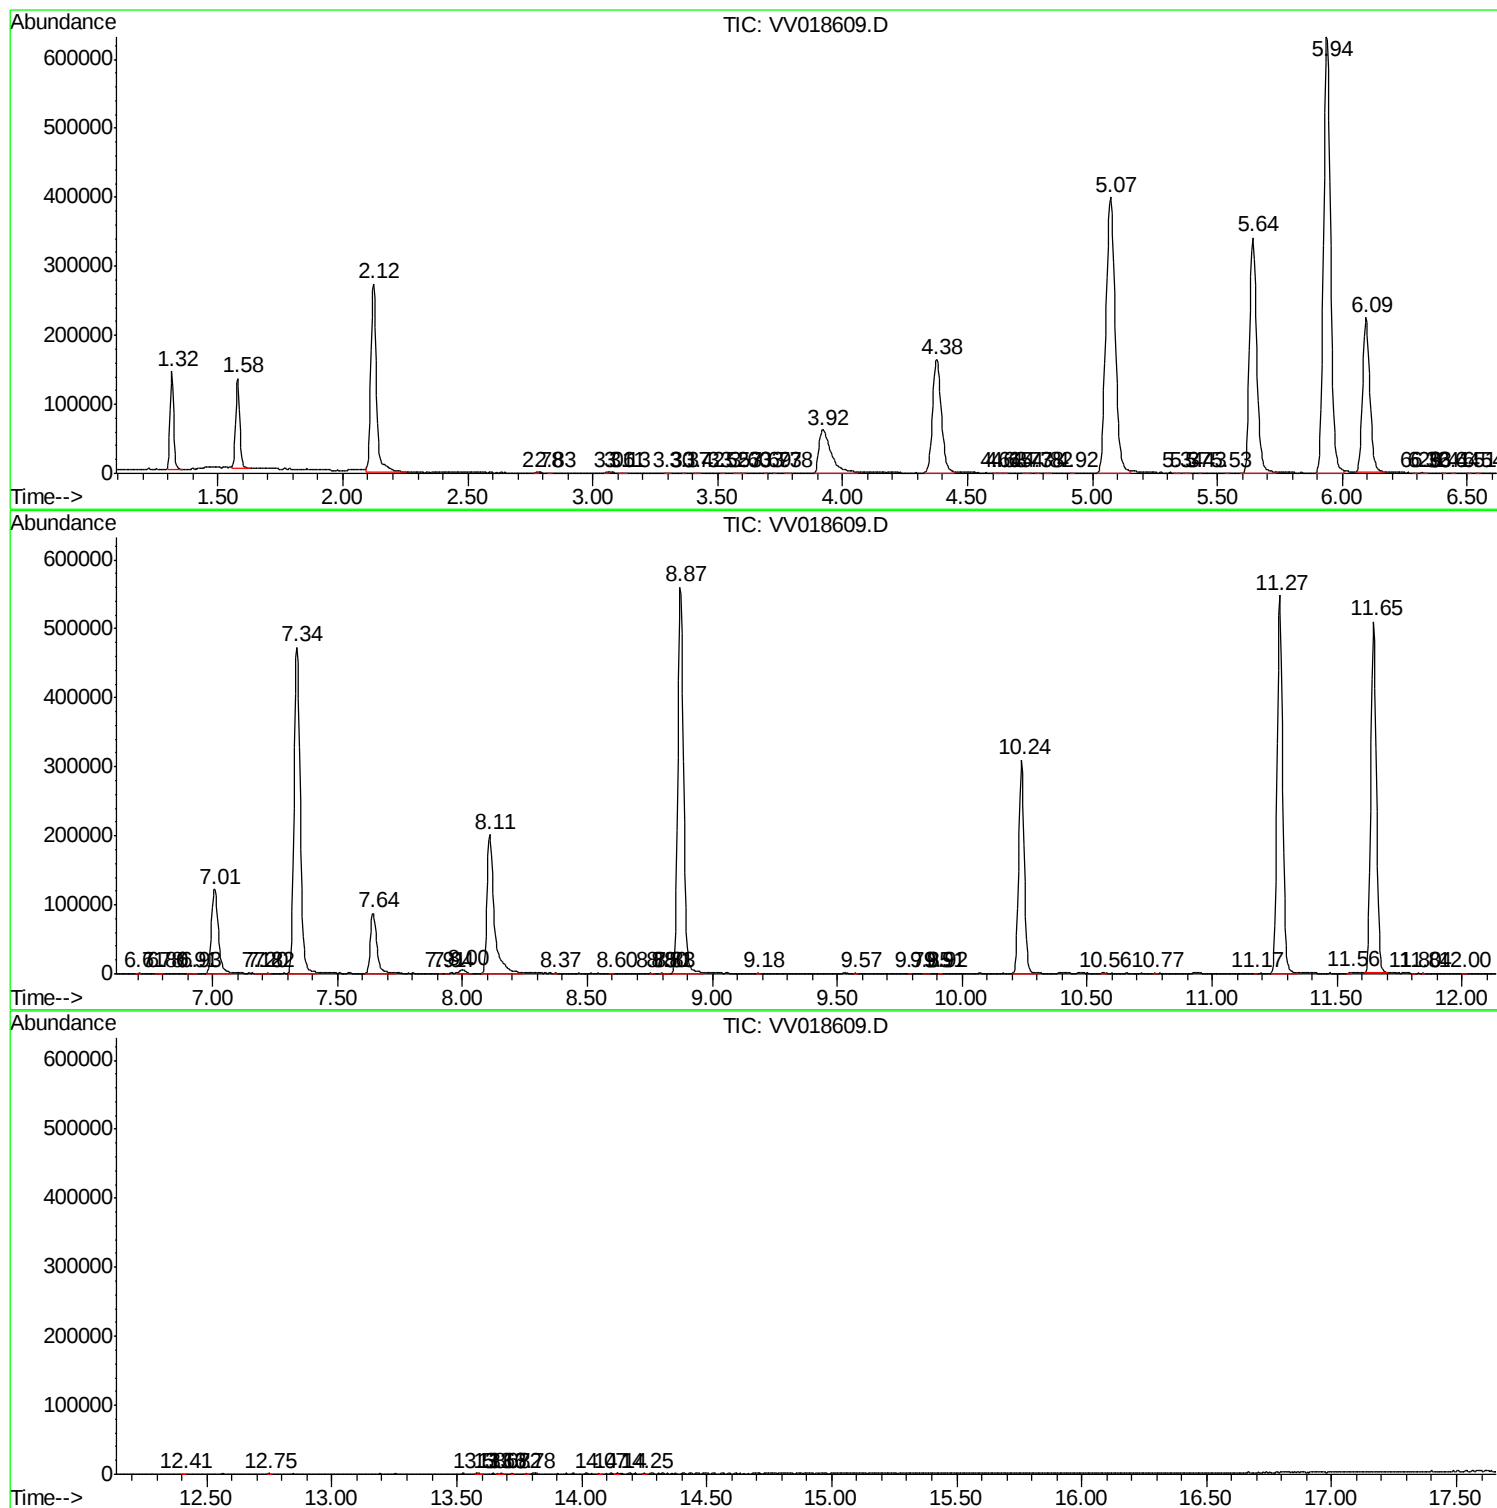

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV100120\
Data File : VV018609.D
Acq On : 01 Oct 2020 23:32
Operator : SY/MD
Sample : L4237-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV100120\
Data File : VV018609.D
Acq On : 01 Oct 2020 23:32
Operator : SY/MD
Sample : L4237-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc