

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100120\
 Data File : VV018610.D
 Acq On : 01 Oct 2020 23:56
 Operator : SY/MD
 Sample : L4237-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	147058	142048	4.84%	1.288%
2	1.579	145	152	165	rVB	139303	156632	5.34%	1.420%
3	2.123	311	321	341	rBV	275154	410785	14.00%	3.724%
4	2.901	561	563	564	rVB2	214	52	0.00%	0.000%
5	2.933	569	573	574	rBV	282	215	0.01%	0.002%
6	2.978	583	587	589	rBV	239	166	0.01%	0.002%
7	3.042	605	607	608	rBV	308	86	0.00%	0.001%
8	3.065	608	614	619	rVV4	1102	1415	0.05%	0.013%
9	3.139	635	637	645	rVB2	274	345	0.01%	0.003%
10	3.171	645	647	649	rBV	288	113	0.00%	0.001%
11	3.190	651	653	656	rVB	217	78	0.00%	0.001%
12	3.341	698	700	702	rVB2	159	72	0.00%	0.001%
13	3.489	742	746	747	rBV2	292	157	0.01%	0.001%
14	3.753	826	828	829	rBV	174	60	0.00%	0.001%
15	3.788	836	839	842	rBV2	174	140	0.00%	0.001%
16	3.923	868	881	922	rBV	64570	215640	7.35%	1.955%
17	4.376	1007	1022	1047	rBV	169630	411726	14.04%	3.732%
18	4.589	1085	1088	1089	rBV	382	250	0.01%	0.002%
19	4.839	1161	1166	1170	rVB2	336	310	0.01%	0.003%
20	4.904	1183	1186	1188	rBV	157	97	0.00%	0.001%
21	4.942	1195	1198	1202	rBV	144	107	0.00%	0.001%
22	4.987	1209	1212	1214	rBV	196	154	0.01%	0.001%
23	5.071	1220	1238	1277	rBV2	400832	1034992	35.28%	9.383%
24	5.447	1353	1355	1358	rVB	217	84	0.00%	0.001%
25	5.511	1373	1375	1379	rVB2	296	160	0.01%	0.001%
26	5.537	1379	1383	1386	rBV	185	195	0.01%	0.002%
27	5.582	1394	1397	1399	rBV2	110	66	0.00%	0.001%
28	5.640	1402	1415	1442	rBV	327803	663630	22.62%	6.016%
29	5.936	1493	1507	1543	rBV	1501199	2933555	100.00%	26.594%
30	6.093	1544	1556	1585	rVB	231871	472544	16.11%	4.284%
31	6.296	1618	1619	1623	rVB	573	241	0.01%	0.002%
32	6.328	1624	1629	1632	rVV4	452	321	0.01%	0.003%
33	6.380	1643	1645	1647	rBV	220	145	0.00%	0.001%
34	6.486	1674	1678	1680	rBV	275	203	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100120\
 Data File : VV018610.D
 Acq On : 01 Oct 2020 23:56
 Operator : SY/MD
 Sample : L4237-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

35	6.563	1701	1702	1703	rBV	135	34	0.00%	0.000%
36	6.640	1725	1726	1728	rBV	241	87	0.00%	0.001%
37	6.695	1741	1743	1747	rBV	220	191	0.01%	0.002%
38	6.791	1770	1773	1775	rBV2	172	131	0.00%	0.001%
39	6.827	1782	1784	1786	rBV2	227	103	0.00%	0.001%
40	6.888	1798	1803	1806	rVB2	249	250	0.01%	0.002%
41	6.907	1806	1809	1811	rBV	109	73	0.00%	0.001%
42	6.942	1818	1820	1823	rVB2	287	100	0.00%	0.001%
43	7.010	1829	1841	1861	rBV	130095	230844	7.87%	2.093%
44	7.257	1916	1918	1920	rBV2	326	153	0.01%	0.001%
45	7.338	1927	1943	1962	rBV	486229	837413	28.55%	7.592%
46	7.589	2018	2021	2024	rBV2	306	234	0.01%	0.002%
47	7.605	2024	2026	2028	rBV3	258	149	0.01%	0.001%
48	7.643	2028	2038	2058	rBV	92248	159010	5.42%	1.441%
49	7.788	2080	2083	2086	rBV	630	468	0.02%	0.004%
50	7.833	2095	2097	2100	rVB3	533	272	0.01%	0.002%
51	7.849	2100	2102	2105	rBV2	176	102	0.00%	0.001%
52	7.942	2129	2131	2132	rBV	212	82	0.00%	0.001%
53	8.000	2142	2149	2160	rVB6	5564	9631	0.33%	0.087%
54	8.109	2173	2183	2220	rBV2	205755	410931	14.01%	3.725%
55	8.347	2255	2257	2259	rBV2	386	140	0.00%	0.001%
56	8.360	2259	2261	2267	rVB2	610	414	0.01%	0.004%
57	8.389	2267	2270	2271	rBV	389	198	0.01%	0.002%
58	8.563	2322	2324	2328	rVB	349	219	0.01%	0.002%
59	8.582	2328	2330	2332	rBV2	209	132	0.00%	0.001%
60	8.685	2358	2362	2364	rBV2	196	162	0.01%	0.001%
61	8.826	2402	2406	2409	rBV2	313	315	0.01%	0.003%
62	8.871	2409	2420	2438	rBV	515209	832607	28.38%	7.548%
63	9.135	2500	2502	2503	rBV	277	103	0.00%	0.001%
64	9.170	2511	2513	2514	rBV	299	126	0.00%	0.001%
65	9.212	2524	2526	2531	rVB2	319	165	0.01%	0.001%
66	9.556	2631	2633	2636	rBV	308	159	0.01%	0.001%
67	9.588	2640	2643	2644	rBV2	163	91	0.00%	0.001%
68	9.614	2648	2651	2654	rBV	326	200	0.01%	0.002%
69	9.939	2749	2752	2755	rBV	219	140	0.00%	0.001%
70	10.026	2777	2779	2787	rVB2	311	287	0.01%	0.003%
71	10.087	2795	2798	2800	rBV	240	118	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100120\
 Data File : VV018610.D
 Acq On : 01 Oct 2020 23:56
 Operator : SY/MD
 Sample : L4237-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

72	10.238	2833	2845	2868	rBV	277781	437172	14.90%	3.963%
73	11.064	3098	3102	3103	rBV2	557	455	0.02%	0.004%
74	11.203	3142	3145	3149	rVB2	269	202	0.01%	0.002%
75	11.270	3152	3166	3189	rBV	545144	833555	28.41%	7.557%
76	11.646	3271	3283	3303	rBV	531180	825677	28.15%	7.485%
77	12.248	3466	3470	3473	rBV2	331	273	0.01%	0.002%
78	12.350	3498	3502	3505	rBV2	374	319	0.01%	0.003%
79	12.370	3505	3508	3510	rVV2	353	223	0.01%	0.002%
80	12.794	3638	3640	3643	rBV2	308	143	0.00%	0.001%
81	13.505	3857	3861	3863	rBV	367	269	0.01%	0.002%


Sum of corrected areas: 11030906

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100120\
Data File : VV018610.D
Acq On : 01 Oct 2020 23:56
Operator : SY/MD
Sample : L4237-12
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

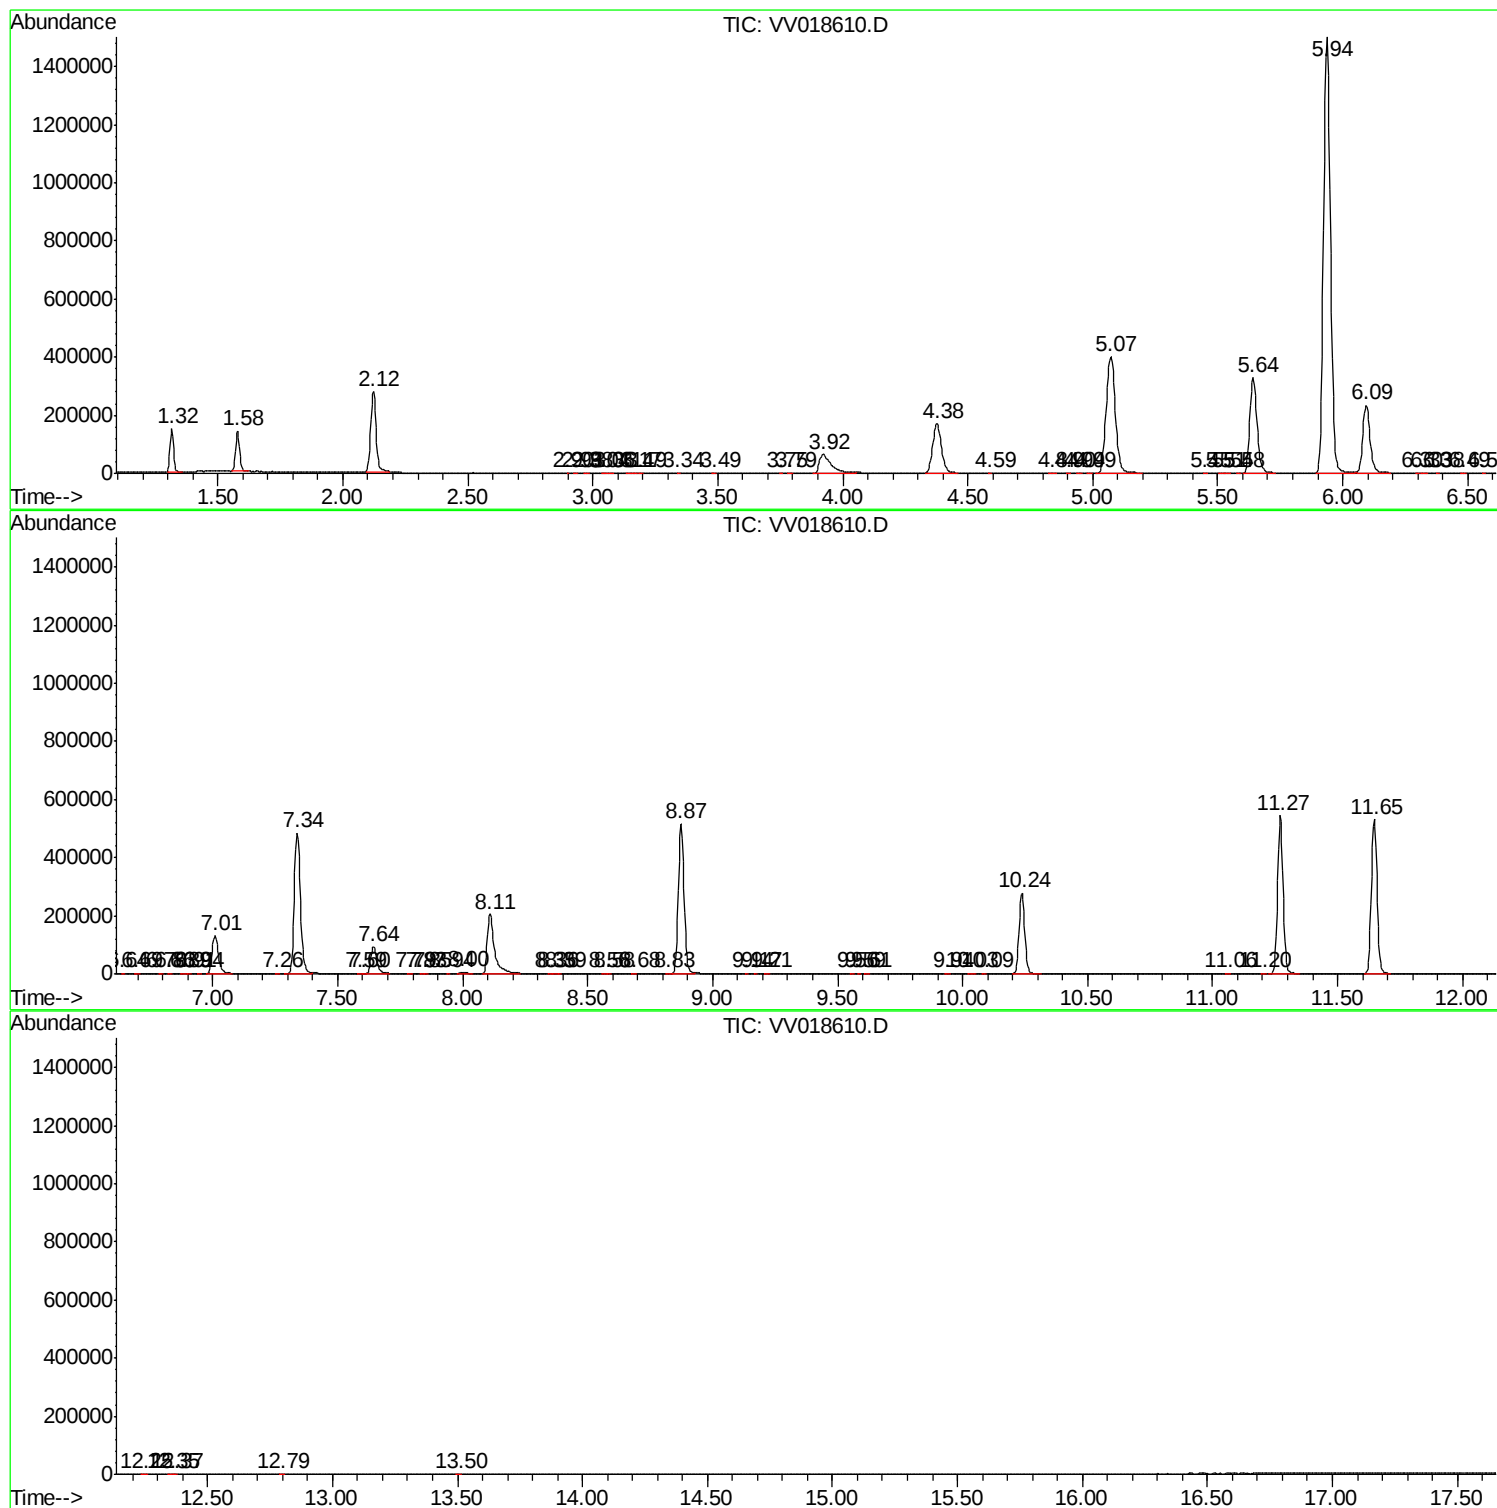

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV100120\
Data File : VV018610.D
Acq On : 01 Oct 2020 23:56
Operator : SY/MD
Sample : L4237-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV100120\
Data File : VV018610.D
Acq On : 01 Oct 2020 23:56
Operator : SY/MD
Sample : L4237-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc