

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100120\
 Data File : VV018611.D
 Acq On : 02 Oct 2020 00:19
 Operator : SY/MD
 Sample : L4237-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	86	rVB	137979	138143	13.83%	1.721%
2	1.579	145	152	163	rVB	135521	148972	14.91%	1.856%
3	2.122	312	321	353	rVB	271160	423232	42.37%	5.272%
4	2.627	475	478	479	rBV2	531	341	0.03%	0.004%
5	2.910	563	566	567	rBV	222	103	0.01%	0.001%
6	3.048	605	609	610	rBV2	393	232	0.02%	0.003%
7	3.061	610	613	621	rVB3	952	1085	0.11%	0.014%
8	3.148	638	640	645	rBV	261	171	0.02%	0.002%
9	3.171	645	647	653	rVB2	372	297	0.03%	0.004%
10	3.203	653	657	660	rBV	249	218	0.02%	0.003%
11	3.219	660	662	664	rBV	190	92	0.01%	0.001%
12	3.293	681	685	686	rBV	387	147	0.01%	0.002%
13	3.328	693	696	699	rBV2	163	131	0.01%	0.002%
14	3.421	720	725	728	rBV2	324	309	0.03%	0.004%
15	3.463	736	738	740	rBV	144	94	0.01%	0.001%
16	3.756	826	829	835	rBV	239	228	0.02%	0.003%
17	3.842	854	856	858	rBV	242	144	0.01%	0.002%
18	3.923	869	881	914	rBV	63060	207428	20.77%	2.584%
19	4.376	1005	1022	1048	rBV	165200	404105	40.46%	5.034%
20	4.643	1104	1105	1107	rBV	232	94	0.01%	0.001%
21	4.669	1109	1113	1114	rBV	339	241	0.02%	0.003%
22	4.733	1130	1133	1136	rBV2	145	125	0.01%	0.002%
23	4.749	1136	1138	1141	rVV	280	136	0.01%	0.002%
24	4.868	1173	1175	1177	rBV	132	48	0.00%	0.001%
25	4.929	1192	1194	1199	rBV2	326	260	0.03%	0.003%
26	5.006	1216	1218	1221	rVB2	247	104	0.01%	0.001%
27	5.071	1221	1238	1274	rBV2	383598	998892	100.00%	12.443%
28	5.350	1323	1325	1327	rBV2	139	73	0.01%	0.001%
29	5.383	1333	1335	1339	rVB2	361	178	0.02%	0.002%
30	5.402	1339	1341	1342	rBV	244	97	0.01%	0.001%
31	5.434	1347	1351	1353	rBV	201	131	0.01%	0.002%
32	5.479	1363	1365	1371	rVB2	251	122	0.01%	0.002%
33	5.511	1371	1375	1378	rBV2	387	284	0.03%	0.004%
34	5.550	1386	1387	1391	rVB2	241	102	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100120\
 Data File : VV018611.D
 Acq On : 02 Oct 2020 00:19
 Operator : SY/MD
 Sample : L4237-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

35	5.640	1403	1415	1442	rBV	338123	670220	67.10%	8.349%
36	5.932	1495	1506	1524	rVB6	23594	53546	5.36%	0.667%
37	6.042	1538	1540	1541	rBV	157	68	0.01%	0.001%
38	6.093	1543	1556	1579	rBV	226364	454135	45.46%	5.657%
39	6.302	1618	1621	1624	rVB2	204	138	0.01%	0.002%
40	6.328	1628	1629	1633	rVB	251	101	0.01%	0.001%
41	6.376	1642	1644	1645	rBV	167	74	0.01%	0.001%
42	6.437	1661	1663	1664	rBV	231	107	0.01%	0.001%
43	6.492	1678	1680	1685	rBV2	288	142	0.01%	0.002%
44	6.598	1710	1713	1715	rBV	384	178	0.02%	0.002%
45	6.627	1719	1722	1724	rBV2	154	91	0.01%	0.001%
46	6.656	1727	1731	1734	rBV2	256	196	0.02%	0.002%
47	6.701	1743	1745	1749	rVB2	339	176	0.02%	0.002%
48	6.730	1751	1754	1759	rVB3	415	285	0.03%	0.004%
49	6.756	1759	1762	1765	rBV	146	121	0.01%	0.002%
50	6.797	1773	1775	1777	rBV	247	126	0.01%	0.002%
51	7.010	1825	1841	1857	rBV	120193	217730	21.80%	2.712%
52	7.338	1931	1943	1968	rBV	468051	809163	81.01%	10.080%
53	7.643	2024	2038	2059	rBV	87094	154129	15.43%	1.920%
54	7.852	2097	2103	2105	rBV3	386	419	0.04%	0.005%
55	7.958	2128	2136	2141	rBV3	915	1417	0.14%	0.018%
56	8.003	2141	2150	2159	rVB5	3730	6499	0.65%	0.081%
57	8.109	2173	2183	2218	rBV2	200317	400533	40.10%	4.989%
58	8.363	2259	2262	2265	rBV3	307	218	0.02%	0.003%
59	8.521	2307	2311	2314	rBV2	191	191	0.02%	0.002%
60	8.540	2314	2317	2318	rBV	229	117	0.01%	0.001%
61	8.569	2324	2326	2328	rVB	152	42	0.00%	0.001%
62	8.595	2330	2334	2336	rBV2	295	237	0.02%	0.003%
63	8.736	2375	2378	2380	rBV	253	159	0.02%	0.002%
64	8.768	2386	2388	2393	rVB	227	109	0.01%	0.001%
65	8.791	2393	2395	2397	rVB	164	67	0.01%	0.001%
66	8.804	2397	2399	2403	rBV2	232	184	0.02%	0.002%
67	8.874	2409	2421	2446	rBV	524776	845368	84.63%	10.531%
68	9.196	2519	2521	2522	rBV2	261	81	0.01%	0.001%
69	9.257	2535	2540	2544	rBV2	409	368	0.04%	0.005%
70	9.276	2544	2546	2547	rBV2	144	40	0.00%	0.000%
71	9.360	2571	2572	2575	rVB2	356	141	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100120\
 Data File : VV018611.D
 Acq On : 02 Oct 2020 00:19
 Operator : SY/MD
 Sample : L4237-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

72	9.444	2595	2598	2600	rBV2	264	185	0.02%	0.002%
73	9.546	2625	2630	2631	rBV2	298	191	0.02%	0.002%
74	9.627	2654	2655	2656	rBV2	143	49	0.00%	0.001%
75	9.685	2671	2673	2674	rBV	153	46	0.00%	0.001%
76	9.701	2674	2678	2680	rVV2	311	203	0.02%	0.003%
77	10.051	2782	2787	2788	rBV	190	160	0.02%	0.002%
78	10.238	2833	2845	2870	rVB	275052	433622	43.41%	5.402%
79	10.399	2888	2895	2907	rVB4	1106	1746	0.17%	0.022%
80	10.444	2907	2909	2912	rVB	169	89	0.01%	0.001%
81	10.463	2912	2915	2917	rBV	192	126	0.01%	0.002%
82	10.588	2951	2954	2956	rBV	217	153	0.02%	0.002%
83	10.704	2986	2990	2995	rBV	240	232	0.02%	0.003%
84	11.019	3085	3088	3091	rBV2	293	195	0.02%	0.002%
85	11.270	3154	3166	3188	rBV	551174	841230	84.22%	10.479%
86	11.488	3231	3234	3236	rBV	320	213	0.02%	0.003%
87	11.501	3236	3238	3239	rBV	258	101	0.01%	0.001%
88	11.559	3250	3256	3264	rBV5	1989	2995	0.30%	0.037%
89	11.646	3271	3283	3311	rBV	516179	801807	80.27%	9.988%
90	12.064	3411	3413	3419	rVB2	419	229	0.02%	0.003%
91	12.099	3419	3424	3426	rBV	275	232	0.02%	0.003%
92	14.029	4021	4024	4026	rBV	433	300	0.03%	0.004%
93	15.266	4407	4409	4414	rBV3	553	423	0.04%	0.005%


Sum of corrected areas: 8027802

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100120\
Data File : VV018611.D
Acq On : 02 Oct 2020 00:19
Operator : SY/MD
Sample : L4237-15
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

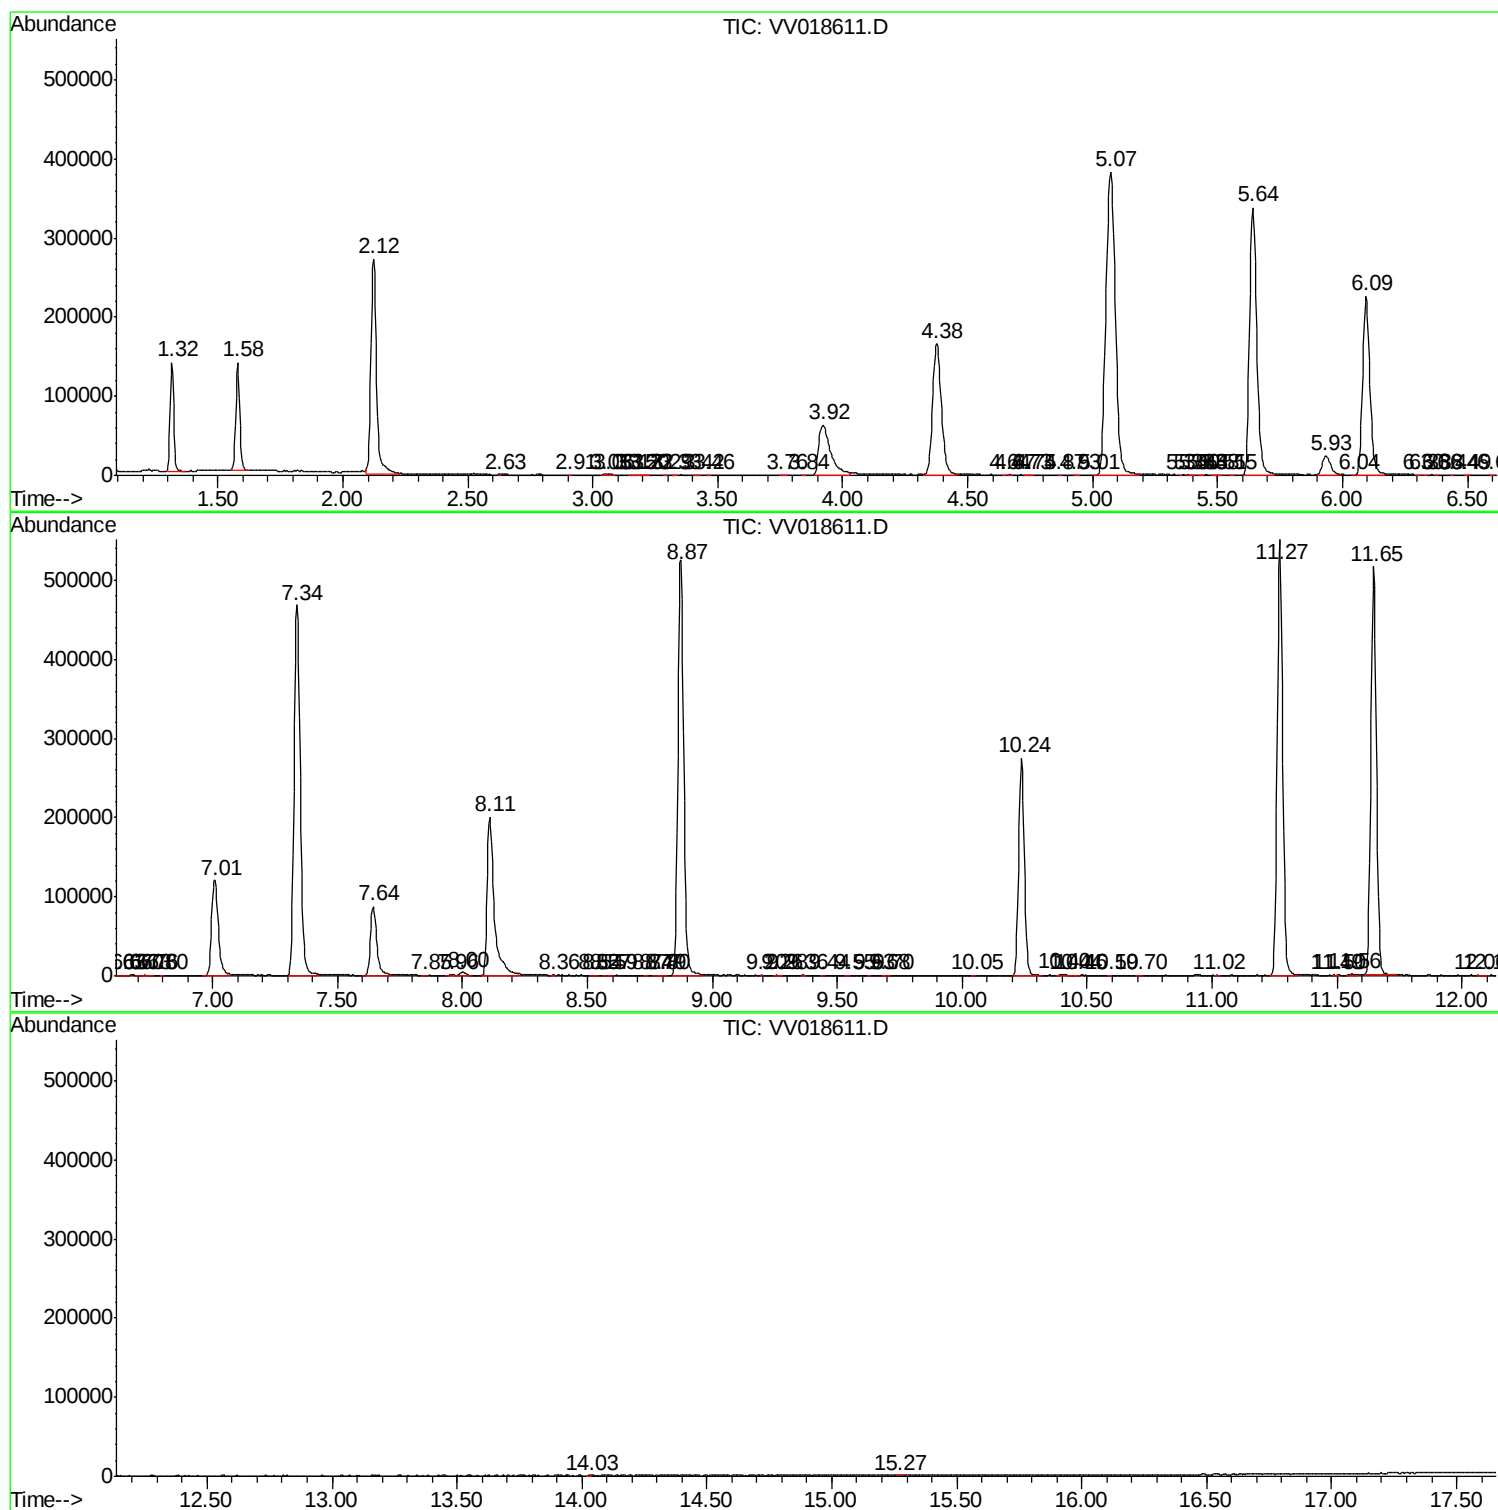

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV100120\
Data File : VV018611.D
Acq On : 02 Oct 2020 00:19
Operator : SY/MD
Sample : L4237-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV100120\
Data File : VV018611.D
Acq On : 02 Oct 2020 00:19
Operator : SY/MD
Sample : L4237-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC8

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc