

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022480.D
 Acq On : 01 Oct 2021 22:30
 Operator : SY/MD
 Sample : VV1001WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK269

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M

Title : VOC Analysis

Signal : TIC: VV022480.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	123757	126151	16.20%	2.030%
2	1.568	156	164	177	rBV	101594	115800	14.87%	1.863%
3	2.108	322	332	352	rBV	211350	306983	39.43%	4.940%
4	2.506	450	456	466	rVB5	3249	4959	0.64%	0.080%
5	2.648	498	500	501	rBV5	290	141	0.02%	0.002%
6	2.696	513	515	521	rVB2	215	175	0.02%	0.003%
7	2.728	523	525	528	rVV2	252	179	0.02%	0.003%
8	2.770	531	538	547	rVB8	1094	2182	0.28%	0.035%
9	2.912	578	582	585	rBV	314	202	0.03%	0.003%
10	3.053	624	626	629	rVB3	315	167	0.02%	0.003%
11	3.095	636	639	644	rBV3	354	317	0.04%	0.005%
12	3.121	644	647	650	rBV2	200	135	0.02%	0.002%
13	3.220	675	678	682	rBV2	305	305	0.04%	0.005%
14	3.426	739	742	744	rBV	300	228	0.03%	0.004%
15	3.465	750	754	756	rBV2	406	237	0.03%	0.004%
16	3.481	756	759	761	rBV2	183	124	0.02%	0.002%
17	3.722	832	834	839	rVV2	197	149	0.02%	0.002%
18	3.895	878	888	922	rBV	34537	122042	15.67%	1.964%
19	4.349	1016	1029	1055	rVB2	120621	298727	38.37%	4.807%
20	4.661	1124	1126	1129	rBV3	459	307	0.04%	0.005%
21	4.979	1222	1225	1226	rBV	370	189	0.02%	0.003%
22	5.047	1230	1246	1277	rBV2	301371	778589	100.00%	12.528%
23	5.349	1338	1340	1344	rBV3	400	306	0.04%	0.005%
24	5.403	1355	1357	1360	rVB2	327	123	0.02%	0.002%
25	5.423	1360	1363	1365	rBV2	336	234	0.03%	0.004%
26	5.619	1411	1424	1448	rBV	285885	569491	73.14%	9.164%
27	5.834	1489	1491	1494	rBV	276	184	0.02%	0.003%
28	5.911	1505	1515	1529	rBV5	9363	19299	2.48%	0.311%
29	6.072	1550	1565	1590	rBV	164714	345684	44.40%	5.562%
30	6.420	1671	1673	1675	rBV	313	123	0.02%	0.002%
31	6.461	1683	1686	1689	rBV2	335	236	0.03%	0.004%
32	6.510	1696	1701	1704	rBV2	252	265	0.03%	0.004%
33	6.792	1786	1789	1792	rBV2	377	245	0.03%	0.004%
34	6.931	1828	1832	1833	rBV	211	177	0.02%	0.003%
35	6.989	1839	1850	1873	rBV2	90424	168415	21.63%	2.710%
36	7.207	1914	1918	1920	rBV2	309	246	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022480.D
 Acq On : 01 Oct 2021 22:30
 Operator : SY/MD
 Sample : VV1001WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK269

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

37	7.317	1940	1952	1971	rBV	360662	631661	81.13%	10.164%
38	7.542	2020	2022	2023	rBV	327	143	0.02%	0.002%
39	7.564	2028	2029	2032	rBV	236	175	0.02%	0.003%
40	7.625	2037	2048	2071	rBV	61289	109802	14.10%	1.767%
41	7.889	2128	2130	2134	rBV2	356	209	0.03%	0.003%
42	7.982	2152	2159	2168	rVB5	1409	1830	0.24%	0.029%
43	8.091	2183	2193	2228	rBV	154293	341881	43.91%	5.501%
44	8.355	2273	2275	2281	rVB3	778	664	0.09%	0.011%
45	8.445	2299	2303	2305	rBV3	246	251	0.03%	0.004%
46	8.464	2307	2309	2312	rVV3	338	144	0.02%	0.002%
47	8.551	2334	2336	2339	rVB	334	163	0.02%	0.003%
48	8.571	2339	2342	2346	rBV2	467	341	0.04%	0.005%
49	8.622	2355	2358	2359	rBV	278	138	0.02%	0.002%
50	8.702	2376	2383	2386	rBV2	491	565	0.07%	0.009%
51	8.853	2419	2430	2457	rBV	424725	677245	86.98%	10.897%
52	9.027	2475	2484	2490	rBV7	998	1485	0.19%	0.024%
53	9.111	2507	2510	2511	rBV	314	146	0.02%	0.002%
54	9.159	2518	2525	2534	rVB6	1447	2231	0.29%	0.036%
55	9.204	2536	2539	2540	rBV2	275	153	0.02%	0.002%
56	9.281	2561	2563	2566	rVB	373	192	0.02%	0.003%
57	9.326	2575	2577	2584	rVB2	487	342	0.04%	0.006%
58	9.358	2584	2587	2590	rBV	250	194	0.02%	0.003%
59	9.651	2676	2678	2682	rBV2	407	293	0.04%	0.005%
60	9.828	2726	2733	2736	rBV	495	543	0.07%	0.009%
61	9.879	2747	2749	2754	rVB2	299	159	0.02%	0.003%
62	9.921	2760	2762	2764	rBV2	310	170	0.02%	0.003%
63	9.940	2764	2768	2773	rVB3	975	948	0.12%	0.015%
64	10.127	2820	2826	2834	rVB4	1816	2449	0.31%	0.039%
65	10.217	2843	2854	2871	rBV2	219387	350063	44.96%	5.633%
66	10.320	2883	2886	2891	rVB5	847	798	0.10%	0.013%
67	10.358	2891	2898	2903	rBV4	360	524	0.07%	0.008%
68	10.384	2903	2906	2908	rBV2	409	228	0.03%	0.004%
69	10.574	2963	2965	2972	rVB4	434	299	0.04%	0.005%
70	10.654	2985	2990	2993	rBV2	385	358	0.05%	0.006%
71	10.747	3017	3019	3022	rVB	424	169	0.02%	0.003%
72	10.767	3023	3025	3027	rVB2	266	127	0.02%	0.002%
73	10.792	3030	3033	3037	rBV2	363	236	0.03%	0.004%
74	10.921	3062	3073	3082	rBV7	2854	4393	0.56%	0.071%
75	10.969	3085	3088	3091	rBV2	286	223	0.03%	0.004%
76	11.030	3104	3107	3112	rBV2	420	399	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022480.D
 Acq On : 01 Oct 2021 22:30
 Operator : SY/MD
 Sample : VV1001WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK269

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

77	11.146	3139	3143	3145	rBV2	839	643	0.08%	0.010%
78	11.188	3151	3156	3164	rBV4	1657	2082	0.27%	0.034%
79	11.249	3164	3175	3195	rBV	420684	643024	82.59%	10.347%
80	11.490	3248	3250	3254	rBV2	252	135	0.02%	0.002%
81	11.532	3261	3263	3265	rVB2	398	161	0.02%	0.003%
82	11.548	3265	3268	3270	rVB	435	220	0.03%	0.004%
83	11.625	3280	3292	3313	rBV	353268	555100	71.30%	8.932%
84	11.757	3331	3333	3336	rVB2	267	152	0.02%	0.002%
85	11.773	3336	3338	3339	rBV2	300	136	0.02%	0.002%
86	12.024	3413	3416	3420	rBV2	351	329	0.04%	0.005%
87	12.197	3467	3470	3472	rBV2	358	243	0.03%	0.004%
88	12.377	3522	3526	3529	rBV	261	249	0.03%	0.004%
89	12.596	3590	3594	3596	rBV	329	292	0.04%	0.005%
90	12.654	3605	3612	3616	rBV4	1875	2317	0.30%	0.037%
91	12.731	3629	3636	3639	rBV2	219	300	0.04%	0.005%
92	12.840	3666	3670	3675	rBV2	505	327	0.04%	0.005%
93	12.898	3685	3688	3691	rVB	386	253	0.03%	0.004%
94	12.988	3713	3716	3718	rBV	247	155	0.02%	0.002%
95	13.268	3797	3803	3812	rBV4	2485	3593	0.46%	0.058%
96	13.326	3819	3821	3822	rBV	375	127	0.02%	0.002%
97	13.509	3870	3878	3887	rBV3	3641	5253	0.67%	0.085%
98	13.747	3946	3952	3963	rVB5	2524	3259	0.42%	0.052%
99	14.162	4078	4081	4083	rBV2	305	203	0.03%	0.003%
100	14.368	4141	4145	4147	rBV3	541	521	0.07%	0.008%




Sum of corrected areas: 6214724

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022480.D
Acq On : 01 Oct 2021 22:30
Operator : SY/MD
Sample : VV1001WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK269

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

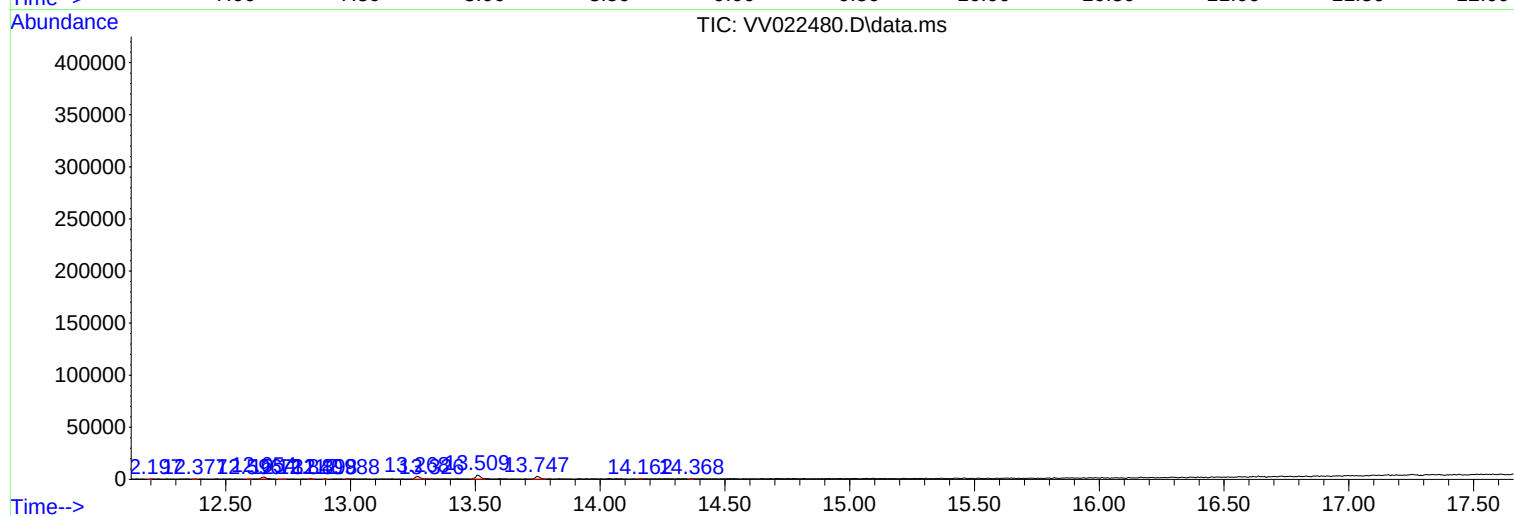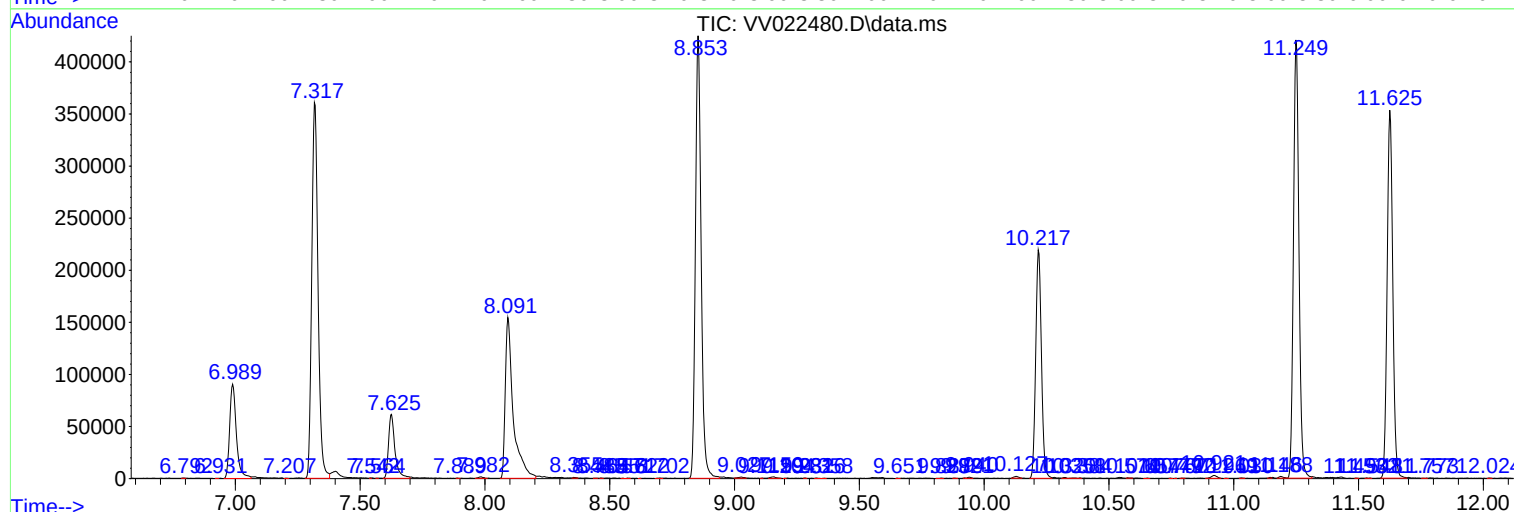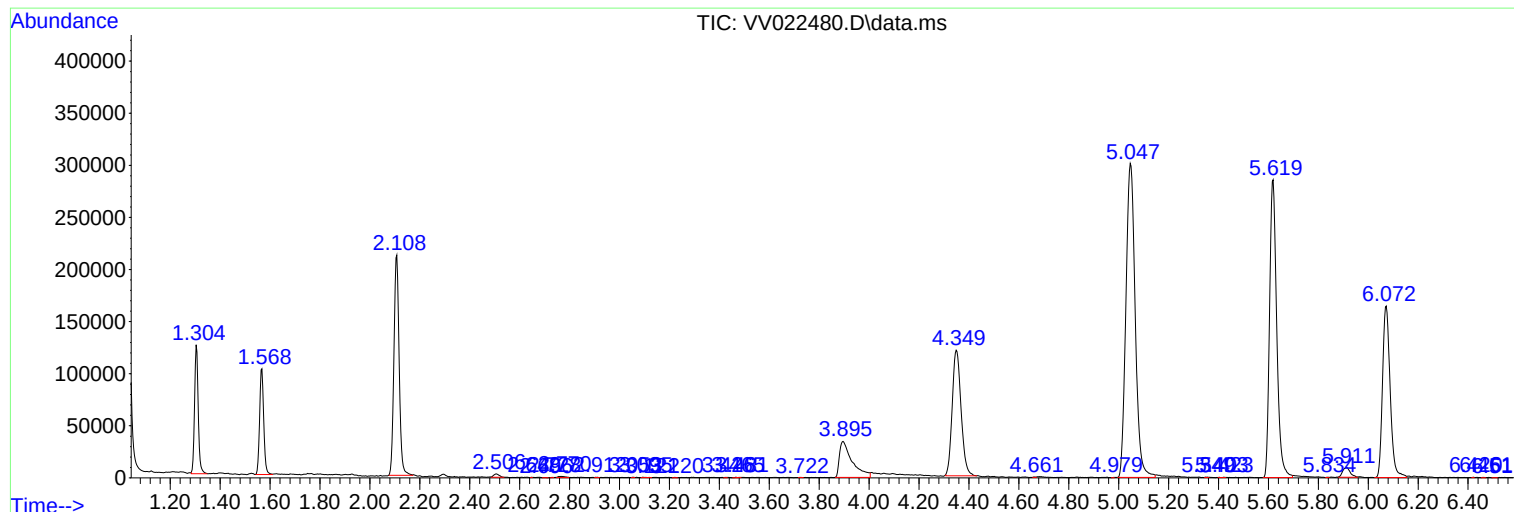

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022480.D
Acq On : 01 Oct 2021 22:30
Operator : SY/MD
Sample : VV1001WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK269

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022480.D
Acq On : 01 Oct 2021 22:30
Operator : SY/MD
Sample : VV1001WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK269

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
