

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022481.D
 Acq On : 01 Oct 2021 22:53
 Operator : SY/MD
 Sample : M4024-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

Signal : TIC: VV022481.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	119881	120373	2.10%	0.928%
2	1.568	157	164	176	rVB	95894	109314	1.91%	0.843%
3	2.111	322	333	360	rVB3	313620	535696	9.34%	4.132%
4	2.510	449	457	464	rBV4	1540	2434	0.04%	0.019%
5	2.635	491	496	498	rBV2	310	289	0.01%	0.002%
6	2.699	513	516	519	rBV	215	210	0.00%	0.002%
7	2.764	527	536	552	rVB2	11436	20784	0.36%	0.160%
8	2.963	597	598	601	rBV	316	155	0.00%	0.001%
9	2.995	606	608	612	rVV2	295	211	0.00%	0.002%
10	3.066	627	630	633	rBV	238	124	0.00%	0.001%
11	3.130	648	650	652	rBV	236	138	0.00%	0.001%
12	3.195	658	670	683	rBV3	6485	13347	0.23%	0.103%
13	3.278	692	696	697	rBV2	313	232	0.00%	0.002%
14	3.426	739	742	749	rBV2	392	472	0.01%	0.004%
15	3.500	762	765	769	rBV2	307	285	0.00%	0.002%
16	3.699	825	827	831	rVB2	279	167	0.00%	0.001%
17	3.767	845	848	851	rBV2	345	246	0.00%	0.002%
18	3.912	878	893	919	rBV2	241295	643596	11.22%	4.964%
19	4.349	1016	1029	1055	rVB2	119957	297562	5.19%	2.295%
20	4.606	1092	1109	1141	rVB2	157186	398948	6.96%	3.077%
21	4.764	1155	1158	1161	rBV2	444	331	0.01%	0.003%
22	4.796	1166	1168	1170	rVV2	350	150	0.00%	0.001%
23	4.834	1177	1180	1188	rVB4	698	702	0.01%	0.005%
24	4.953	1214	1217	1220	rBV2	210	123	0.00%	0.001%
25	5.050	1229	1247	1271	rBV2	294220	749978	13.08%	5.785%
26	5.339	1335	1337	1339	rBV	319	189	0.00%	0.001%
27	5.497	1383	1386	1388	rBV2	457	273	0.00%	0.002%
28	5.545	1398	1401	1403	rBV	262	131	0.00%	0.001%
29	5.619	1411	1424	1453	rBV	277879	565251	9.86%	4.360%
30	5.915	1500	1516	1550	rBV	2983809	5734626	100.00%	44.232%
31	6.072	1554	1565	1594	rVB	163241	339854	5.93%	2.621%
32	6.378	1658	1660	1663	rBV	412	174	0.00%	0.001%
33	6.439	1675	1679	1680	rBV	226	139	0.00%	0.001%
34	6.538	1706	1710	1716	rBV3	504	405	0.01%	0.003%
35	6.574	1719	1721	1725	rVB2	453	304	0.01%	0.002%
36	6.677	1751	1753	1756	rBV	245	127	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100121\
 Data File : VW022481.D
 Acq On : 01 Oct 2021 22:53
 Operator : SY/MD
 Sample : M4024-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

37	6.744	1771	1774	1778	rBV3	506	498	0.01%	0.004%
38	6.796	1787	1790	1792	rBV2	287	149	0.00%	0.001%
39	6.937	1830	1834	1838	rBV2	392	344	0.01%	0.003%
40	6.989	1839	1850	1874	rBV	91120	165440	2.88%	1.276%
41	7.198	1912	1915	1917	rBV2	583	234	0.00%	0.002%
42	7.230	1923	1925	1927	rBV2	330	146	0.00%	0.001%
43	7.317	1941	1952	1971	rBV	355158	615413	10.73%	4.747%
44	7.580	2031	2034	2035	rBV	308	195	0.00%	0.002%
45	7.625	2038	2048	2070	rBV	59428	107724	1.88%	0.831%
46	7.850	2110	2118	2127	rBV6	3748	6199	0.11%	0.048%
47	7.985	2152	2160	2166	rBV6	1902	2635	0.05%	0.020%
48	8.091	2182	2193	2230	rBV	145248	322221	5.62%	2.485%
49	8.333	2266	2268	2271	rVB3	514	207	0.00%	0.002%
50	8.410	2289	2292	2293	rBV	204	151	0.00%	0.001%
51	8.448	2302	2304	2307	rBV	320	201	0.00%	0.002%
52	8.648	2364	2366	2369	rVB2	264	121	0.00%	0.001%
53	8.715	2384	2387	2390	rBV2	543	313	0.01%	0.002%
54	8.854	2419	2430	2453	rBV	422359	676308	11.79%	5.216%
55	9.153	2518	2523	2527	rBV	730	676	0.01%	0.005%
56	9.387	2594	2596	2599	rBV	197	140	0.00%	0.001%
57	9.519	2634	2637	2638	rBV	306	154	0.00%	0.001%
58	9.542	2641	2644	2645	rBV	515	245	0.00%	0.002%
59	9.792	2715	2722	2726	rBV2	333	332	0.01%	0.003%
60	9.860	2738	2743	2746	rBV2	310	285	0.00%	0.002%
61	9.882	2747	2750	2755	rBV2	255	259	0.00%	0.002%
62	9.908	2756	2758	2760	rBV2	272	121	0.00%	0.001%
63	10.091	2812	2815	2817	rBV2	172	144	0.00%	0.001%
64	10.130	2819	2827	2835	rVB5	2153	2909	0.05%	0.022%
65	10.217	2843	2854	2873	rBV	216251	340210	5.93%	2.624%
66	10.297	2877	2879	2881	rVB3	753	287	0.01%	0.002%
67	10.490	2937	2939	2942	rVB2	418	193	0.00%	0.001%
68	10.548	2951	2957	2962	rBV2	706	1088	0.02%	0.008%
69	10.635	2979	2984	2986	rBV2	222	200	0.00%	0.002%
70	10.670	2991	2995	3000	rBV2	446	324	0.01%	0.002%
71	10.699	3000	3004	3008	rBV2	587	444	0.01%	0.003%
72	10.738	3013	3016	3018	rBV	192	150	0.00%	0.001%
73	10.882	3059	3061	3066	rBV2	253	245	0.00%	0.002%
74	10.918	3066	3072	3079	rBV4	2066	2887	0.05%	0.022%
75	11.017	3099	3103	3106	rBV	265	292	0.01%	0.002%
76	11.101	3123	3129	3135	rVB3	714	841	0.01%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022481.D
 Acq On : 01 Oct 2021 22:53
 Operator : SY/MD
 Sample : M4024-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

77	11.152	3139	3145	3150	rVB4	1096	1390	0.02%	0.011%
78	11.191	3150	3157	3161	rBV5	1249	1897	0.03%	0.015%
79	11.249	3164	3175	3197	rBV	410395	634858	11.07%	4.897%
80	11.574	3273	3276	3278	rBV2	341	162	0.00%	0.001%
81	11.625	3280	3292	3310	rVV	336229	529288	9.23%	4.082%
82	11.828	3352	3355	3358	rBV3	444	371	0.01%	0.003%
83	11.937	3388	3389	3393	rBV2	313	234	0.00%	0.002%
84	12.095	3436	3438	3442	rBV	373	231	0.00%	0.002%
85	12.230	3478	3480	3485	rVB2	295	166	0.00%	0.001%
86	12.361	3518	3521	3527	rVB3	501	388	0.01%	0.003%
87	12.538	3573	3576	3581	rVB3	295	208	0.00%	0.002%
88	12.564	3581	3584	3586	rBV3	235	154	0.00%	0.001%
89	12.651	3603	3611	3612	rBV5	1360	1506	0.03%	0.012%
90	13.046	3730	3734	3736	rBV2	228	220	0.00%	0.002%
91	13.175	3772	3774	3776	rBV	262	142	0.00%	0.001%
92	13.265	3797	3802	3813	rVB5	2158	2844	0.05%	0.022%
93	13.332	3819	3823	3825	rBV2	399	325	0.01%	0.003%
94	13.416	3847	3849	3853	rBV2	243	178	0.00%	0.001%
95	13.564	3893	3895	3898	rVB2	405	185	0.00%	0.001%
96	13.638	3915	3918	3920	rBV2	231	177	0.00%	0.001%
97	13.747	3947	3952	3953	rBV4	1109	935	0.02%	0.007%
98	14.512	4188	4190	4191	rBV4	315	142	0.00%	0.001%
99	14.853	4292	4296	4299	rBV3	430	448	0.01%	0.003%
100	15.030	4349	4351	4354	rBV2	380	182	0.00%	0.001%




Sum of corrected areas: 12964896

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022481.D
Acq On : 01 Oct 2021 22:53
Operator : SY/MD
Sample : M4024-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

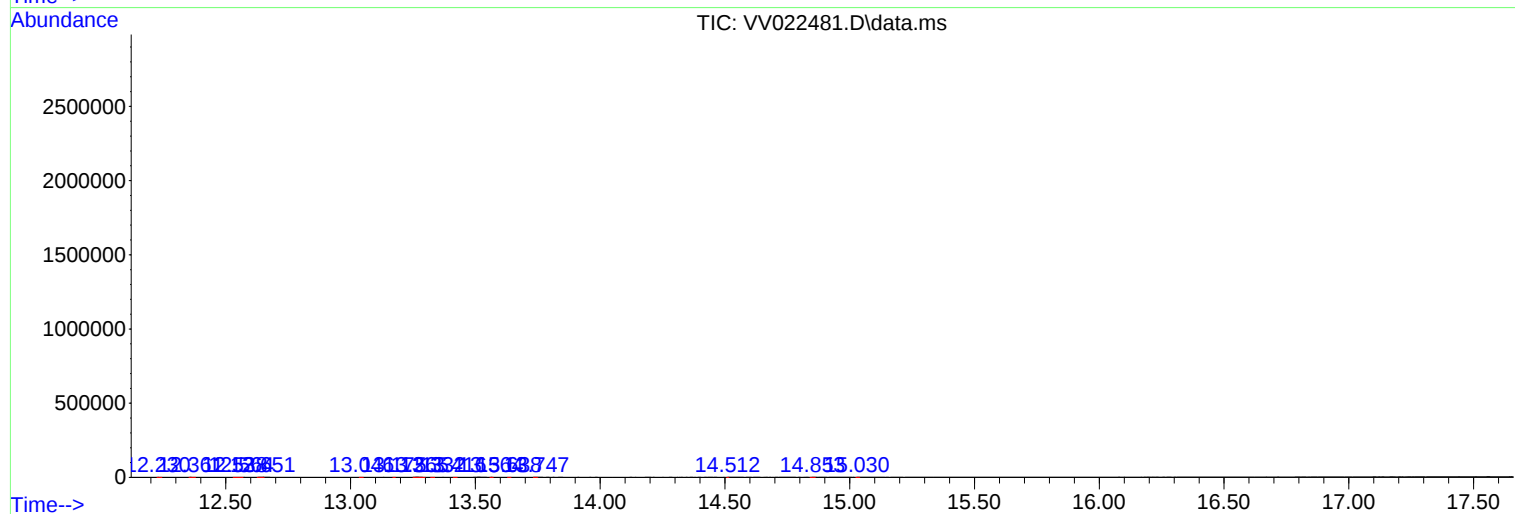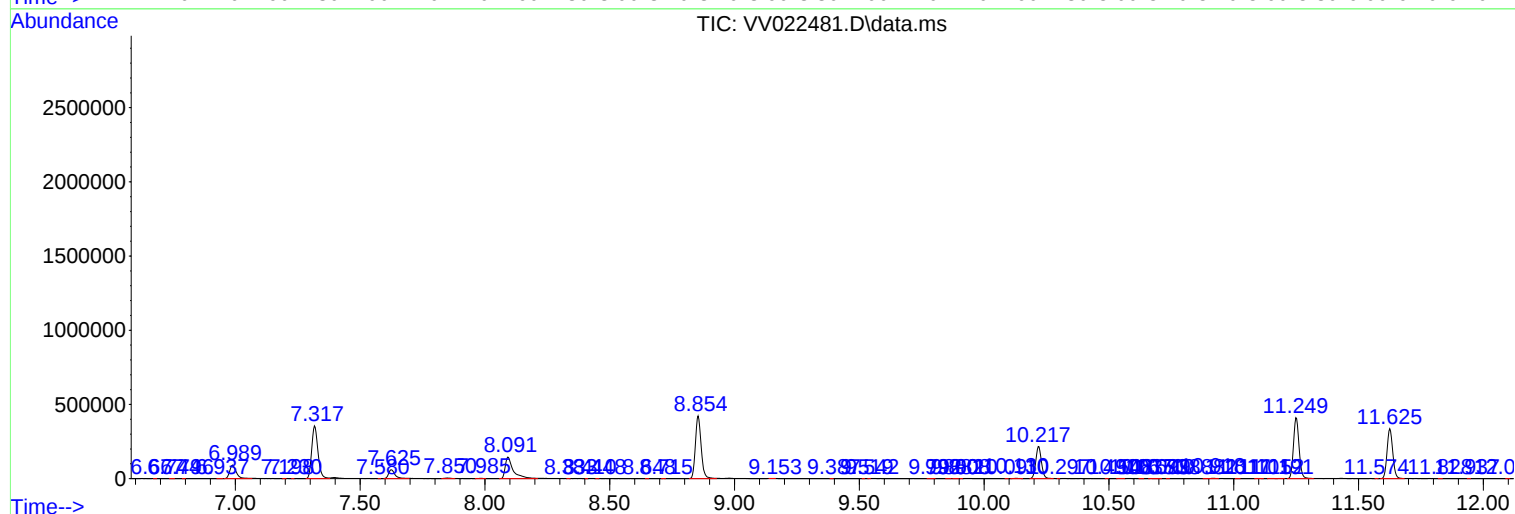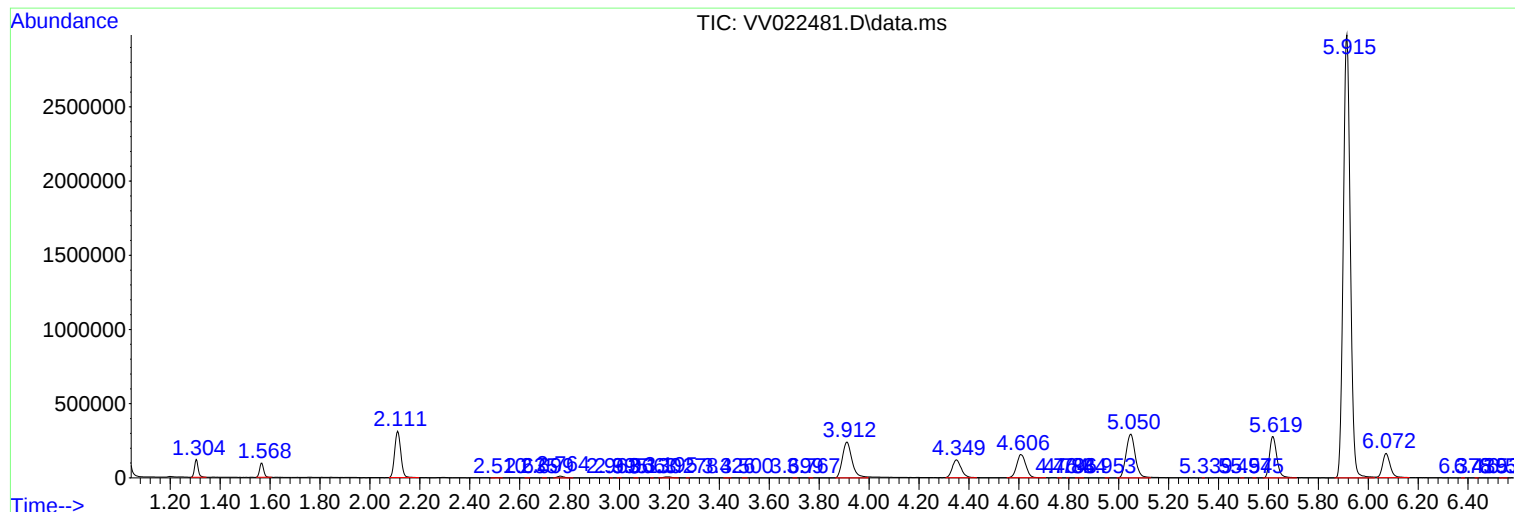

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022481.D
Acq On : 01 Oct 2021 22:53
Operator : SY/MD
Sample : M4024-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022481.D
Acq On : 01 Oct 2021 22:53
Operator : SY/MD
Sample : M4024-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
