

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022483.D
 Acq On : 01 Oct 2021 23:41
 Operator : SY/MD
 Sample : M4024-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M

Title : VOC Analysis

Signal : TIC: VV022483.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rVB	115511	118760	16.24%	2.025%
2	1.565	157	163	175	rVB	92875	104707	14.32%	1.785%
3	2.105	321	331	351	rBV	201679	293330	40.12%	5.001%
4	2.320	395	398	402	rVB	7588	4466	0.61%	0.076%
5	2.394	417	421	422	rBV2	471	275	0.04%	0.005%
6	2.703	515	517	518	rBV2	348	169	0.02%	0.003%
7	2.757	528	534	537	rBV4	659	681	0.09%	0.012%
8	2.950	592	594	597	rVB2	552	270	0.04%	0.005%
9	3.121	643	647	650	rBV	332	279	0.04%	0.005%
10	3.188	655	668	678	rVV7	3330	7281	1.00%	0.124%
11	3.246	684	686	690	rVB2	265	135	0.02%	0.002%
12	3.278	693	696	699	rBV3	344	272	0.04%	0.005%
13	3.327	707	711	714	rBV2	391	236	0.03%	0.004%
14	3.433	739	744	745	rBV2	275	179	0.02%	0.003%
15	3.484	755	760	762	rBV3	320	203	0.03%	0.003%
16	3.564	782	785	789	rVV	272	143	0.02%	0.002%
17	3.584	789	791	797	rVB2	361	301	0.04%	0.005%
18	3.613	797	800	803	rBV2	259	232	0.03%	0.004%
19	3.709	826	830	831	rBV	250	153	0.02%	0.003%
20	3.738	835	839	844	rBV2	319	403	0.06%	0.007%
21	3.767	845	848	850	rBV2	288	147	0.02%	0.003%
22	3.905	878	891	920	rBV3	49666	176422	24.13%	3.008%
23	4.349	1016	1029	1054	rVB2	115047	282683	38.66%	4.819%
24	4.802	1169	1170	1173	rVB	234	94	0.01%	0.002%
25	4.825	1173	1177	1178	rBV	230	135	0.02%	0.002%
26	4.934	1209	1211	1213	rVB	239	95	0.01%	0.002%
27	4.960	1217	1219	1222	rBV3	314	152	0.02%	0.003%
28	5.047	1229	1246	1272	rBV2	286479	731123	100.00%	12.465%
29	5.359	1336	1343	1348	rBV3	321	584	0.08%	0.010%
30	5.458	1370	1374	1376	rBV2	400	239	0.03%	0.004%
31	5.484	1380	1382	1384	rBV2	282	120	0.02%	0.002%
32	5.497	1384	1386	1389	rVB	307	147	0.02%	0.003%
33	5.516	1389	1392	1394	rVB3	278	146	0.02%	0.002%
34	5.542	1395	1400	1406	rVB3	322	377	0.05%	0.006%
35	5.571	1406	1409	1411	rBV2	302	173	0.02%	0.003%
36	5.616	1411	1423	1449	rBV	270067	542440	74.19%	9.248%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022483.D
 Acq On : 01 Oct 2021 23:41
 Operator : SY/MD
 Sample : M4024-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

37	5.912	1504	1515	1534	rVB7	11785	28813	3.94%	0.491%
38	5.998	1540	1542	1544	rBV	400	230	0.03%	0.004%
39	6.069	1551	1564	1587	rBV	159456	326251	44.62%	5.562%
40	6.285	1628	1631	1632	rBV	194	116	0.02%	0.002%
41	6.465	1685	1687	1691	rBV2	175	105	0.01%	0.002%
42	6.529	1703	1707	1708	rBV	344	232	0.03%	0.004%
43	6.645	1740	1743	1747	rBV	180	165	0.02%	0.003%
44	6.989	1839	1850	1869	rBV	81041	150091	20.53%	2.559%
45	7.278	1935	1940	1941	rBV2	166	156	0.02%	0.003%
46	7.317	1941	1952	1970	rBV	342952	591644	80.92%	10.087%
47	7.625	2038	2048	2068	rBV	54531	98244	13.44%	1.675%
48	7.899	2131	2133	2135	rBV	302	172	0.02%	0.003%
49	8.092	2184	2193	2237	rBV	136624	308986	42.26%	5.268%
50	8.320	2261	2264	2269	rVB2	421	273	0.04%	0.005%
51	8.600	2344	2351	2353	rBV2	338	376	0.05%	0.006%
52	8.616	2353	2356	2357	rBV2	261	109	0.01%	0.002%
53	8.854	2418	2430	2458	rBV	398455	639896	87.52%	10.909%
54	9.153	2515	2523	2527	rBV3	1085	1523	0.21%	0.026%
55	9.291	2562	2566	2570	rBV	242	237	0.03%	0.004%
56	9.333	2576	2579	2584	rBV3	226	205	0.03%	0.003%
57	9.545	2643	2645	2646	rBV	272	109	0.01%	0.002%
58	9.664	2681	2682	2687	rVB3	427	301	0.04%	0.005%
59	9.686	2687	2689	2690	rBV	269	98	0.01%	0.002%
60	10.088	2812	2814	2816	rBV	219	114	0.02%	0.002%
61	10.127	2819	2826	2839	rVB5	1626	2779	0.38%	0.047%
62	10.175	2839	2841	2842	rBV	224	112	0.02%	0.002%
63	10.217	2843	2854	2876	rVV	206575	329642	45.09%	5.620%
64	10.362	2894	2899	2903	rVV3	544	521	0.07%	0.009%
65	10.378	2903	2904	2906	rVB	399	93	0.01%	0.002%
66	10.506	2941	2944	2946	rBV2	237	192	0.03%	0.003%
67	10.522	2946	2949	2950	rVV	261	128	0.02%	0.002%
68	10.657	2988	2991	2992	rBV2	336	191	0.03%	0.003%
69	10.725	3011	3012	3015	rBV2	257	115	0.02%	0.002%
70	10.760	3020	3023	3027	rVB2	212	112	0.02%	0.002%
71	10.780	3027	3029	3034	rBV	265	178	0.02%	0.003%
72	10.802	3034	3036	3041	rBV2	153	101	0.01%	0.002%
73	10.837	3044	3047	3049	rBV2	273	193	0.03%	0.003%
74	11.056	3113	3115	3117	rBV	414	189	0.03%	0.003%
75	11.133	3136	3139	3140	rBV2	490	262	0.04%	0.004%
76	11.249	3164	3175	3195	rBV	387804	596670	81.61%	10.173%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022483.D
 Acq On : 01 Oct 2021 23:41
 Operator : SY/MD
 Sample : M4024-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

77	11.362	3208	3210	3214	rBV3	455	261	0.04%	0.004%
78	11.625	3281	3292	3309	rBV	332831	513626	70.25%	8.757%
79	11.850	3361	3362	3365	rBV2	310	116	0.02%	0.002%
80	11.976	3396	3401	3403	rBV2	180	178	0.02%	0.003%
81	12.018	3410	3414	3417	rBV	249	245	0.03%	0.004%
82	12.149	3452	3455	3456	rBV	268	111	0.02%	0.002%
83	12.255	3486	3488	3491	rBV	213	135	0.02%	0.002%
84	12.603	3594	3596	3598	rBV2	287	145	0.02%	0.002%
85	12.616	3598	3600	3604	rBB2	223	116	0.02%	0.002%
86	12.648	3607	3610	3613	rBV2	807	621	0.08%	0.011%
87	12.882	3682	3683	3685	rBV	232	95	0.01%	0.002%
88	13.037	3727	3731	3733	rBV2	196	160	0.02%	0.003%
89	13.127	3757	3759	3761	rBV	363	133	0.02%	0.002%
90	13.255	3797	3799	3800	rBV	483	199	0.03%	0.003%
91	13.506	3875	3877	3878	rBV	515	207	0.03%	0.004%
92	13.603	3905	3907	3909	rBV	168	112	0.02%	0.002%
93	13.625	3912	3914	3916	rBV	344	191	0.03%	0.003%
94	13.673	3926	3929	3930	rBV	251	107	0.01%	0.002%
95	13.747	3949	3952	3954	rBV2	478	269	0.04%	0.005%
96	13.979	4021	4024	4025	rBV2	301	179	0.02%	0.003%
97	14.053	4045	4047	4051	rBV3	379	236	0.03%	0.004%
98	14.120	4065	4068	4073	rBV	362	261	0.04%	0.004%
99	14.159	4077	4080	4082	rBV2	322	160	0.02%	0.003%
100	14.181	4085	4087	4092	rVB2	312	174	0.02%	0.003%




Sum of corrected areas: 5865513

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022483.D
Acq On : 01 Oct 2021 23:41
Operator : SY/MD
Sample : M4024-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

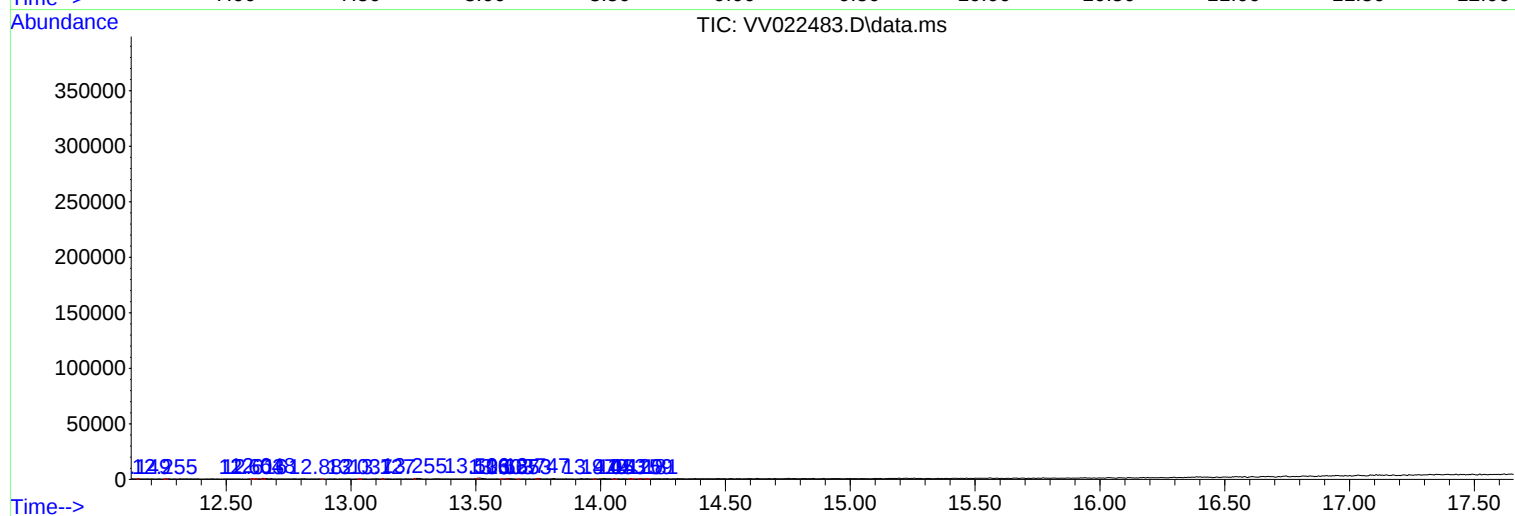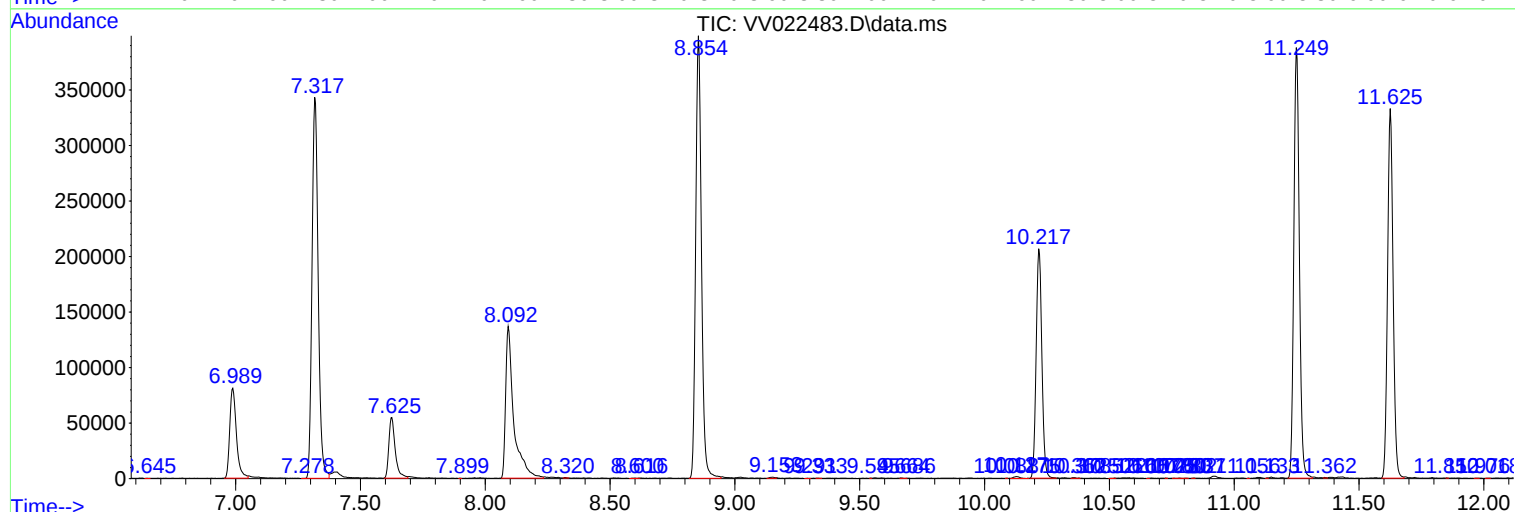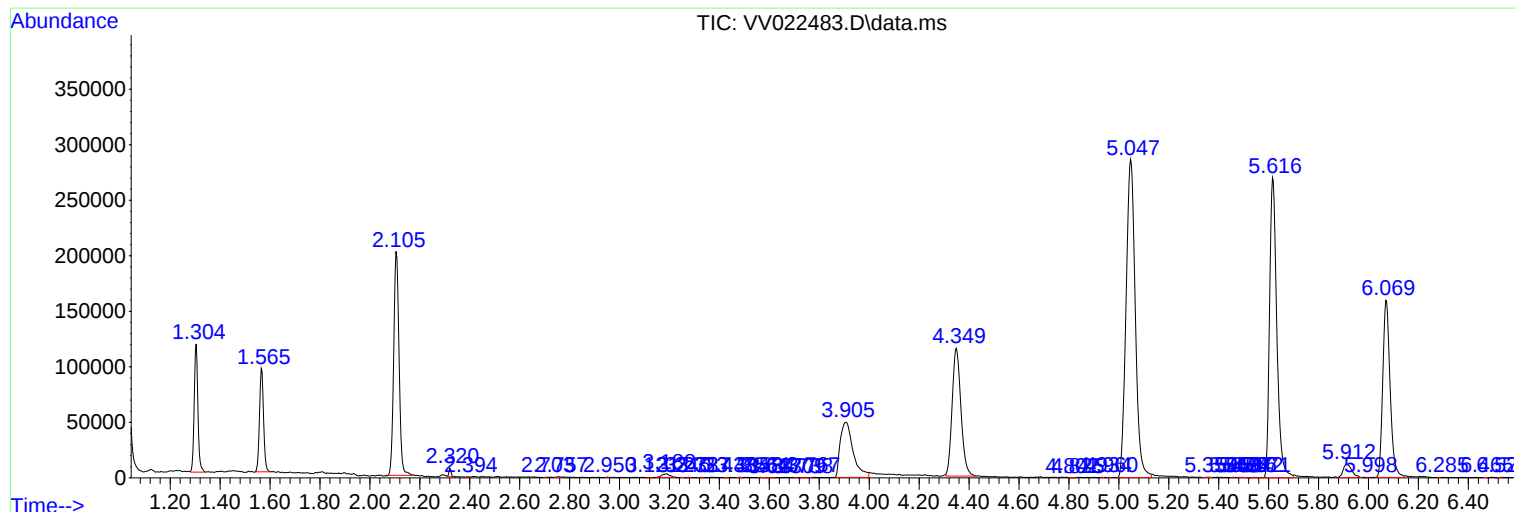

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022483.D
Acq On : 01 Oct 2021 23:41
Operator : SY/MD
Sample : M4024-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022483.D
Acq On : 01 Oct 2021 23:41
Operator : SY/MD
Sample : M4024-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
