

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022484.D
 Acq On : 02 Oct 2021 00:05
 Operator : SY/MD
 Sample : M4024-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

Signal : TIC: VV022484.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	77	82	105	rVB2	192235	216882	30.90%	3.545%
2	1.564	157	163	178	rVB	92561	104611	14.90%	1.710%
3	2.105	322	331	345	rVB2	200479	297387	42.37%	4.861%
4	3.188	656	668	689	rVB	37961	80562	11.48%	1.317%
5	3.426	740	742	744	rBV	293	116	0.02%	0.002%
6	3.699	820	827	828	rBV	316	319	0.05%	0.005%
7	3.802	856	859	860	rBV2	195	119	0.02%	0.002%
8	3.908	877	892	923	rBV4	149325	426670	60.78%	6.975%
9	4.349	1015	1029	1052	rVB	113481	274373	39.09%	4.485%
10	4.609	1097	1110	1129	rVB3	11558	28530	4.06%	0.466%
11	4.677	1129	1131	1132	rBV3	465	180	0.03%	0.003%
12	4.815	1172	1174	1177	rBV	185	147	0.02%	0.002%
13	5.047	1230	1246	1271	rBV3	274802	701948	100.00%	11.475%
14	5.336	1334	1336	1338	rBV2	276	140	0.02%	0.002%
15	5.567	1405	1408	1411	rBV3	203	202	0.03%	0.003%
16	5.616	1411	1423	1447	rBV	255013	512686	73.04%	8.381%
17	5.912	1505	1515	1531	rVB7	9004	20408	2.91%	0.334%
18	6.005	1543	1544	1547	rVB	258	117	0.02%	0.002%
19	6.072	1550	1565	1585	rBV2	150953	311411	44.36%	5.091%
20	6.301	1634	1636	1640	rVB2	439	325	0.05%	0.005%
21	6.333	1640	1646	1651	rBV	383	473	0.07%	0.008%
22	6.375	1653	1659	1665	rBV3	434	388	0.06%	0.006%
23	6.612	1729	1733	1734	rBV3	264	170	0.02%	0.003%
24	6.728	1766	1769	1772	rBV	326	175	0.02%	0.003%
25	6.767	1777	1781	1783	rBV2	194	120	0.02%	0.002%
26	6.834	1797	1802	1808	rBV3	438	461	0.07%	0.008%
27	6.866	1809	1812	1815	rVB3	199	131	0.02%	0.002%
28	6.895	1818	1821	1822	rBV3	245	130	0.02%	0.002%
29	6.989	1839	1850	1870	rBV	79736	145626	20.75%	2.381%
30	7.162	1903	1904	1907	rBV	258	126	0.02%	0.002%
31	7.223	1921	1923	1927	rVB2	428	258	0.04%	0.004%
32	7.317	1940	1952	1971	rBV	331252	571743	81.45%	9.346%
33	7.625	2038	2048	2067	rBV	51750	94115	13.41%	1.539%
34	7.773	2092	2094	2096	rVB3	459	177	0.03%	0.003%
35	7.786	2096	2098	2101	rBV2	321	284	0.04%	0.005%
36	7.879	2124	2127	2130	rVB2	296	161	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022484.D
 Acq On : 02 Oct 2021 00:05
 Operator : SY/MD
 Sample : M4024-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

37	7.911	2133	2137	2140	rBV2	365	203	0.03%	0.003%
38	7.985	2156	2160	2162	rVV3	381	272	0.04%	0.004%
39	8.059	2179	2183	2184	rBV	203	127	0.02%	0.002%
40	8.091	2184	2193	2224	rBV	127735	294139	41.90%	4.808%
41	8.355	2272	2275	2280	rVB3	537	462	0.07%	0.008%
42	8.461	2305	2308	2311	rBV	517	354	0.05%	0.006%
43	8.564	2338	2340	2342	rVB	237	133	0.02%	0.002%
44	8.622	2354	2358	2361	rBV2	314	237	0.03%	0.004%
45	8.702	2382	2383	2387	rVB2	249	138	0.02%	0.002%
46	8.770	2401	2404	2405	rVB	454	159	0.02%	0.003%
47	8.802	2409	2414	2417	rBV2	326	351	0.05%	0.006%
48	8.854	2418	2430	2451	rBV	380512	614526	87.55%	10.046%
49	9.098	2503	2506	2508	rBV3	238	135	0.02%	0.002%
50	9.149	2516	2522	2527	rBV4	1002	1340	0.19%	0.022%
51	9.191	2532	2535	2539	rBV	183	189	0.03%	0.003%
52	9.236	2546	2549	2550	rBV	282	136	0.02%	0.002%
53	9.316	2567	2574	2576	rBV2	258	301	0.04%	0.005%
54	9.403	2599	2601	2604	rBV	268	175	0.02%	0.003%
55	9.445	2610	2614	2617	rBV3	354	309	0.04%	0.005%
56	9.487	2625	2627	2631	rVB2	343	199	0.03%	0.003%
57	9.558	2647	2649	2650	rBV	396	197	0.03%	0.003%
58	9.876	2745	2748	2750	rBV	236	162	0.02%	0.003%
59	10.001	2784	2787	2788	rBV	243	120	0.02%	0.002%
60	10.027	2793	2795	2797	rBV2	176	119	0.02%	0.002%
61	10.130	2817	2827	2835	rBV3	1877	2820	0.40%	0.046%
62	10.172	2835	2840	2843	rBV	255	196	0.03%	0.003%
63	10.220	2843	2855	2873	rBV	204087	326243	46.48%	5.333%
64	10.413	2911	2915	2917	rBV2	295	249	0.04%	0.004%
65	10.445	2922	2925	2926	rBV2	183	122	0.02%	0.002%
66	10.503	2938	2943	2945	rBV2	170	185	0.03%	0.003%
67	10.596	2970	2972	2974	rBV3	426	210	0.03%	0.003%
68	10.654	2988	2990	2993	rVB2	325	162	0.02%	0.003%
69	10.731	3007	3014	3016	rBV2	140	177	0.03%	0.003%
70	10.763	3021	3024	3025	rBV	294	156	0.02%	0.003%
71	10.850	3048	3051	3053	rVV	210	126	0.02%	0.002%
72	10.915	3066	3071	3074	rBV2	1656	1837	0.26%	0.030%
73	11.146	3139	3143	3144	rBV2	645	472	0.07%	0.008%
74	11.188	3150	3156	3161	rBV2	528	616	0.09%	0.010%
75	11.249	3164	3175	3194	rBV	375535	572897	81.62%	9.365%
76	11.516	3256	3258	3263	rVB2	252	193	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022484.D
 Acq On : 02 Oct 2021 00:05
 Operator : SY/MD
 Sample : M4024-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

77	11.580	3277	3278	3280	rBV	377	165	0.02%	0.003%
78	11.625	3280	3292	3312	rVV	314027	499270	71.13%	8.162%
79	11.914	3379	3382	3384	rVB2	390	168	0.02%	0.003%
80	12.191	3465	3468	3470	rBV	208	169	0.02%	0.003%
81	12.255	3482	3488	3493	rVB3	457	551	0.08%	0.009%
82	12.355	3516	3519	3522	rVB2	437	250	0.04%	0.004%
83	12.394	3528	3531	3534	rBV2	221	210	0.03%	0.003%
84	12.435	3542	3544	3545	rBV2	261	129	0.02%	0.002%
85	12.468	3551	3554	3558	rBV3	308	248	0.04%	0.004%
86	12.570	3584	3586	3589	rVB	239	134	0.02%	0.002%
87	12.651	3609	3611	3617	rVB3	478	353	0.05%	0.006%
88	12.895	3682	3687	3690	rVB2	421	414	0.06%	0.007%
89	12.914	3690	3693	3696	rBV	220	192	0.03%	0.003%
90	12.937	3696	3700	3702	rBV	298	234	0.03%	0.004%
91	13.117	3753	3756	3758	rBV	147	110	0.02%	0.002%
92	13.358	3829	3831	3832	rBV	312	133	0.02%	0.002%
93	13.644	3918	3920	3923	rVB2	440	129	0.02%	0.002%
94	13.747	3949	3952	3956	rBV3	542	398	0.06%	0.007%
95	13.940	4008	4012	4013	rBV	331	206	0.03%	0.003%
96	13.979	4021	4024	4028	rBV2	248	166	0.02%	0.003%
97	14.127	4067	4070	4073	rBV	189	148	0.02%	0.002%
98	14.194	4088	4091	4094	rBV2	317	258	0.04%	0.004%
99	14.406	4155	4157	4159	rBV	383	172	0.02%	0.003%
100	14.438	4164	4167	4169	rBV	354	225	0.03%	0.004%




Sum of corrected areas: 6117247

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022484.D
Acq On : 02 Oct 2021 00:05
Operator : SY/MD
Sample : M4024-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

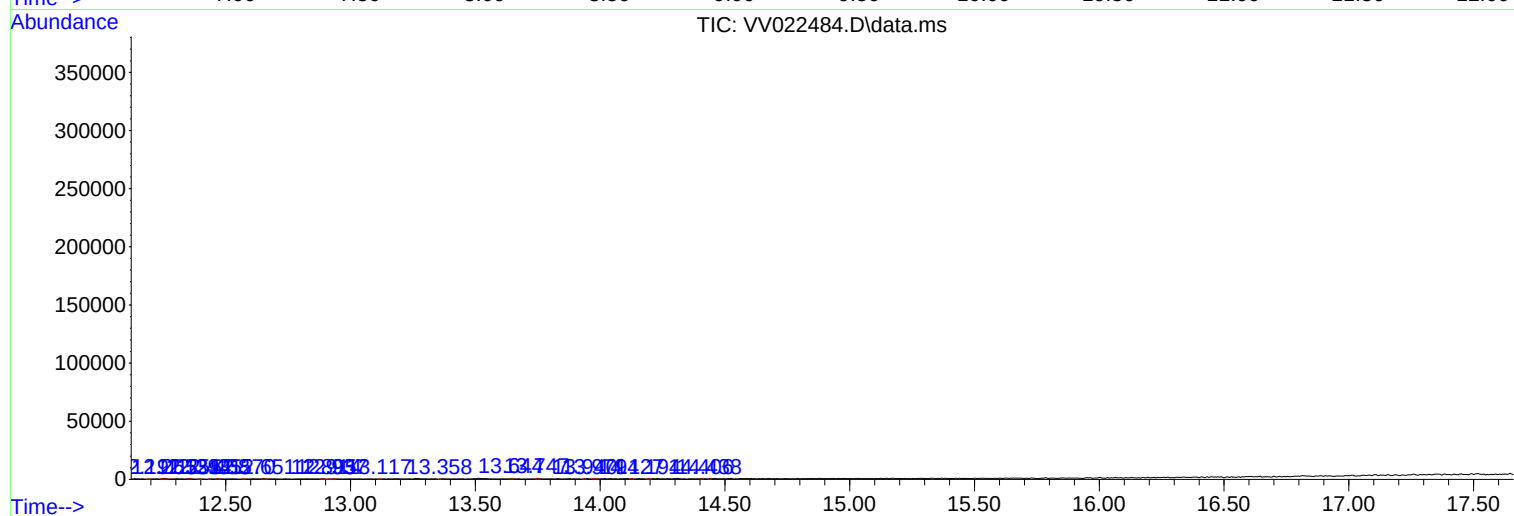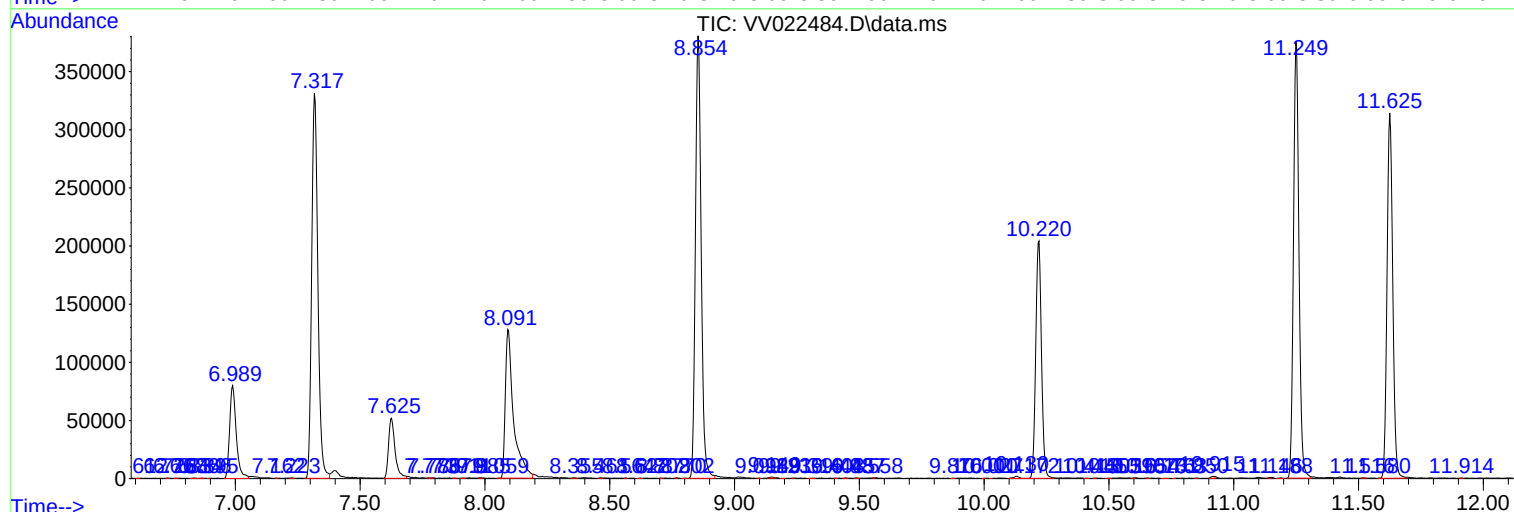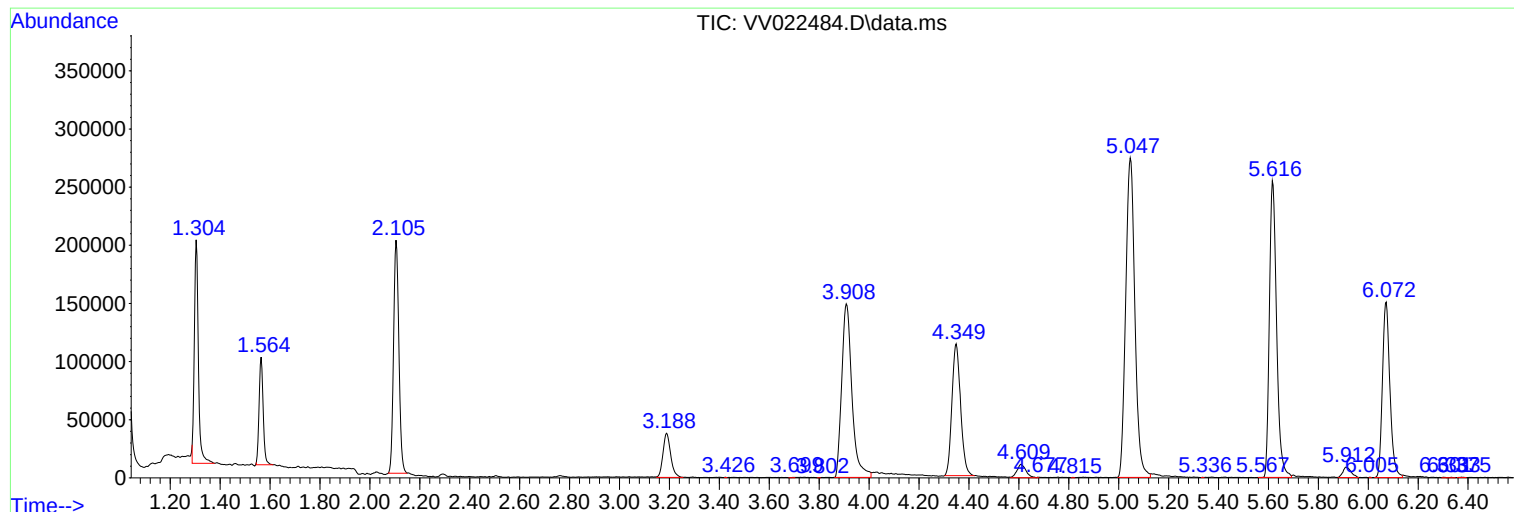

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022484.D
Acq On : 02 Oct 2021 00:05
Operator : SY/MD
Sample : M4024-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022484.D
Acq On : 02 Oct 2021 00:05
Operator : SY/MD
Sample : M4024-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
