

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022485.D
 Acq On : 02 Oct 2021 00:29
 Operator : SY/MD
 Sample : M4024-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

Signal : TIC: VV022485.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	124940	127340	17.08%	2.133%
2	1.568	157	164	176	rVB	98018	109525	14.69%	1.835%
3	2.108	323	332	354	rVB	203163	295107	39.57%	4.943%
4	2.940	588	591	593	rBV3	756	478	0.06%	0.008%
5	3.185	665	667	670	rBV3	337	198	0.03%	0.003%
6	3.375	724	726	727	rVB	356	99	0.01%	0.002%
7	3.384	727	729	732	rBV2	309	159	0.02%	0.003%
8	3.410	735	737	740	rBV	242	131	0.02%	0.002%
9	3.426	740	742	745	rBV2	293	150	0.02%	0.003%
10	3.522	771	772	773	rBV2	207	48	0.01%	0.001%
11	3.728	834	836	838	rBV2	181	100	0.01%	0.002%
12	3.866	877	879	880	rBV2	310	125	0.02%	0.002%
13	3.899	880	889	922	rBV2	32641	127983	17.16%	2.144%
14	4.352	1017	1030	1055	rVB	121850	294250	39.46%	4.929%
15	4.863	1186	1189	1192	rBV	500	324	0.04%	0.005%
16	4.921	1205	1207	1208	rBV	213	51	0.01%	0.001%
17	4.963	1218	1220	1223	rBV2	241	101	0.01%	0.002%
18	5.046	1230	1246	1276	rBV2	290804	745751	100.00%	12.492%
19	5.355	1340	1342	1343	rBV	386	156	0.02%	0.003%
20	5.381	1348	1350	1352	rBV	316	145	0.02%	0.002%
21	5.500	1384	1387	1390	rBV	314	247	0.03%	0.004%
22	5.619	1411	1424	1445	rBV	279158	559927	75.08%	9.379%
23	5.969	1531	1533	1534	rBV	153	48	0.01%	0.001%
24	6.072	1551	1565	1587	rBV	159539	328545	44.06%	5.503%
25	6.265	1624	1625	1630	rVB	325	151	0.02%	0.003%
26	6.574	1720	1721	1726	rVB3	360	156	0.02%	0.003%
27	6.657	1744	1747	1751	rVB3	322	184	0.02%	0.003%
28	6.805	1792	1793	1796	rBV2	246	107	0.01%	0.002%
29	6.989	1839	1850	1878	rBV	84315	155609	20.87%	2.607%
30	7.239	1926	1928	1931	rBV2	458	286	0.04%	0.005%
31	7.255	1931	1933	1936	rBV2	312	132	0.02%	0.002%
32	7.316	1940	1952	1970	rBV	351261	603210	80.89%	10.104%
33	7.625	2038	2048	2065	rBV	55629	99956	13.40%	1.674%
34	7.847	2115	2117	2122	rVB	852	641	0.09%	0.011%
35	7.876	2122	2126	2127	rBV	486	332	0.04%	0.006%
36	8.091	2183	2193	2236	rBV	148574	329402	44.17%	5.518%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022485.D
 Acq On : 02 Oct 2021 00:29
 Operator : SY/MD
 Sample : M4024-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

37	8.371	2279	2280	2283	rBV2	436	214	0.03%	0.004%
38	8.853	2419	2430	2450	rBV	410703	666809	89.41%	11.170%
39	9.230	2545	2547	2548	rBV	363	128	0.02%	0.002%
40	9.429	2607	2609	2610	rBV	225	112	0.02%	0.002%
41	9.615	2665	2667	2676	rBV3	425	464	0.06%	0.008%
42	9.693	2689	2691	2693	rBV	358	165	0.02%	0.003%
43	9.863	2741	2744	2749	rBV3	268	208	0.03%	0.003%
44	9.905	2756	2757	2760	rVB2	349	135	0.02%	0.002%
45	9.934	2764	2766	2768	rBV2	249	88	0.01%	0.001%
46	10.127	2819	2826	2836	rVB5	1944	3105	0.42%	0.052%
47	10.165	2836	2838	2841	rBV	349	242	0.03%	0.004%
48	10.220	2842	2855	2871	rBV	221032	349902	46.92%	5.861%
49	10.574	2961	2965	2968	rBV3	611	596	0.08%	0.010%
50	10.770	3024	3026	3027	rBV	229	86	0.01%	0.001%
51	10.831	3039	3045	3047	rBV2	534	445	0.06%	0.007%
52	10.956	3082	3084	3087	rBV	248	174	0.02%	0.003%
53	11.252	3164	3176	3201	rBV	407629	631588	84.69%	10.580%
54	11.625	3280	3292	3313	rBV	334467	531379	71.25%	8.901%
55	12.059	3425	3427	3428	rBV	382	156	0.02%	0.003%
56	12.091	3435	3437	3438	rBV	389	110	0.01%	0.002%
57	12.377	3523	3526	3528	rBV	340	179	0.02%	0.003%
58	12.647	3607	3610	3613	rBV2	584	344	0.05%	0.006%
59	12.680	3618	3620	3622	rBV	320	188	0.03%	0.003%
60	12.709	3627	3629	3631	rBV3	306	172	0.02%	0.003%
61	12.750	3640	3642	3644	rVB2	277	74	0.01%	0.001%
62	12.802	3656	3658	3660	rBV	257	97	0.01%	0.002%
63	12.927	3695	3697	3698	rBV	256	103	0.01%	0.002%
64	13.271	3801	3804	3810	rBV3	611	752	0.10%	0.013%
65	13.348	3826	3828	3830	rBV	344	145	0.02%	0.002%
66	13.705	3936	3939	3942	rBV2	521	355	0.05%	0.006%
67	14.435	4165	4166	4167	rBV2	296	108	0.01%	0.002%




Sum of corrected areas: 5969777

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022485.D
Acq On : 02 Oct 2021 00:29
Operator : SY/MD
Sample : M4024-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

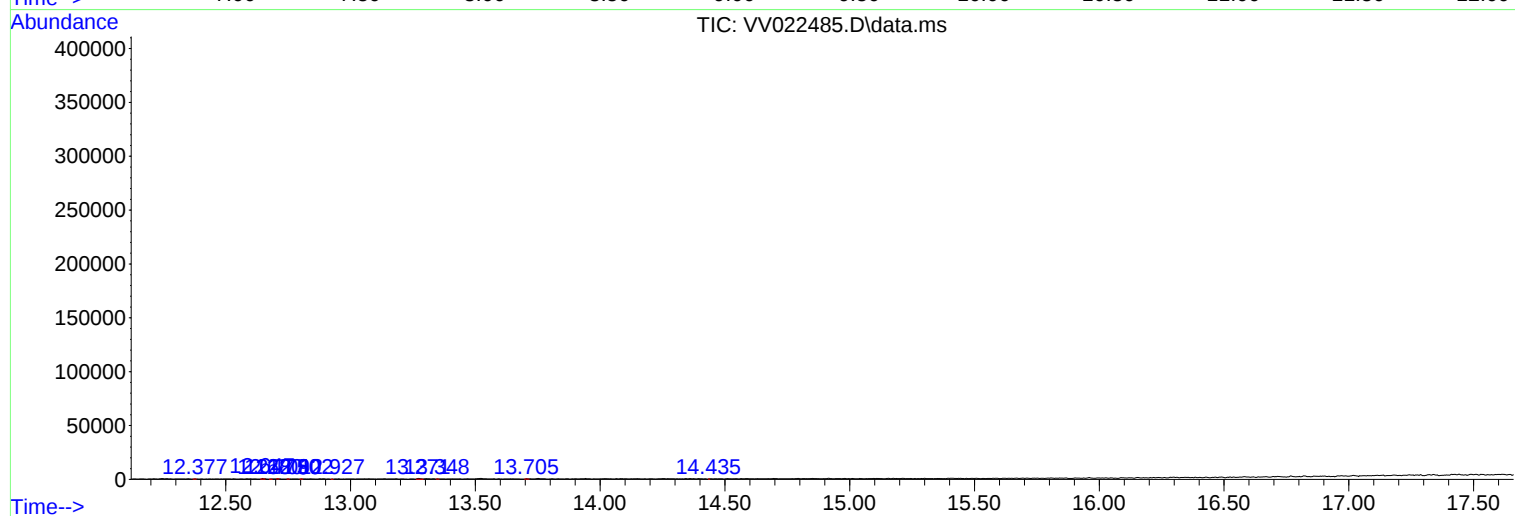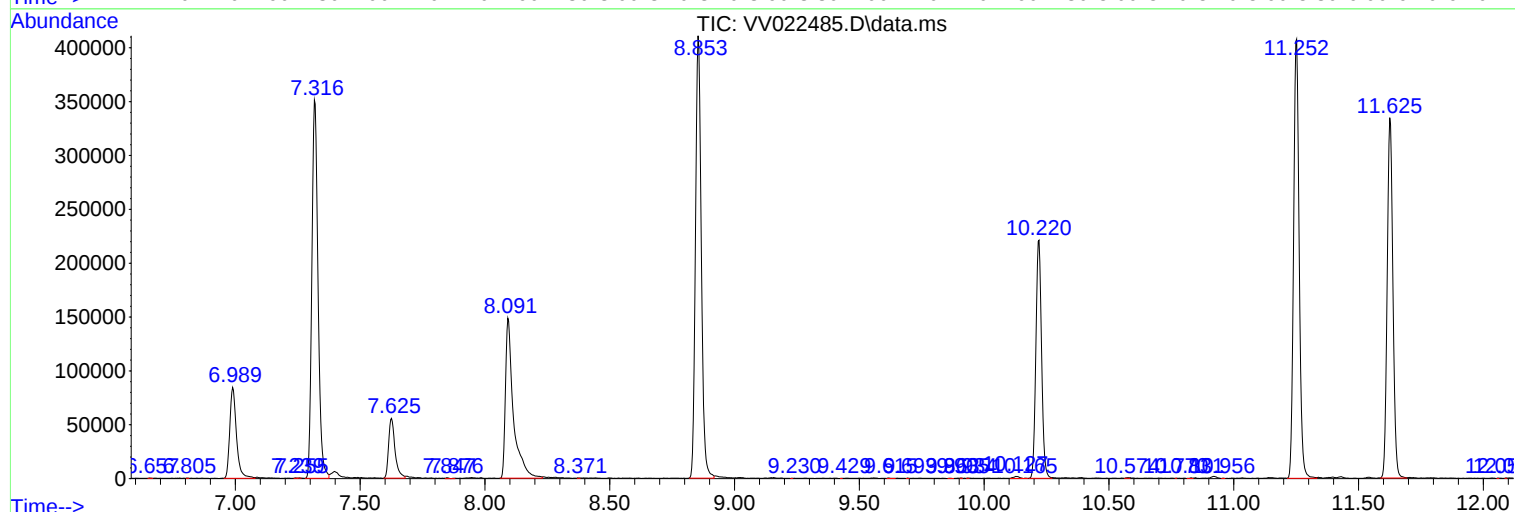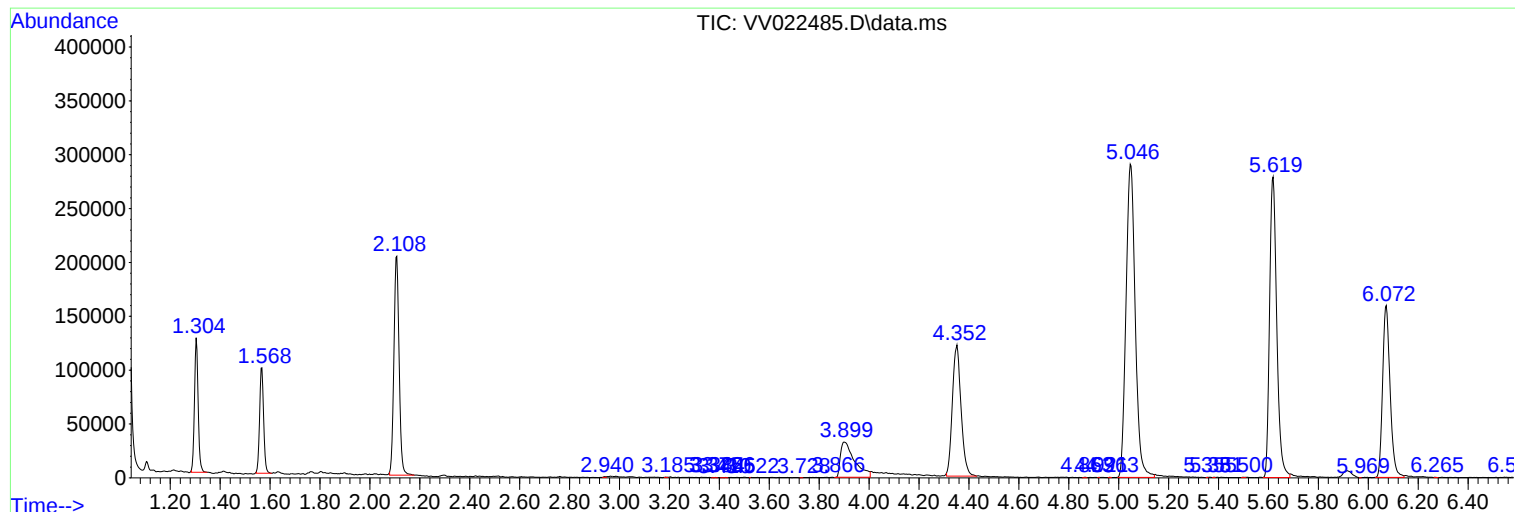

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022485.D
Acq On : 02 Oct 2021 00:29
Operator : SY/MD
Sample : M4024-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022485.D
Acq On : 02 Oct 2021 00:29
Operator : SY/MD
Sample : M4024-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
