

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022486.D
 Acq On : 02 Oct 2021 00:52
 Operator : SY/MD
 Sample : M4024-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M

Title : VOC Analysis

Signal : TIC: VV022486.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	119574	118504	10.69%	1.677%
2	1.568	156	164	177	rBV	96347	109627	9.89%	1.552%
3	2.108	322	332	351	rVB2	217634	332179	29.96%	4.702%
4	2.635	495	496	501	rBV3	401	300	0.03%	0.004%
5	2.680	508	510	512	rBV	330	142	0.01%	0.002%
6	2.790	542	544	545	rBV	346	154	0.01%	0.002%
7	2.854	562	564	566	rVB	353	138	0.01%	0.002%
8	2.928	585	587	590	rVB3	462	266	0.02%	0.004%
9	2.979	600	603	604	rBV	238	148	0.01%	0.002%
10	3.053	622	626	631	rBV2	549	525	0.05%	0.007%
11	3.175	661	664	665	rBV2	533	294	0.03%	0.004%
12	3.413	732	738	741	rBV2	442	470	0.04%	0.007%
13	3.452	748	750	751	rBV2	365	135	0.01%	0.002%
14	3.545	775	779	781	rBV2	320	160	0.01%	0.002%
15	3.661	814	815	819	rVB2	432	182	0.02%	0.003%
16	3.683	819	822	823	rBV2	249	138	0.01%	0.002%
17	3.905	879	891	923	rBV2	33747	134967	12.17%	1.910%
18	4.349	1017	1029	1054	rVB	118398	292203	26.35%	4.136%
19	4.683	1131	1133	1137	rVB2	315	170	0.02%	0.002%
20	4.709	1137	1141	1142	rBV2	329	190	0.02%	0.003%
21	4.761	1153	1157	1159	rBV2	303	203	0.02%	0.003%
22	4.892	1193	1198	1203	rBV2	209	264	0.02%	0.004%
23	4.921	1203	1207	1209	rBV2	188	141	0.01%	0.002%
24	4.937	1209	1212	1214	rBV2	342	206	0.02%	0.003%
25	5.047	1229	1246	1270	rBV2	289452	733373	66.14%	10.381%
26	5.388	1348	1352	1353	rBV2	243	143	0.01%	0.002%
27	5.449	1368	1371	1377	rVB2	631	483	0.04%	0.007%
28	5.478	1377	1380	1384	rBV2	167	179	0.02%	0.003%
29	5.503	1384	1388	1389	rBV2	242	142	0.01%	0.002%
30	5.619	1411	1424	1453	rBV	276077	560629	50.56%	7.935%
31	5.812	1481	1484	1485	rBV2	441	234	0.02%	0.003%
32	5.915	1502	1516	1539	rBV	567927	1108786	100.00%	15.694%
33	6.072	1553	1565	1586	rVB	159110	321264	28.97%	4.547%
34	6.243	1616	1618	1622	rVB3	497	371	0.03%	0.005%
35	6.664	1746	1749	1751	rBV2	174	142	0.01%	0.002%
36	6.680	1751	1754	1757	rVV2	240	152	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022486.D
 Acq On : 02 Oct 2021 00:52
 Operator : SY/MD
 Sample : M4024-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

37	6.728	1767	1769	1774	rVB	225	204	0.02%	0.003%
38	6.796	1787	1790	1793	rBV2	301	170	0.02%	0.002%
39	6.841	1799	1804	1806	rBV2	282	290	0.03%	0.004%
40	6.989	1840	1850	1875	rBV	84362	156941	14.15%	2.221%
41	7.317	1940	1952	1969	rBV	343255	597002	53.84%	8.450%
42	7.516	2011	2014	2016	rBV2	420	229	0.02%	0.003%
43	7.574	2027	2032	2034	rBV2	498	381	0.03%	0.005%
44	7.622	2034	2047	2067	rBV2	55020	100131	9.03%	1.417%
45	7.773	2091	2094	2096	rBV2	354	189	0.02%	0.003%
46	7.889	2129	2130	2133	rBV2	238	134	0.01%	0.002%
47	7.989	2157	2161	2164	rVV4	616	488	0.04%	0.007%
48	8.092	2184	2193	2228	rBV	142291	313015	28.23%	4.431%
49	8.375	2278	2281	2284	rBV3	450	321	0.03%	0.005%
50	8.432	2293	2299	2306	rBV3	674	778	0.07%	0.011%
51	8.461	2306	2308	2311	rVB2	420	195	0.02%	0.003%
52	8.603	2350	2352	2355	rBV	439	268	0.02%	0.004%
53	8.854	2418	2430	2458	rBV	412971	670885	60.51%	9.496%
54	9.018	2477	2481	2485	rBV5	538	604	0.05%	0.009%
55	9.085	2500	2502	2506	rBV	246	171	0.02%	0.002%
56	9.146	2518	2521	2523	rBV2	445	342	0.03%	0.005%
57	9.182	2531	2532	2537	rVB	491	278	0.03%	0.004%
58	9.207	2537	2540	2542	rBV2	217	144	0.01%	0.002%
59	9.368	2587	2590	2592	rBV2	385	261	0.02%	0.004%
60	9.403	2596	2601	2603	rVV3	289	279	0.03%	0.004%
61	9.638	2672	2674	2677	rBV3	302	168	0.02%	0.002%
62	9.677	2683	2686	2689	rBV2	324	280	0.03%	0.004%
63	9.728	2700	2702	2710	rVB3	304	336	0.03%	0.005%
64	9.776	2713	2717	2721	rBV2	188	178	0.02%	0.003%
65	10.021	2790	2793	2796	rBV3	296	253	0.02%	0.004%
66	10.082	2808	2812	2814	rBV2	150	144	0.01%	0.002%
67	10.137	2819	2829	2835	rVV5	1585	2762	0.25%	0.039%
68	10.217	2843	2854	2872	rBV	215197	344948	31.11%	4.883%
69	10.381	2896	2905	2908	rBV3	853	1030	0.09%	0.015%
70	10.497	2939	2941	2945	rBV2	283	187	0.02%	0.003%
71	10.712	3007	3008	3011	rBV	232	134	0.01%	0.002%
72	10.854	3047	3052	3055	rBV3	345	351	0.03%	0.005%
73	10.918	3066	3072	3080	rVB6	1712	2299	0.21%	0.033%
74	11.001	3091	3098	3100	rBV2	274	293	0.03%	0.004%
75	11.095	3123	3127	3128	rBV2	625	457	0.04%	0.006%
76	11.137	3138	3140	3141	rBV	395	142	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022486.D
 Acq On : 02 Oct 2021 00:52
 Operator : SY/MD
 Sample : M4024-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

77	11.249	3164	3175	3195	rBV	401883	622440	56.14%	8.810%
78	11.381	3212	3216	3218	rBV4	812	784	0.07%	0.011%
79	11.625	3280	3292	3311	rBV	328378	521825	47.06%	7.386%
80	11.854	3361	3363	3368	rVB3	393	190	0.02%	0.003%
81	11.899	3375	3377	3380	rBV2	387	173	0.02%	0.002%
82	12.043	3416	3422	3424	rBV	359	302	0.03%	0.004%
83	12.153	3454	3456	3458	rBV2	368	169	0.02%	0.002%
84	12.368	3520	3523	3527	rBV2	160	179	0.02%	0.003%
85	12.776	3647	3650	3653	rBV2	192	153	0.01%	0.002%
86	12.860	3673	3676	3678	rBV3	432	256	0.02%	0.004%
87	13.037	3729	3731	3734	rBV	271	163	0.01%	0.002%
88	13.053	3734	3736	3738	rVV	279	145	0.01%	0.002%
89	13.082	3742	3745	3747	rBV	294	173	0.02%	0.002%
90	13.220	3786	3788	3793	rBV2	257	180	0.02%	0.003%
91	13.265	3799	3802	3810	rBV3	523	671	0.06%	0.009%
92	13.317	3816	3818	3820	rBV	281	134	0.01%	0.002%
93	13.452	3856	3860	3864	rBV2	298	328	0.03%	0.005%
94	13.480	3867	3869	3873	rVB2	325	158	0.01%	0.002%
95	13.673	3926	3929	3931	rBV2	286	171	0.02%	0.002%
96	13.722	3942	3944	3950	rVB2	224	140	0.01%	0.002%
97	13.760	3952	3956	3958	rVB2	436	310	0.03%	0.004%
98	13.789	3963	3965	3969	rVB2	428	217	0.02%	0.003%
99	14.124	4066	4069	4073	rBV3	197	157	0.01%	0.002%
100	14.397	4151	4154	4155	rBV	279	157	0.01%	0.002%




Sum of corrected areas: 7064841

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022486.D
Acq On : 02 Oct 2021 00:52
Operator : SY/MD
Sample : M4024-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

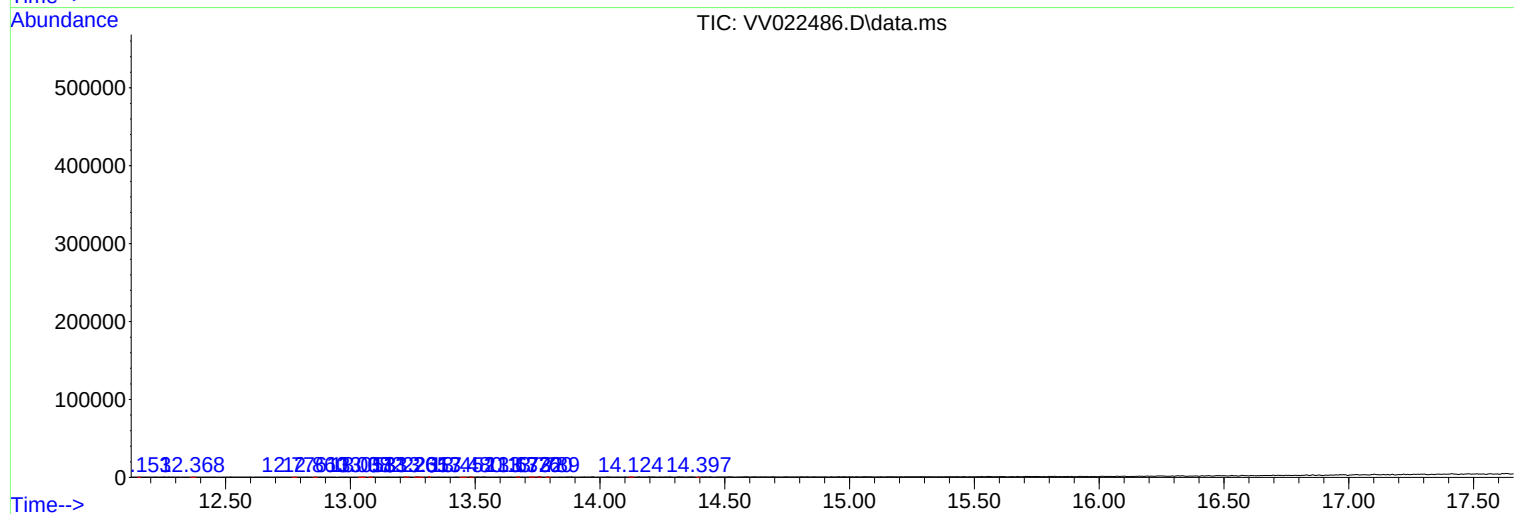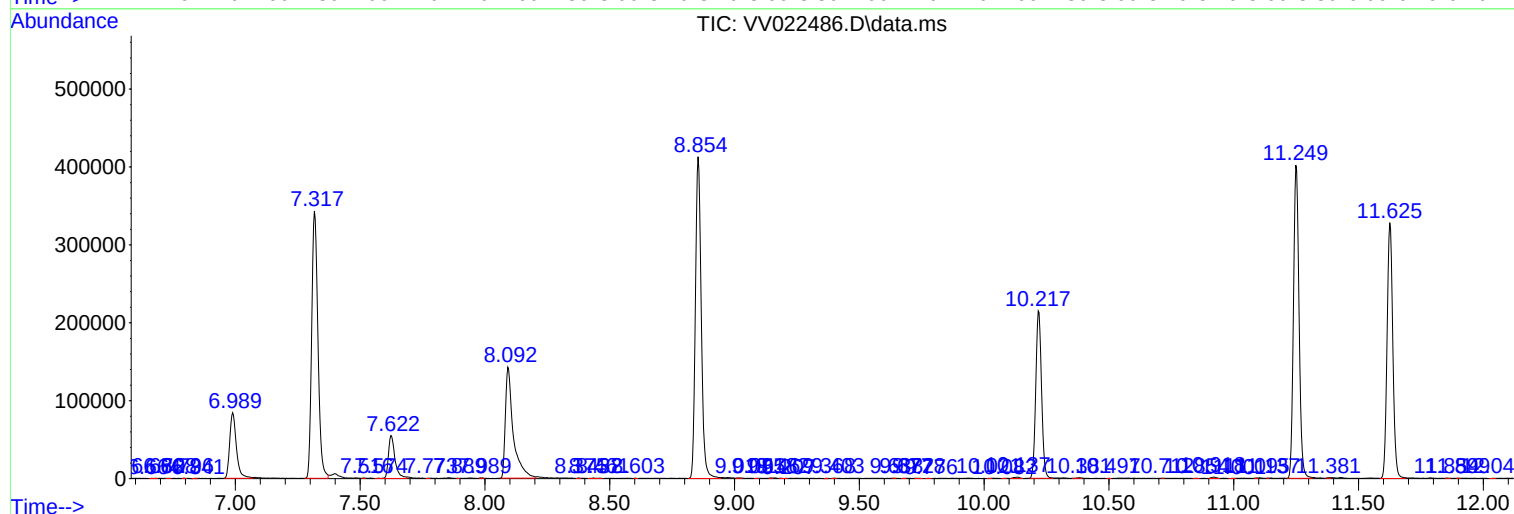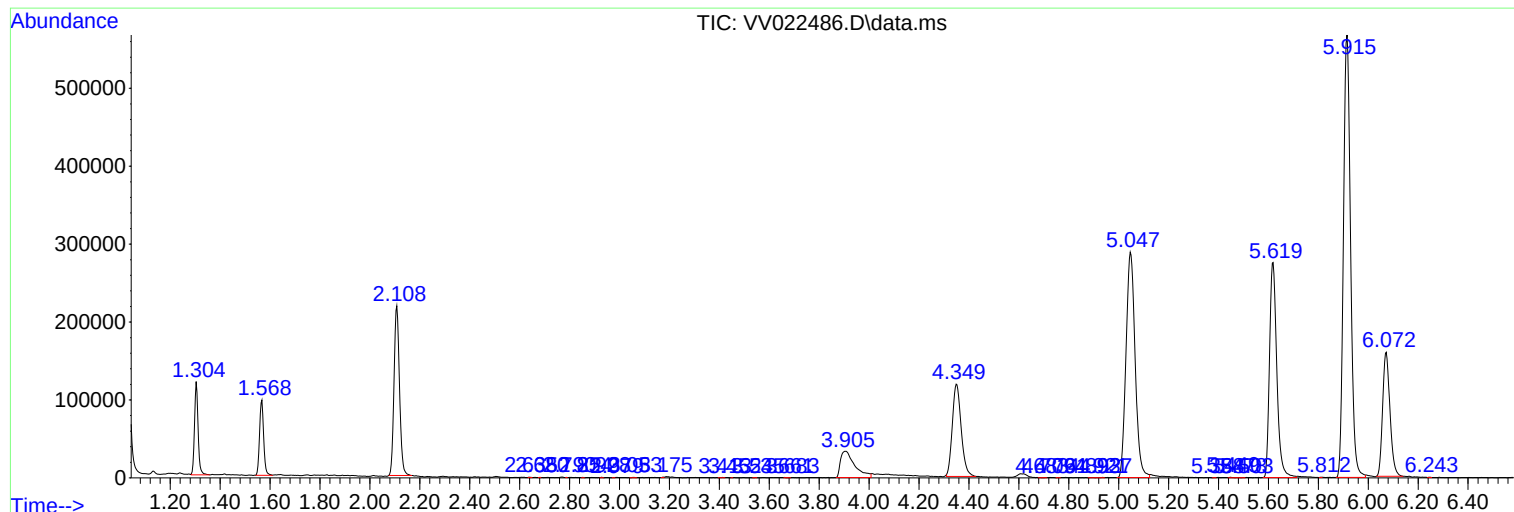

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022486.D
Acq On : 02 Oct 2021 00:52
Operator : SY/MD
Sample : M4024-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022486.D
Acq On : 02 Oct 2021 00:52
Operator : SY/MD
Sample : M4024-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
