

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022488.D
 Acq On : 02 Oct 2021 01:40
 Operator : SY/MD
 Sample : M4024-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

Signal : TIC: VV022488.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	77	82	94	rVB	110980	112758	15.85%	1.964%
2	1.568	157	164	175	rVB	91517	103459	14.54%	1.802%
3	2.108	323	332	356	rVB	186659	276319	38.85%	4.812%
4	3.282	693	697	699	rBV2	352	270	0.04%	0.005%
5	3.336	711	714	716	rBV	312	146	0.02%	0.003%
6	3.349	716	718	722	rVB2	624	335	0.05%	0.006%
7	3.378	725	727	730	rVB2	237	115	0.02%	0.002%
8	3.761	843	846	847	rBV	305	159	0.02%	0.003%
9	3.896	878	888	920	rBV2	34176	122292	17.19%	2.130%
10	4.349	1016	1029	1060	rVB2	113749	286351	40.26%	4.987%
11	4.661	1123	1126	1128	rBV	225	183	0.03%	0.003%
12	4.783	1162	1164	1166	rBV	389	199	0.03%	0.003%
13	4.847	1180	1184	1188	rBV2	244	223	0.03%	0.004%
14	5.047	1229	1246	1276	rBV3	277170	711306	100.00%	12.387%
15	5.381	1347	1350	1352	rBV2	298	160	0.02%	0.003%
16	5.487	1381	1383	1385	rVB2	279	106	0.01%	0.002%
17	5.619	1411	1424	1455	rBV	257606	522977	73.52%	9.107%
18	5.918	1506	1517	1530	rVB9	5747	12806	1.80%	0.223%
19	6.072	1552	1565	1586	rBV	154141	316150	44.45%	5.506%
20	6.259	1621	1623	1626	rBV	274	237	0.03%	0.004%
21	6.291	1630	1633	1638	rVV3	491	315	0.04%	0.005%
22	6.384	1659	1662	1664	rVB2	251	106	0.01%	0.002%
23	6.439	1676	1679	1681	rBV	263	172	0.02%	0.003%
24	6.516	1699	1703	1706	rBV2	405	359	0.05%	0.006%
25	6.587	1720	1725	1730	rBV2	330	350	0.05%	0.006%
26	6.654	1744	1746	1750	rVB2	375	173	0.02%	0.003%
27	6.674	1750	1752	1754	rBV	339	137	0.02%	0.002%
28	6.715	1762	1765	1770	rVB2	291	215	0.03%	0.004%
29	6.851	1800	1807	1810	rBV2	237	337	0.05%	0.006%
30	6.989	1840	1850	1872	rBV2	79112	147496	20.74%	2.569%
31	7.175	1904	1908	1911	rVB2	370	214	0.03%	0.004%
32	7.207	1915	1918	1919	rBV	500	173	0.02%	0.003%
33	7.317	1941	1952	1971	rBV	327531	564911	79.42%	9.838%
34	7.555	2022	2026	2027	rBV2	348	189	0.03%	0.003%
35	7.580	2031	2034	2035	rBV	362	182	0.03%	0.003%
36	7.625	2038	2048	2064	rBV2	52645	93274	13.11%	1.624%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100121\
 Data File : VW022488.D
 Acq On : 02 Oct 2021 01:40
 Operator : SY/MD
 Sample : M4024-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

37	7.789	2097	2099	2101	rVB2	455	217	0.03%	0.004%
38	7.812	2104	2106	2108	rBV	242	126	0.02%	0.002%
39	7.825	2108	2110	2112	rBV	363	130	0.02%	0.002%
40	7.976	2155	2157	2158	rBV	477	162	0.02%	0.003%
41	8.037	2173	2176	2178	rBV2	230	147	0.02%	0.003%
42	8.053	2179	2181	2183	rVV	302	161	0.02%	0.003%
43	8.092	2184	2193	2236	rVV	148697	328826	46.23%	5.726%
44	8.600	2348	2351	2352	rBV	212	145	0.02%	0.003%
45	8.658	2367	2369	2374	rVB2	287	157	0.02%	0.003%
46	8.854	2418	2430	2451	rBV	381812	620173	87.19%	10.800%
47	9.069	2494	2497	2500	rBV	603	323	0.05%	0.006%
48	9.130	2514	2516	2517	rBV	318	132	0.02%	0.002%
49	9.233	2546	2548	2552	rBV3	511	326	0.05%	0.006%
50	9.821	2729	2731	2736	rVB2	313	197	0.03%	0.003%
51	9.860	2740	2743	2744	rVV	337	124	0.02%	0.002%
52	9.915	2758	2760	2761	rBV	253	105	0.01%	0.002%
53	10.002	2784	2787	2789	rBV2	383	260	0.04%	0.005%
54	10.217	2843	2854	2872	rBV	210924	342478	48.15%	5.964%
55	10.410	2912	2914	2915	rBV	239	118	0.02%	0.002%
56	10.590	2969	2970	2974	rVB2	373	184	0.03%	0.003%
57	10.686	2996	3000	3002	rBV	221	153	0.02%	0.003%
58	10.725	3010	3012	3014	rBV	246	122	0.02%	0.002%
59	10.841	3043	3048	3051	rBV2	230	270	0.04%	0.005%
60	10.866	3054	3056	3059	rVB	394	180	0.03%	0.003%
61	10.886	3059	3062	3064	rBV2	379	234	0.03%	0.004%
62	10.924	3065	3074	3081	rVV7	1186	1879	0.26%	0.033%
63	10.956	3081	3084	3089	rVB2	453	311	0.04%	0.005%
64	11.053	3112	3114	3120	rBV3	442	427	0.06%	0.007%
65	11.082	3120	3123	3124	rBV2	706	333	0.05%	0.006%
66	11.137	3137	3140	3141	rBV	676	340	0.05%	0.006%
67	11.249	3163	3175	3196	rBV	368392	572265	80.45%	9.966%
68	11.452	3236	3238	3241	rBV	735	397	0.06%	0.007%
69	11.625	3279	3292	3316	rBV	312831	497947	70.00%	8.671%
70	11.747	3325	3330	3333	rBV5	1033	956	0.13%	0.017%
71	11.905	3373	3379	3381	rBV2	368	295	0.04%	0.005%
72	11.921	3382	3384	3385	rBV	359	132	0.02%	0.002%
73	12.024	3411	3416	3420	rBV2	372	422	0.06%	0.007%
74	12.233	3479	3481	3485	rBV2	547	241	0.03%	0.004%
75	12.262	3488	3490	3491	rBV	357	117	0.02%	0.002%
76	12.284	3494	3497	3498	rBV2	748	459	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022488.D
 Acq On : 02 Oct 2021 01:40
 Operator : SY/MD
 Sample : M4024-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

77	12.342	3512	3515	3518	rBV2	301	204	0.03%	0.004%
78	12.384	3524	3528	3533	rBV6	1043	1056	0.15%	0.018%
79	12.551	3573	3580	3583	rBV3	1451	1607	0.23%	0.028%
80	12.625	3599	3603	3606	rVB3	457	284	0.04%	0.005%
81	12.757	3638	3644	3652	rVB3	1621	2070	0.29%	0.036%
82	12.796	3652	3656	3658	rBV2	278	186	0.03%	0.003%
83	12.963	3704	3708	3716	rVB4	1041	1081	0.15%	0.019%
84	13.011	3721	3723	3724	rBV	355	176	0.02%	0.003%
85	13.124	3755	3758	3760	rBV	437	277	0.04%	0.005%
86	13.243	3793	3795	3796	rBV	313	113	0.02%	0.002%
87	13.271	3798	3804	3809	rVV6	1139	1473	0.21%	0.026%
88	13.336	3810	3824	3836	rVB4	5760	13107	1.84%	0.228%
89	13.468	3861	3865	3866	rBV	252	159	0.02%	0.003%
90	13.490	3866	3872	3874	rBV4	800	932	0.13%	0.016%
91	13.616	3902	3911	3923	rVB4	13399	19866	2.79%	0.346%
92	13.677	3927	3930	3931	rBV	530	305	0.04%	0.005%
93	13.706	3931	3939	3951	rVV5	15195	24686	3.47%	0.430%
94	14.095	4052	4060	4066	rBV7	5076	9744	1.37%	0.170%
95	14.197	4089	4092	4095	rBV3	713	658	0.09%	0.011%
96	14.365	4139	4144	4148	rBV5	1674	2084	0.29%	0.036%
97	14.452	4162	4171	4179	rBV4	5826	8970	1.26%	0.156%
98	14.767	4261	4269	4277	rBV10	3171	5306	0.75%	0.092%
99	14.976	4332	4334	4336	rBV	805	379	0.05%	0.007%
100	15.474	4487	4489	4492	rBV3	793	556	0.08%	0.010%




Sum of corrected areas: 5742404

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022488.D
Acq On : 02 Oct 2021 01:40
Operator : SY/MD
Sample : M4024-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

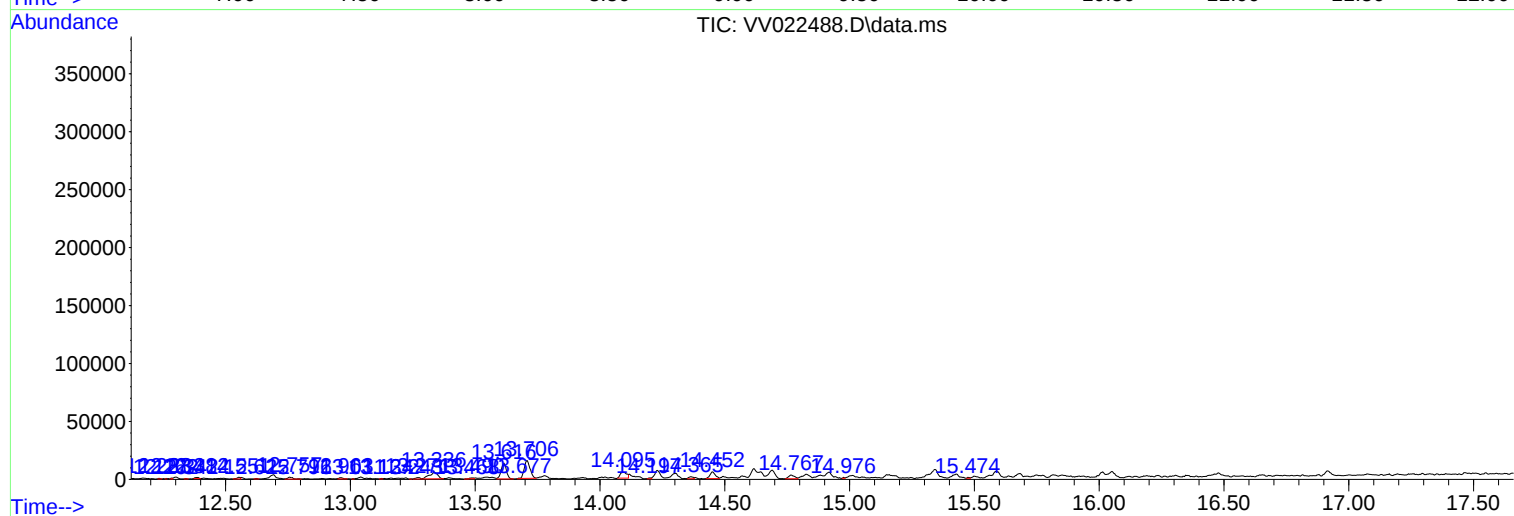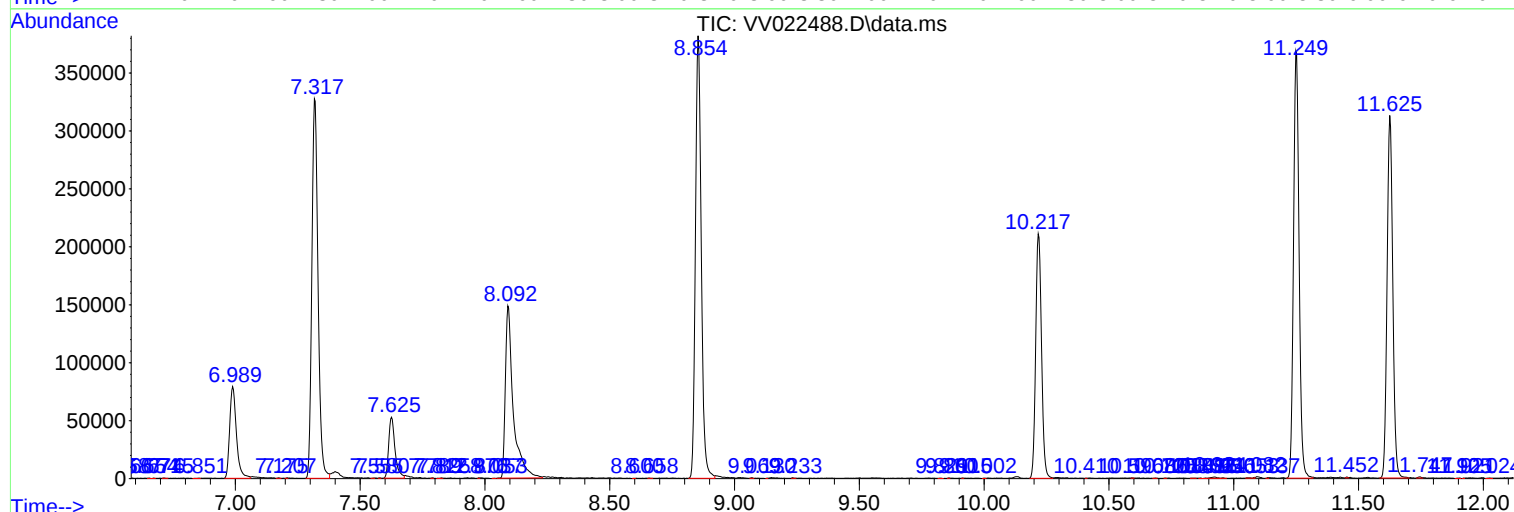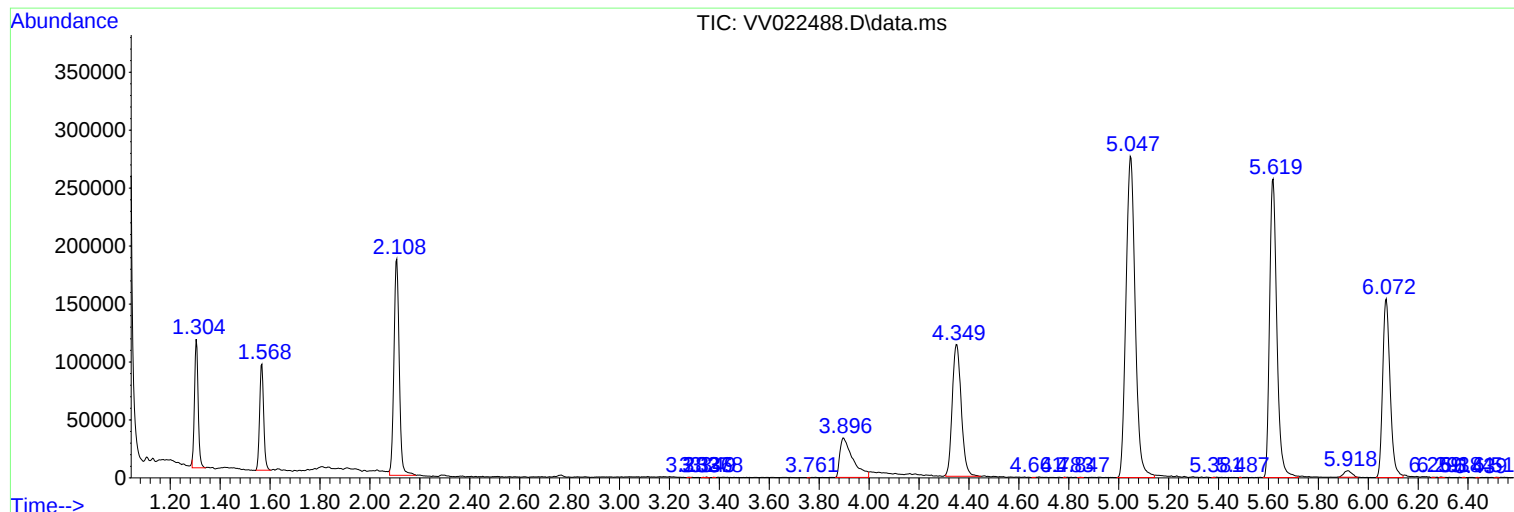

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022488.D
Acq On : 02 Oct 2021 01:40
Operator : SY/MD
Sample : M4024-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022488.D
Acq On : 02 Oct 2021 01:40
Operator : SY/MD
Sample : M4024-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
