

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022490.D
 Acq On : 02 Oct 2021 02:27
 Operator : SY/MD
 Sample : M4024-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

Signal : TIC: VV022490.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	113003	113420	15.69%	1.935%
2	1.568	157	164	175	rVB	91152	103123	14.27%	1.759%
3	2.108	321	332	355	rBV	195903	284899	39.42%	4.859%
4	2.558	469	472	479	rBV4	490	496	0.07%	0.008%
5	2.626	491	493	498	rBV2	282	268	0.04%	0.005%
6	2.699	514	516	517	rBV2	402	139	0.02%	0.002%
7	2.751	529	532	534	rVB2	426	194	0.03%	0.003%
8	2.773	537	539	542	rVV	379	230	0.03%	0.004%
9	2.992	605	607	610	rBV	351	188	0.03%	0.003%
10	3.085	633	636	640	rVB2	155	116	0.02%	0.002%
11	3.288	696	699	700	rBV2	260	137	0.02%	0.002%
12	3.487	759	761	765	rBV2	166	120	0.02%	0.002%
13	3.654	810	813	816	rBV2	246	149	0.02%	0.003%
14	3.757	842	845	849	rVB2	166	120	0.02%	0.002%
15	3.844	869	872	875	rBV2	311	227	0.03%	0.004%
16	3.902	879	890	912	rBV2	32658	111683	15.45%	1.905%
17	4.349	1014	1029	1057	rVB2	116184	285409	39.49%	4.868%
18	4.664	1125	1127	1131	rBV3	276	145	0.02%	0.002%
19	4.683	1131	1133	1140	rVB2	446	416	0.06%	0.007%
20	4.715	1140	1143	1146	rBV	259	239	0.03%	0.004%
21	4.728	1146	1147	1150	rVB	280	143	0.02%	0.002%
22	4.809	1170	1172	1175	rBV2	301	196	0.03%	0.003%
23	4.857	1184	1187	1188	rBV2	232	122	0.02%	0.002%
24	4.896	1197	1199	1202	rBV2	143	106	0.01%	0.002%
25	4.941	1211	1213	1214	rBV2	271	119	0.02%	0.002%
26	5.047	1230	1246	1270	rBV2	284587	722782	100.00%	12.328%
27	5.313	1323	1329	1331	rBV2	185	178	0.02%	0.003%
28	5.362	1342	1344	1345	rBV2	318	142	0.02%	0.002%
29	5.423	1361	1363	1365	rBV	251	138	0.02%	0.002%
30	5.494	1383	1385	1387	rVB	258	101	0.01%	0.002%
31	5.561	1400	1406	1407	rBV3	363	372	0.05%	0.006%
32	5.619	1411	1424	1453	rBV	267780	538489	74.50%	9.185%
33	5.918	1505	1517	1538	rBV5	45055	97143	13.44%	1.657%
34	6.018	1546	1548	1551	rVB3	397	187	0.03%	0.003%
35	6.072	1551	1565	1592	rBV	157234	324624	44.91%	5.537%
36	6.333	1642	1646	1649	rVB3	443	302	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100121\
 Data File : VW022490.D
 Acq On : 02 Oct 2021 02:27
 Operator : SY/MD
 Sample : M4024-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

37	6.413	1668	1671	1674	rVB	188	153	0.02%	0.003%
38	6.474	1688	1690	1693	rBV	281	100	0.01%	0.002%
39	6.625	1733	1737	1739	rBV	282	218	0.03%	0.004%
40	6.657	1745	1747	1750	rVB2	356	177	0.02%	0.003%
41	6.680	1750	1754	1755	rBV	275	157	0.02%	0.003%
42	6.989	1839	1850	1870	rBV	81913	149568	20.69%	2.551%
43	7.317	1941	1952	1971	rBV	336040	588974	81.49%	10.046%
44	7.625	2038	2048	2071	rBV	55483	97633	13.51%	1.665%
45	7.776	2093	2095	2098	rVB	377	159	0.02%	0.003%
46	7.866	2120	2123	2125	rBV2	260	199	0.03%	0.003%
47	7.915	2133	2138	2142	rBV2	624	550	0.08%	0.009%
48	7.931	2142	2143	2144	rBV2	375	137	0.02%	0.002%
49	7.989	2157	2161	2164	rBV3	558	401	0.06%	0.007%
50	8.037	2173	2176	2179	rBV	208	143	0.02%	0.002%
51	8.092	2183	2193	2229	rBV	145285	322173	44.57%	5.495%
52	8.452	2302	2305	2311	rBV2	393	288	0.04%	0.005%
53	8.481	2312	2314	2317	rBV2	201	133	0.02%	0.002%
54	8.564	2337	2340	2343	rBV	181	115	0.02%	0.002%
55	8.747	2395	2397	2401	rBV2	231	198	0.03%	0.003%
56	8.770	2401	2404	2408	rVB	265	188	0.03%	0.003%
57	8.854	2419	2430	2459	rBV	396959	643170	88.99%	10.970%
58	9.130	2514	2516	2517	rBV	385	163	0.02%	0.003%
59	9.185	2532	2533	2535	rVB	290	105	0.01%	0.002%
60	9.204	2535	2539	2543	rBV	305	328	0.05%	0.006%
61	9.259	2554	2556	2558	rVB2	330	152	0.02%	0.003%
62	9.519	2635	2637	2639	rVV	293	110	0.02%	0.002%
63	9.561	2644	2650	2655	rVV3	598	736	0.10%	0.013%
64	9.937	2764	2767	2768	rBV	205	101	0.01%	0.002%
65	9.976	2778	2779	2783	rBV	285	173	0.02%	0.003%
66	10.017	2789	2792	2795	rBV2	389	238	0.03%	0.004%
67	10.133	2819	2828	2833	rVB3	2003	2843	0.39%	0.048%
68	10.165	2833	2838	2841	rBV2	212	260	0.04%	0.004%
69	10.217	2841	2854	2872	rBV	213461	341948	47.31%	5.833%
70	10.362	2896	2899	2901	rBV2	675	388	0.05%	0.007%
71	10.461	2927	2930	2933	rBV3	286	226	0.03%	0.004%
72	10.535	2949	2953	2954	rBV	445	228	0.03%	0.004%
73	10.670	2991	2995	2996	rBV	356	225	0.03%	0.004%
74	10.696	3000	3003	3008	rBV2	385	395	0.05%	0.007%
75	10.924	3067	3074	3080	rVB4	1596	2031	0.28%	0.035%
76	10.956	3082	3084	3087	rBV	235	111	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022490.D
 Acq On : 02 Oct 2021 02:27
 Operator : SY/MD
 Sample : M4024-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

77	10.972	3087	3089	3094	rVB2	290	132	0.02%	0.002%
78	11.030	3105	3107	3109	rBV2	211	107	0.01%	0.002%
79	11.252	3164	3176	3193	rBV	393894	603115	83.44%	10.287%
80	11.625	3280	3292	3315	rVV	325822	512723	70.94%	8.745%
81	11.796	3341	3345	3349	rBV2	496	466	0.06%	0.008%
82	11.860	3363	3365	3369	rBV2	180	103	0.01%	0.002%
83	12.326	3506	3510	3513	rBV2	199	185	0.03%	0.003%
84	12.419	3537	3539	3541	rBV	259	109	0.02%	0.002%
85	12.503	3562	3565	3566	rBV	210	140	0.02%	0.002%
86	12.812	3659	3661	3664	rBV2	168	143	0.02%	0.002%
87	12.831	3664	3667	3670	rVV2	315	196	0.03%	0.003%
88	13.152	3764	3767	3772	rBV2	165	163	0.02%	0.003%
89	13.194	3777	3780	3783	rBV2	159	141	0.02%	0.002%
90	13.268	3800	3803	3805	rBV	217	175	0.02%	0.003%
91	13.365	3825	3833	3837	rBV2	369	535	0.07%	0.009%
92	13.416	3846	3849	3850	rBV	218	144	0.02%	0.002%
93	13.583	3899	3901	3902	rBV	414	166	0.02%	0.003%
94	13.763	3955	3957	3960	rVB	329	159	0.02%	0.003%
95	13.988	4025	4027	4030	rBV	333	222	0.03%	0.004%
96	14.143	4071	4075	4081	rBV2	425	384	0.05%	0.007%
97	14.204	4091	4094	4098	rBV	236	195	0.03%	0.003%
98	14.239	4102	4105	4107	rBV2	271	185	0.03%	0.003%
99	14.821	4282	4286	4288	rBV2	378	278	0.04%	0.005%
100	14.898	4308	4310	4311	rBV2	279	107	0.01%	0.002%


Sum of corrected areas: 5862730

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022490.D
Acq On : 02 Oct 2021 02:27
Operator : SY/MD
Sample : M4024-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AL8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

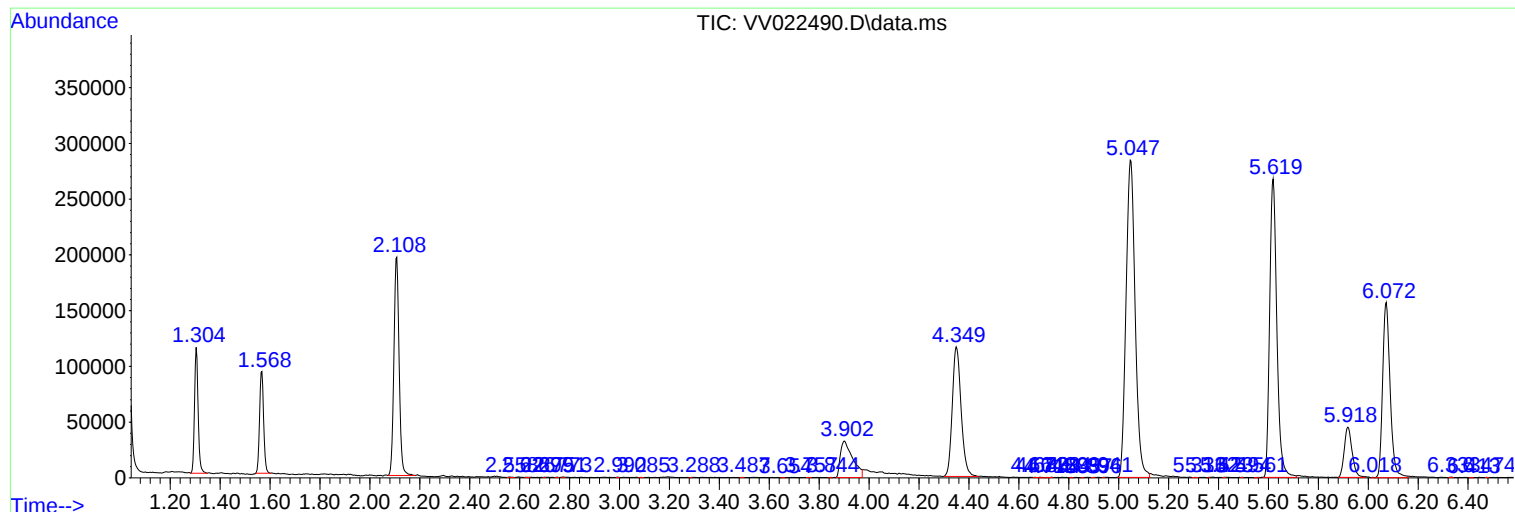

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022490.D
Acq On : 02 Oct 2021 02:27
Operator : SY/MD
Sample : M4024-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AL8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022490.D
Acq On : 02 Oct 2021 02:27
Operator : SY/MD
Sample : M4024-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AL8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
