

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022491.D
 Acq On : 02 Oct 2021 02:51
 Operator : SY/MD
 Sample : M4024-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

Signal : TIC: VV022491.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	112765	117807	16.23%	1.939%
2	1.568	157	164	174	rVB	95206	106383	14.66%	1.751%
3	2.108	322	332	347	rBV2	202408	299014	41.19%	4.923%
4	2.535	461	465	467	rBV2	407	316	0.04%	0.005%
5	2.658	501	503	505	rBV2	367	163	0.02%	0.003%
6	2.857	563	565	570	rVB3	322	222	0.03%	0.004%
7	2.966	596	599	604	rBV4	380	380	0.05%	0.006%
8	3.150	653	656	658	rBV2	296	183	0.03%	0.003%
9	3.198	663	671	676	rVV3	614	831	0.11%	0.014%
10	3.346	712	717	720	rBV2	203	225	0.03%	0.004%
11	3.394	727	732	736	rBV2	358	238	0.03%	0.004%
12	3.555	777	782	786	rBV2	216	275	0.04%	0.005%
13	3.645	807	810	814	rVB2	233	203	0.03%	0.003%
14	3.670	814	818	819	rBV	299	183	0.03%	0.003%
15	3.709	826	830	832	rBV2	259	227	0.03%	0.004%
16	3.754	840	844	847	rBV2	162	159	0.02%	0.003%
17	3.905	876	891	919	rBV3	42769	160391	22.10%	2.641%
18	4.352	1017	1030	1054	rVB2	115701	282211	38.88%	4.646%
19	4.568	1095	1097	1098	rBV	375	155	0.02%	0.003%
20	4.690	1132	1135	1136	rBV	394	197	0.03%	0.003%
21	4.735	1147	1149	1152	rBV2	258	155	0.02%	0.003%
22	5.047	1230	1246	1269	rBV2	285160	725853	100.00%	11.950%
23	5.442	1366	1369	1372	rBV	206	159	0.02%	0.003%
24	5.487	1380	1383	1386	rVB2	302	172	0.02%	0.003%
25	5.510	1389	1390	1393	rVB	366	158	0.02%	0.003%
26	5.551	1397	1403	1407	rBV2	370	412	0.06%	0.007%
27	5.619	1411	1424	1446	rBV	273945	545910	75.21%	8.987%
28	5.860	1496	1499	1502	rBV2	397	312	0.04%	0.005%
29	5.918	1504	1517	1537	rVV2	105741	215405	29.68%	3.546%
30	6.069	1553	1564	1591	rBV	156838	319623	44.03%	5.262%
31	6.243	1616	1618	1622	rVV3	401	230	0.03%	0.004%
32	6.320	1638	1642	1646	rVV2	350	251	0.03%	0.004%
33	6.352	1648	1652	1655	rVV3	379	290	0.04%	0.005%
34	6.596	1726	1728	1732	rVB	288	147	0.02%	0.002%
35	6.744	1768	1774	1775	rBV3	299	303	0.04%	0.005%
36	6.776	1780	1784	1786	rBV2	352	260	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100121\
 Data File : VW022491.D
 Acq On : 02 Oct 2021 02:51
 Operator : SY/MD
 Sample : M4024-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

37	6.989	1838	1850	1874	rBV	82373	151529	20.88%	2.495%
38	7.198	1912	1915	1920	rVB2	471	288	0.04%	0.005%
39	7.220	1920	1922	1923	rBV2	399	143	0.02%	0.002%
40	7.317	1940	1952	1972	rBV	337845	591533	81.49%	9.738%
41	7.625	2037	2048	2069	rBV2	53851	99880	13.76%	1.644%
42	7.931	2138	2143	2144	rBV	290	186	0.03%	0.003%
43	7.989	2158	2161	2165	rVB2	456	274	0.04%	0.005%
44	8.091	2183	2193	2238	rBV	144267	319908	44.07%	5.267%
45	8.439	2298	2301	2306	rVB2	475	365	0.05%	0.006%
46	8.474	2310	2312	2315	rVB	484	195	0.03%	0.003%
47	8.513	2321	2324	2330	rBV3	337	409	0.06%	0.007%
48	8.854	2419	2430	2458	rBV	398147	648403	89.33%	10.675%
49	9.133	2514	2517	2519	rBV2	284	180	0.02%	0.003%
50	9.149	2520	2522	2528	rVV2	579	514	0.07%	0.008%
51	9.181	2528	2532	2536	rVB4	512	377	0.05%	0.006%
52	9.278	2561	2562	2566	rVB	302	186	0.03%	0.003%
53	9.317	2569	2574	2575	rBV	420	264	0.04%	0.004%
54	9.474	2621	2623	2630	rVB2	301	173	0.02%	0.003%
55	9.509	2630	2634	2636	rVB	283	162	0.02%	0.003%
56	9.580	2654	2656	2659	rBV2	379	171	0.02%	0.003%
57	9.609	2663	2665	2669	rBV	251	176	0.02%	0.003%
58	9.680	2685	2687	2689	rBV	236	158	0.02%	0.003%
59	9.747	2705	2708	2709	rBV	306	156	0.02%	0.003%
60	9.934	2763	2766	2771	rBV2	319	298	0.04%	0.005%
61	10.075	2806	2810	2813	rBV2	258	196	0.03%	0.003%
62	10.133	2819	2828	2836	rBV7	1448	2389	0.33%	0.039%
63	10.217	2843	2854	2878	rVB	213513	340315	46.88%	5.603%
64	10.307	2878	2882	2883	rBV2	393	225	0.03%	0.004%
65	10.378	2901	2904	2907	rBV2	272	189	0.03%	0.003%
66	10.551	2954	2958	2959	rBV	403	312	0.04%	0.005%
67	10.596	2969	2972	2974	rVB2	484	266	0.04%	0.004%
68	10.911	3065	3070	3073	rBV6	888	1057	0.15%	0.017%
69	11.095	3122	3127	3128	rBV2	711	529	0.07%	0.009%
70	11.146	3139	3143	3150	rBV4	765	702	0.10%	0.012%
71	11.249	3163	3175	3197	rBV	393671	608203	83.79%	10.013%
72	11.538	3262	3265	3270	rVB3	394	333	0.05%	0.005%
73	11.625	3280	3292	3315	rBV	323160	517639	71.31%	8.522%
74	11.783	3338	3341	3346	rVB4	513	493	0.07%	0.008%
75	11.844	3354	3360	3363	rBV2	333	332	0.05%	0.005%
76	11.931	3383	3387	3389	rBV2	210	192	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022491.D
 Acq On : 02 Oct 2021 02:51
 Operator : SY/MD
 Sample : M4024-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

77	12.011	3410	3412	3417	rBV3	471	440	0.06%	0.007%
78	12.117	3442	3445	3449	rVB	209	148	0.02%	0.002%
79	12.278	3492	3495	3498	rBV2	207	181	0.02%	0.003%
80	12.320	3506	3508	3512	rVB	324	147	0.02%	0.002%
81	12.699	3623	3626	3628	rBV	199	162	0.02%	0.003%
82	12.763	3643	3646	3647	rBV	329	149	0.02%	0.002%
83	12.828	3662	3666	3668	rBV2	275	236	0.03%	0.004%
84	12.879	3679	3682	3684	rBV2	223	187	0.03%	0.003%
85	12.979	3711	3713	3717	rBV2	271	182	0.03%	0.003%
86	13.040	3729	3732	3734	rVB2	484	231	0.03%	0.004%
87	13.307	3812	3815	3820	rBV2	303	224	0.03%	0.004%
88	13.390	3837	3841	3845	rBV2	330	256	0.04%	0.004%
89	13.493	3868	3873	3875	rBV	343	303	0.04%	0.005%
90	13.644	3917	3920	3924	rVB	319	235	0.03%	0.004%
91	13.670	3924	3928	3929	rBV	284	169	0.02%	0.003%
92	13.728	3943	3946	3949	rVB3	311	221	0.03%	0.004%
93	13.747	3949	3952	3953	rBV	272	154	0.02%	0.003%
94	14.062	4048	4050	4053	rBV3	390	210	0.03%	0.003%
95	14.098	4059	4061	4064	rBV	345	196	0.03%	0.003%
96	14.239	4103	4105	4110	rBV2	320	243	0.03%	0.004%
97	14.467	4172	4176	4181	rBV2	333	420	0.06%	0.007%
98	14.599	4214	4217	4219	rBV3	275	217	0.03%	0.004%
99	15.072	4361	4364	4366	rBV2	364	231	0.03%	0.004%
100	15.104	4372	4374	4378	rBV2	481	377	0.05%	0.006%


Sum of corrected areas: 6074222

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022491.D
Acq On : 02 Oct 2021 02:51
Operator : SY/MD
Sample : M4024-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AL9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

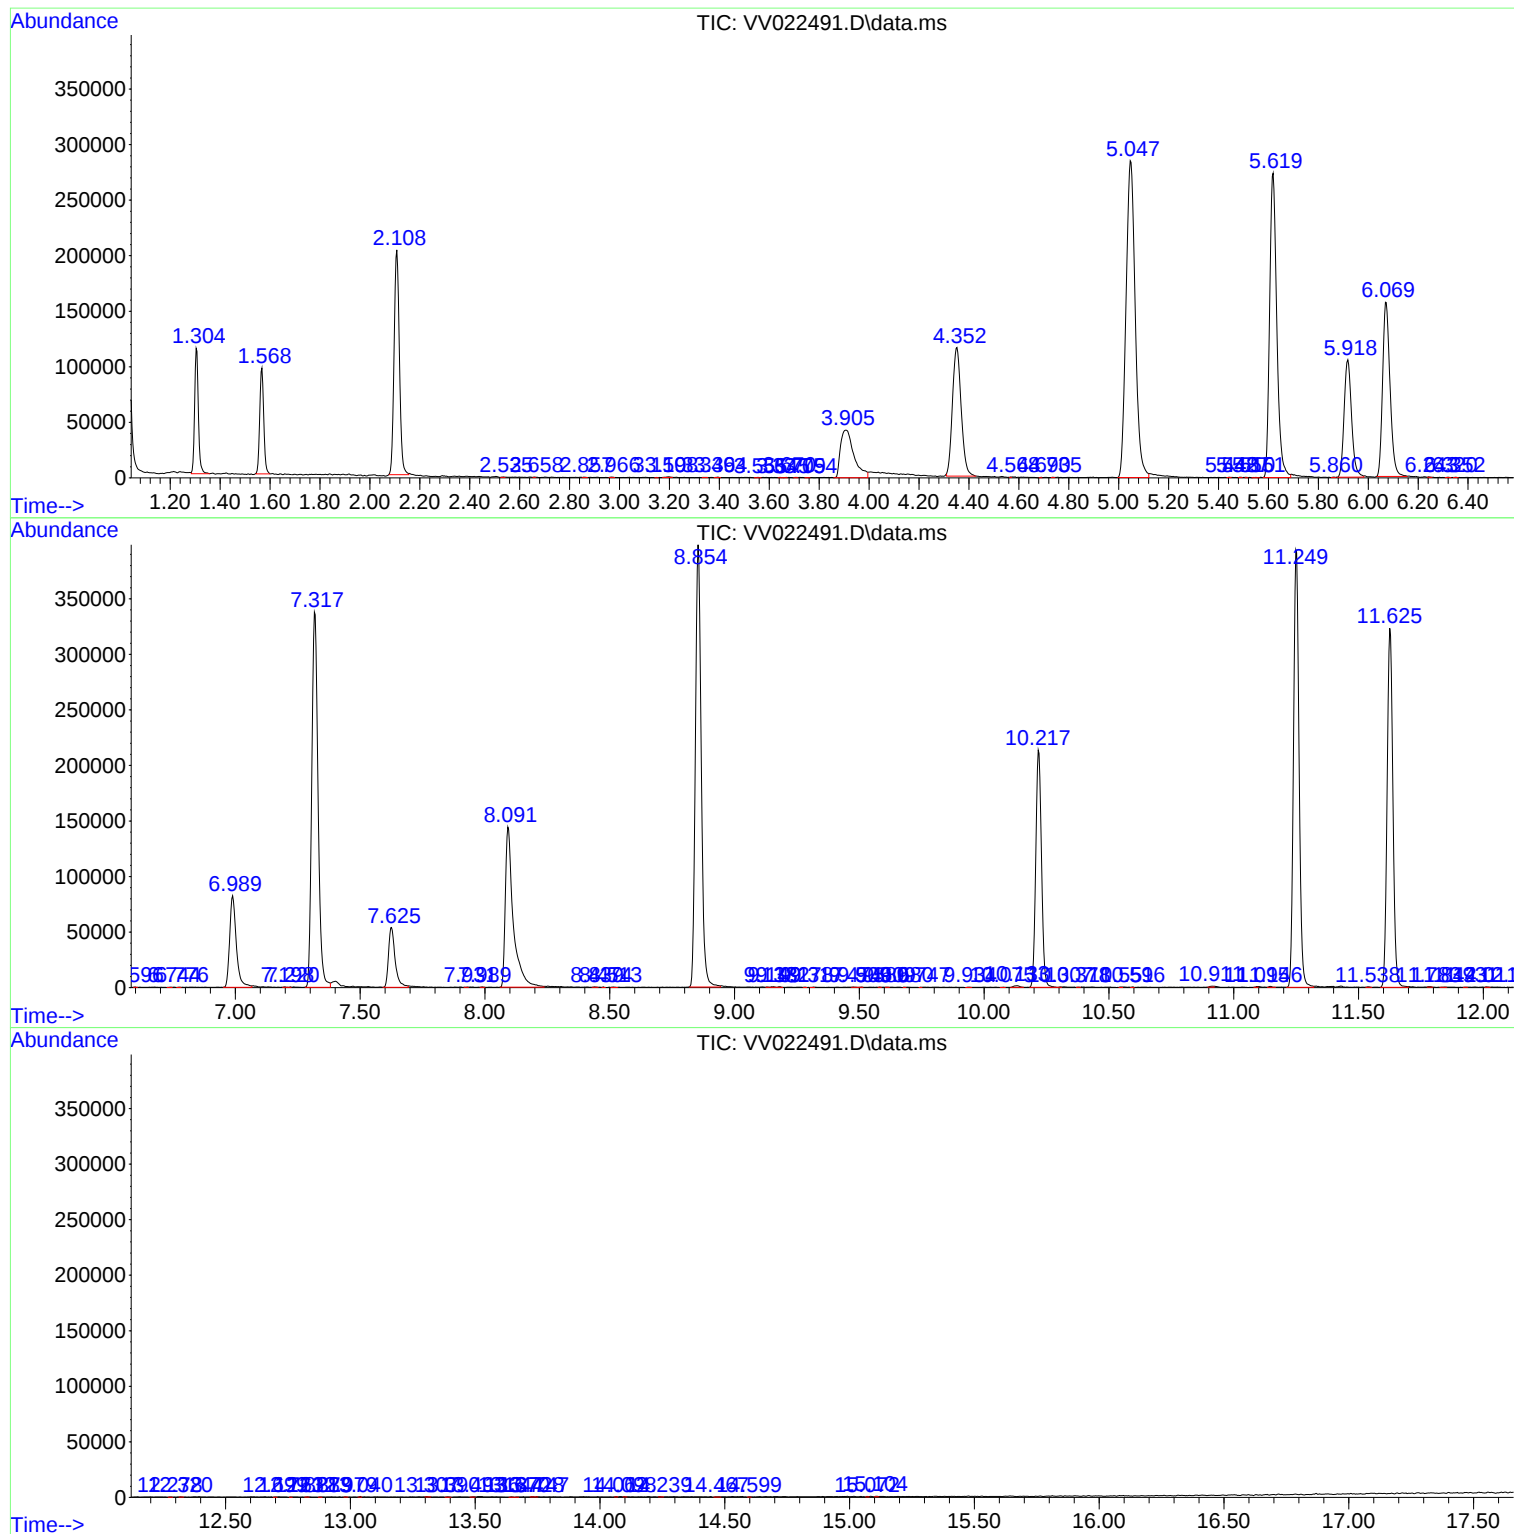

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022491.D
Acq On : 02 Oct 2021 02:51
Operator : SY/MD
Sample : M4024-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AL9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022491.D
Acq On : 02 Oct 2021 02:51
Operator : SY/MD
Sample : M4024-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AL9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
