

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100121\
 Data File : VW022492.D
 Acq On : 02 Oct 2021 03:15
 Operator : SY/MD
 Sample : M4024-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAMO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M

Title : VOC Analysis

Signal : TIC: VW022492.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	112111	114088	8.05%	1.465%
2	1.568	156	164	178	rBV	93995	108613	7.66%	1.395%
3	2.108	321	332	353	rBV3	238566	389208	27.46%	4.997%
4	2.497	448	453	454	rBV3	1016	872	0.06%	0.011%
5	2.584	478	480	481	rVB3	431	158	0.01%	0.002%
6	2.760	532	535	542	rBV4	903	993	0.07%	0.013%
7	2.944	590	592	597	rVB2	464	264	0.02%	0.003%
8	3.014	610	614	617	rVB	312	216	0.02%	0.003%
9	3.117	644	646	649	rVB2	347	152	0.01%	0.002%
10	3.166	658	661	662	rBV	414	231	0.02%	0.003%
11	3.191	662	669	683	rVB3	4442	8469	0.60%	0.109%
12	3.259	686	690	694	rBV2	310	311	0.02%	0.004%
13	3.297	699	702	705	rVB2	371	180	0.01%	0.002%
14	3.423	739	741	749	rVV2	212	214	0.02%	0.003%
15	3.500	761	765	767	rVB2	308	199	0.01%	0.003%
16	3.912	877	893	924	rBV2	210473	574596	40.55%	7.378%
17	4.349	1016	1029	1057	rVB2	115996	291534	20.57%	3.743%
18	4.622	1110	1114	1118	rVB3	454	357	0.03%	0.005%
19	4.748	1145	1153	1155	rBV2	444	382	0.03%	0.005%
20	4.802	1167	1170	1173	rBV2	168	152	0.01%	0.002%
21	4.918	1203	1206	1207	rBV2	295	188	0.01%	0.002%
22	5.047	1229	1246	1278	rBV2	282068	730925	51.58%	9.385%
23	5.256	1309	1311	1315	rVB3	432	254	0.02%	0.003%
24	5.355	1339	1342	1345	rBV4	374	253	0.02%	0.003%
25	5.423	1361	1363	1366	rVV	252	174	0.01%	0.002%
26	5.452	1369	1372	1376	rBV	281	159	0.01%	0.002%
27	5.481	1378	1381	1385	rVB2	330	201	0.01%	0.003%
28	5.513	1389	1391	1395	rBV	342	286	0.02%	0.004%
29	5.619	1411	1424	1448	rBV	271251	547100	38.61%	7.025%
30	5.915	1502	1516	1547	rVV	726610	1417154	100.00%	18.196%
31	6.072	1554	1565	1591	rVB	156294	316692	22.35%	4.066%
32	6.259	1621	1623	1627	rVB3	419	237	0.02%	0.003%
33	6.294	1631	1634	1636	rBV	311	179	0.01%	0.002%
34	6.400	1664	1667	1670	rBV2	271	157	0.01%	0.002%
35	6.532	1704	1708	1709	rBV2	341	200	0.01%	0.003%
36	6.757	1775	1778	1784	rBV	251	276	0.02%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022492.D
 Acq On : 02 Oct 2021 03:15
 Operator : SY/MD
 Sample : M4024-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAMO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

37	6.989	1839	1850	1867	rBV	80986	146996	10.37%	1.887%
38	7.210	1917	1919	1922	rVB2	473	278	0.02%	0.004%
39	7.317	1940	1952	1970	rBV	337230	584448	41.24%	7.504%
40	7.625	2038	2048	2064	rBV	56409	97367	6.87%	1.250%
41	7.789	2097	2099	2106	rVB2	479	276	0.02%	0.004%
42	7.847	2109	2117	2120	rBV4	2009	2092	0.15%	0.027%
43	7.934	2141	2144	2154	rVB4	389	595	0.04%	0.008%
44	8.034	2171	2175	2176	rBV2	259	153	0.01%	0.002%
45	8.091	2183	2193	2222	rBV	142561	308565	21.77%	3.962%
46	8.313	2259	2262	2265	rBV2	457	279	0.02%	0.004%
47	8.390	2283	2286	2291	rBV2	352	405	0.03%	0.005%
48	8.551	2333	2336	2339	rBV	282	201	0.01%	0.003%
49	8.606	2351	2353	2358	rVB	269	166	0.01%	0.002%
50	8.744	2392	2396	2398	rBV3	339	313	0.02%	0.004%
51	8.853	2418	2430	2461	rBV	403817	658678	46.48%	8.457%
52	9.053	2491	2492	2495	rVB2	600	197	0.01%	0.003%
53	9.152	2517	2523	2524	rBV3	689	636	0.04%	0.008%
54	9.297	2564	2568	2570	rBV	278	172	0.01%	0.002%
55	9.333	2575	2579	2582	rBV2	312	217	0.02%	0.003%
56	9.384	2593	2595	2598	rBV2	303	148	0.01%	0.002%
57	9.452	2613	2616	2618	rBV	219	177	0.01%	0.002%
58	9.487	2625	2627	2631	rBV	278	238	0.02%	0.003%
59	9.554	2645	2648	2656	rVB3	456	380	0.03%	0.005%
60	9.677	2682	2686	2690	rVB2	311	253	0.02%	0.003%
61	10.085	2808	2813	2815	rBV2	208	212	0.01%	0.003%
62	10.130	2820	2827	2835	rVB5	1767	2422	0.17%	0.031%
63	10.217	2843	2854	2873	rBV	215027	341342	24.09%	4.383%
64	10.500	2936	2942	2945	rBV2	282	332	0.02%	0.004%
65	10.587	2965	2969	2970	rBV2	538	250	0.02%	0.003%
66	10.612	2975	2977	2983	rVB	340	283	0.02%	0.004%
67	10.741	3015	3017	3021	rVB2	209	169	0.01%	0.002%
68	10.763	3021	3024	3029	rBV	175	212	0.01%	0.003%
69	10.821	3038	3042	3044	rBV	336	266	0.02%	0.003%
70	10.850	3048	3051	3054	rVB	293	148	0.01%	0.002%
71	10.873	3054	3058	3060	rBV	360	271	0.02%	0.003%
72	10.921	3067	3073	3082	rVB5	1341	1955	0.14%	0.025%
73	11.101	3125	3129	3136	rVB4	960	1157	0.08%	0.015%
74	11.146	3136	3143	3147	rBV3	1017	1086	0.08%	0.014%
75	11.165	3147	3149	3152	rBV	273	160	0.01%	0.002%
76	11.249	3165	3175	3193	rBV	397205	609452	43.01%	7.825%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022492.D
 Acq On : 02 Oct 2021 03:15
 Operator : SY/MD
 Sample : M4024-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAMO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

77	11.545	3265	3267	3271	rVB2	414	218	0.02%	0.003%
78	11.625	3281	3292	3317	rVV	330878	513927	36.26%	6.599%
79	11.773	3334	3338	3341	rBV3	455	353	0.02%	0.005%
80	11.840	3357	3359	3361	rBV	387	171	0.01%	0.002%
81	11.972	3398	3400	3405	rBV2	312	276	0.02%	0.004%
82	12.320	3505	3508	3510	rBV2	327	238	0.02%	0.003%
83	12.400	3530	3533	3536	rBV	502	277	0.02%	0.004%
84	12.416	3536	3538	3542	rVV	256	184	0.01%	0.002%
85	12.474	3554	3556	3558	rBV	272	186	0.01%	0.002%
86	12.985	3710	3715	3721	rBV3	337	442	0.03%	0.006%
87	13.255	3796	3799	3803	rBV2	400	312	0.02%	0.004%
88	13.561	3892	3894	3897	rBV2	211	149	0.01%	0.002%
89	13.580	3897	3900	3902	rBV	297	179	0.01%	0.002%
90	13.673	3927	3929	3933	rBV2	163	148	0.01%	0.002%
91	13.963	4014	4019	4021	rBV2	269	303	0.02%	0.004%
92	14.040	4041	4043	4047	rVB3	352	247	0.02%	0.003%
93	14.062	4047	4050	4052	rBV2	272	221	0.02%	0.003%
94	14.236	4101	4104	4106	rBV	330	206	0.01%	0.003%
95	14.281	4115	4118	4122	rVB	302	254	0.02%	0.003%
96	14.307	4123	4126	4127	rBV2	294	168	0.01%	0.002%
97	14.419	4160	4161	4165	rBV3	235	164	0.01%	0.002%
98	14.496	4181	4185	4189	rVB3	494	392	0.03%	0.005%
99	14.522	4190	4193	4196	rBV2	622	402	0.03%	0.005%
100	14.760	4264	4267	4270	rBV	506	421	0.03%	0.005%




Sum of corrected areas: 7788409

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022492.D
Acq On : 02 Oct 2021 03:15
Operator : SY/MD
Sample : M4024-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COAM0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

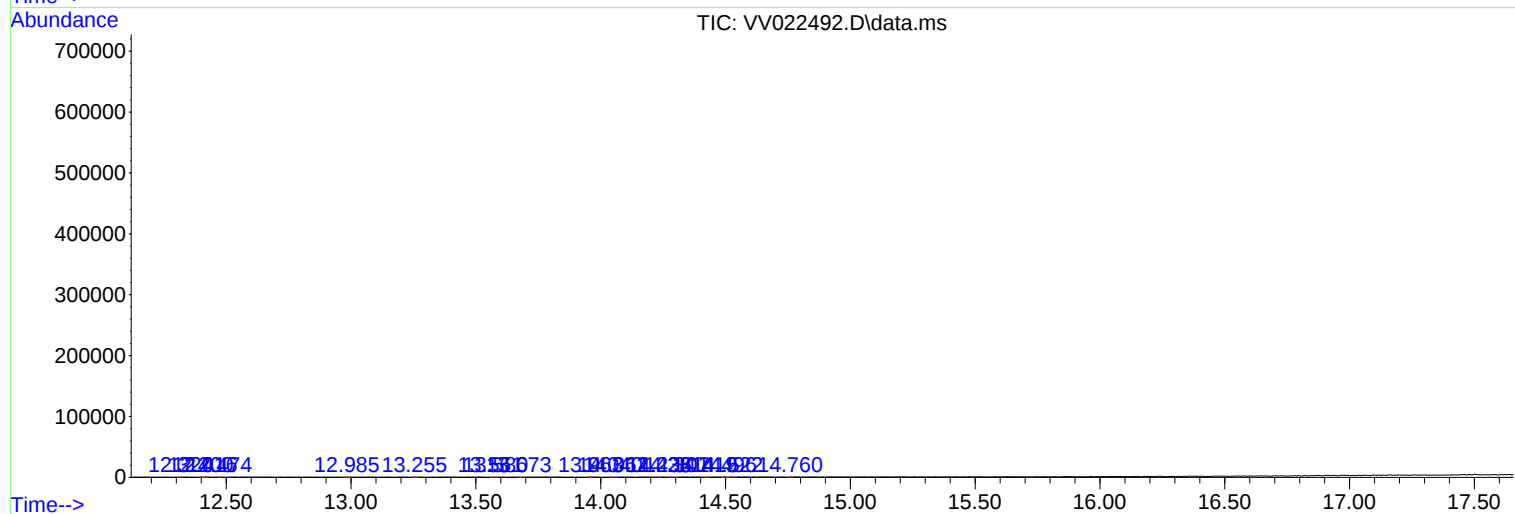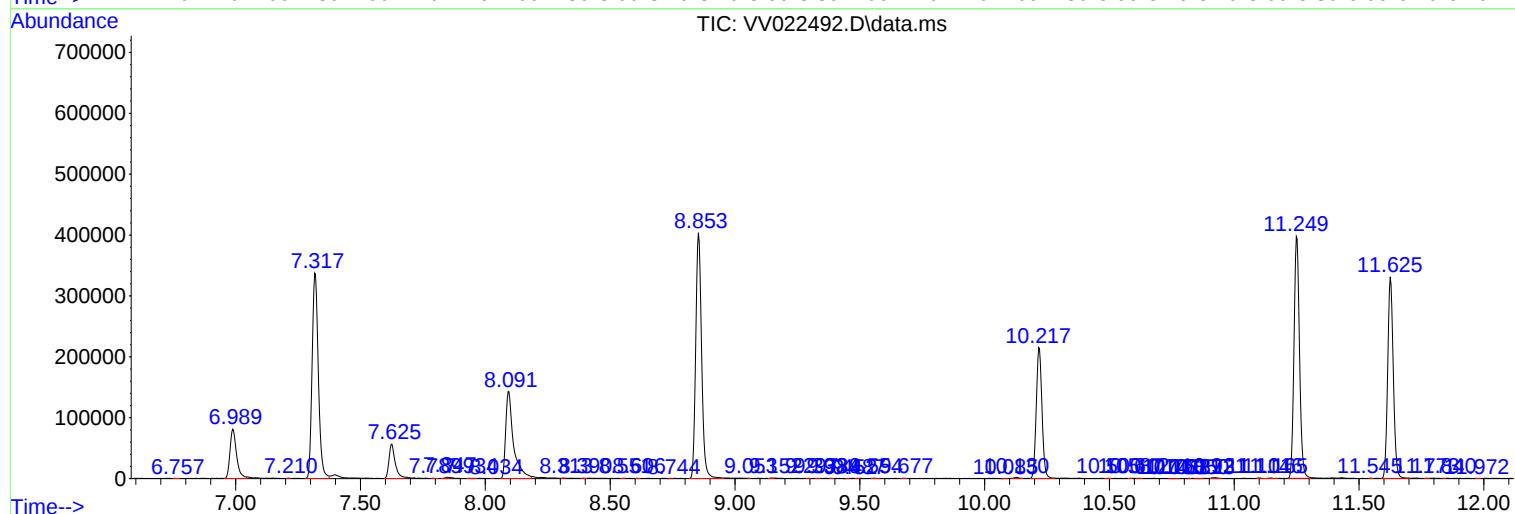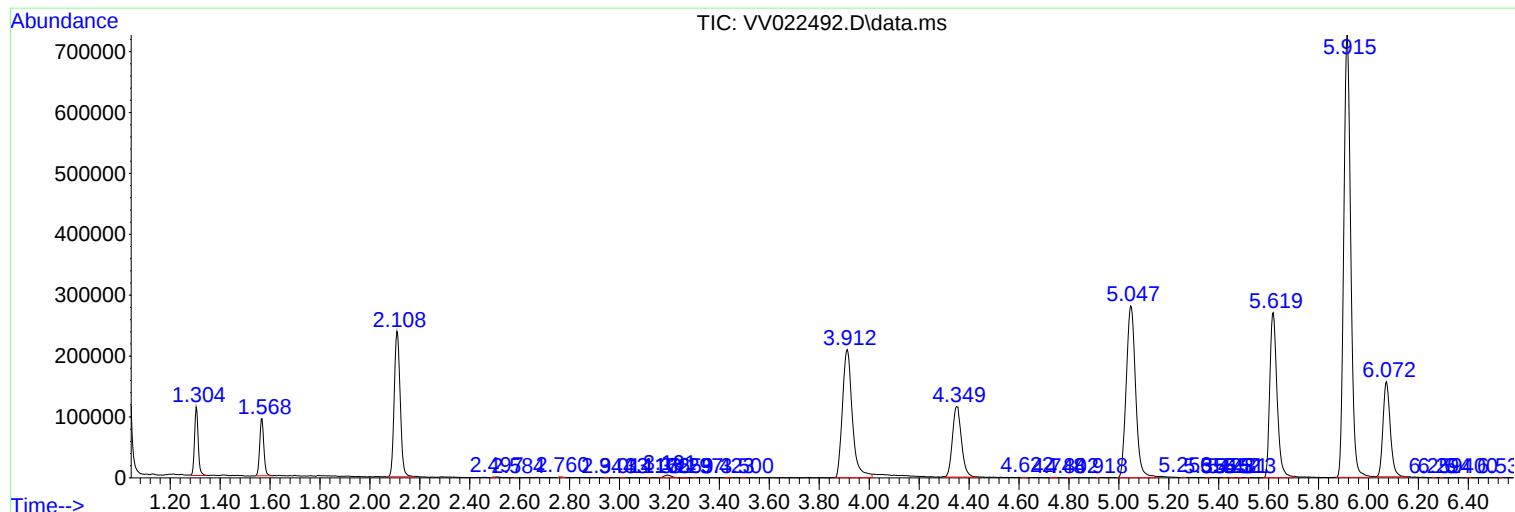

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022492.D
Acq On : 02 Oct 2021 03:15
Operator : SY/MD
Sample : M4024-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022492.D
Acq On : 02 Oct 2021 03:15
Operator : SY/MD
Sample : M4024-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
