

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022495.D
 Acq On : 02 Oct 2021 04:26
 Operator : SY/MD
 Sample : M4023-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

Signal : TIC: VV022495.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB2	130638	136489	5.59%	1.183%
2	1.564	157	163	177	rVB	89768	103611	4.24%	0.898%
3	2.111	322	333	355	rVB3	335615	570894	23.38%	4.947%
4	2.764	528	536	547	rVB3	7371	12853	0.53%	0.111%
5	2.957	593	596	597	rBV2	318	211	0.01%	0.002%
6	2.998	607	609	612	rBV	300	181	0.01%	0.002%
7	3.066	628	630	633	rVB3	297	160	0.01%	0.001%
8	3.092	633	638	640	rBV3	325	210	0.01%	0.002%
9	3.191	657	669	686	rBV	21549	44203	1.81%	0.383%
10	3.304	701	704	706	rBV	356	259	0.01%	0.002%
11	3.580	784	790	791	rBV	255	184	0.01%	0.002%
12	3.629	803	805	808	rBV	347	270	0.01%	0.002%
13	3.683	820	822	827	rBV	212	173	0.01%	0.001%
14	3.722	832	834	837	rBV	245	170	0.01%	0.001%
15	3.841	867	871	876	rBV3	303	248	0.01%	0.002%
16	3.908	876	892	922	rBV	995582	2441447	100.00%	21.154%
17	4.349	1016	1029	1057	rVB2	117586	295667	12.11%	2.562%
18	4.609	1094	1110	1130	rVB2	264034	652212	26.71%	5.651%
19	4.892	1192	1198	1202	rBV3	414	628	0.03%	0.005%
20	4.928	1207	1209	1213	rBV	272	170	0.01%	0.001%
21	4.973	1219	1223	1227	rVB	468	363	0.01%	0.003%
22	5.047	1227	1246	1269	rBV2	284569	725404	29.71%	6.285%
23	5.326	1330	1333	1335	rBV3	405	274	0.01%	0.002%
24	5.474	1376	1379	1380	rBV2	401	239	0.01%	0.002%
25	5.497	1384	1386	1387	rBV2	341	147	0.01%	0.001%
26	5.619	1411	1424	1453	rBV	263609	535371	21.93%	4.639%
27	5.847	1492	1495	1501	rVB4	547	332	0.01%	0.003%
28	5.915	1501	1516	1551	rBV	1247411	2412522	98.82%	20.904%
29	6.072	1554	1565	1587	rVB	159363	320378	13.12%	2.776%
30	6.288	1629	1632	1635	rBV2	670	509	0.02%	0.004%
31	6.339	1646	1648	1656	rVB3	409	344	0.01%	0.003%
32	6.426	1672	1675	1676	rBV	423	250	0.01%	0.002%
33	6.494	1690	1696	1699	rVB3	427	368	0.02%	0.003%
34	6.564	1713	1718	1722	rBV3	269	243	0.01%	0.002%
35	6.603	1726	1730	1736	rVB3	349	312	0.01%	0.003%
36	6.654	1743	1746	1747	rBV	283	134	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022495.D
 Acq On : 02 Oct 2021 04:26
 Operator : SY/MD
 Sample : M4023-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

37	6.780	1781	1785	1790	rBV3	375	336	0.01%	0.003%
38	6.989	1839	1850	1870	rBV	83520	154485	6.33%	1.339%
39	7.194	1911	1914	1917	rBV3	349	211	0.01%	0.002%
40	7.243	1926	1929	1934	rBV5	468	442	0.02%	0.004%
41	7.317	1940	1952	1971	rBV	341169	590893	24.20%	5.120%
42	7.625	2037	2048	2071	rBV2	55549	102233	4.19%	0.886%
43	7.802	2101	2103	2106	rVB3	493	261	0.01%	0.002%
44	7.847	2109	2117	2130	rBV5	6636	10981	0.45%	0.095%
45	7.944	2142	2147	2148	rBV2	338	268	0.01%	0.002%
46	7.979	2154	2158	2161	rBV4	613	462	0.02%	0.004%
47	8.008	2165	2167	2168	rBV2	243	135	0.01%	0.001%
48	8.092	2184	2193	2228	rBV	145050	317882	13.02%	2.754%
49	8.490	2314	2317	2319	rBV2	359	293	0.01%	0.003%
50	8.571	2340	2342	2344	rBV	271	165	0.01%	0.001%
51	8.792	2409	2411	2412	rBV	338	156	0.01%	0.001%
52	8.854	2418	2430	2462	rBV	383860	632187	25.89%	5.478%
53	9.056	2491	2493	2497	rVB2	332	127	0.01%	0.001%
54	9.108	2505	2509	2512	rBV2	464	320	0.01%	0.003%
55	9.149	2514	2522	2531	rBV3	3311	5697	0.23%	0.049%
56	9.217	2540	2543	2544	rBV	323	147	0.01%	0.001%
57	9.284	2560	2564	2567	rBV3	163	154	0.01%	0.001%
58	9.497	2627	2630	2633	rBV3	434	333	0.01%	0.003%
59	9.545	2641	2645	2646	rBV3	1130	836	0.03%	0.007%
60	9.670	2679	2684	2689	rVV2	334	390	0.02%	0.003%
61	10.050	2797	2802	2803	rBV	254	183	0.01%	0.002%
62	10.130	2818	2827	2832	rBV3	1373	2058	0.08%	0.018%
63	10.172	2837	2840	2842	rBV2	203	151	0.01%	0.001%
64	10.217	2843	2854	2875	rVV	218982	342783	14.04%	2.970%
65	10.345	2890	2894	2895	rBV	274	200	0.01%	0.002%
66	10.455	2925	2928	2931	rBV2	249	201	0.01%	0.002%
67	10.567	2961	2963	2967	rVB3	336	205	0.01%	0.002%
68	10.805	3036	3037	3041	rVB2	424	170	0.01%	0.001%
69	10.857	3051	3053	3057	rVB2	264	160	0.01%	0.001%
70	11.037	3105	3109	3111	rBV2	390	343	0.01%	0.003%
71	11.101	3125	3129	3131	rVB	472	233	0.01%	0.002%
72	11.149	3140	3144	3150	rVB5	676	723	0.03%	0.006%
73	11.175	3150	3152	3155	rBV2	248	168	0.01%	0.001%
74	11.249	3164	3175	3195	rBV	388204	594081	24.33%	5.147%
75	11.416	3225	3227	3228	rBV	470	195	0.01%	0.002%
76	11.538	3261	3265	3267	rBV2	551	392	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022495.D
 Acq On : 02 Oct 2021 04:26
 Operator : SY/MD
 Sample : M4023-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

77	11.570	3273	3275	3280	rBV3	314	239	0.01%	0.002%
78	11.625	3280	3292	3312	rBV	334788	516477	21.15%	4.475%
79	11.747	3328	3330	3336	rVB4	384	324	0.01%	0.003%
80	11.802	3346	3347	3351	rBV	405	214	0.01%	0.002%
81	11.844	3358	3360	3367	rBV2	379	344	0.01%	0.003%
82	11.950	3387	3393	3394	rBV3	322	336	0.01%	0.003%
83	12.188	3465	3467	3470	rBV2	299	190	0.01%	0.002%
84	12.242	3481	3484	3486	rBV3	324	205	0.01%	0.002%
85	12.355	3517	3519	3521	rBV	251	145	0.01%	0.001%
86	12.500	3561	3564	3566	rVB3	443	239	0.01%	0.002%
87	12.532	3566	3574	3576	rBV2	425	578	0.02%	0.005%
88	12.660	3612	3614	3619	rVB2	329	199	0.01%	0.002%
89	12.853	3670	3674	3675	rBV	276	159	0.01%	0.001%
90	12.959	3705	3707	3710	rVB3	298	143	0.01%	0.001%
91	13.005	3719	3721	3725	rVB2	436	196	0.01%	0.002%
92	13.062	3733	3739	3741	rBV	391	376	0.02%	0.003%
93	13.297	3810	3812	3815	rVB	370	167	0.01%	0.001%
94	13.384	3836	3839	3841	rBV	309	212	0.01%	0.002%
95	13.651	3919	3922	3926	rBV	294	236	0.01%	0.002%
96	13.969	4018	4021	4024	rBV	233	193	0.01%	0.002%
97	14.024	4034	4038	4041	rBV3	300	296	0.01%	0.003%
98	14.130	4068	4071	4072	rBV2	337	198	0.01%	0.002%
99	14.294	4119	4122	4126	rVB3	366	264	0.01%	0.002%
100	14.644	4227	4231	4232	rBV2	254	196	0.01%	0.002%




Sum of corrected areas: 11541196

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022495.D
Acq On : 02 Oct 2021 04:26
Operator : SY/MD
Sample : M4023-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

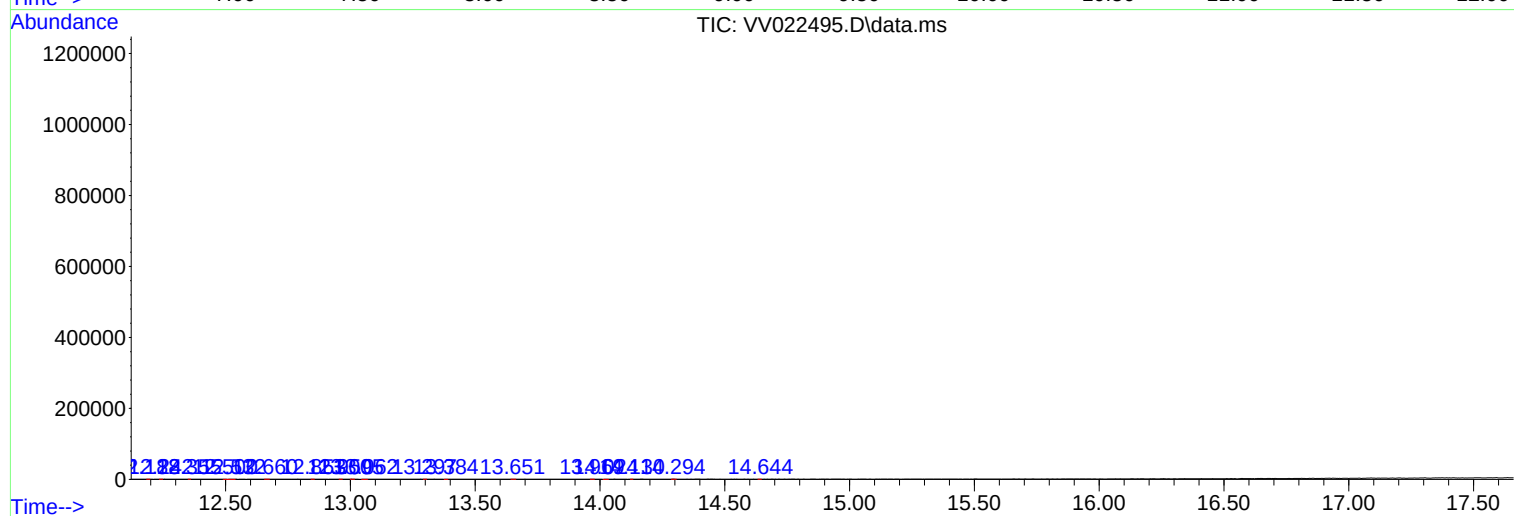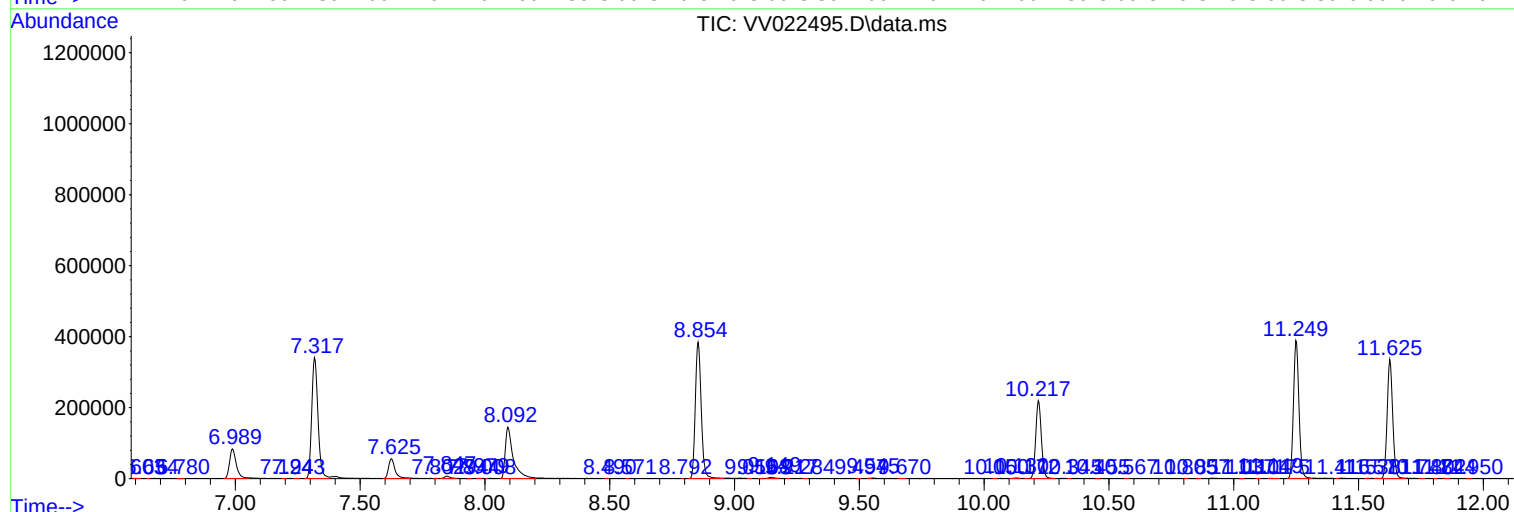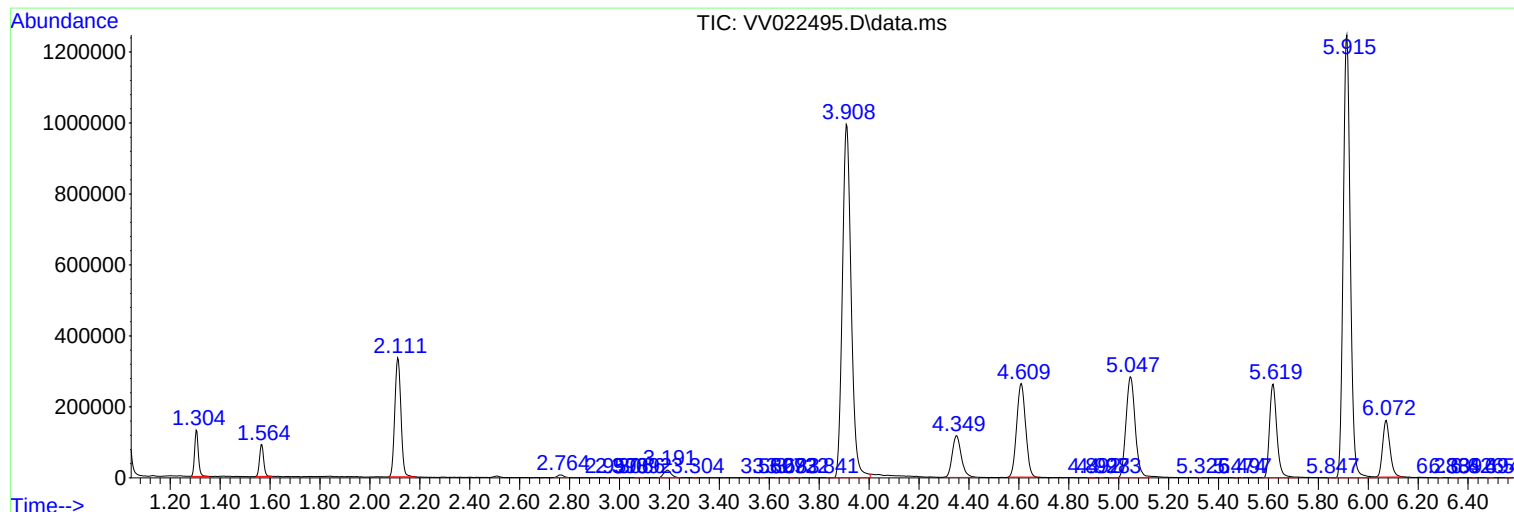

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022495.D
Acq On : 02 Oct 2021 04:26
Operator : SY/MD
Sample : M4023-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022495.D
Acq On : 02 Oct 2021 04:26
Operator : SY/MD
Sample : M4023-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
