

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022496.D
 Acq On : 02 Oct 2021 04:50
 Operator : SY/MD
 Sample : M4023-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

Signal : TIC: VV022496.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	116378	121692	16.87%	2.069%
2	1.568	156	164	173	rBV	93084	106431	14.76%	1.809%
3	2.108	322	332	355	rVB	199720	294960	40.89%	5.014%
4	2.551	467	470	472	rBV2	411	257	0.04%	0.004%
5	3.066	624	630	637	rVB2	394	485	0.07%	0.008%
6	3.101	638	641	645	rBV	183	150	0.02%	0.003%
7	3.178	661	665	674	rVB4	487	402	0.06%	0.007%
8	3.625	802	804	807	rBV2	293	159	0.02%	0.003%
9	3.648	809	811	813	rVB2	372	166	0.02%	0.003%
10	3.699	824	827	830	rBV3	296	153	0.02%	0.003%
11	3.776	848	851	852	rBV	234	162	0.02%	0.003%
12	3.825	863	866	869	rVB2	303	225	0.03%	0.004%
13	3.905	879	891	920	rBV5	43977	157824	21.88%	2.683%
14	4.349	1017	1029	1059	rVB	115959	290082	40.22%	4.931%
15	4.674	1129	1130	1133	rVB	466	167	0.02%	0.003%
16	4.715	1140	1143	1145	rBV3	365	223	0.03%	0.004%
17	4.747	1151	1153	1157	rVB3	342	151	0.02%	0.003%
18	4.866	1188	1190	1193	rVB2	304	162	0.02%	0.003%
19	4.889	1193	1197	1198	rBV	343	252	0.03%	0.004%
20	4.928	1207	1209	1215	rBV2	401	446	0.06%	0.008%
21	5.047	1228	1246	1275	rBV2	283487	721296	100.00%	12.261%
22	5.313	1321	1329	1334	rBV3	447	634	0.09%	0.011%
23	5.349	1338	1340	1346	rBV3	470	290	0.04%	0.005%
24	5.619	1411	1424	1452	rBV	261063	529833	73.46%	9.006%
25	5.873	1500	1503	1505	rBV2	441	322	0.04%	0.005%
26	5.918	1505	1517	1535	rVV3	50766	106270	14.73%	1.806%
27	6.069	1552	1564	1590	rBV	155546	323742	44.88%	5.503%
28	6.284	1628	1631	1633	rBV	252	173	0.02%	0.003%
29	6.439	1675	1679	1680	rBV2	284	170	0.02%	0.003%
30	6.474	1687	1690	1692	rBV	263	159	0.02%	0.003%
31	6.526	1702	1706	1708	rBV2	339	239	0.03%	0.004%
32	6.651	1744	1745	1747	rVB	469	159	0.02%	0.003%
33	6.683	1752	1755	1758	rBV2	283	238	0.03%	0.004%
34	6.783	1782	1786	1793	rBV2	242	237	0.03%	0.004%
35	6.989	1839	1850	1873	rBV	78537	149964	20.79%	2.549%
36	7.140	1895	1897	1901	rVB2	482	281	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100121\
 Data File : VW022496.D
 Acq On : 02 Oct 2021 04:50
 Operator : SY/MD
 Sample : M4023-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

37	7.159	1901	1903	1906	rBV2	355	179	0.02%	0.003%
38	7.207	1914	1918	1921	rVB2	388	278	0.04%	0.005%
39	7.233	1923	1926	1930	rVB4	415	267	0.04%	0.005%
40	7.317	1940	1952	1972	rBV	331092	585807	81.22%	9.958%
41	7.519	2012	2015	2018	rBV2	471	327	0.05%	0.006%
42	7.625	2033	2048	2064	rBV	54677	96905	13.43%	1.647%
43	7.789	2096	2099	2101	rBV2	472	270	0.04%	0.005%
44	7.937	2142	2145	2147	rBV2	419	241	0.03%	0.004%
45	7.998	2160	2164	2166	rBV2	263	210	0.03%	0.004%
46	8.091	2184	2193	2233	rBV	137767	313668	43.49%	5.332%
47	8.439	2298	2301	2305	rBV2	368	356	0.05%	0.006%
48	8.590	2345	2348	2351	rBV2	201	158	0.02%	0.003%
49	8.715	2386	2387	2391	rVB	457	190	0.03%	0.003%
50	8.744	2394	2396	2399	rBV2	279	200	0.03%	0.003%
51	8.770	2402	2404	2406	rBV	248	150	0.02%	0.003%
52	8.853	2418	2430	2458	rBV	394586	636371	88.23%	10.817%
53	9.053	2489	2492	2496	rBV2	432	243	0.03%	0.004%
54	9.120	2510	2513	2514	rBV2	325	177	0.02%	0.003%
55	9.146	2514	2521	2529	rVV4	1479	2266	0.31%	0.039%
56	9.259	2551	2556	2558	rBV2	195	154	0.02%	0.003%
57	9.365	2586	2589	2595	rVB2	366	293	0.04%	0.005%
58	9.416	2602	2605	2608	rBV2	277	151	0.02%	0.003%
59	9.493	2627	2629	2634	rVB2	314	205	0.03%	0.003%
60	9.529	2635	2640	2642	rBV	304	244	0.03%	0.004%
61	9.545	2642	2645	2646	rBV2	471	250	0.03%	0.004%
62	9.953	2768	2772	2779	rVB3	188	163	0.02%	0.003%
63	9.982	2779	2781	2787	rVB2	275	210	0.03%	0.004%
64	10.017	2787	2792	2795	rVB2	236	247	0.03%	0.004%
65	10.043	2795	2800	2802	rBV2	421	384	0.05%	0.007%
66	10.130	2820	2827	2836	rVB6	1567	2347	0.33%	0.040%
67	10.172	2836	2840	2841	rBV2	416	271	0.04%	0.005%
68	10.217	2842	2854	2876	rVV	205927	335333	46.49%	5.700%
69	10.336	2889	2891	2894	rBV2	433	211	0.03%	0.004%
70	10.461	2926	2930	2933	rBV3	485	359	0.05%	0.006%
71	10.760	3019	3023	3025	rBV	177	177	0.02%	0.003%
72	10.799	3031	3035	3037	rBV2	227	197	0.03%	0.003%
73	10.911	3063	3070	3072	rBV3	1068	947	0.13%	0.016%
74	11.098	3124	3128	3138	rBV3	675	936	0.13%	0.016%
75	11.143	3138	3142	3146	rBV3	870	777	0.11%	0.013%
76	11.213	3159	3164	3165	rBV	321	231	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022496.D
 Acq On : 02 Oct 2021 04:50
 Operator : SY/MD
 Sample : M4023-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

77	11.252	3165	3176	3192	rVV	375901	580607	80.49%	9.869%
78	11.535	3261	3264	3265	rBV	286	149	0.02%	0.003%
79	11.583	3275	3279	3281	rBV2	305	262	0.04%	0.004%
80	11.625	3281	3292	3312	rVV	325742	506586	70.23%	8.611%
81	11.779	3337	3340	3342	rBV2	250	146	0.02%	0.002%
82	11.799	3344	3346	3348	rVB3	481	201	0.03%	0.003%
83	11.969	3394	3399	3401	rBV2	209	149	0.02%	0.003%
84	12.188	3464	3467	3470	rBV2	248	181	0.03%	0.003%
85	12.207	3471	3473	3477	rVV2	223	160	0.02%	0.003%
86	12.381	3521	3527	3531	rBV3	386	366	0.05%	0.006%
87	12.477	3555	3557	3560	rVB	436	192	0.03%	0.003%
88	12.548	3577	3579	3581	rVB	395	173	0.02%	0.003%
89	12.776	3644	3650	3653	rBV2	321	381	0.05%	0.006%
90	13.471	3864	3866	3868	rBV	271	153	0.02%	0.003%
91	13.522	3879	3882	3884	rBV2	267	170	0.02%	0.003%
92	13.602	3904	3907	3909	rBV2	395	252	0.03%	0.004%
93	13.718	3940	3943	3946	rBV2	233	178	0.02%	0.003%
94	13.795	3964	3967	3970	rBV2	463	284	0.04%	0.005%
95	13.811	3970	3972	3976	rVB2	282	232	0.03%	0.004%
96	13.866	3985	3989	3992	rBV2	341	316	0.04%	0.005%
97	14.046	4041	4045	4047	rBV	372	182	0.03%	0.003%
98	14.159	4074	4080	4082	rBV	303	322	0.04%	0.005%
99	14.262	4109	4112	4113	rBV	420	202	0.03%	0.003%
100	15.056	4358	4359	4364	rBV2	296	209	0.03%	0.004%



Sum of corrected areas: 5882959

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022496.D
Acq On : 02 Oct 2021 04:50
Operator : SY/MD
Sample : M4023-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

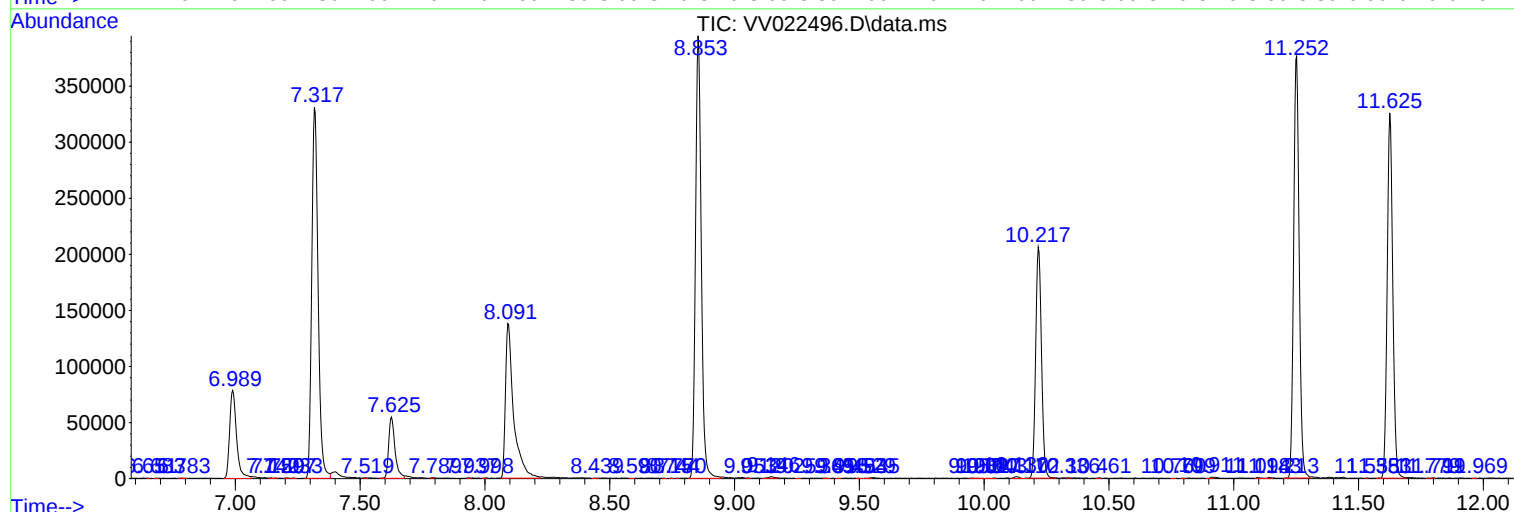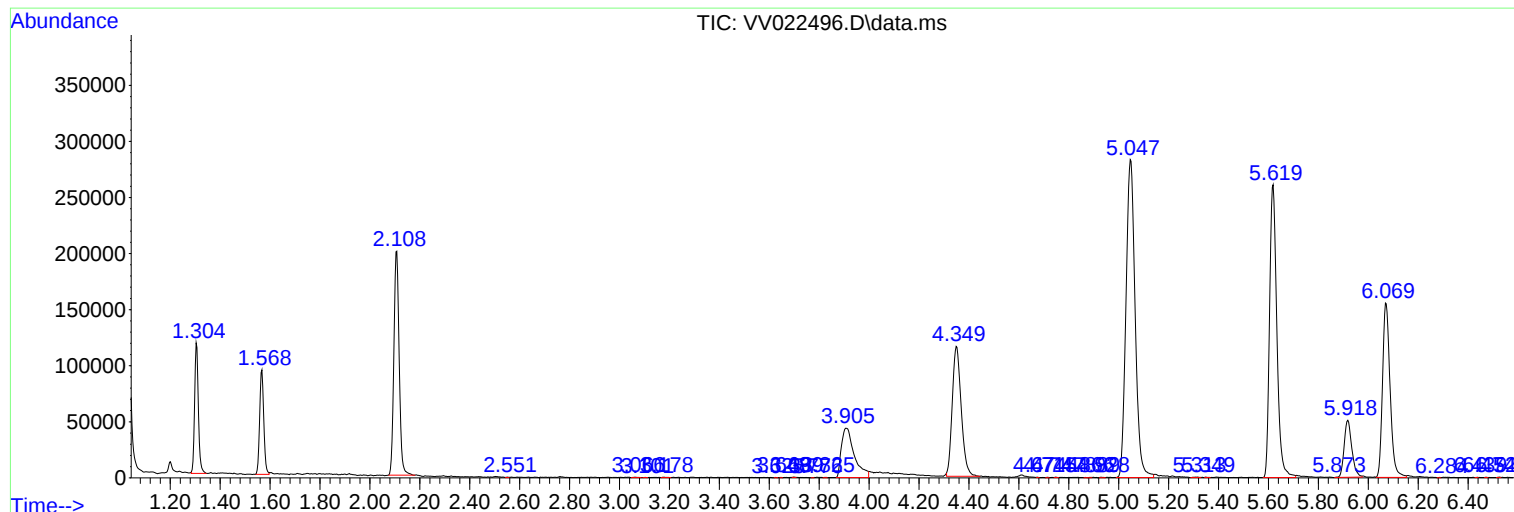

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022496.D
Acq On : 02 Oct 2021 04:50
Operator : SY/MD
Sample : M4023-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
Data File : VV022496.D
Acq On : 02 Oct 2021 04:50
Operator : SY/MD
Sample : M4023-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
