


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100121\
 Data File : VV022472.D
 Acq On : 01 Oct 2021 14:10
 Operator : SY/MD
 Sample : BFB239
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB239

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis
 Last Update : Mon Oct 04 04:27:20 2021

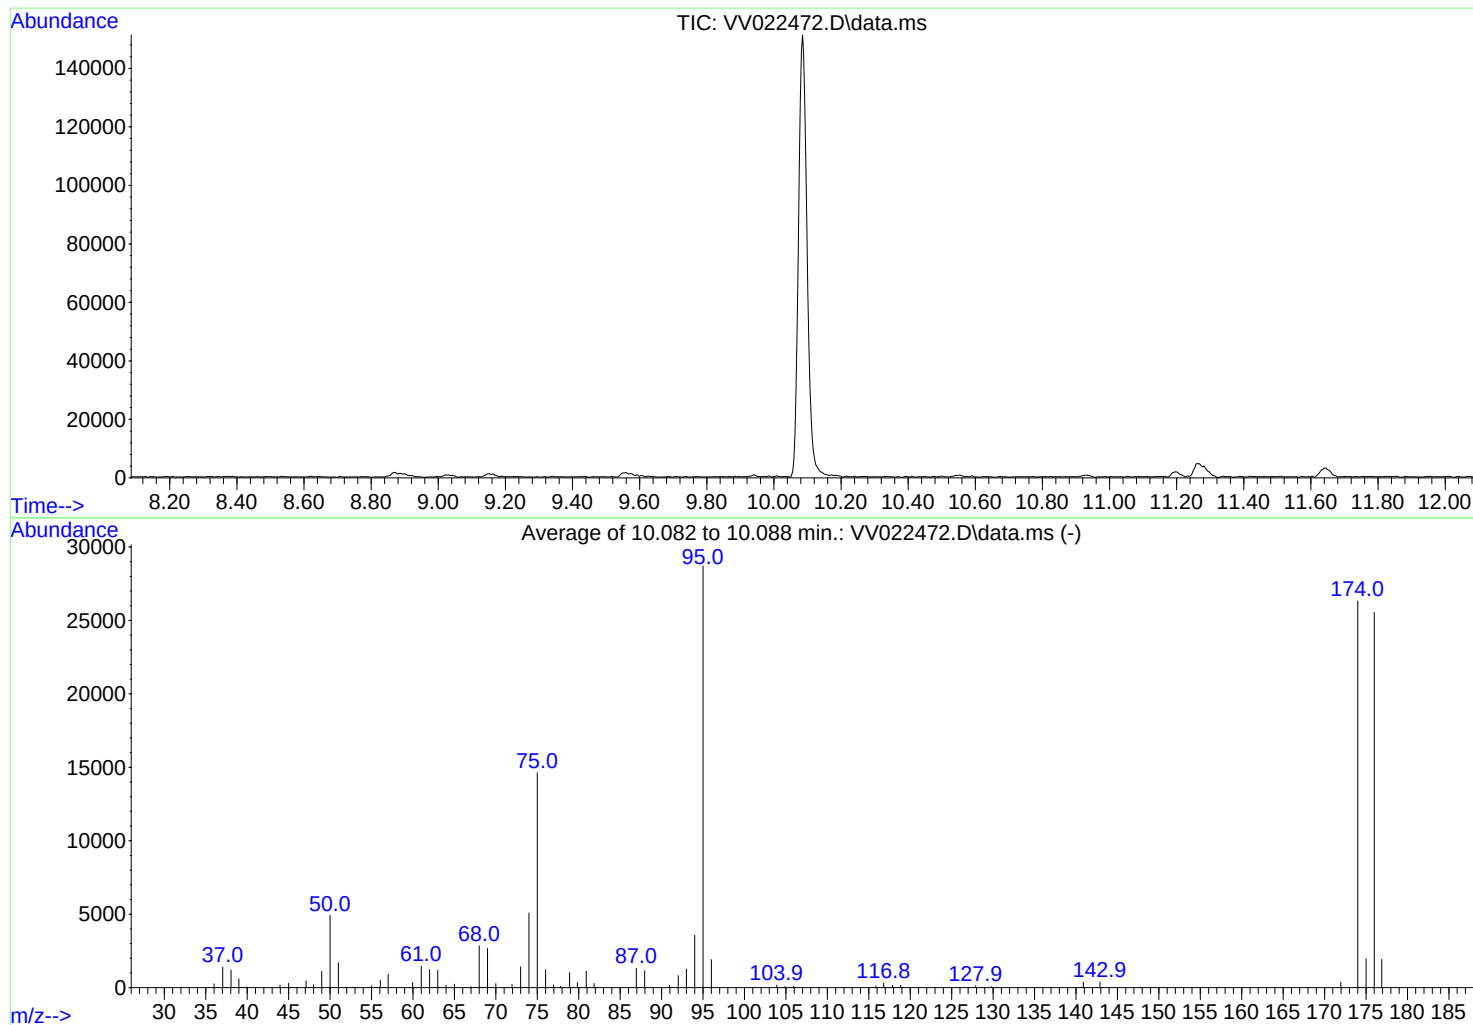

AutoFind: Scans 2812, 2813, 2814; Background Corrected with Scan 2801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	4923	PASS
75	95	30	80	51.0	14632	PASS
95	95	100	100	100.0	28717	PASS
96	95	5	9	6.6	1905	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	91.7	26333	PASS
175	174	5	9	7.4	1957	PASS
176	174	95	105	97.0	25544	PASS
177	176	5	10	7.6	1930	PASS

Scan 2801 (10.047 min): VV022472.D\data.ms
BFB239

m/z	Abundance
40.00	128.0
44.00	198.0

Instrument :
MSVOA_V
ClientSampleId :
BFB239

m/z	Abundance
36.00	272.0
37.00	1435.0
38.00	1184.0
39.00	593.0
39.80	193.0
43.90	371.0
45.00	329.0
47.00	438.0
48.00	199.0
49.00	1122.0
50.00	4932.0
51.00	1740.0
51.90	119.0
52.80	109.0
55.10	124.0
56.10	546.0
57.00	900.0
59.90	313.0
61.00	1436.0
62.00	1083.0
63.00	1191.0
64.00	150.0
65.00	239.0
68.00	2885.0
69.00	2546.0
70.00	333.0
71.90	240.0
73.00	1398.0
74.00	5068.0
75.00	14641.0
76.00	1128.0
76.90	143.0
77.80	128.0
78.90	1032.0
79.80	364.0
80.90	1095.0
81.80	262.0
87.00	1337.0
87.90	1150.0
90.90	144.0
92.00	851.0
93.00	1189.0
94.00	3476.0
95.00	28680.0
96.00	1786.0
103.90	195.0
105.90	149.0
115.80	111.0
116.80	297.0
117.80	141.0
118.80	170.0
127.90	121.0
129.80	116.0
140.90	359.0
142.90	386.0
147.80	103.0
171.90	425.0
174.00	26008.0
175.00	1896.0
176.00	24648.0
176.90	1859.0

Instrument :
MSVOA_V
ClientSampleId :
BFB239

m/z	Abundance
36.00	263.0
37.00	1415.0
38.10	1221.0
39.00	617.0
39.90	179.0
43.90	356.0
45.00	304.0
47.10	481.0
48.00	211.0
49.00	1166.0
50.00	5060.0
51.00	1747.0
55.00	132.0
56.10	520.0
57.00	941.0
60.00	358.0
61.00	1508.0
62.00	1255.0
63.00	1202.0
64.00	174.0
65.00	252.0
67.00	102.0
68.00	2929.0
69.00	2716.0
70.00	286.0
71.90	236.0
73.00	1465.0
74.00	5213.0
75.00	15133.0
76.00	1260.0
76.90	198.0
77.80	122.0
78.90	1037.0
79.80	337.0
80.90	1178.0
81.90	304.0
86.90	1364.0
88.00	1142.0
90.90	152.0
92.00	826.0
93.00	1274.0
94.00	3641.0
95.00	29224.0
96.00	1934.0
103.90	178.0
104.90	123.0
105.90	120.0
115.80	123.0
116.80	325.0
117.80	145.0
118.80	173.0
127.90	138.0
129.80	102.0
140.90	358.0
142.90	396.0
172.00	397.0
174.00	26960.0
175.00	2002.0
176.00	26304.0
176.90	2022.0
178.00	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB239

m/z	Abundance
36.00	253.0
37.10	1325.0
38.10	1172.0
39.00	586.0
39.90	179.0
44.00	383.0
45.00	237.0
47.20	471.0
48.00	201.0
49.00	1044.0
50.00	4778.0
51.00	1594.0
54.90	116.0
56.00	428.0
57.00	877.0
60.00	362.0
61.00	1436.0
62.00	1352.0
63.00	1144.0
64.00	174.0
65.00	225.0
67.00	102.0
68.00	2757.0
69.00	2747.0
70.00	213.0
72.00	180.0
73.00	1373.0
74.00	4985.0
75.00	14121.0
76.00	1280.0
77.00	257.0
78.90	1005.0
79.90	317.0
80.90	1097.0
81.90	297.0
86.90	1250.0
88.00	1156.0
91.00	147.0
92.00	785.0
93.00	1343.0
94.00	3559.0
95.00	28248.0
96.00	1995.0
103.90	155.0
104.90	124.0
106.10	132.0
115.90	132.0
116.80	306.0
117.90	133.0
118.90	165.0
127.90	149.0
140.90	354.0
142.90	388.0
172.00	338.0
174.00	26032.0
175.00	1972.0
176.00	25680.0
176.90	1908.0

Instrument :
MSVOA_V
ClientSampleId :
BFB239