

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100218\
 Data File : VV008028.D
 Acq On : 02 Oct 2018 14:00
 Operator : SY/MD
 Sample : J5160-18
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GACC1

Quant Time: Oct 03 05:59:15 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Oct 03 05:34:53 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	90041	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	85960	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	42355	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	22948	4.75	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.00%
7) Chloroethane-d5	1.59	69	20234	4.85	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.00%
11) 1,1-Dichloroethene-d2	2.13	63	37361	3.43	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.60%
20) 2-Butanone-d5	3.96	46	65543	45.14	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.28%
24) Chloroform-d	4.41	84	53115	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.60%
26) 1,2-Dichloroethane-d4	5.09	65	27971	4.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.60%
32) Benzene-d6	5.10	84	102928	5.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.40%
36) 1,2-Dichloropropane-d6	6.12	67	31986	4.92	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.40%
41) Toluene-d8	7.36	98	95656	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.60%
43) trans-1,3-Dichloropropene-	7.67	79	10753	4.29	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.80%
46) 2-Hexanone-d5	8.14	63	44545	40.29	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.58%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	21446	4.27	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	38966	4.75	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.00%


Target Compounds					Ovalue
13) Acetone	2.21	43	4171	3.943 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100218\
Data File : VV008028.D
Acq On : 02 Oct 2018 14:00
Operator : SY/MD
Sample : J5160-18
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GACC1

Quant Time: Oct 03 05:59:15 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Oct 03 05:34:53 2018
Response via : Initial Calibration

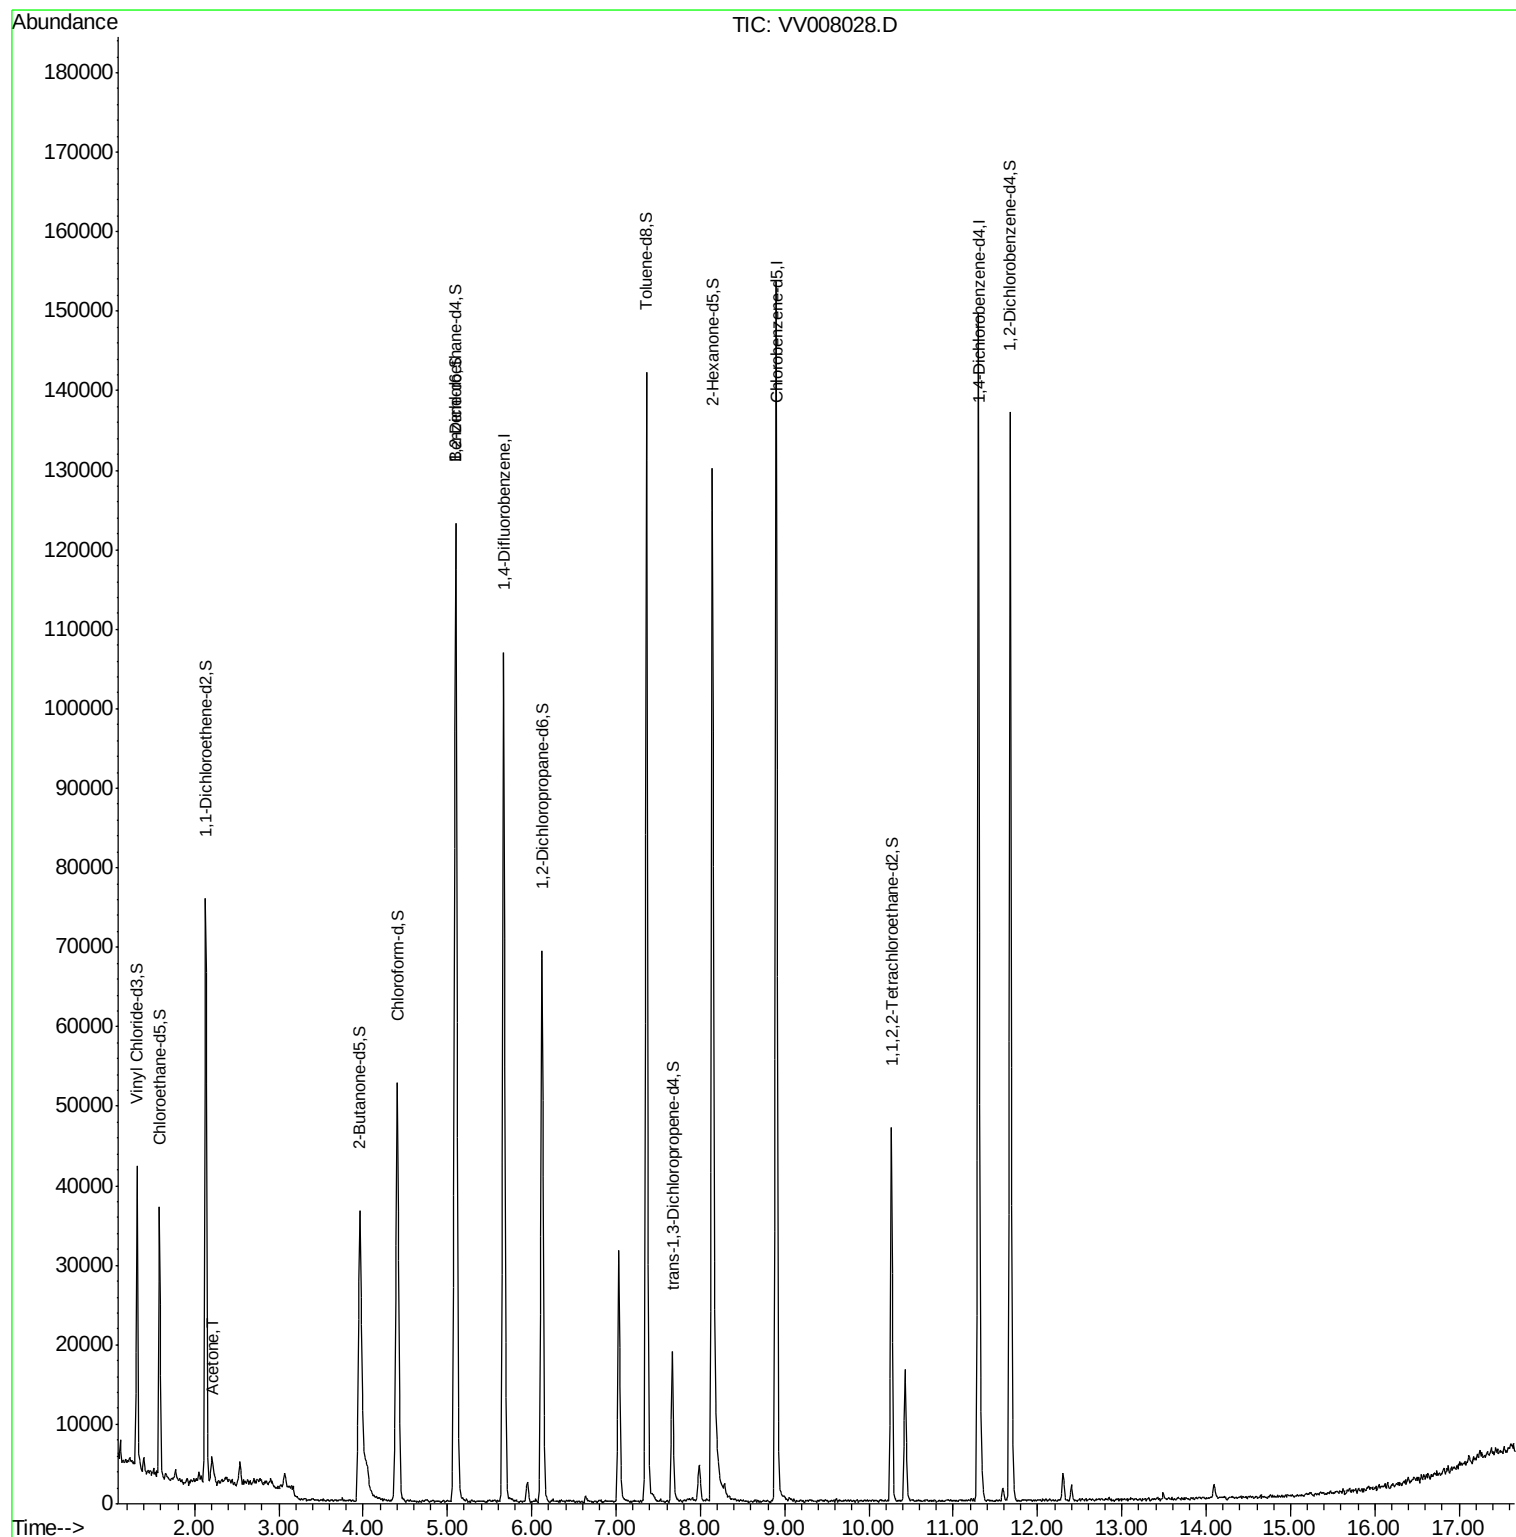

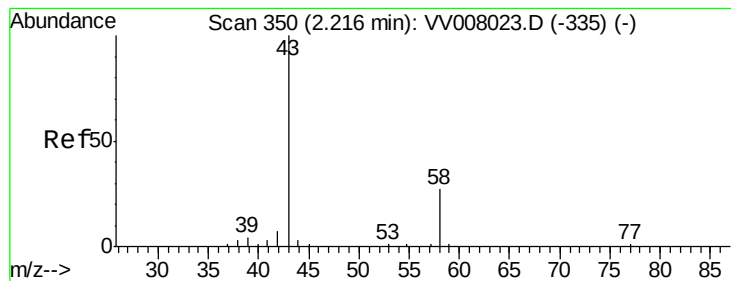

#13

Acetone

Concen: 3.943 ug/L

RT: 2.21 min Scan# 349

Delta R.T. -0.00 min

Lab File: VV008028.D

Acq: 02 Oct 2018 14:00

Instrument :
MSVOA_V
ClientSampleId :
GACC1

Tot Ion: 43 Resp: 4171

Ion Ratio Lower Upper

43 100

58 31.3 0.0 62.0

