

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100218\
 Data File : VV008029.D
 Acq On : 02 Oct 2018 14:27
 Operator : SY/MD
 Sample : J5160-19
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GACC2

Quant Time: Oct 03 06:35:36 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Oct 03 05:34:53 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	88482	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	87036	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	42437	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	23868	5.03	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.60%
7) Chloroethane-d5	1.59	69	21222	5.18	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.60%
11) 1,1-Dichloroethene-d2	2.14	63	37473	3.50	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.00%
20) 2-Butanone-d5	3.96	46	68621	48.10	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.20%
24) Chloroform-d	4.41	84	53834	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.60%
26) 1,2-Dichloroethane-d4	5.09	65	29192	4.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.20%
32) Benzene-d6	5.10	84	104703	5.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.80%
36) 1,2-Dichloropropane-d6	6.12	67	32873	4.99	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.80%
41) Toluene-d8	7.36	98	100032	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.60%
43) trans-1,3-Dichloropropene-	7.67	79	11705	4.61	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.20%
46) 2-Hexanone-d5	8.14	63	46379	41.43	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.86%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	22634	4.45	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	41527	5.06	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.20%


Target Compounds					Ovalue
13) Acetone	2.21	43	4609	4.434 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100218\
Data File : VV008029.D
Acq On : 02 Oct 2018 14:27
Operator : SY/MD
Sample : J5160-19
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GACC2

Quant Time: Oct 03 06:35:36 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Oct 03 05:34:53 2018
Response via : Initial Calibration

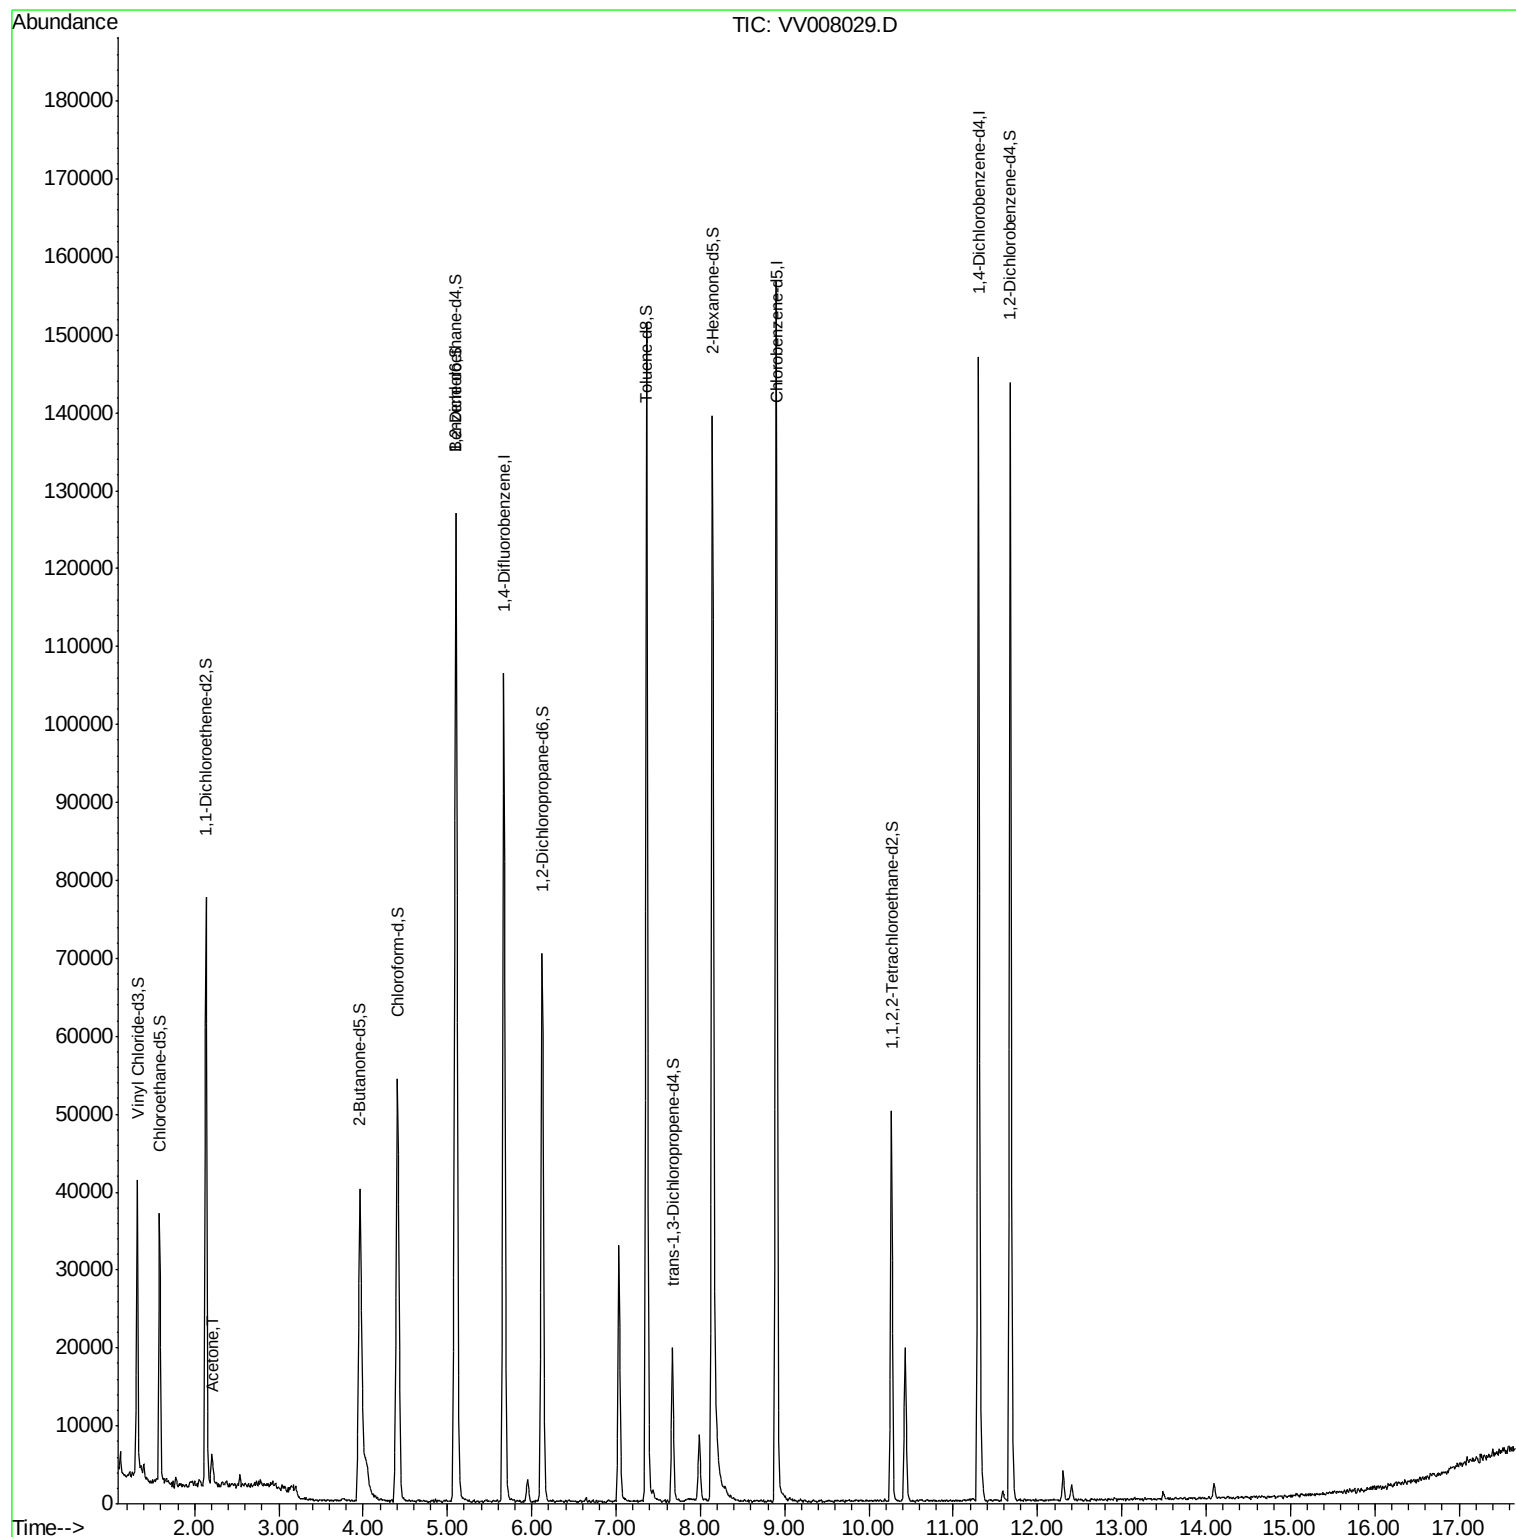

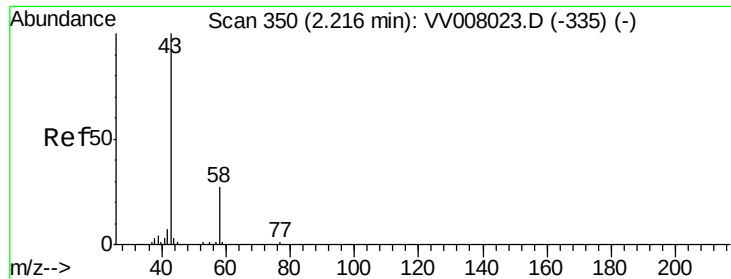

#13

Acetone

Concen: 4.434 ug/L

RT: 2.21 min Scan# 348

Delta R.T. -0.01 min

Lab File: VV008029.D

Acq: 02 Oct 2018 14:27

Instrument :
MSVOA_V
ClientSampleId :
GACC2

Tot Ion: 43 Resp: 4609

Ion Ratio Lower Upper

43 100

58 30.8 0.0 62.0

