

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100218\
 Data File : VV008039.D
 Acq On : 02 Oct 2018 20:17
 Operator : SY/MD
 Sample : J5185-09
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JLC87

Quant Time: Oct 03 07:01:01 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Oct 03 05:34:53 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	85236	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	83031	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	39683	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	21886	4.79	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.80%
7) Chloroethane-d5	1.59	69	19870	5.03	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.60%
11) 1,1-Dichloroethene-d2	2.13	63	35947	3.48	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.60%
20) 2-Butanone-d5	3.96	46	65478	47.64	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.28%
24) Chloroform-d	4.41	84	55378	5.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.40%
26) 1,2-Dichloroethane-d4	5.09	65	27816	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.20%
32) Benzene-d6	5.10	84	100463	5.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.40%
36) 1,2-Dichloropropane-d6	6.12	67	31823	5.06	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.20%
41) Toluene-d8	7.36	98	92929	4.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.00%
43) trans-1,3-Dichloropropene-	7.67	79	10398	4.30	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.00%
46) 2-Hexanone-d5	8.14	63	44453	41.62	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.24%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	21866	4.51	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	38813	5.05	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.00%


Target Compounds					Ovalue
25) Chloroform	4.43	83	80034	6.983 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100218\
Data File : VV008039.D
Acq On : 02 Oct 2018 20:17
Operator : SY/MD
Sample : J5185-09
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JLC87

Quant Time: Oct 03 07:01:01 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Oct 03 05:34:53 2018
Response via : Initial Calibration

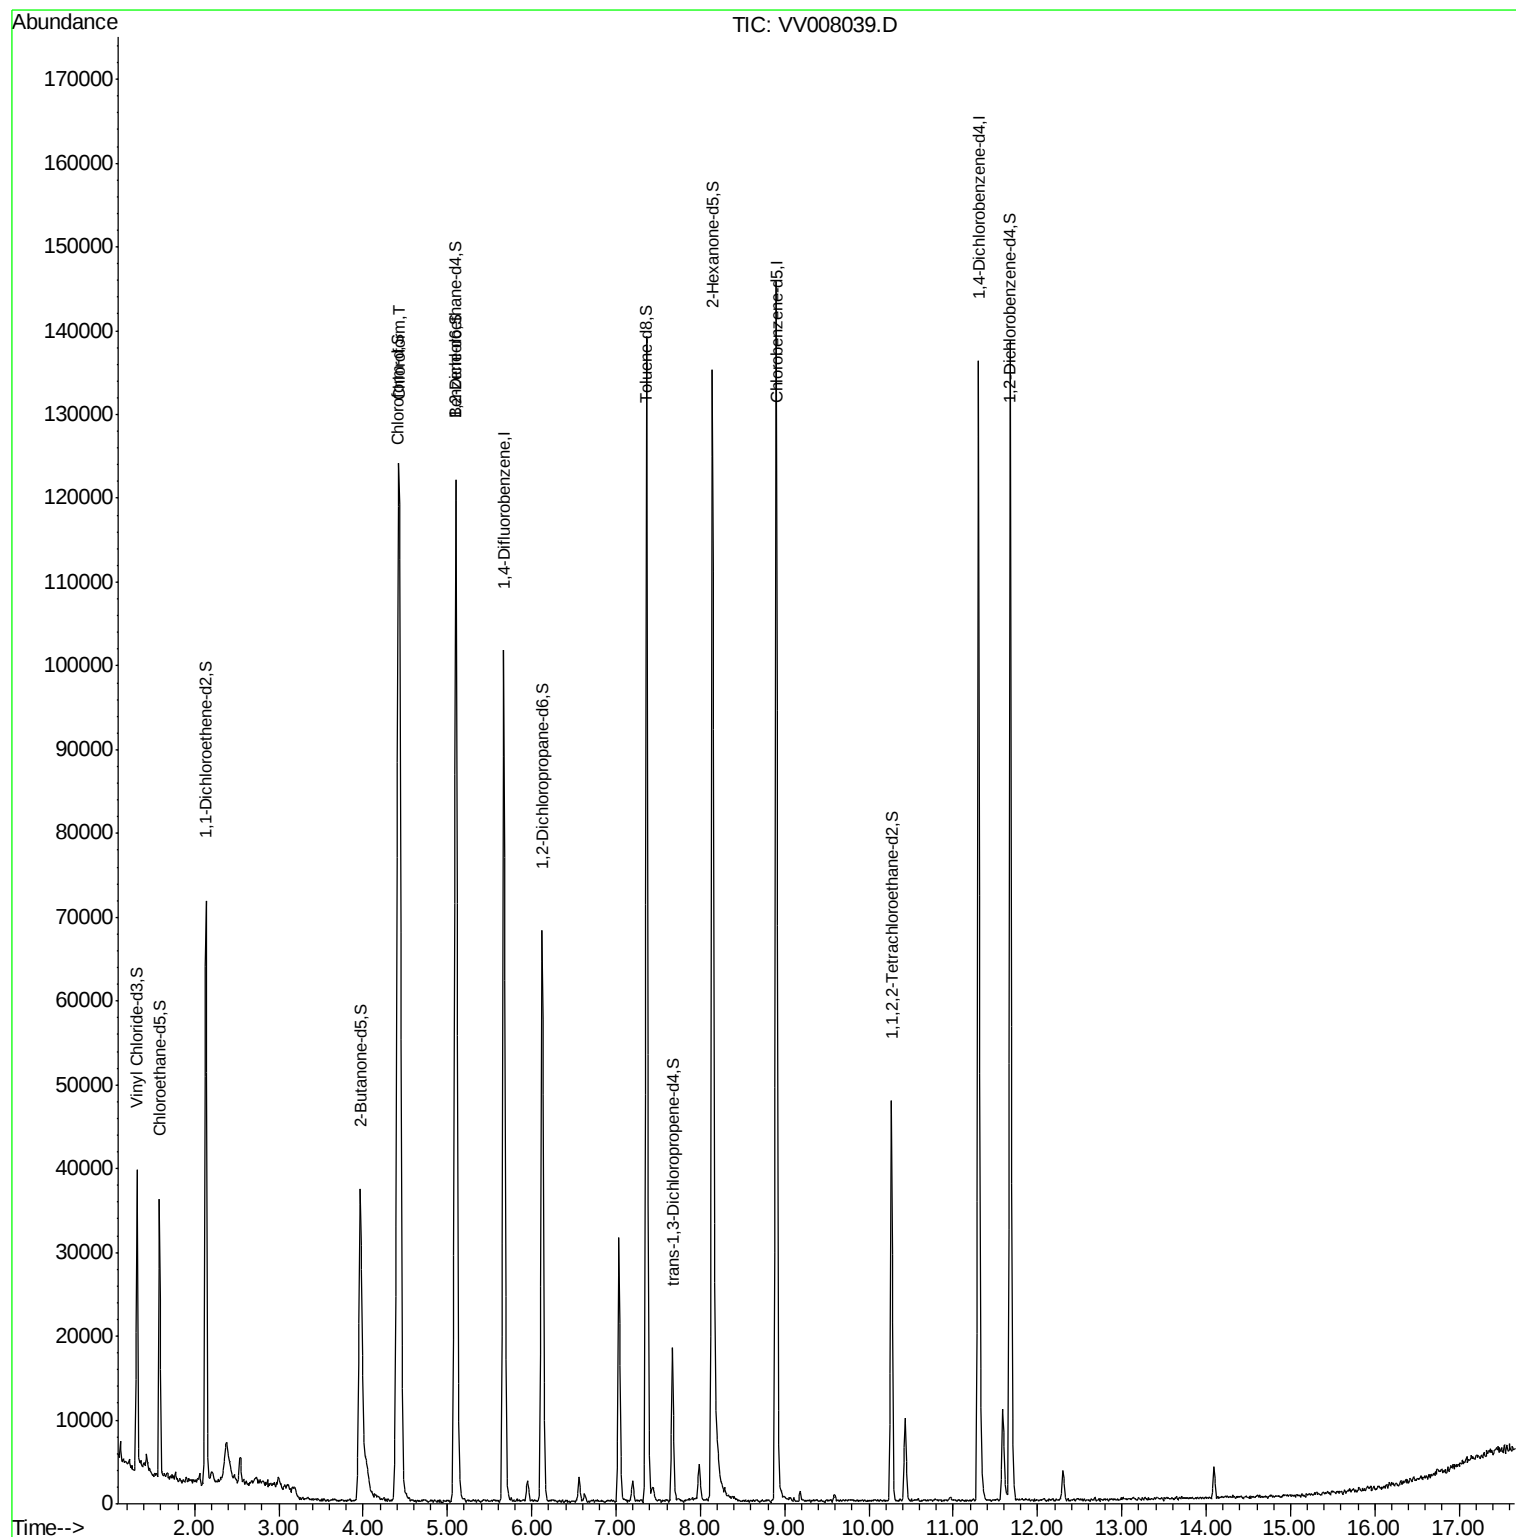

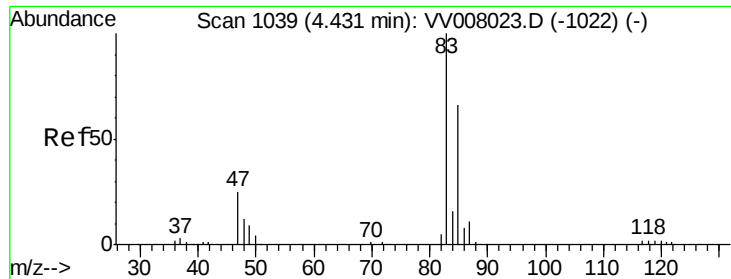

#25
 Chloroform
 Concen: 6.983 ug/L
 RT: 4.43 min Scan# 1040
 Delta R.T. 0.00 min
 Lab File: VV008039.D
 Acq: 02 Oct 2018 20:17

Instrument :
 MSVOA_V
 ClientSampleId :
 JLC87

Tot Ion: 83 Resp: 80034
 Ion Ratio Lower Upper
 83 100
 85 65.4 44.8 83.2

