


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100218\
Data File : VV008022.D
Acq On : 02 Oct 2018 09:55
Operator : SY/MD
Sample : BFB79
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB79

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR092718WMA.M
Title : TRACE VOA SOM01.0
Last Update : Wed Oct 03 05:34:53 2018

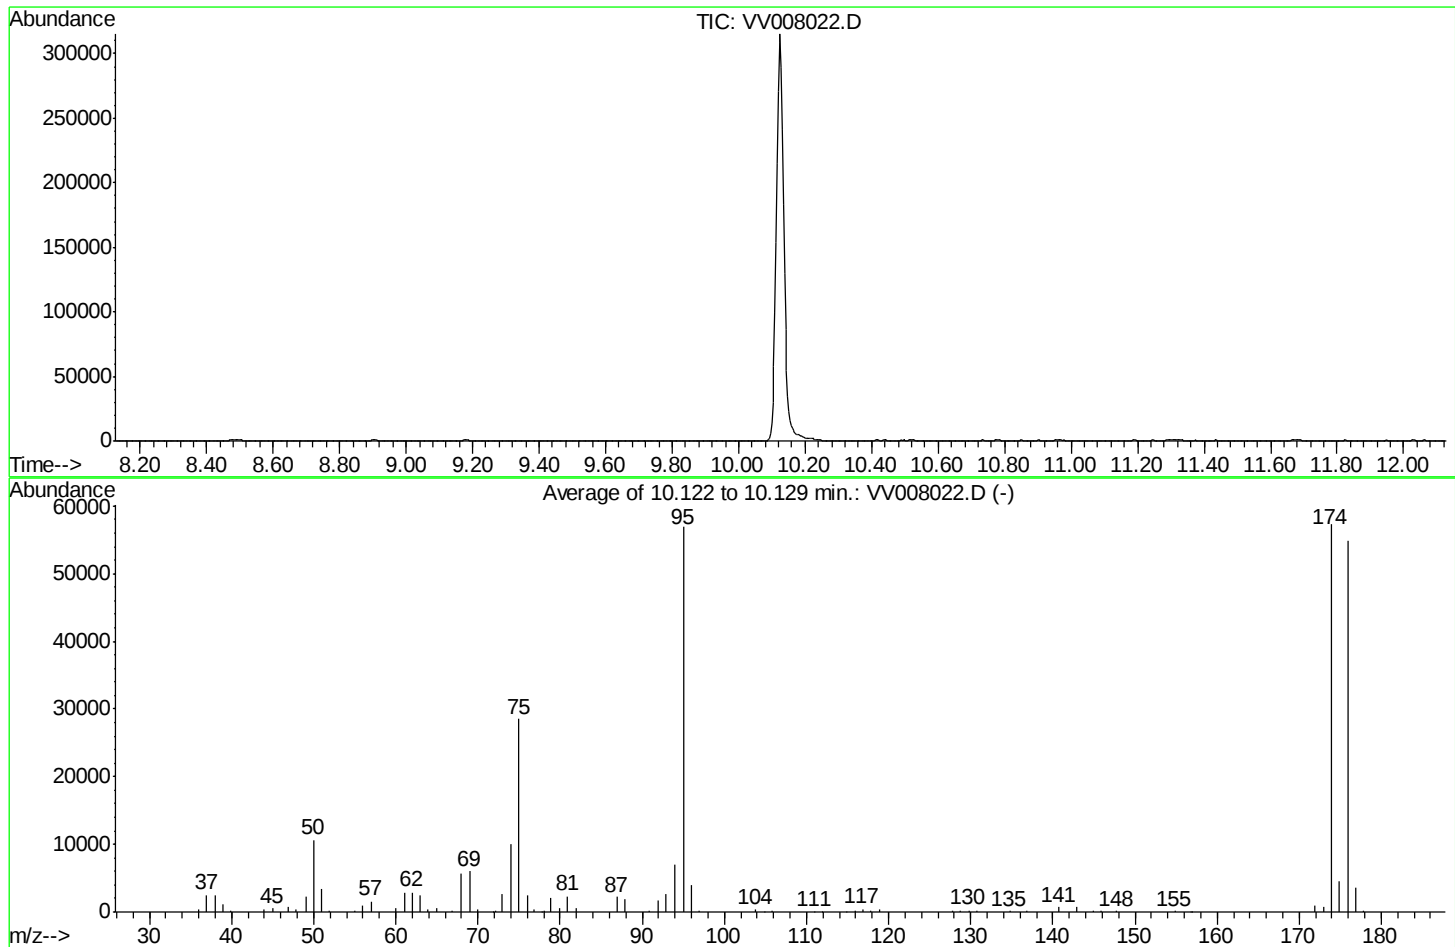

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	10607	PASS
75	95	30	80	50.1	28544	PASS
95	95	100	100	100.0	57029	PASS
96	95	5	9	7.0	3989	PASS
173	174	0.00	2	1.4	812	PASS
174	95	50	120	100.5	57290	PASS
175	174	5	9	7.8	4475	PASS
176	174	95	101	95.6	54776	PASS
177	176	5	9	6.4	3533	PASS

m/z	Abundance
43.90	256.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79

m/z	Abundance
35.90	433.0
36.90	2725.0
38.00	2529.0
38.90	1085.0
40.00	149.0
43.90	576.0
44.90	555.0
46.90	764.0
47.90	446.0
49.00	2270.0
50.00	11052.0
51.00	3547.0
51.90	162.0
55.00	178.0
56.00	981.0
57.00	1664.0
60.00	615.0
61.00	2967.0
62.00	2787.0
63.00	2550.0
63.90	269.0
64.90	515.0
66.90	190.0
68.00	5934.0
69.00	6069.0
70.00	490.0
71.90	305.0
72.90	2811.0
74.00	10525.0
75.00	29464.0
76.00	2511.0
76.80	351.0
77.70	205.0
78.10	216.0
78.90	2161.0
79.90	624.0
80.90	2347.0
81.90	481.0
86.90	2191.0
87.90	2162.0
90.90	288.0
91.90	1667.0
92.90	2785.0
94.00	7389.0
95.00	58136.0
96.00	4121.0
96.90	167.0
103.80	348.0
104.80	104.0
105.80	249.0
111.00	113.0
114.90	113.0
115.90	263.0
116.80	458.0
117.80	223.0
118.90	393.0
127.80	231.0
128.60	130.0
129.80	224.0
130.80	108.0
134.80	195.0
136.70	116.0
140.80	779.0
142.90	779.0
144.90	178.0
145.80	116.0
147.80	154.0
154.90	177.0
156.80	108.0
172.00	851.0
173.00	808.0
173.90	56584.0
174.90	4567.0
175.90	54120.0
176.90	3569.0
177.80	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79

m/z	Abundance
35.90	432.0
37.00	2637.0
38.00	2587.0
38.90	1160.0
40.00	154.0
43.90	568.0
45.00	585.0
46.90	790.0
47.90	409.0
49.00	2390.0
50.00	10889.0
51.00	3612.0
51.90	135.0
55.00	191.0
56.00	1018.0
57.00	1668.0
60.00	619.0
61.00	2883.0
62.00	2984.0
63.00	2625.0
64.00	306.0
64.90	520.0
66.90	155.0
68.00	6004.0
69.00	6221.0
70.00	489.0
72.10	297.0
72.90	2818.0
74.00	10478.0
75.00	29488.0
76.00	2467.0
76.70	344.0
78.10	237.0
78.90	2182.0
79.90	674.0
80.90	2447.0
81.90	506.0
86.90	2235.0
87.90	1980.0
90.90	286.0
91.90	1662.0
92.90	2710.0
94.00	7305.0
95.00	59000.0
96.00	4180.0
96.90	159.0
103.80	382.0
105.80	242.0
114.90	103.0
115.90	279.0
116.80	447.0
117.80	229.0
118.90	355.0
127.80	237.0
128.70	119.0
129.80	233.0
130.80	128.0
134.80	189.0
136.70	134.0
140.80	779.0
142.80	773.0
144.90	215.0
145.80	127.0
147.80	160.0
154.80	186.0
157.00	111.0
172.00	971.0
173.00	823.0
173.90	59552.0
174.90	4653.0
175.90	56624.0
176.90	3618.0
177.80	124.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79

m/z	Abundance
35.90	393.0
37.00	2266.0
38.00	2286.0
38.90	1066.0
39.80	160.0
43.90	572.0
44.90	554.0
46.90	728.0
47.90	302.0
49.00	2261.0
50.00	9880.0
51.00	3294.0
51.90	113.0
55.00	180.0
55.90	972.0
57.00	1489.0
60.00	543.0
61.00	2579.0
62.00	2848.0
63.00	2342.0
64.00	332.0
64.90	490.0
66.90	119.0
68.00	5375.0
69.00	5672.0
70.00	445.0
72.10	261.0
73.00	2479.0
74.00	9362.0
75.00	26680.0
76.00	2185.0
76.70	289.0
78.00	237.0
78.90	1912.0
79.90	599.0
80.90	2207.0
81.90	518.0
86.90	2147.0
87.90	1760.0
90.80	255.0
91.90	1532.0
92.90	2317.0
94.00	6479.0
95.00	53952.0
96.00	3667.0
96.90	116.0
103.80	358.0
105.70	227.0
111.90	105.0
115.90	244.0
116.80	393.0
117.80	210.0
118.90	324.0
127.80	209.0
128.80	105.0
129.80	231.0
130.80	125.0
134.80	125.0
136.80	130.0
140.80	714.0
142.80	720.0
144.90	219.0
145.80	123.0
147.80	148.0
154.80	160.0
171.90	992.0
173.00	806.0
173.90	55736.0
174.90	4207.0
175.90	53584.0
176.90	3413.0
177.80	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79