


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV100219\
 Data File : VV013022.D
 Acq On : 02 Oct 2019 08:45
 Operator : SY/MD
 Sample : BFB63
 Misc : 5.00G/10ML/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB63

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM093019SMA.M
 Title : VOC Analysis
 Last Update : Fri Oct 04 03:45:22 2019

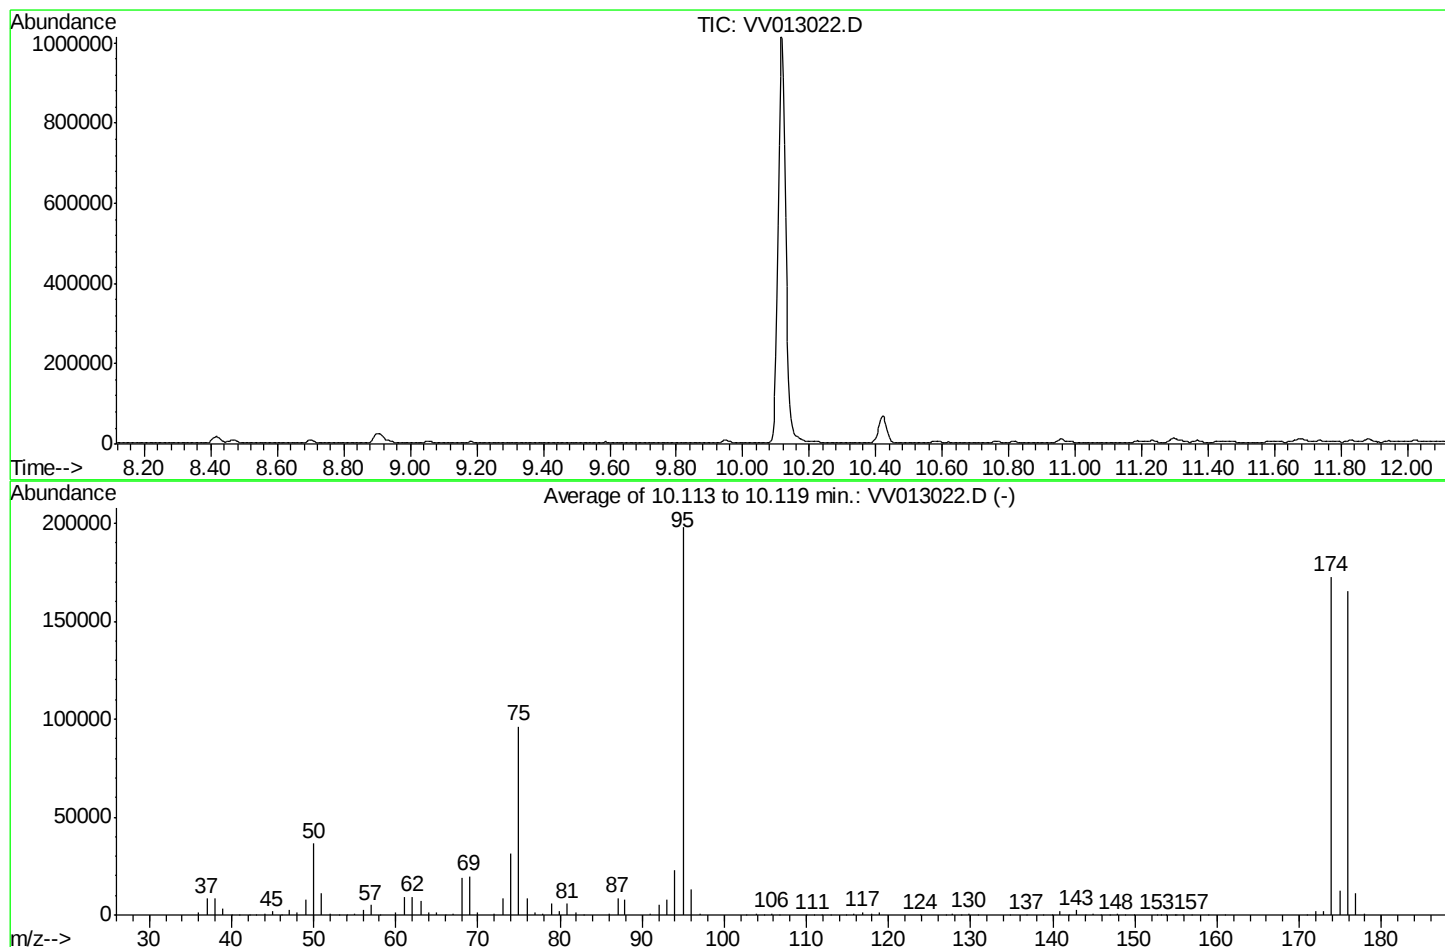

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	36578	PASS
75	95	30	80	48.7	96386	PASS
95	95	100	100	100.0	197930	PASS
96	95	5	9	6.6	13093	PASS
173	174	0.00	2	1.1	1909	PASS
174	95	50	120	87.3	172885	PASS
175	174	5	9	7.3	12669	PASS
176	174	95	101	95.7	165504	PASS
177	176	5	9	6.8	11316	PASS

m/z	Abundance
36.00	1485.0
37.00	8100.0
38.00	8016.0
39.00	3286.0
40.00	1467.0
42.20	118.0
42.90	203.0
44.00	1918.0
45.00	1731.0
46.10	305.0
47.00	2575.0
48.00	1097.0
49.00	7426.0
50.00	35296.0
51.00	10603.0
52.00	445.0
53.00	170.0
55.00	556.0
56.00	2372.0
57.00	5120.0
58.10	235.0
60.00	1502.0
61.00	8578.0
62.00	8981.0
63.10	7255.0
64.00	1172.0
65.00	1583.0
66.10	290.0
67.10	570.0
68.00	17664.0
69.00	19136.0
70.00	1510.0
72.00	718.0
73.00	8418.0
74.00	29520.0
75.00	90792.0
76.00	8192.0
76.90	1111.0
77.90	895.0
78.90	5612.0
79.90	1786.0
80.90	5350.0
82.00	1348.0
82.90	144.0
85.90	296.0
87.00	8252.0
87.90	7332.0
90.90	687.0
92.00	4949.0
93.00	7635.0
94.00	21608.0
95.00	185728.0
96.00	12507.0
97.00	397.0
104.00	720.0
104.90	315.0
105.80	784.0
106.70	135.0
110.00	155.0
110.90	124.0
113.00	128.0
114.90	278.0
115.80	587.0
116.90	1295.0
117.90	697.0
118.90	976.0
127.80	582.0
128.80	290.0
129.80	707.0
130.80	260.0
134.80	273.0
136.80	291.0
139.90	110.0
140.90	1786.0
142.90	2144.0
143.90	239.0
144.90	539.0
146.00	294.0
146.90	193.0
147.80	424.0
148.90	144.0
149.80	196.0
152.80	167.0
153.10	150.0
154.80	458.0
155.90	102.0
157.00	264.0
158.90	239.0
160.90	200.0
170.90	295.0
172.00	1694.0
173.00	1752.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

173.90	158016.0
174.90	11802.0
175.90	150720.0
176.90	10647.0
177.90	410.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
36.00	1572.0
37.00	8549.0
38.00	8565.0
39.00	3697.0
40.00	1461.0
42.20	130.0
43.00	205.0
44.00	1990.0
45.00	1945.0
46.10	241.0
47.00	2855.0
47.90	1324.0
49.00	7882.0
50.00	37776.0
51.00	11613.0
52.00	541.0
53.10	203.0
54.00	107.0
55.00	562.0
56.00	2621.0
57.00	5341.0
58.10	221.0
60.00	1689.0
61.00	9381.0
62.00	9760.0
63.10	7637.0
64.00	1169.0
65.00	1581.0
66.10	315.0
67.00	640.0
68.00	19504.0
69.00	20472.0
70.00	1601.0
71.90	803.0
73.00	9133.0
74.00	32464.0
75.00	99648.0
76.00	8814.0
76.90	1170.0
77.80	989.0
78.90	6207.0
79.90	1862.0
80.90	5898.0
82.00	1548.0
82.90	142.0
85.90	409.0
87.00	8845.0
87.90	8035.0
90.90	790.0
92.00	5717.0
93.00	8466.0
94.00	23296.0
95.00	205312.0
96.00	13586.0
97.00	424.0
104.00	758.0
104.90	338.0
105.80	958.0
106.80	162.0
109.90	167.0
110.90	178.0
113.00	150.0
114.90	283.0
115.80	694.0
116.90	1597.0
117.90	743.0
118.90	1198.0
127.80	682.0
128.80	309.0
129.90	722.0
130.80	235.0
134.80	325.0
136.80	340.0
139.90	154.0
140.90	1979.0
141.90	173.0
142.90	2437.0
143.90	228.0
144.90	569.0
145.90	342.0
146.90	244.0
147.80	460.0
148.80	174.0
149.90	232.0
152.80	161.0
153.20	163.0
153.80	133.0
155.00	457.0
155.80	147.0
156.90	319.0
158.90	271.0
161.00	256.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

170.90	319.0
172.00	1932.0
173.00	1965.0
173.90	178944.0
174.90	13144.0
175.90	171328.0
176.90	11662.0
177.90	459.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
36.00	1676.0
37.00	8478.0
38.00	8324.0
39.00	3754.0
40.00	1418.0
41.00	109.0
43.00	209.0
44.00	1959.0
45.00	1787.0
46.20	195.0
47.00	2823.0
48.00	1360.0
49.00	7498.0
50.00	36664.0
51.00	11218.0
52.00	616.0
53.10	201.0
54.00	116.0
54.90	513.0
56.00	2662.0
57.00	5076.0
58.00	229.0
60.00	1688.0
61.00	9344.0
62.00	9601.0
63.10	7206.0
64.00	1114.0
65.00	1476.0
66.10	283.0
67.00	647.0
68.00	19344.0
69.00	19864.0
70.00	1490.0
71.90	841.0
73.00	8961.0
74.00	32024.0
75.00	98720.0
76.00	8530.0
77.00	1141.0
77.80	918.0
78.90	6073.0
79.90	1781.0
80.90	5871.0
82.00	1509.0
82.90	163.0
86.00	419.0
87.00	8566.0
87.90	7830.0
90.90	775.0
92.00	5822.0
93.00	8274.0
94.00	22848.0
95.00	202752.0
96.00	13187.0
97.00	358.0
102.70	112.0
103.90	739.0
104.90	332.0
105.90	1001.0
106.80	167.0
109.90	151.0
110.90	191.0
111.80	116.0
112.90	147.0
114.80	250.0
115.80	749.0
116.90	1662.0
117.90	646.0
118.90	1267.0
123.90	128.0
126.90	104.0
127.80	732.0
128.80	291.0
129.90	703.0
130.90	220.0
134.80	344.0
136.80	350.0
138.80	104.0
139.90	183.0
140.90	1790.0
141.90	173.0
142.90	2441.0
143.90	165.0
144.90	536.0
145.80	337.0
146.90	214.0
147.90	459.0
148.70	169.0
149.90	265.0
152.70	169.0
153.20	130.0
153.80	174.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

155.00	478.0
155.80	162.0
156.80	373.0
158.90	241.0
161.00	269.0
170.90	308.0
171.90	2081.0
173.00	2010.0
173.90	181696.0
174.90	13062.0
175.90	174464.0
176.90	11641.0
177.90	440.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

Scan 2794 (10.074 min): VV013022.D
BFB63

m/z	Abundance
40.00	1157.0
44.00	955.0
81.90	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63