

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100220\
 Data File : VV018622.D
 Acq On : 02 Oct 2020 13:50
 Operator : SY/MD
 Sample : L4237-14MSD
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC7MSD

Quant Time: Oct 03 01:26:37 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 03 00:50:30 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	238642	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	238713	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	119842	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	83969	60.00	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	120.00%
7) Chloroethane-d5	1.58	69	71966	62.19	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	124.38%
11) 1,1-Dichloroethene-d2	2.12	63	183935	64.50	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	129.00%#
21) 2-Butanone-d5	3.91	46	109651	105.03	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	105.03%
24) Chloroform-d	4.38	84	169234	55.92	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	111.84%
26) 1,2-Dichloroethane-d4	5.06	65	113833	59.25	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	118.50%
32) Benzene-d6	5.07	84	328850	54.39	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	108.78%
36) 1,2-Dichloropropane-d6	6.09	67	101429	55.52	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	111.04%
41) Toluene-d8	7.34	98	302711	53.22	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.44%
43) trans-1,3-Dichloropropene-	7.64	79	51526	52.21	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	104.42%
47) 2-Hexanone-d5	8.11	63	66689	96.10	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	96.10%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	121213	50.04	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	100.08%
64) 1,2-Dichlorobenzene-d4	11.65	152	131790	57.18	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	114.36%

Target Compounds


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
12) 1,1-Dichloroethene	2.13	96	73808	49.545	ug/L	92
33) Benzene	5.13	78	302174	43.087	ug/L	100
34) Trichloroethene	5.94	95	563306	276.672	ug/L	99
42) Toluene	7.41	91	331692	43.720	ug/L	100
51) Chlorobenzene	8.90	112	229472	44.710	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100220\
Data File : VV018622.D
Acq On : 02 Oct 2020 13:50
Operator : SY/MD
Sample : L4237-14MSD
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC7MSD

Quant Time: Oct 03 01:26:37 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 03 00:50:30 2020
Response via : Initial Calibration




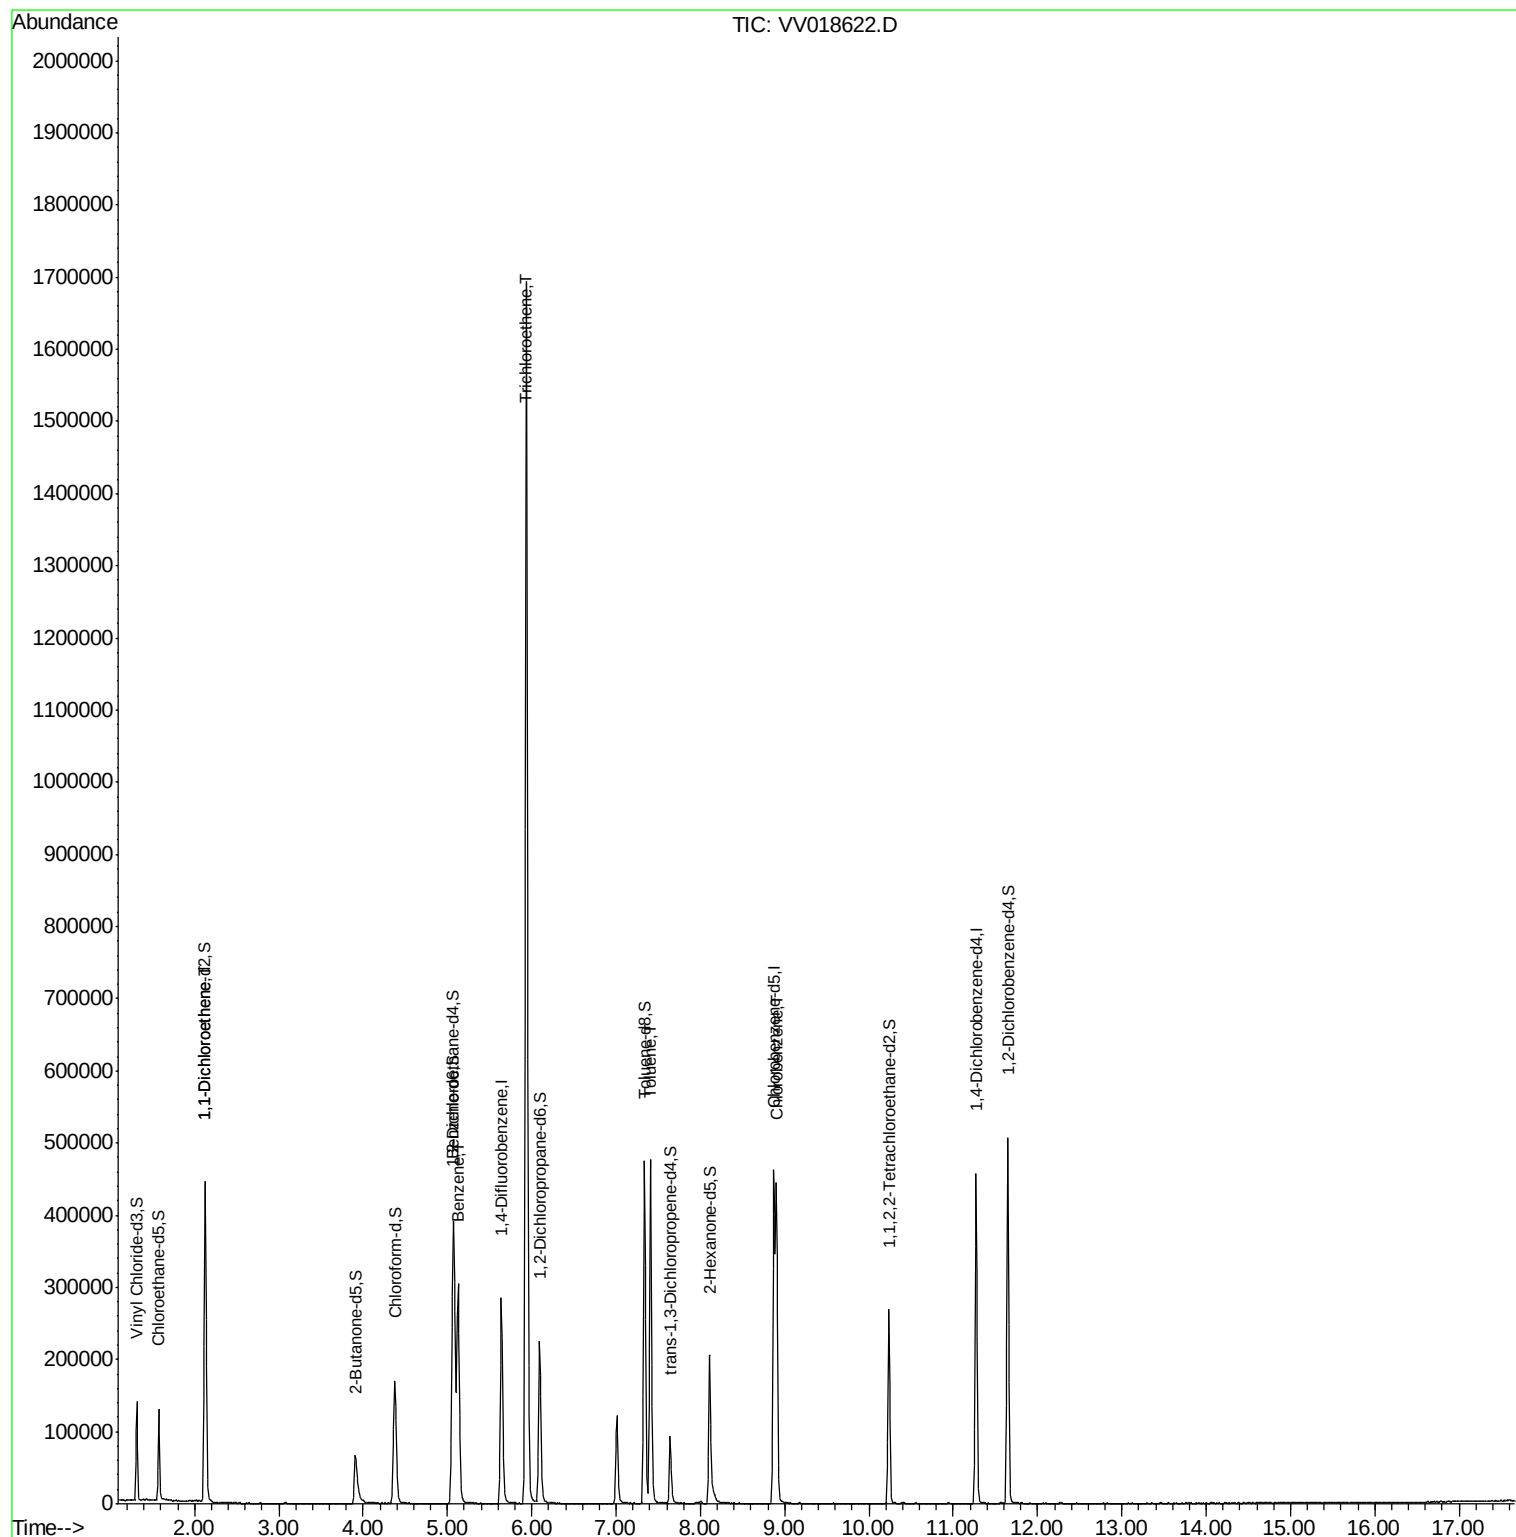


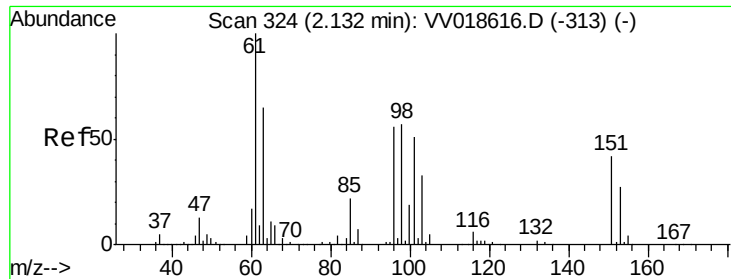

#12
 1,1-Dichloroethene
 Concen: 49.545 ug/L
 RT: 2.13 min Scan# 324
 Delta R.T. 0.00 min
 Lab File: VV018622.D
 Acq: 02 Oct 2020 13:50




Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC7MSD


Tot Ion: 96 Resp: 73808
 Ion Ratio Lower Upper
 96 100
 61 178.6 122.8 228.1
 63 150.3 91.9 170.7

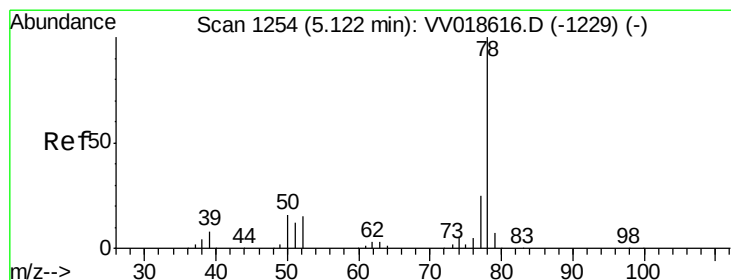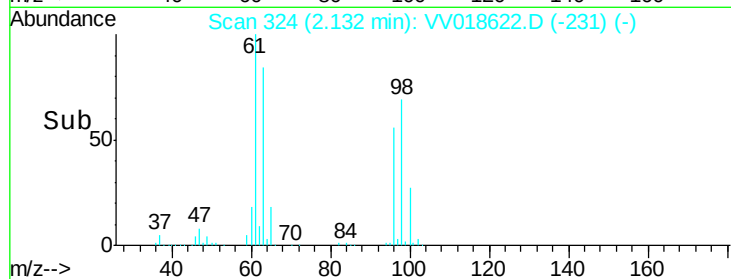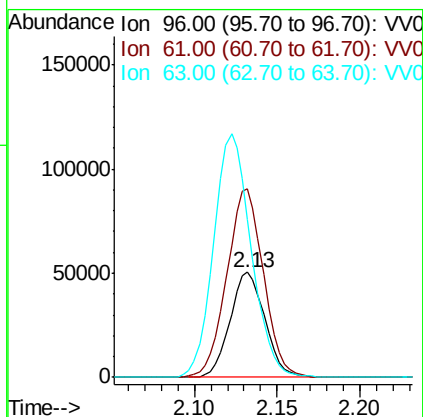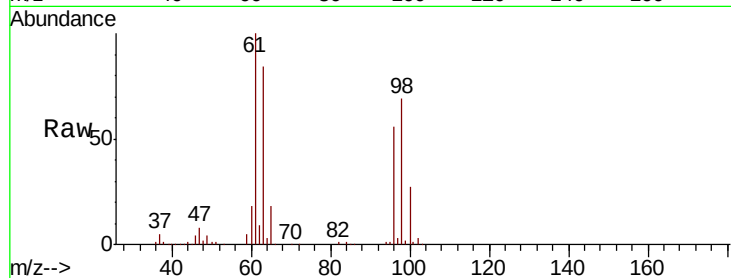

#33
 Benzene
 Concen: 43.087 ug/L
 RT: 5.13 min Scan# 1255
 Delta R.T. 0.00 min
 Lab File: VV018622.D
 Acq: 02 Oct 2020 13:50

Tgt Ion: 78 Resp: 302174

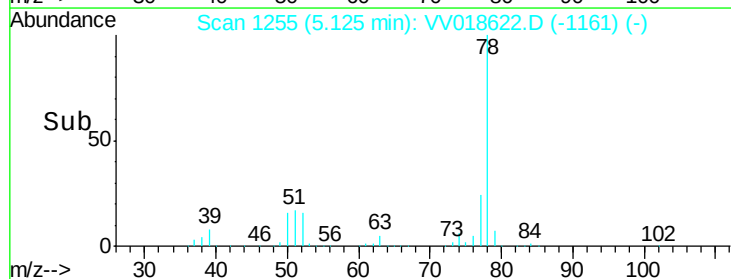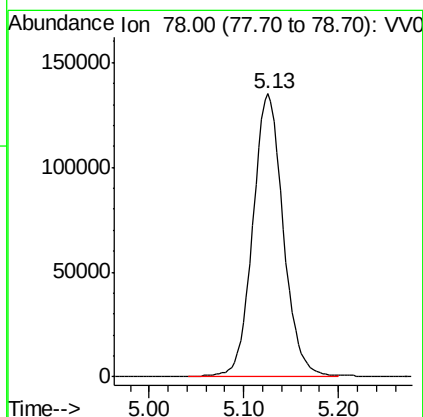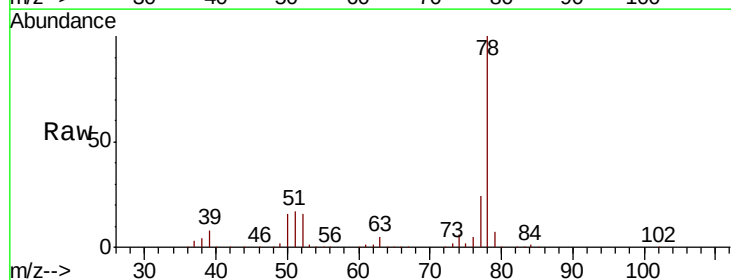


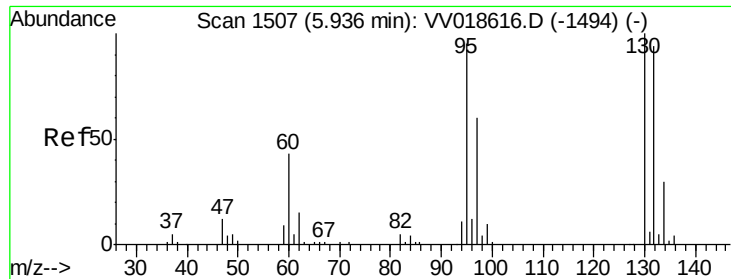




#34
 Trichloroethene
 Concen: 276.672 ug/L
 RT: 5.94 min Scan# 1507
 Delta R.T. 0.00 min
 Lab File: VV018622.D
 Acq: 02 Oct 2020 13:50

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC7MSD

Tot Ion: 95 Resp: 563306
 Ion Ratio Lower Upper
 95 100
 97 65.0 45.9 85.3
 132 102.1 70.8 131.4
 130 105.2 75.3 139.8

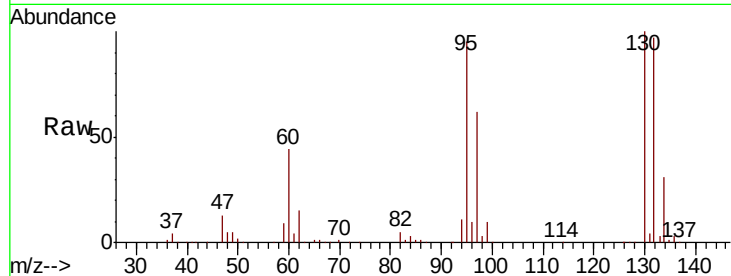


Abundance Ion 95.00 (94.70 to 95.70): VV0
 Ion 97.00 (96.70 to 97.70): VV0
 Ion 132.00 (131.70 to 132.70): VV0
 Ion 130.00 (129.70 to 130.70): VV0

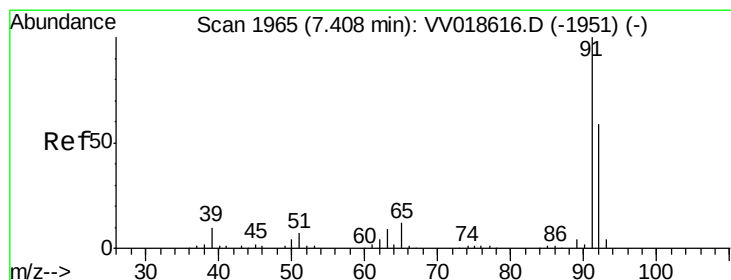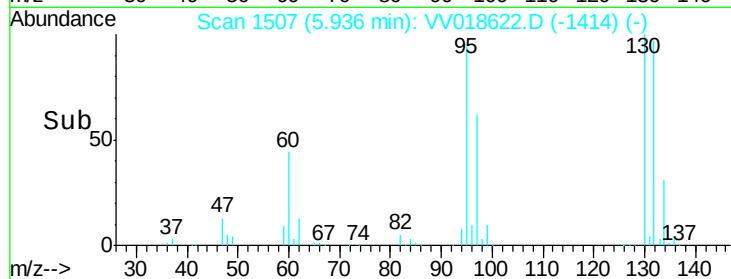
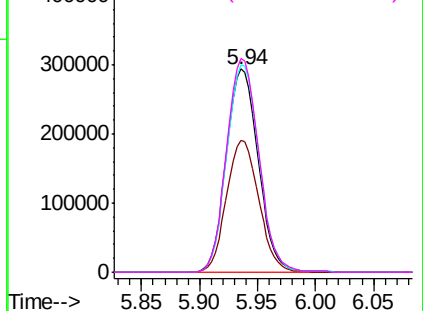



#42
 Toluene
 Concen: 43.720 ug/L
 RT: 7.41 min Scan# 1965
 Delta R.T. 0.00 min
 Lab File: VV018622.D
 Acq: 02 Oct 2020 13:50

Tgt Ion: 91 Resp: 331692
 Ion Ratio Lower Upper
 91 100
 92 59.4 41.6 77.3

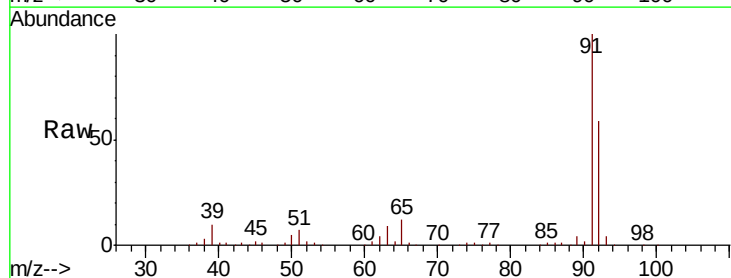

Abundance Ion 91.00 (90.70 to 91.70): VV0
 Ion 92.00 (91.70 to 92.70): VV0

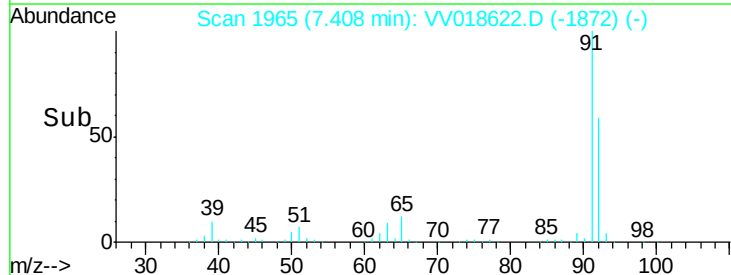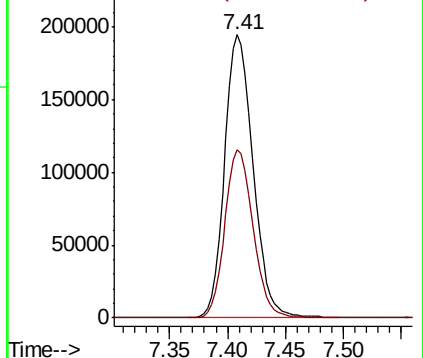

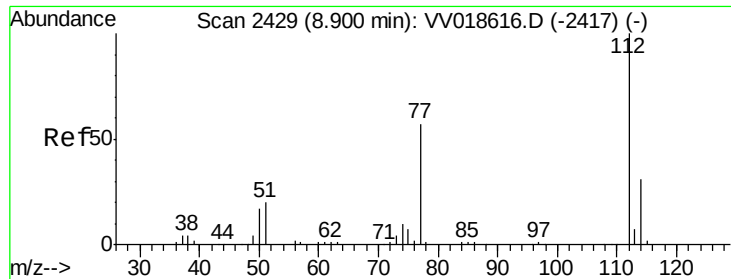

#51
 Chlorobenzene
 Concen: 44.710 ug/L
 RT: 8.90 min Scan# 2430
 Delta R.T. 0.00 min
 Lab File: VV018622.D
 Acq: 02 Oct 2020 13:50

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC7MSD

Tot Ion	Ratio	Lower	Upper
112	100		
114	32.1	22.4	41.6
77	55.1	44.8	67.2

