

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100220\
 Data File : VV018627.D
 Acq On : 02 Oct 2020 15:54
 Operator : SY/MD
 Sample : L4203-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3S0

Quant Time: Oct 03 02:02:14 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 03 00:50:30 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	286525	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	283175	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	144763	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	96776	57.59	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	115.18%
7) Chloroethane-d5	1.58	69	90475	65.12	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	130.24%#
11) 1,1-Dichloroethene-d2	2.12	63	165116	48.22	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	96.44%
21) 2-Butanone-d5	3.91	46	116687	93.09	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	93.09%
24) Chloroform-d	4.37	84	183990	50.63	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.26%
26) 1,2-Dichloroethane-d4	5.05	65	126385	54.79	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	109.58%
32) Benzene-d6	5.07	84	367820	51.28	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.56%
36) 1,2-Dichloropropane-d6	6.09	67	111782	51.58	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	103.16%
41) Toluene-d8	7.33	98	333566	49.43	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.86%
43) trans-1,3-Dichloropropene-	7.64	79	52592	44.92	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.84%
47) 2-Hexanone-d5	8.11	63	58928	71.59	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	71.59%
57) 1,1,2,2-Tetrachloroethane-	10.23	84	113602	39.54	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	79.08%
64) 1,2-Dichlorobenzene-d4	11.65	152	141895	50.97	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.94%


Target Compounds					Ovalue
13) Acetone	2.20	43	5271	4.867 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100220\
Data File : VV018627.D
Acq On : 02 Oct 2020 15:54
Operator : SY/MD
Sample : L4203-11
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3S0

Quant Time: Oct 03 02:02:14 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 03 00:50:30 2020
Response via : Initial Calibration

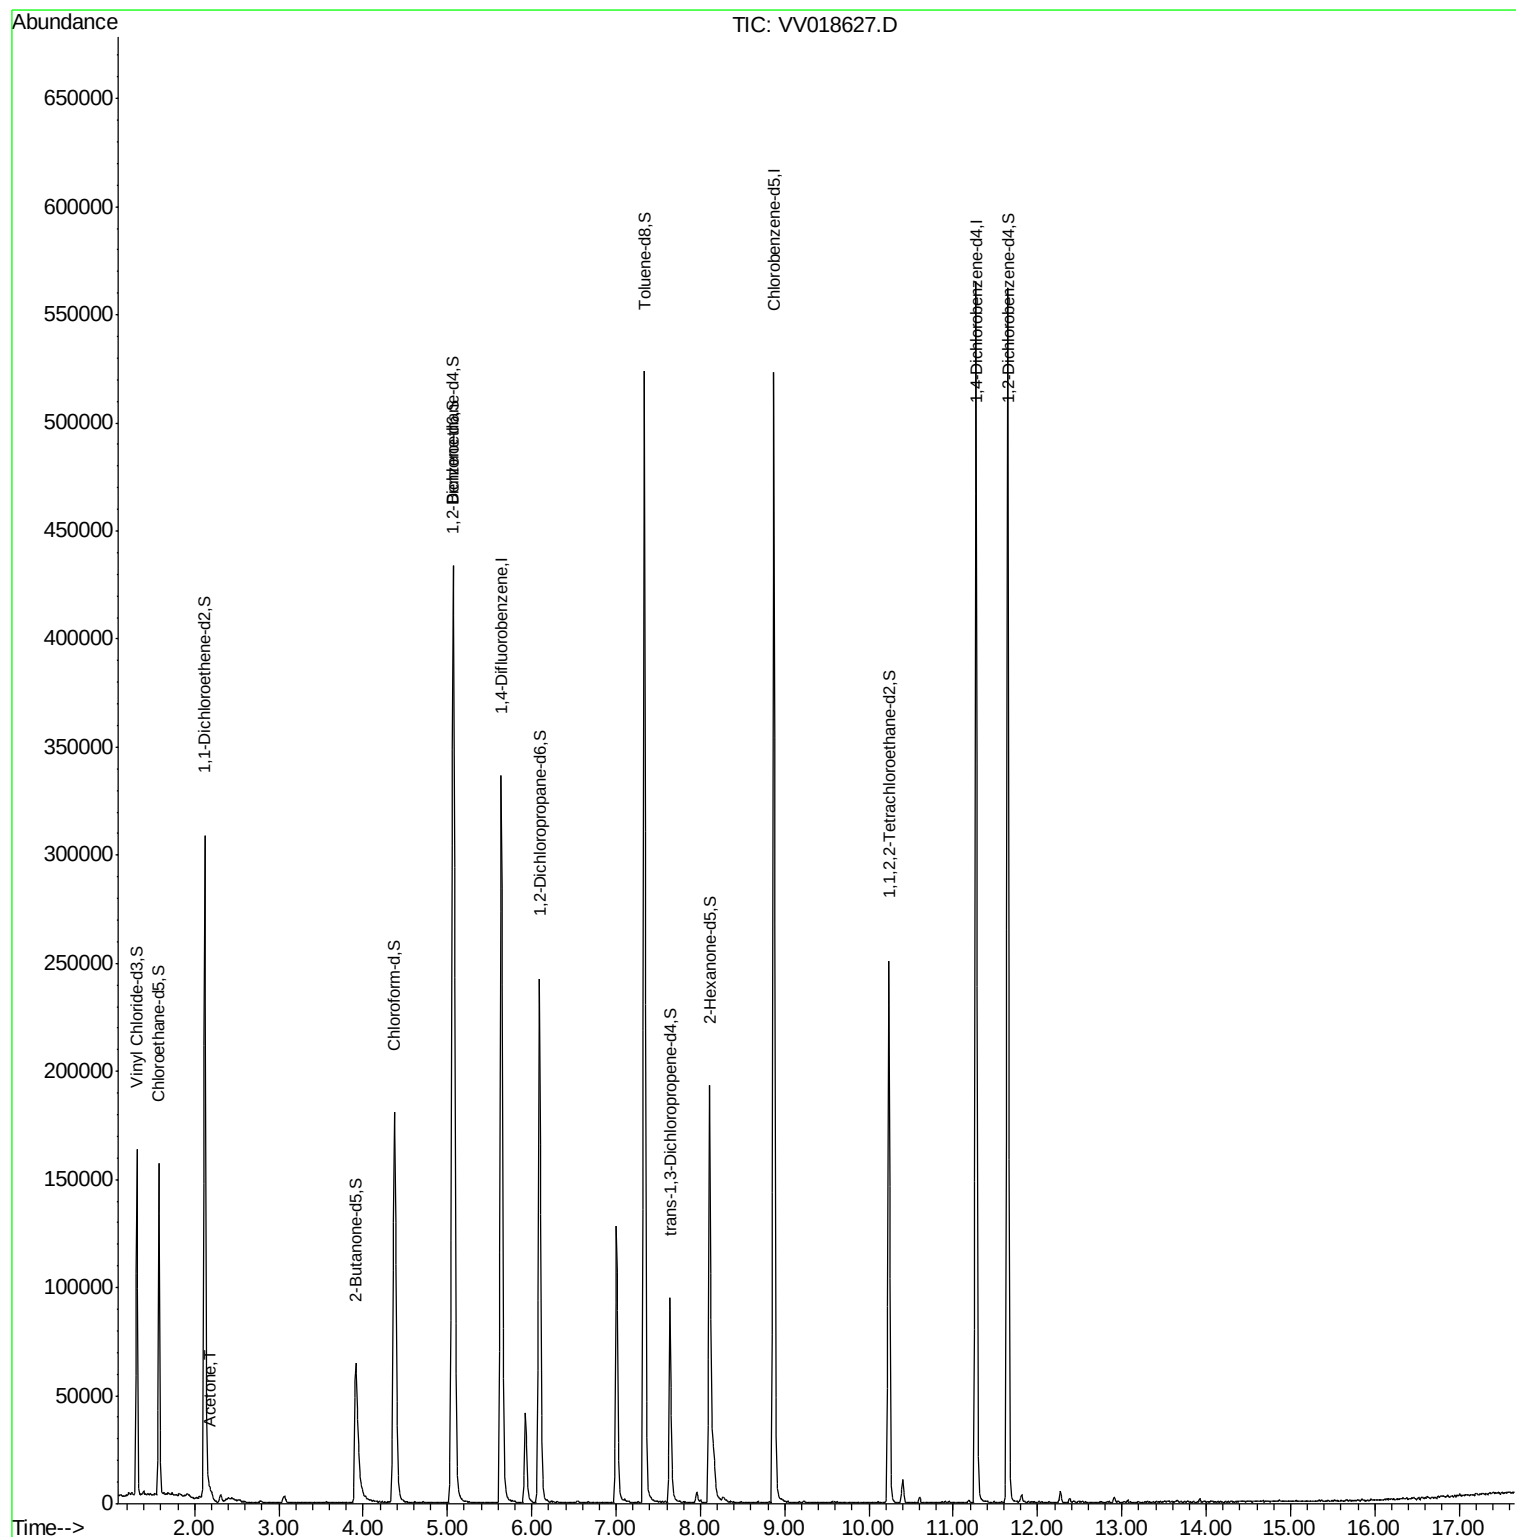

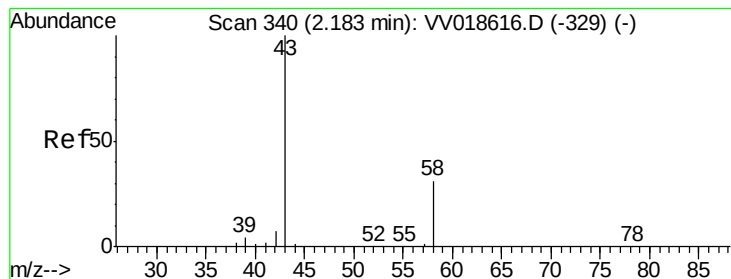

#13
 Acetone
 Concen: 4.867 ug/L
 RT: 2.20 min Scan# 344
 Delta R.T. 0.01 min
 Lab File: VV018627.D
 Acq: 02 Oct 2020 15:54

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3S0

Tot Ion: 43 Resp: 5271
 Ion Ratio Lower Upper
 43 100
 58 29.8 0.0 64.0

