

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100220\
 Data File : VV018639.D
 Acq On : 02 Oct 2020 20:45
 Operator : SY/MD
 Sample : L4203-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3R8

Quant Time: Oct 03 03:11:53 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 03 02:08:43 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	299231	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	297352	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	144407	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	74538	42.47	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	84.94%
7) Chloroethane-d5	1.58	69	69072	47.60	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	95.20%
11) 1,1-Dichloroethene-d2	2.12	63	132743	37.12	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.24%
21) 2-Butanone-d5	3.90	46	110098	84.11	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	84.11%
24) Chloroform-d	4.38	84	163518	43.09	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.18%
26) 1,2-Dichloroethane-d4	5.06	65	112502	46.70	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.40%
32) Benzene-d6	5.07	84	316808	42.06	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.12%
36) 1,2-Dichloropropane-d6	6.09	67	98439	43.26	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	86.52%
41) Toluene-d8	7.34	98	292425	41.27	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.54%
43) trans-1,3-Dichloropropene-	7.64	79	48278	39.27	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.54%
47) 2-Hexanone-d5	8.11	63	58046	67.15	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	67.15%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	108387	35.92	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	71.84%
64) 1,2-Dichlorobenzene-d4	11.65	152	129467	46.62	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.24%


Target Compounds					Ovalue
13) Acetone	2.18	43	4833	4.273 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100220\
Data File : VV018639.D
Acq On : 02 Oct 2020 20:45
Operator : SY/MD
Sample : L4203-04
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3R8

Quant Time: Oct 03 03:11:53 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 03 02:08:43 2020
Response via : Initial Calibration

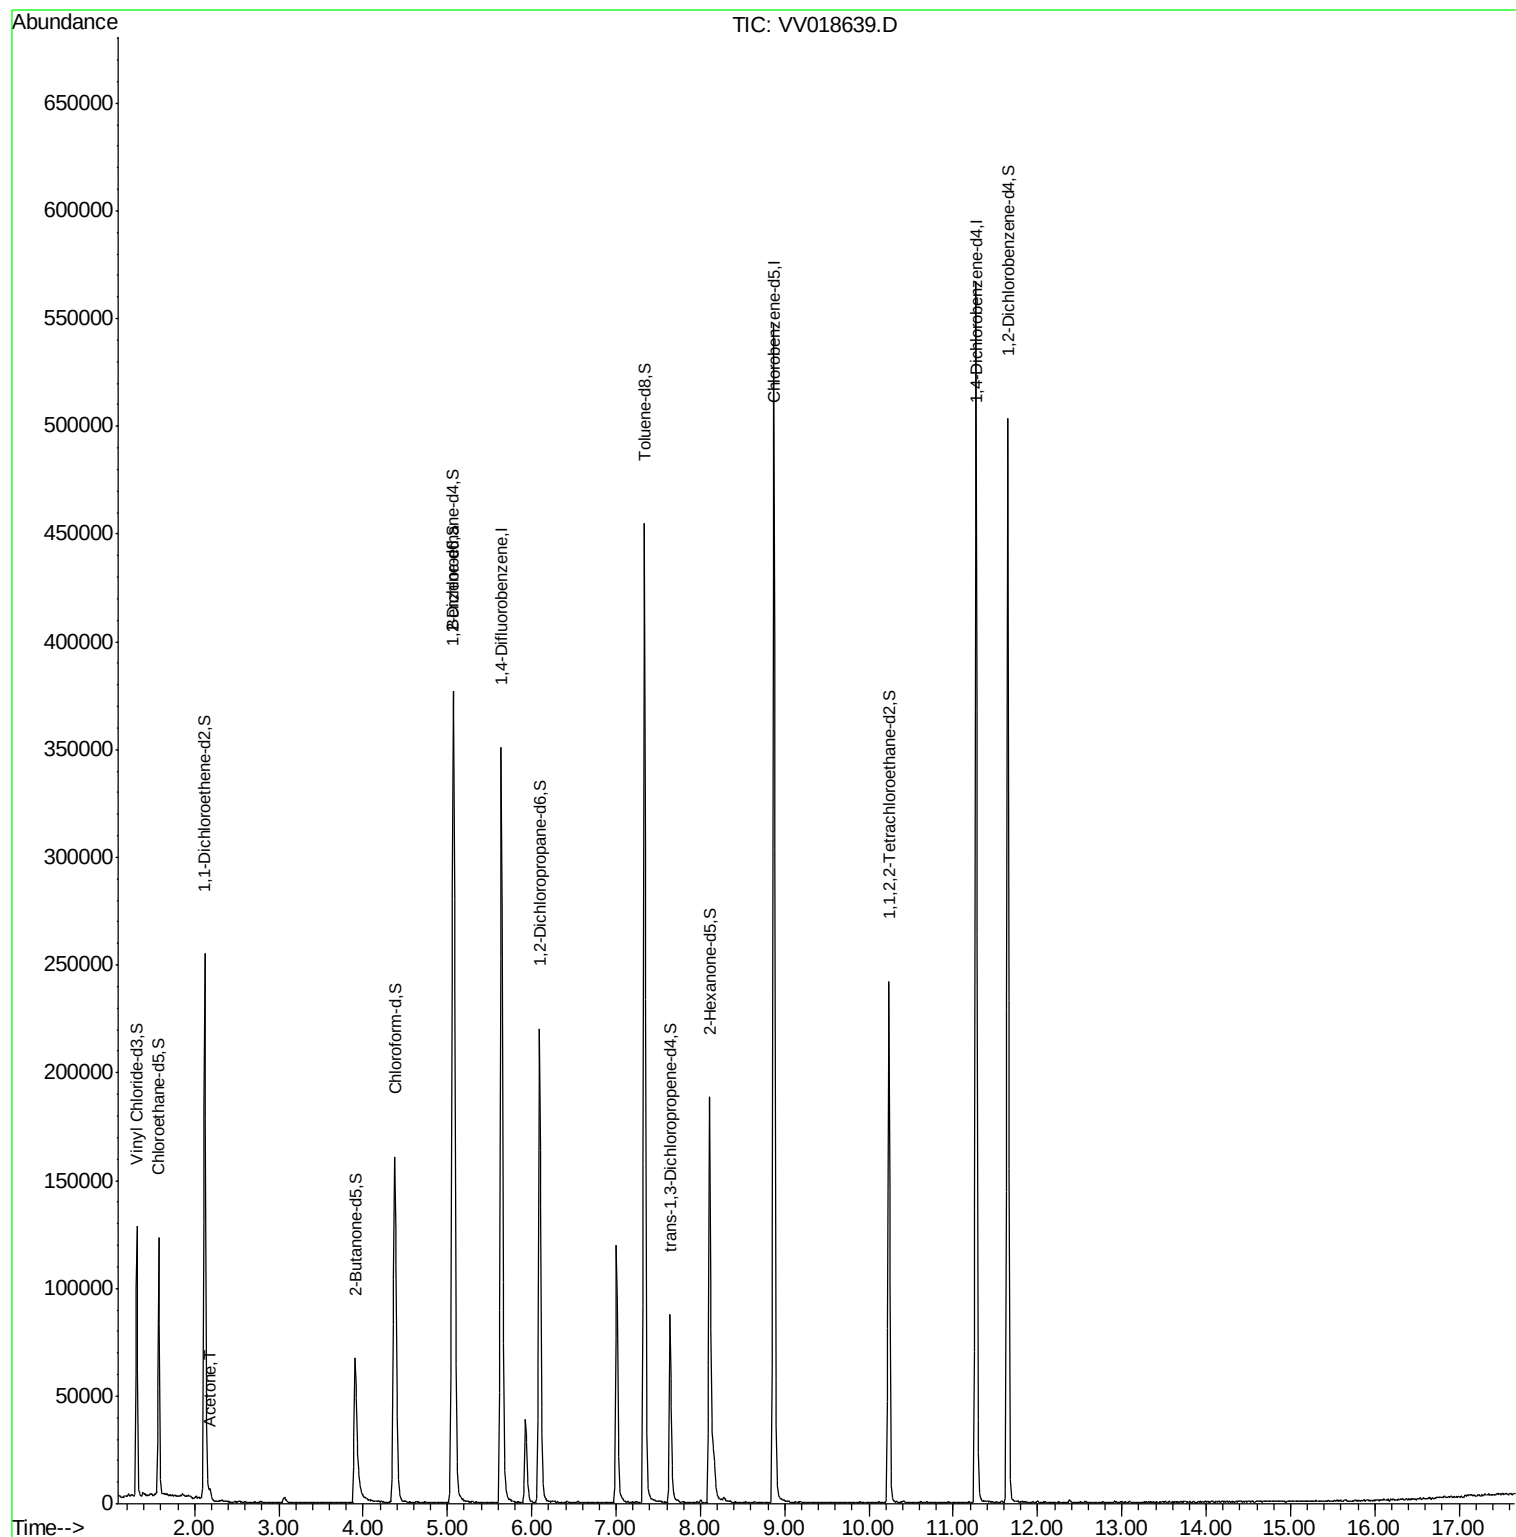

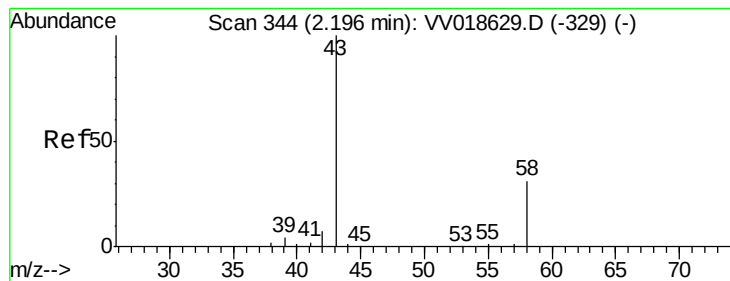

#13
 Acetone
 Concen: 4.273 ug/L
 RT: 2.18 min Scan# 340
 Delta R.T. -0.01 min
 Lab File: VV018639.D
 Acq: 02 Oct 2020 20:45

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3R8

Tot Ion: 43 Resp: 4833
 Ion Ratio Lower Upper
 43 100
 58 28.1 0.0 64.0

