

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100220\
 Data File : VV018631.D
 Acq On : 02 Oct 2020 17:36
 Operator : SY/MD
 Sample : L4237-01DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AB6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	87	rVB	134738	137174	13.44%	1.461%
2	1.579	144	152	165	rBV	130070	150027	14.70%	1.598%
3	2.122	311	321	344	rBV	267546	395805	38.78%	4.215%
4	2.267	364	366	369	rBV	446	257	0.03%	0.003%
5	2.399	404	407	410	rBV	447	328	0.03%	0.003%
6	2.524	440	446	452	rBV3	1778	2612	0.26%	0.028%
7	2.646	481	484	488	rVB	442	256	0.03%	0.003%
8	2.724	506	508	513	rBV	275	240	0.02%	0.003%
9	2.769	518	522	523	rBV2	410	275	0.03%	0.003%
10	2.933	572	573	579	rVB	226	134	0.01%	0.001%
11	3.055	605	611	612	rBV3	1061	892	0.09%	0.009%
12	3.151	639	641	645	rVB2	205	120	0.01%	0.001%
13	3.347	701	702	705	rVB	205	102	0.01%	0.001%
14	3.379	709	712	716	rVB	224	147	0.01%	0.002%
15	3.428	720	727	728	rBV2	211	207	0.02%	0.002%
16	3.502	748	750	752	rVB2	228	109	0.01%	0.001%
17	3.550	761	765	767	rBV2	139	121	0.01%	0.001%
18	3.566	767	770	774	rBV2	248	146	0.01%	0.002%
19	3.720	815	818	820	rBV	332	200	0.02%	0.002%
20	3.797	839	842	846	rVB2	198	147	0.01%	0.002%
21	3.830	846	852	857	rBV2	392	436	0.04%	0.005%
22	3.920	869	880	926	rBV	61561	209744	20.55%	2.234%
23	4.209	968	970	974	rVB3	457	294	0.03%	0.003%
24	4.376	1005	1022	1053	rBV	166546	414087	40.57%	4.410%
25	4.534	1068	1071	1074	rBV2	300	207	0.02%	0.002%
26	4.592	1088	1089	1094	rVB2	235	123	0.01%	0.001%
27	4.617	1094	1097	1101	rVB3	229	177	0.02%	0.002%
28	4.643	1101	1105	1107	rBV2	401	354	0.03%	0.004%
29	4.730	1129	1132	1135	rBV2	307	170	0.02%	0.002%
30	4.923	1189	1192	1197	rVB2	185	139	0.01%	0.001%
31	4.994	1210	1214	1220	rBV3	253	337	0.03%	0.004%
32	5.071	1220	1238	1265	rBV2	396012	1020564	100.00%	10.868%
33	5.428	1347	1349	1352	rBV	209	105	0.01%	0.001%
34	5.441	1352	1353	1356	rVB	391	149	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100220\
 Data File : VV018631.D
 Acq On : 02 Oct 2020 17:36
 Operator : SY/MD
 Sample : L4237-01DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleID :
 E0AB6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

35	5.508	1371	1374	1375	rBV	218	108	0.01%	0.001%
36	5.640	1401	1415	1444	rBV	388407	768393	75.29%	8.183%
37	5.936	1493	1507	1536	rBV2	509299	1017107	99.66%	10.831%
38	6.093	1543	1556	1581	rBV	227011	457763	44.85%	4.875%
39	6.190	1585	1586	1587	rBV	397	143	0.01%	0.002%
40	6.270	1609	1611	1615	rVB2	750	360	0.04%	0.004%
41	6.293	1615	1618	1621	rVB2	439	251	0.02%	0.003%
42	6.309	1621	1623	1629	rVB2	381	279	0.03%	0.003%
43	6.347	1629	1635	1636	rBV2	150	112	0.01%	0.001%
44	6.363	1638	1640	1643	rVB2	215	120	0.01%	0.001%
45	6.399	1648	1651	1654	rBV2	211	158	0.02%	0.002%
46	6.653	1726	1730	1731	rBV	293	201	0.02%	0.002%
47	6.749	1758	1760	1763	rVB	348	164	0.02%	0.002%
48	6.772	1763	1767	1771	rBV	221	204	0.02%	0.002%
49	6.817	1780	1781	1784	rBV2	238	139	0.01%	0.001%
50	6.916	1810	1812	1814	rBV	220	104	0.01%	0.001%
51	7.006	1829	1840	1867	rBV	133587	236504	23.17%	2.519%
52	7.202	1899	1901	1903	rVB	423	161	0.02%	0.002%
53	7.231	1906	1910	1913	rVV3	801	575	0.06%	0.006%
54	7.338	1931	1943	1965	rBV	484077	833117	81.63%	8.872%
55	7.592	2020	2022	2026	rBV	399	288	0.03%	0.003%
56	7.643	2026	2038	2061	rBV	93559	164556	16.12%	1.752%
57	7.810	2087	2090	2094	rBV2	558	377	0.04%	0.004%
58	7.881	2102	2112	2115	rBV2	246	434	0.04%	0.005%
59	7.942	2128	2131	2134	rBV	415	332	0.03%	0.004%
60	7.997	2144	2148	2159	rBV4	862	1283	0.13%	0.014%
61	8.038	2159	2161	2164	rVB2	248	137	0.01%	0.001%
62	8.109	2173	2183	2219	rBV2	198926	396995	38.90%	4.228%
63	8.563	2322	2324	2325	rBV	244	106	0.01%	0.001%
64	8.585	2329	2331	2332	rBV2	297	126	0.01%	0.001%
65	8.772	2387	2389	2392	rVB	286	111	0.01%	0.001%
66	8.794	2392	2396	2400	rBV2	232	204	0.02%	0.002%
67	8.871	2409	2420	2446	rBV	593078	955576	93.63%	10.176%
68	9.096	2489	2490	2493	rVB	342	125	0.01%	0.001%
69	9.116	2493	2496	2499	rBV2	443	280	0.03%	0.003%
70	9.289	2546	2550	2555	rBV2	240	179	0.02%	0.002%
71	9.321	2557	2560	2562	rBV2	240	122	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100220\
 Data File : VV018631.D
 Acq On : 02 Oct 2020 17:36
 Operator : SY/MD
 Sample : L4237-01DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AB6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

72	9.373	2573	2576	2578	rVV2	351	162	0.02%	0.002%
73	9.434	2590	2595	2597	rBV2	297	294	0.03%	0.003%
74	9.540	2625	2628	2635	rBV2	360	375	0.04%	0.004%
75	9.572	2635	2638	2640	rVV2	315	184	0.02%	0.002%
76	9.636	2655	2658	2667	rVV	290	244	0.02%	0.003%
77	9.678	2668	2671	2673	rVB	232	130	0.01%	0.001%
78	9.939	2749	2752	2753	rBV	266	143	0.01%	0.002%
79	10.238	2833	2845	2864	rBV	268971	417754	40.93%	4.449%
80	10.360	2881	2883	2885	rBV2	294	138	0.01%	0.001%
81	10.562	2944	2946	2948	rBV	357	182	0.02%	0.002%
82	10.601	2954	2958	2963	rVB4	1186	1145	0.11%	0.012%
83	10.897	3047	3050	3053	rBV2	298	171	0.02%	0.002%
84	10.939	3059	3063	3064	rBV2	332	256	0.03%	0.003%
85	10.993	3078	3080	3083	rBV	205	105	0.01%	0.001%
86	11.206	3143	3146	3148	rBV2	348	185	0.02%	0.002%
87	11.270	3154	3166	3186	rBV	632560	960834	94.15%	10.232%
88	11.482	3229	3232	3233	rBV	228	133	0.01%	0.001%
89	11.582	3262	3263	3265	rBV	315	147	0.01%	0.002%
90	11.646	3271	3283	3300	rBV	533673	830795	81.41%	8.847%
91	11.807	3326	3333	3335	rBV4	1459	1529	0.15%	0.016%
92	12.177	3445	3448	3451	rBV	402	231	0.02%	0.002%
93	12.222	3460	3462	3463	rBV	320	114	0.01%	0.001%
94	12.427	3524	3526	3528	rBV2	197	130	0.01%	0.001%
95	12.437	3528	3529	3533	rVV2	218	104	0.01%	0.001%
96	12.508	3548	3551	3552	rBV	196	128	0.01%	0.001%
97	12.591	3575	3577	3583	rBV2	212	115	0.01%	0.001%
98	13.070	3723	3726	3728	rBV	243	142	0.01%	0.002%
99	13.778	3939	3946	3950	rBV2	591	824	0.08%	0.009%
100	14.578	4192	4195	4200	rBV2	564	501	0.05%	0.005%


Sum of corrected areas: 9390574

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100220\
Data File : VV018631.D
Acq On : 02 Oct 2020 17:36
Operator : SY/MD
Sample : L4237-01DL 5X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
E0AB6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

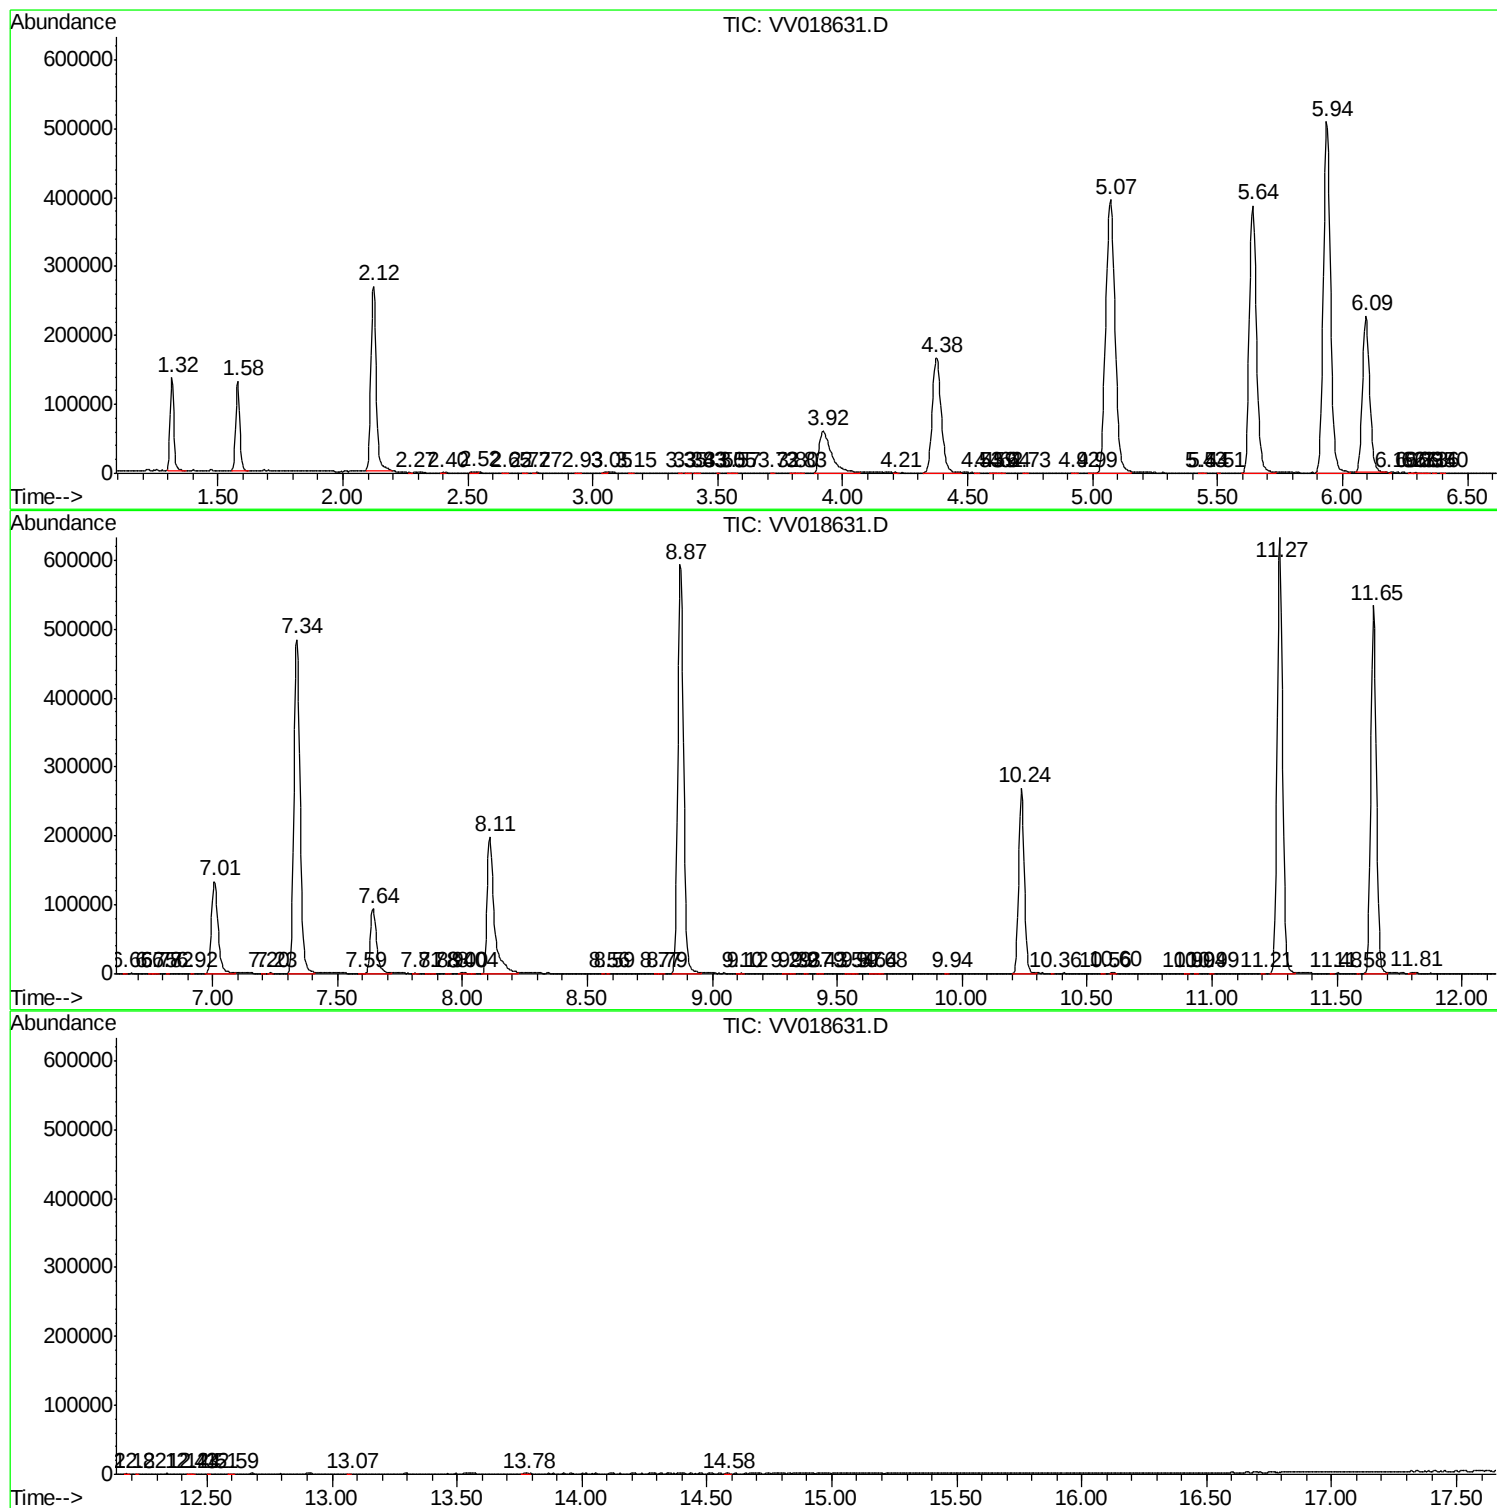

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV100220\
Data File : VV018631.D
Acq On : 02 Oct 2020 17:36
Operator : SY/MD
Sample : L4237-01DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AB6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV100220\
Data File : VV018631.D
Acq On : 02 Oct 2020 17:36
Operator : SY/MD
Sample : L4237-01DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AB6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc