

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100220\
 Data File : VV018632.D
 Acq On : 02 Oct 2020 18:00
 Operator : SY/MD
 Sample : L4237-02DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AB7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	85	rVB	132079	133859	13.39%	1.503%
2	1.579	145	152	165	rVB	125981	145126	14.52%	1.630%
3	2.123	312	321	353	rVB	266989	413151	41.32%	4.640%
4	2.377	397	400	406	rBV3	460	474	0.05%	0.005%
5	2.711	502	504	507	rBV	146	72	0.01%	0.001%
6	2.762	518	520	521	rBV	186	46	0.00%	0.001%
7	2.772	521	523	525	rBV2	695	455	0.05%	0.005%
8	2.820	536	538	542	rBV	151	63	0.01%	0.001%
9	2.910	563	566	570	rVB	267	185	0.02%	0.002%
10	2.939	570	575	577	rBV	197	156	0.02%	0.002%
11	2.975	584	586	589	rVB	225	113	0.01%	0.001%
12	3.145	637	639	643	rBV2	183	144	0.01%	0.002%
13	3.164	643	645	647	rVV	183	79	0.01%	0.001%
14	3.286	677	683	686	rBV2	341	375	0.04%	0.004%
15	3.412	717	722	724	rBV2	231	231	0.02%	0.003%
16	3.450	730	734	736	rVB	209	126	0.01%	0.001%
17	3.463	736	738	740	rBV	178	93	0.01%	0.001%
18	3.579	770	774	776	rBV2	334	206	0.02%	0.002%
19	3.643	788	794	795	rBV	174	141	0.01%	0.002%
20	3.785	833	838	839	rBV2	469	291	0.03%	0.003%
21	3.836	852	854	857	rBV	152	110	0.01%	0.001%
22	3.917	868	879	916	rBV	63778	195838	19.59%	2.200%
23	4.376	1005	1022	1051	rBV	162962	406732	40.68%	4.568%
24	4.605	1090	1093	1099	rBV4	304	352	0.04%	0.004%
25	4.820	1158	1160	1162	rBV	227	93	0.01%	0.001%
26	4.833	1162	1164	1166	rVV2	171	59	0.01%	0.001%
27	5.071	1221	1238	1267	rBV2	390431	999793	100.00%	11.229%
28	5.312	1310	1313	1315	rBV3	251	178	0.02%	0.002%
29	5.364	1326	1329	1331	rVB2	269	130	0.01%	0.001%
30	5.380	1331	1334	1338	rBV	263	191	0.02%	0.002%
31	5.482	1359	1366	1368	rBV	432	411	0.04%	0.005%
32	5.537	1381	1383	1387	rVB	321	146	0.01%	0.002%
33	5.582	1395	1397	1403	rBV3	189	154	0.02%	0.002%
34	5.640	1403	1415	1440	rBV	370680	740448	74.06%	8.316%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100220\
 Data File : VV018632.D
 Acq On : 02 Oct 2020 18:00
 Operator : SY/MD
 Sample : L4237-02DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AB7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

35	5.936	1493	1507	1535	rBV2	371009	743477	74.36%	8.350%
36	6.093	1543	1556	1584	rBV	225821	449455	44.95%	5.048%
37	6.206	1589	1591	1593	rBV2	417	255	0.03%	0.003%
38	6.283	1612	1615	1618	rVB3	483	272	0.03%	0.003%
39	6.318	1624	1626	1627	rBV2	148	71	0.01%	0.001%
40	6.399	1648	1651	1652	rBV	222	125	0.01%	0.001%
41	6.457	1667	1669	1670	rBV	197	92	0.01%	0.001%
42	6.592	1709	1711	1715	rBV2	215	118	0.01%	0.001%
43	6.669	1732	1735	1739	rVB2	353	230	0.02%	0.003%
44	6.720	1748	1751	1755	rBV2	292	168	0.02%	0.002%
45	6.769	1763	1766	1769	rBV2	291	159	0.02%	0.002%
46	6.891	1802	1804	1807	rBV	192	119	0.01%	0.001%
47	6.907	1807	1809	1813	rVV2	159	97	0.01%	0.001%
48	6.962	1823	1826	1830	rBV	319	272	0.03%	0.003%
49	7.007	1830	1840	1863	rBV	128185	230630	23.07%	2.590%
50	7.257	1915	1918	1920	rVB	294	176	0.02%	0.002%
51	7.273	1920	1923	1928	rBV	279	202	0.02%	0.002%
52	7.338	1930	1943	1969	rBV	475919	809357	80.95%	9.090%
53	7.643	2027	2038	2060	rBV	92294	160094	16.01%	1.798%
54	7.897	2114	2117	2120	rBV2	233	125	0.01%	0.001%
55	7.955	2132	2135	2140	rBV3	440	379	0.04%	0.004%
56	8.000	2143	2149	2157	rVV4	1824	2481	0.25%	0.028%
57	8.039	2159	2161	2164	rBV	129	102	0.01%	0.001%
58	8.109	2173	2183	2217	rBV3	193862	391857	39.19%	4.401%
59	8.553	2317	2321	2324	rBV2	285	186	0.02%	0.002%
60	8.627	2342	2344	2346	rBV	92	59	0.01%	0.001%
61	8.871	2408	2420	2443	rBV	576976	931995	93.22%	10.468%
62	9.068	2480	2481	2484	rBV2	250	126	0.01%	0.001%
63	9.402	2582	2585	2587	rBV	185	143	0.01%	0.002%
64	9.463	2601	2604	2607	rBV	233	144	0.01%	0.002%
65	10.077	2790	2795	2799	rVB2	421	388	0.04%	0.004%
66	10.100	2800	2802	2806	rBV	249	133	0.01%	0.001%
67	10.180	2823	2827	2831	rBV2	219	224	0.02%	0.003%
68	10.235	2832	2844	2869	rVV	260732	414234	41.43%	4.653%
69	10.325	2869	2872	2874	rVV	226	126	0.01%	0.001%
70	10.521	2929	2933	2938	rBV2	240	272	0.03%	0.003%
71	10.547	2938	2941	2945	rVB	346	234	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100220\
 Data File : VV018632.D
 Acq On : 02 Oct 2020 18:00
 Operator : SY/MD
 Sample : L4237-02DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AB7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

72	10.576	2945	2950	2952	rBV2	325	254	0.03%	0.003%
73	10.707	2989	2991	2992	rBV2	219	81	0.01%	0.001%
74	10.865	3037	3040	3042	rBV2	278	163	0.02%	0.002%
75	10.932	3059	3061	3062	rBV	252	82	0.01%	0.001%
76	11.010	3082	3085	3087	rBV	290	211	0.02%	0.002%
77	11.180	3135	3138	3143	rBV3	332	282	0.03%	0.003%
78	11.215	3147	3149	3154	rVB	274	139	0.01%	0.002%
79	11.270	3154	3166	3187	rBV	608565	917842	91.80%	10.309%
80	11.447	3219	3221	3224	rBV	250	121	0.01%	0.001%
81	11.646	3271	3283	3303	rBV	513911	802609	80.28%	9.015%
82	11.813	3330	3335	3342	rVB4	1322	1329	0.13%	0.015%
83	11.971	3379	3384	3389	rBV2	258	308	0.03%	0.003%
84	12.093	3420	3422	3425	rBV	270	181	0.02%	0.002%
85	12.157	3439	3442	3443	rBV	322	168	0.02%	0.002%
86	12.376	3508	3510	3511	rBV	213	74	0.01%	0.001%
87	13.289	3792	3794	3798	rBV2	326	252	0.03%	0.003%
88	13.910	3985	3987	3991	rBV3	266	181	0.02%	0.002%
89	14.910	4294	4298	4302	rBV3	542	532	0.05%	0.006%


Sum of corrected areas: 8903407

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100220\
Data File : VV018632.D
Acq On : 02 Oct 2020 18:00
Operator : SY/MD
Sample : L4237-02DL 5X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AB7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

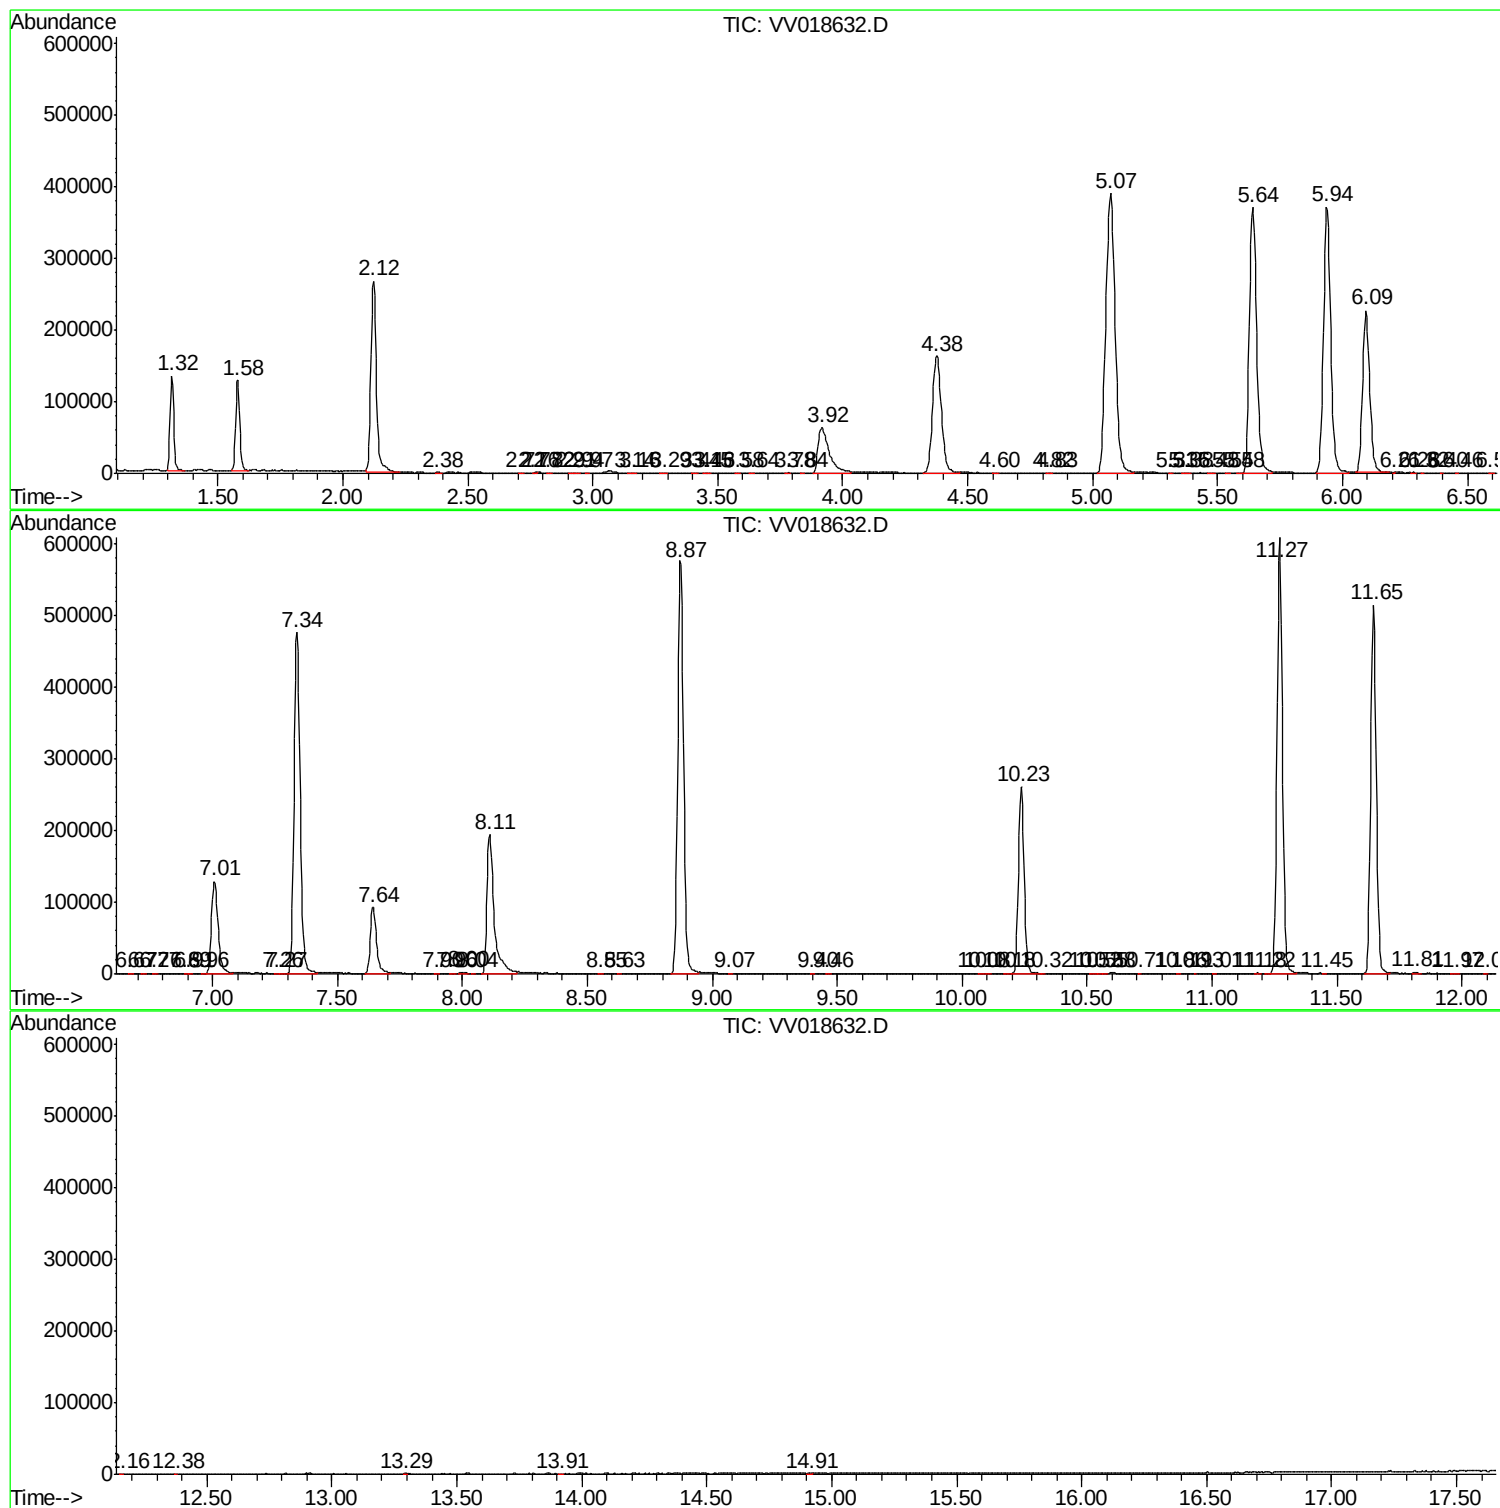

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV100220\
Data File : VV018632.D
Acq On : 02 Oct 2020 18:00
Operator : SY/MD
Sample : L4237-02DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AB7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV100220\
Data File : VV018632.D
Acq On : 02 Oct 2020 18:00
Operator : SY/MD
Sample : L4237-02DL 5X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
E0AB7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc