

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100220\
 Data File : VV018634.D
 Acq On : 02 Oct 2020 18:47
 Operator : SY/MD
 Sample : L4237-05DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0ACODL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	63	70	83	rBV	138891	134436	13.01%	1.438%
2	1.579	145	152	163	rVB	126839	142891	13.83%	1.529%
3	2.123	311	321	353	rVB	267065	413454	40.02%	4.424%
4	2.528	440	447	453	rBV5	1781	2510	0.24%	0.027%
5	2.743	513	514	515	rBV5	139	33	0.00%	0.000%
6	2.869	549	553	554	rBV	218	163	0.02%	0.002%
7	2.965	581	583	584	rBV	157	50	0.00%	0.001%
8	3.061	606	613	627	rVB6	2999	5383	0.52%	0.058%
9	3.168	643	646	647	rBV	115	66	0.01%	0.001%
10	3.415	718	723	726	rBV	388	396	0.04%	0.004%
11	3.614	779	785	791	rBV2	253	336	0.03%	0.004%
12	3.669	799	802	804	rBV2	191	143	0.01%	0.002%
13	3.913	867	878	918	rBV2	66297	212899	20.61%	2.278%
14	4.377	1004	1022	1045	rBV	168049	413686	40.04%	4.426%
15	4.743	1133	1136	1138	rBV	241	163	0.02%	0.002%
16	4.804	1152	1155	1156	rBV	190	98	0.01%	0.001%
17	4.894	1181	1183	1185	rBV	193	98	0.01%	0.001%
18	5.071	1221	1238	1264	rBV2	400268	1019139	98.64%	10.904%
19	5.360	1324	1328	1330	rVB2	300	245	0.02%	0.003%
20	5.380	1330	1334	1337	rBV2	413	245	0.02%	0.003%
21	5.486	1364	1367	1372	rVB	11570	6621	0.64%	0.071%
22	5.521	1377	1378	1379	rBV	203	57	0.01%	0.001%
23	5.640	1402	1415	1447	rBV	378568	751624	72.75%	8.042%
24	5.862	1482	1484	1485	rBV2	174	76	0.01%	0.001%
25	5.881	1489	1490	1493	rVB2	289	68	0.01%	0.001%
26	5.936	1493	1507	1533	rBV2	515672	1033230	100.00%	11.055%
27	6.093	1544	1556	1587	rVB	229220	463695	44.88%	4.961%
28	6.296	1617	1619	1623	rBV2	417	301	0.03%	0.003%
29	6.598	1711	1713	1714	rBV	256	114	0.01%	0.001%
30	6.637	1724	1725	1726	rBV	103	20	0.00%	0.000%
31	6.672	1732	1736	1740	rBV2	380	416	0.04%	0.004%
32	6.708	1744	1747	1751	rBV2	446	306	0.03%	0.003%
33	6.791	1770	1773	1776	rBV2	183	133	0.01%	0.001%
34	6.952	1819	1823	1828	rBV2	209	273	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100220\
 Data File : VV018634.D
 Acq On : 02 Oct 2020 18:47
 Operator : SY/MD
 Sample : L4237-05DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0ACODL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

35	7.007	1828	1840	1857	rBV	126921	229818	22.24%	2.459%
36	7.228	1907	1909	1913	rBV3	302	201	0.02%	0.002%
37	7.338	1930	1943	1968	rBV	475823	827137	80.05%	8.850%
38	7.643	2028	2038	2061	rBV	93620	164286	15.90%	1.758%
39	7.814	2088	2091	2094	rVB	495	290	0.03%	0.003%
40	8.003	2143	2150	2159	rVB3	1445	1977	0.19%	0.021%
41	8.074	2170	2172	2173	rBV3	292	103	0.01%	0.001%
42	8.109	2173	2183	2223	rVV2	201959	403766	39.08%	4.320%
43	8.383	2266	2268	2270	rBV	256	117	0.01%	0.001%
44	8.421	2278	2280	2283	rBV2	279	163	0.02%	0.002%
45	8.502	2302	2305	2307	rBV2	358	261	0.03%	0.003%
46	8.550	2317	2320	2323	rBV	357	284	0.03%	0.003%
47	8.630	2338	2345	2347	rBV	269	296	0.03%	0.003%
48	8.666	2354	2356	2358	rBV	141	61	0.01%	0.001%
49	8.753	2378	2383	2385	rBV2	311	233	0.02%	0.002%
50	8.781	2389	2392	2394	rBV	291	186	0.02%	0.002%
51	8.871	2408	2420	2442	rBV	582449	940931	91.07%	10.067%
52	9.058	2476	2478	2480	rBV	208	78	0.01%	0.001%
53	9.116	2494	2496	2498	rBV	317	140	0.01%	0.001%
54	9.241	2529	2535	2536	rBV2	320	249	0.02%	0.003%
55	9.283	2545	2548	2549	rBV2	144	66	0.01%	0.001%
56	9.473	2605	2607	2608	rBV2	159	71	0.01%	0.001%
57	9.502	2612	2616	2619	rBV3	200	185	0.02%	0.002%
58	9.588	2641	2643	2645	rBV	125	53	0.01%	0.001%
59	9.769	2697	2699	2701	rBV2	248	114	0.01%	0.001%
60	9.794	2705	2707	2708	rBV2	192	89	0.01%	0.001%
61	9.814	2712	2713	2716	rVB2	287	81	0.01%	0.001%
62	10.045	2782	2785	2786	rBV	148	92	0.01%	0.001%
63	10.190	2828	2830	2832	rVB2	215	63	0.01%	0.001%
64	10.238	2833	2845	2861	rBV	265795	417866	40.44%	4.471%
65	10.354	2878	2881	2882	rBV	294	158	0.02%	0.002%
66	10.437	2905	2907	2909	rBV	198	101	0.01%	0.001%
67	10.621	2962	2964	2969	rBV2	161	135	0.01%	0.001%
68	10.994	3078	3080	3082	rBV	196	66	0.01%	0.001%
69	11.058	3097	3100	3101	rBV	217	99	0.01%	0.001%
70	11.119	3113	3119	3123	rBV2	279	335	0.03%	0.004%
71	11.270	3154	3166	3197	rBV	611448	927048	89.72%	9.919%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100220\
 Data File : VV018634.D
 Acq On : 02 Oct 2020 18:47
 Operator : SY/MD
 Sample : L4237-05DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC0DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

72	11.392	3199	3204	3205	rBV3	580	437	0.04%	0.005%
73	11.405	3205	3208	3212	rVB2	612	359	0.03%	0.004%
74	11.646	3271	3283	3306	rBV	527338	822463	79.60%	8.800%
75	11.810	3329	3334	3340	rBV4	1254	1450	0.14%	0.016%
76	11.833	3340	3341	3342	rBV4	205	62	0.01%	0.001%
77	11.891	3357	3359	3362	rBV2	245	121	0.01%	0.001%
78	12.164	3442	3444	3448	rVB	266	148	0.01%	0.002%
79	12.807	3640	3644	3646	rBV2	440	309	0.03%	0.003%
80	12.897	3669	3672	3673	rBV2	267	140	0.01%	0.001%
81	14.013	4015	4019	4022	rBV	312	251	0.02%	0.003%


Sum of corrected areas: 9346307

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100220\
Data File : VV018634.D
Acq On : 02 Oct 2020 18:47
Operator : SY/MD
Sample : L4237-05DL 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0ACODL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

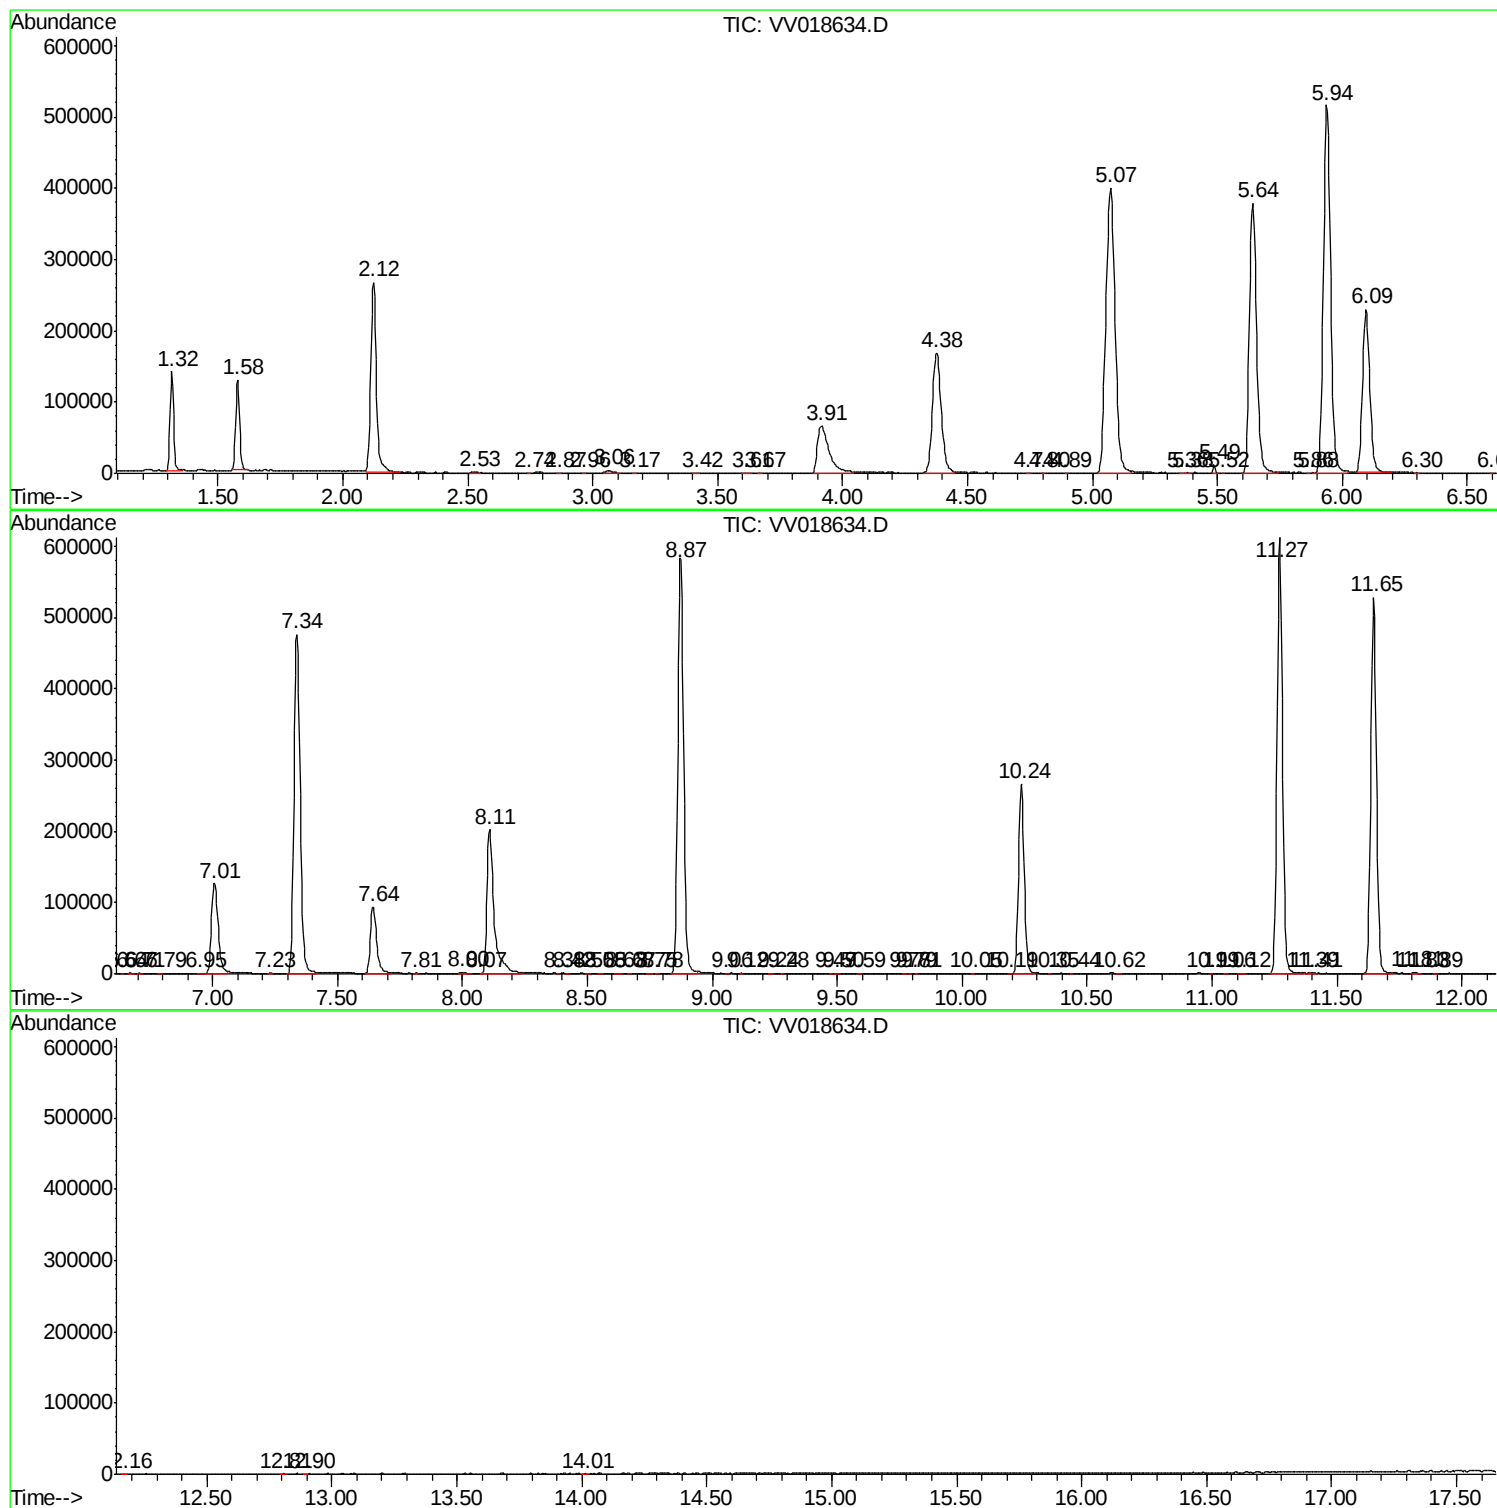

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV100220\
Data File : VV018634.D
Acq On : 02 Oct 2020 18:47
Operator : SY/MD
Sample : L4237-05DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC0DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV100220\
Data File : VV018634.D
Acq On : 02 Oct 2020 18:47
Operator : SY/MD
Sample : L4237-05DL 10X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
E0AC0DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc