

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100220\
 Data File : VV018636.D
 Acq On : 02 Oct 2020 19:34
 Operator : SY/MD
 Sample : L4237-10DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	81	rBV	131621	127667	11.04%	1.376%
2	1.579	144	152	167	rBV	124744	144058	12.46%	1.553%
3	2.122	311	321	351	rVB	263283	402843	34.84%	4.343%
4	2.351	389	392	393	rBV	355	199	0.02%	0.002%
5	2.528	440	447	460	rVB6	2183	3774	0.33%	0.041%
6	2.637	476	481	487	rVB3	627	740	0.06%	0.008%
7	2.772	519	523	524	rBV2	432	303	0.03%	0.003%
8	2.833	539	542	548	rBV2	199	258	0.02%	0.003%
9	2.962	580	582	588	rVB	475	380	0.03%	0.004%
10	2.997	588	593	597	rBV2	389	465	0.04%	0.005%
11	3.061	601	613	626	rBV6	2716	5857	0.51%	0.063%
12	3.315	687	692	693	rBV2	247	161	0.01%	0.002%
13	3.402	715	719	725	rVB2	255	245	0.02%	0.003%
14	3.634	787	791	794	rBV2	174	167	0.01%	0.002%
15	3.656	794	798	802	rVB2	181	207	0.02%	0.002%
16	3.920	869	880	916	rBV	61951	207126	17.91%	2.233%
17	4.376	1004	1022	1053	rBV	165733	404591	34.99%	4.362%
18	4.502	1058	1061	1065	rVV	446	353	0.03%	0.004%
19	4.560	1076	1079	1083	rVB2	603	492	0.04%	0.005%
20	4.685	1115	1118	1121	rBV	436	278	0.02%	0.003%
21	4.769	1141	1144	1148	rVB2	350	251	0.02%	0.003%
22	5.071	1220	1238	1264	rBV2	389737	994089	85.98%	10.717%
23	5.360	1325	1328	1330	rBV	258	204	0.02%	0.002%
24	5.396	1337	1339	1346	rVB3	495	554	0.05%	0.006%
25	5.441	1346	1353	1358	rBV4	785	1054	0.09%	0.011%
26	5.518	1374	1377	1382	rVB	469	317	0.03%	0.003%
27	5.598	1399	1402	1403	rBV	297	154	0.01%	0.002%
28	5.640	1403	1415	1443	rVV	366068	728235	62.99%	7.851%
29	5.936	1491	1507	1540	rBV	581135	1156187	100.00%	12.464%
30	6.093	1543	1556	1576	rBV	224344	446575	38.62%	4.814%
31	6.232	1596	1599	1602	rVB3	819	502	0.04%	0.005%
32	6.296	1617	1619	1624	rVB	475	310	0.03%	0.003%
33	6.605	1710	1715	1719	rBV2	257	288	0.02%	0.003%
34	6.627	1719	1722	1727	rVV2	231	203	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100220\
 Data File : VV018636.D
 Acq On : 02 Oct 2020 19:34
 Operator : SY/MD
 Sample : L4237-10DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

35	6.672	1734	1736	1738	rBV	277	154	0.01%	0.002%
36	6.814	1774	1780	1781	rBV	323	227	0.02%	0.002%
37	7.006	1829	1840	1861	rBV	123813	224451	19.41%	2.420%
38	7.225	1905	1908	1914	rBV3	427	366	0.03%	0.004%
39	7.338	1929	1943	1969	rBV	479929	810282	70.08%	8.735%
40	7.643	2027	2038	2059	rBV	93123	157804	13.65%	1.701%
41	7.842	2095	2100	2102	rBV3	487	386	0.03%	0.004%
42	7.997	2144	2148	2150	rBV3	1160	949	0.08%	0.010%
43	8.035	2156	2160	2164	rBV2	163	165	0.01%	0.002%
44	8.109	2171	2183	2220	rBV2	200546	403259	34.88%	4.347%
45	8.373	2262	2265	2267	rBV	638	245	0.02%	0.003%
46	8.476	2293	2297	2300	rVB	475	371	0.03%	0.004%
47	8.595	2330	2334	2336	rVB2	423	241	0.02%	0.003%
48	8.871	2408	2420	2452	rBV	569210	926974	80.18%	9.993%
49	9.103	2489	2492	2496	rBV3	277	242	0.02%	0.003%
50	9.248	2534	2537	2542	rBV	404	339	0.03%	0.004%
51	9.379	2574	2578	2581	rBV2	490	290	0.03%	0.003%
52	9.569	2634	2637	2642	rBV	237	232	0.02%	0.003%
53	9.640	2655	2659	2663	rBV2	280	197	0.02%	0.002%
54	9.675	2665	2670	2674	rBV2	188	194	0.02%	0.002%
55	9.698	2674	2677	2681	rBV	272	193	0.02%	0.002%
56	9.900	2737	2740	2743	rVV2	276	156	0.01%	0.002%
57	10.058	2787	2789	2794	rVB2	279	197	0.02%	0.002%
58	10.154	2815	2819	2822	rBV2	278	256	0.02%	0.003%
59	10.238	2833	2845	2865	rBV	256878	408464	35.33%	4.403%
60	10.386	2888	2891	2897	rVB	243	236	0.02%	0.003%
61	10.440	2902	2908	2909	rBV2	330	297	0.03%	0.003%
62	10.473	2915	2918	2921	rBV2	250	179	0.02%	0.002%
63	10.569	2945	2948	2952	rBV2	378	266	0.02%	0.003%
64	10.598	2955	2957	2960	rBV2	501	286	0.02%	0.003%
65	10.836	3026	3031	3033	rBV2	233	166	0.01%	0.002%
66	10.932	3056	3061	3062	rBV2	204	161	0.01%	0.002%
67	10.945	3062	3065	3075	rVB2	690	851	0.07%	0.009%
68	10.987	3075	3078	3079	rBV	235	158	0.01%	0.002%
69	11.270	3154	3166	3187	rBV	590291	903321	78.13%	9.738%
70	11.399	3203	3206	3208	rBV2	444	294	0.03%	0.003%
71	11.424	3211	3214	3220	rVB3	541	556	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100220\
 Data File : VV018636.D
 Acq On : 02 Oct 2020 19:34
 Operator : SY/MD
 Sample : L4237-10DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

72	11.460	3222	3225	3227	rVB	380	201	0.02%	0.002%
73	11.530	3244	3247	3251	rBV2	292	265	0.02%	0.003%
74	11.569	3256	3259	3262	rBV	171	170	0.01%	0.002%
75	11.646	3271	3283	3300	rBV	513759	795456	68.80%	8.575%
76	11.752	3314	3316	3320	rVB	508	281	0.02%	0.003%
77	11.804	3328	3332	3335	rBV2	575	524	0.05%	0.006%
78	11.817	3335	3336	3342	rVB	884	625	0.05%	0.007%
79	11.874	3352	3354	3357	rVB	347	162	0.01%	0.002%
80	12.334	3495	3497	3501	rVB	331	157	0.01%	0.002%
81	12.562	3565	3568	3569	rBV	278	166	0.01%	0.002%
82	12.636	3588	3591	3594	rBV	253	194	0.02%	0.002%
83	12.903	3669	3674	3675	rBV	525	304	0.03%	0.003%
84	13.273	3786	3789	3793	rVB2	234	174	0.02%	0.002%
85	13.308	3797	3800	3804	rVV	277	204	0.02%	0.002%
86	13.807	3953	3955	3961	rVB2	315	164	0.01%	0.002%
87	13.903	3982	3985	3990	rVV	411	432	0.04%	0.005%
88	14.058	4030	4033	4035	rBV2	314	209	0.02%	0.002%
89	14.074	4036	4038	4040	rVV	395	183	0.02%	0.002%
90	14.099	4042	4046	4049	rVB3	194	185	0.02%	0.002%
91	14.160	4062	4065	4068	rBV2	407	299	0.03%	0.003%
92	14.289	4102	4105	4107	rBV	289	178	0.02%	0.002%
93	14.566	4187	4191	4193	rBV2	373	334	0.03%	0.004%
94	14.582	4194	4196	4200	rVB3	331	236	0.02%	0.003%
95	15.183	4381	4383	4386	rBV	331	152	0.01%	0.002%
96	15.238	4398	4400	4404	rVB2	473	273	0.02%	0.003%
97	15.450	4464	4466	4469	rBV2	350	203	0.02%	0.002%
98	15.540	4492	4494	4497	rBV3	490	259	0.02%	0.003%
99	16.414	4761	4766	4767	rBV3	678	600	0.05%	0.006%
100	16.652	4837	4840	4844	rBV3	1075	1046	0.09%	0.011%


Sum of corrected areas: 9276128

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100220\
Data File : VV018636.D
Acq On : 02 Oct 2020 19:34
Operator : SY/MD
Sample : L4237-10DL 20X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

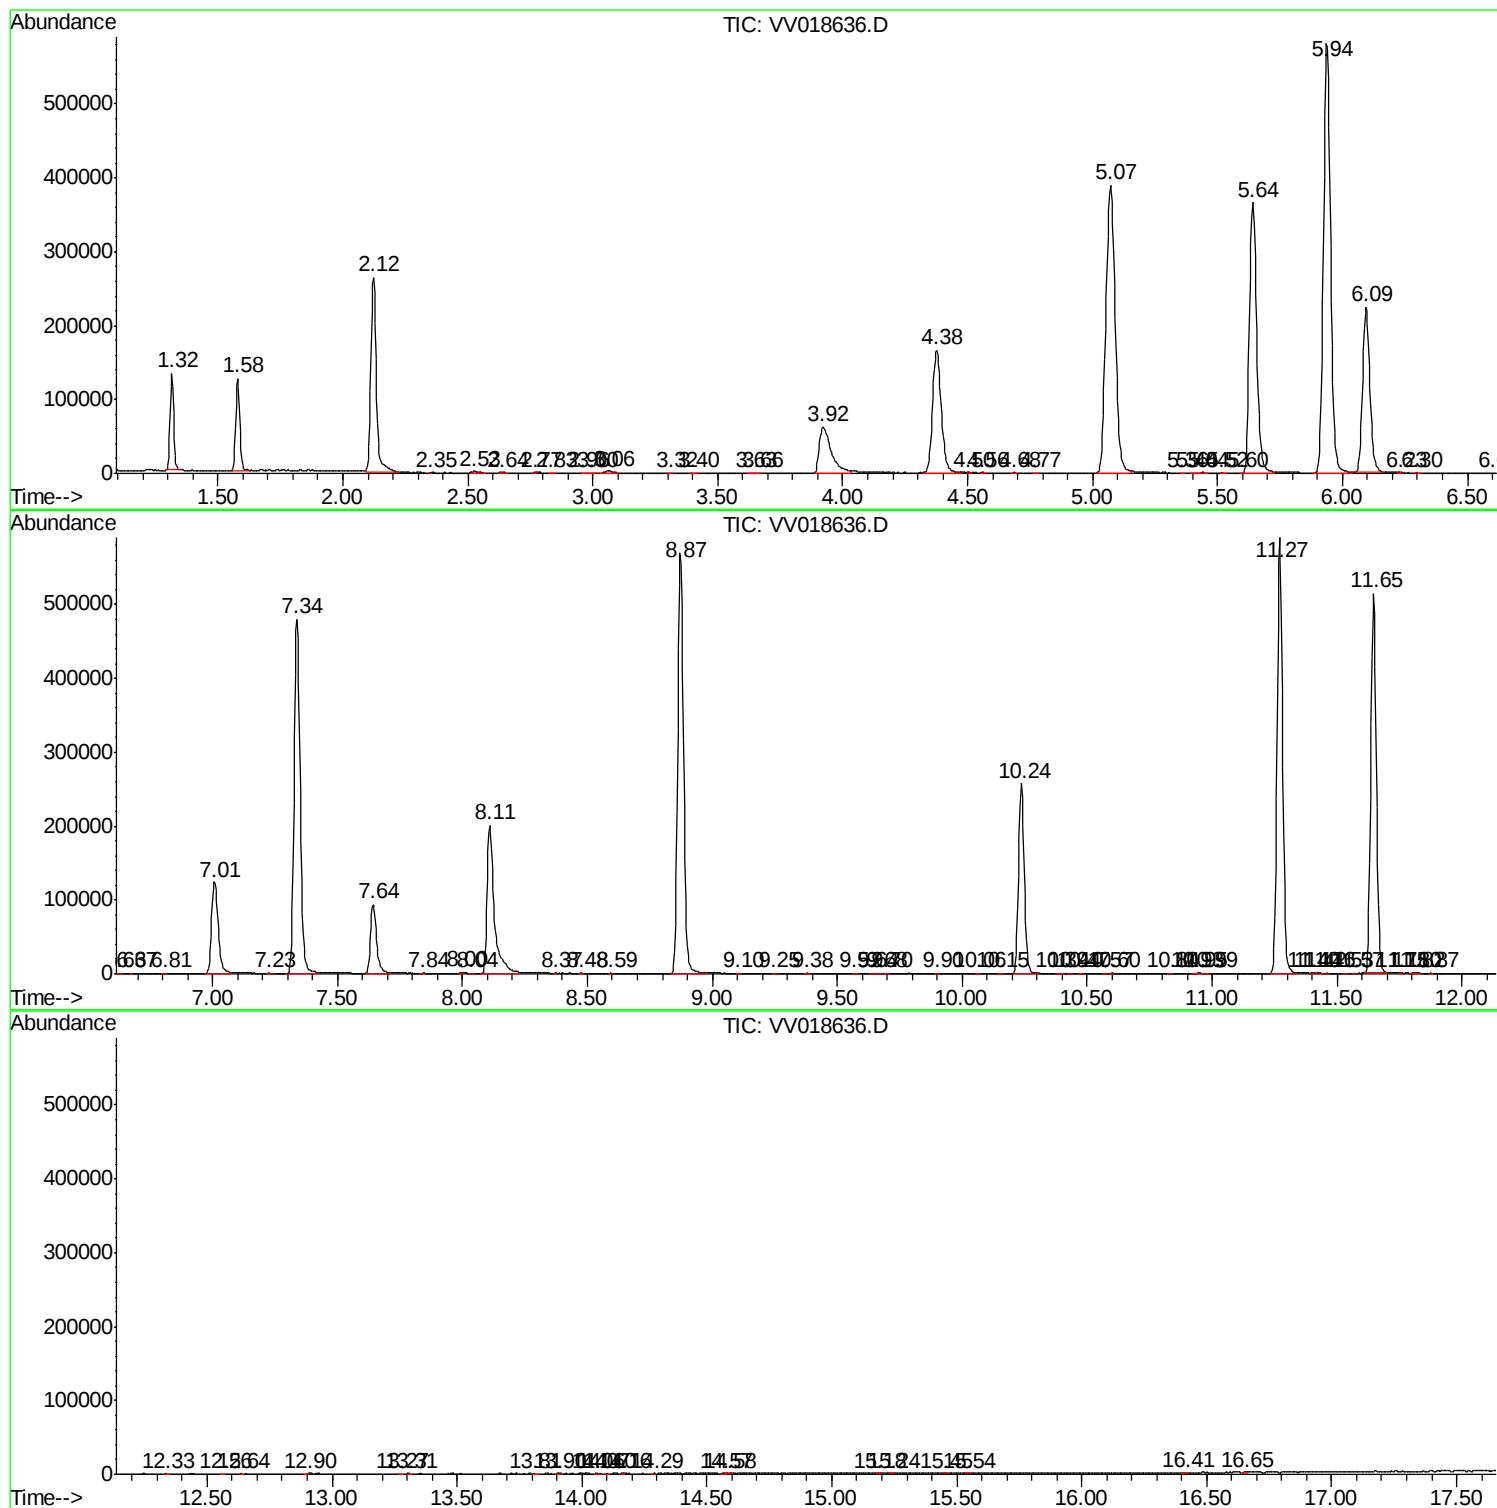

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV100220\
Data File : VV018636.D
Acq On : 02 Oct 2020 19:34
Operator : SY/MD
Sample : L4237-10DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV100220\
Data File : VV018636.D
Acq On : 02 Oct 2020 19:34
Operator : SY/MD
Sample : L4237-10DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC5DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
