

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100220\
 Data File : VV018649.D
 Acq On : 03 Oct 2020 00:43
 Operator : SY/MD
 Sample : L4203-08DL2 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3N9DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	82	rVB	128841	130831	13.86%	1.515%
2	1.576	144	151	162	rVB	115759	126648	13.41%	1.467%
3	2.119	310	320	349	rVB	239695	372952	39.50%	4.319%
4	2.633	476	480	482	rBV2	472	332	0.04%	0.004%
5	2.662	487	489	491	rBV	344	124	0.01%	0.001%
6	2.781	523	526	532	rVB4	461	422	0.04%	0.005%
7	2.833	540	542	544	rBV2	216	148	0.02%	0.002%
8	3.016	596	599	600	rBV	183	102	0.01%	0.001%
9	3.318	687	693	699	rBV	225	342	0.04%	0.004%
10	3.473	739	741	744	rVB	206	116	0.01%	0.001%
11	3.543	760	763	764	rBV	185	110	0.01%	0.001%
12	3.698	809	811	813	rBV2	178	96	0.01%	0.001%
13	3.743	821	825	827	rBV	453	311	0.03%	0.004%
14	3.797	839	842	845	rBV	281	189	0.02%	0.002%
15	3.817	845	848	854	rVV2	172	170	0.02%	0.002%
16	3.904	866	875	909	rBV	68149	197925	20.96%	2.292%
17	4.376	1006	1022	1047	rBV	155748	385096	40.79%	4.460%
18	4.550	1071	1076	1080	rBV3	509	525	0.06%	0.006%
19	4.614	1094	1096	1097	rBV	302	122	0.01%	0.001%
20	4.656	1106	1109	1111	rBV2	315	150	0.02%	0.002%
21	4.675	1113	1115	1117	rBV	251	133	0.01%	0.002%
22	4.772	1143	1145	1152	rVB2	349	289	0.03%	0.003%
23	4.804	1152	1155	1157	rBV2	206	111	0.01%	0.001%
24	4.820	1157	1160	1163	rBV2	409	279	0.03%	0.003%
25	4.833	1163	1164	1165	rBV2	214	54	0.01%	0.001%
26	4.920	1189	1191	1193	rBV	196	124	0.01%	0.001%
27	5.003	1212	1217	1219	rBV2	207	214	0.02%	0.002%
28	5.071	1221	1238	1272	rVV2	370114	944129	100.00%	10.934%
29	5.399	1338	1340	1343	rVB2	301	134	0.01%	0.002%
30	5.434	1349	1351	1357	rVB2	248	214	0.02%	0.002%
31	5.489	1365	1368	1370	rBV2	196	119	0.01%	0.001%
32	5.582	1394	1397	1403	rBV	273	251	0.03%	0.003%
33	5.640	1403	1415	1440	rBV	350871	692537	73.35%	8.021%
34	5.929	1494	1505	1530	rVB4	35130	82092	8.69%	0.951%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100220\
 Data File : VV018649.D
 Acq On : 03 Oct 2020 00:43
 Operator : SY/MD
 Sample : L4203-08DL2 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3N9DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

35	6.093	1542	1556	1580	rBV	214234	430695	45.62%	4.988%
36	6.305	1619	1622	1624	rBV	282	133	0.01%	0.002%
37	6.318	1624	1626	1627	rVB2	244	58	0.01%	0.001%
38	6.370	1640	1642	1646	rVB	411	206	0.02%	0.002%
39	6.392	1646	1649	1652	rBV2	351	241	0.03%	0.003%
40	6.431	1656	1661	1665	rBV2	181	132	0.01%	0.002%
41	6.659	1730	1732	1734	rBV	214	121	0.01%	0.001%
42	6.765	1762	1765	1766	rBV	214	103	0.01%	0.001%
43	7.006	1829	1840	1865	rBV	113618	208316	22.06%	2.413%
44	7.186	1894	1896	1897	rBV	190	64	0.01%	0.001%
45	7.251	1915	1916	1917	rBV	141	38	0.00%	0.000%
46	7.286	1925	1927	1928	rBV	190	84	0.01%	0.001%
47	7.337	1931	1943	1965	rBV	441833	754067	79.87%	8.733%
48	7.643	2028	2038	2056	rBV2	84495	145565	15.42%	1.686%
49	7.919	2121	2124	2125	rBV2	113	63	0.01%	0.001%
50	7.997	2135	2148	2170	rBV	516070	868710	92.01%	10.061%
51	8.109	2173	2183	2221	rVV2	195411	392034	41.52%	4.540%
52	8.392	2269	2271	2274	rBV	292	154	0.02%	0.002%
53	8.434	2278	2284	2287	rBV3	466	582	0.06%	0.007%
54	8.485	2299	2300	2302	rBV3	222	75	0.01%	0.001%
55	8.775	2388	2390	2391	rVB	258	82	0.01%	0.001%
56	8.871	2408	2420	2448	rBV	543602	882421	93.46%	10.220%
57	9.164	2507	2511	2512	rBV	264	126	0.01%	0.001%
58	9.177	2512	2515	2517	rBV	220	151	0.02%	0.002%
59	9.231	2528	2532	2535	rBV2	249	205	0.02%	0.002%
60	9.260	2537	2541	2544	rBV2	283	199	0.02%	0.002%
61	9.292	2549	2551	2552	rBV2	230	74	0.01%	0.001%
62	9.347	2565	2568	2572	rBV	301	219	0.02%	0.003%
63	9.418	2586	2590	2592	rBV	240	184	0.02%	0.002%
64	9.447	2597	2599	2602	rBV2	325	185	0.02%	0.002%
65	9.842	2718	2722	2723	rBV	403	248	0.03%	0.003%
66	9.900	2733	2740	2743	rVB2	274	301	0.03%	0.003%
67	9.919	2743	2746	2749	rBV	338	231	0.02%	0.003%
68	10.238	2833	2845	2864	rBV	254654	399391	42.30%	4.626%
69	10.485	2920	2922	2923	rBV	327	145	0.02%	0.002%
70	10.704	2984	2990	2994	rBV2	281	364	0.04%	0.004%
71	10.836	3028	3031	3036	rVB2	340	285	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100220\
Data File : VV018649.D
Acq On : 03 Oct 2020 00:43
Operator : SY/MD
Sample : L4203-08DL2 200X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3N9DL2

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Title : VOC Analysis

72	10.916	3053	3056	3057	rBV	181	80	0.01%	0.001%
73	11.189	3138	3141	3143	rBV2	312	239	0.03%	0.003%
74	11.270	3155	3166	3193	rBV	561711	846668	89.68%	9.806%
75	11.646	3271	3283	3300	rBV	485908	763068	80.82%	8.837%
76	11.906	3362	3364	3369	rBV	349	199	0.02%	0.002%
77	12.154	3438	3441	3444	rBV	306	217	0.02%	0.003%
78	13.604	3889	3892	3895	rBV	420	300	0.03%	0.003%
79	13.881	3977	3978	3980	rVB2	256	75	0.01%	0.001%


Sum of corrected areas: 8634489

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100220\
Data File : VV018649.D
Acq On : 03 Oct 2020 00:43
Operator : SY/MD
Sample : L4203-08DL2 200X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
BG3N9DL2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

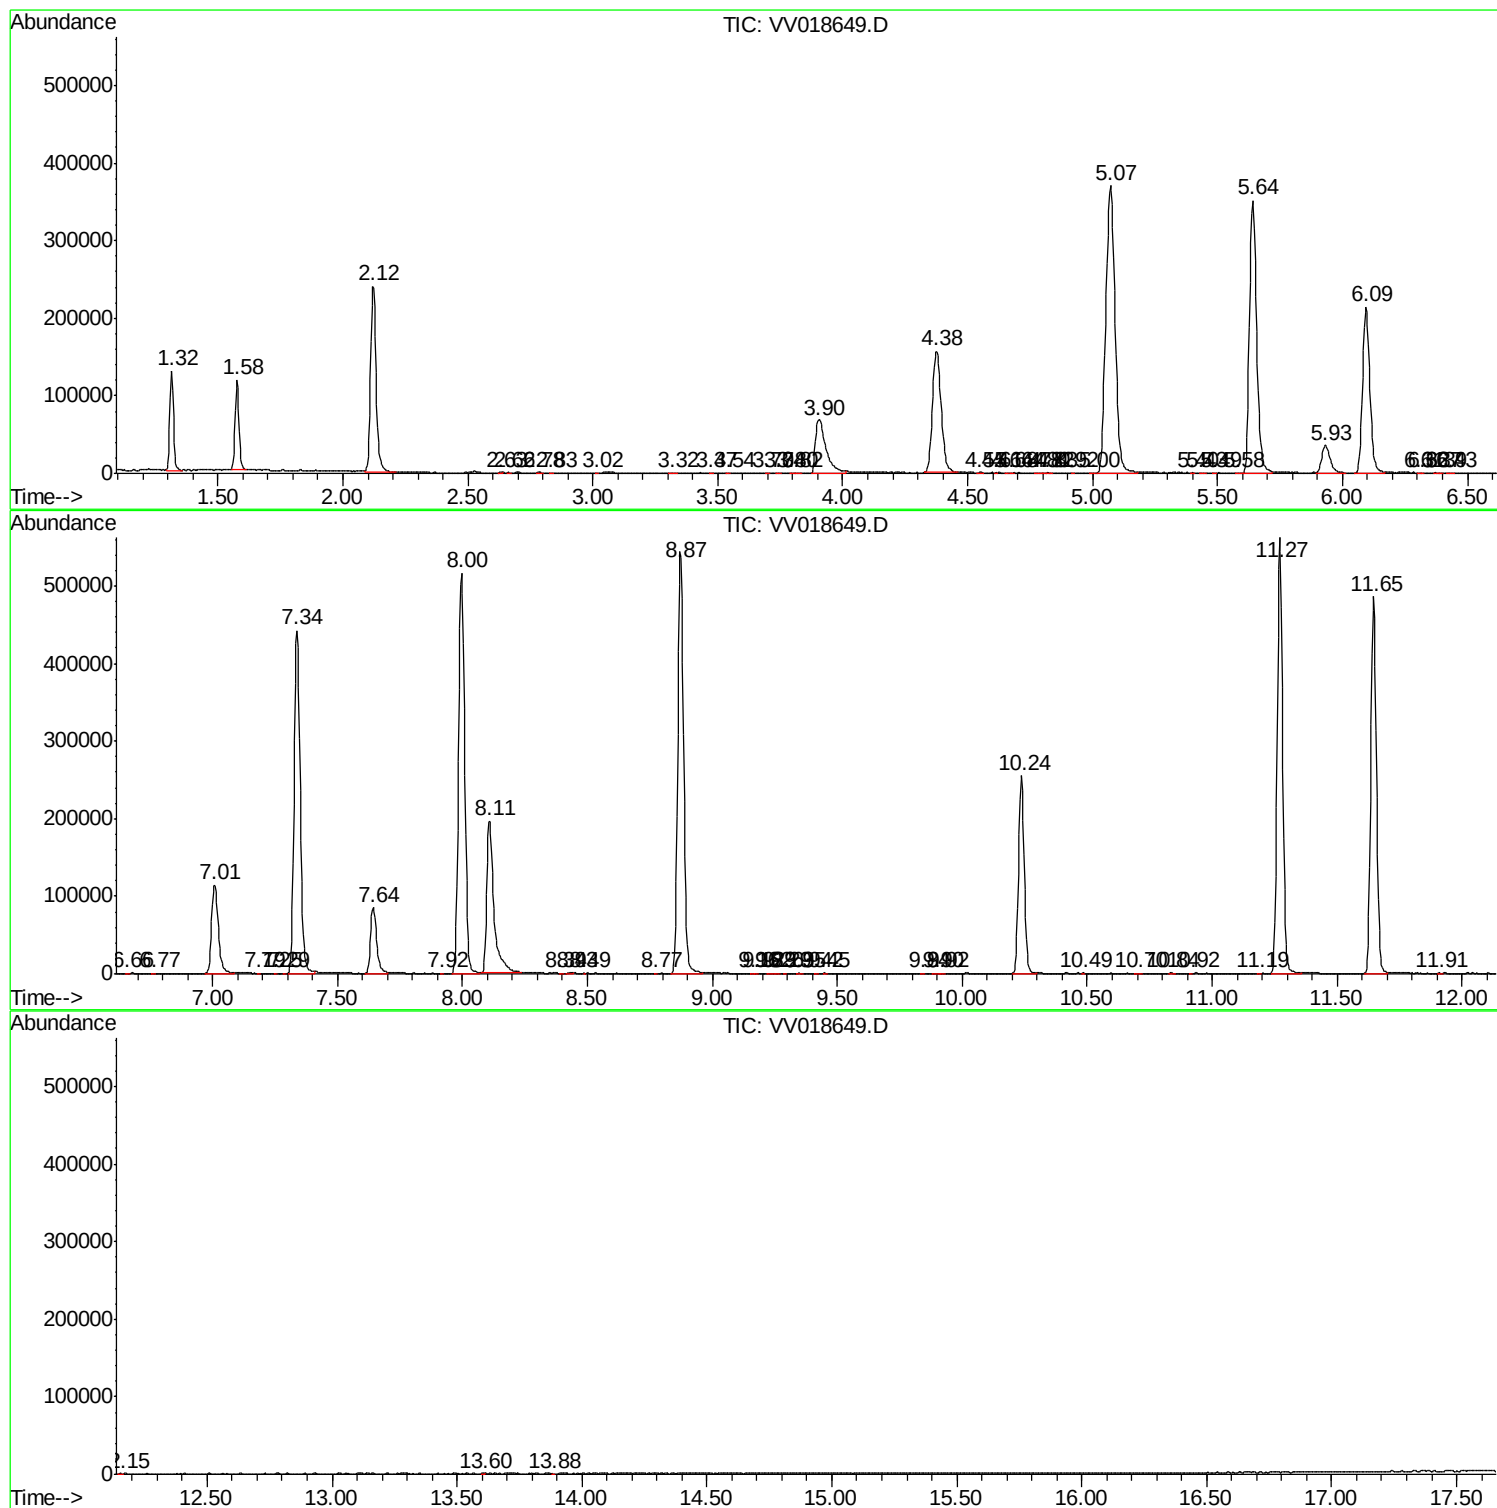

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV100220\
Data File : VV018649.D
Acq On : 03 Oct 2020 00:43
Operator : SY/MD
Sample : L4203-08DL2 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3N9DL2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV100220\
Data File : VV018649.D
Acq On : 03 Oct 2020 00:43
Operator : SY/MD
Sample : L4203-08DL2 200X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG3N9DL2

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc