


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV100220\
 Data File : VV018615.D
 Acq On : 02 Oct 2020 10:41
 Operator : SY/MD
 Sample : BFB65
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB65

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis
 Last Update : Fri Oct 16 00:56:49 2020

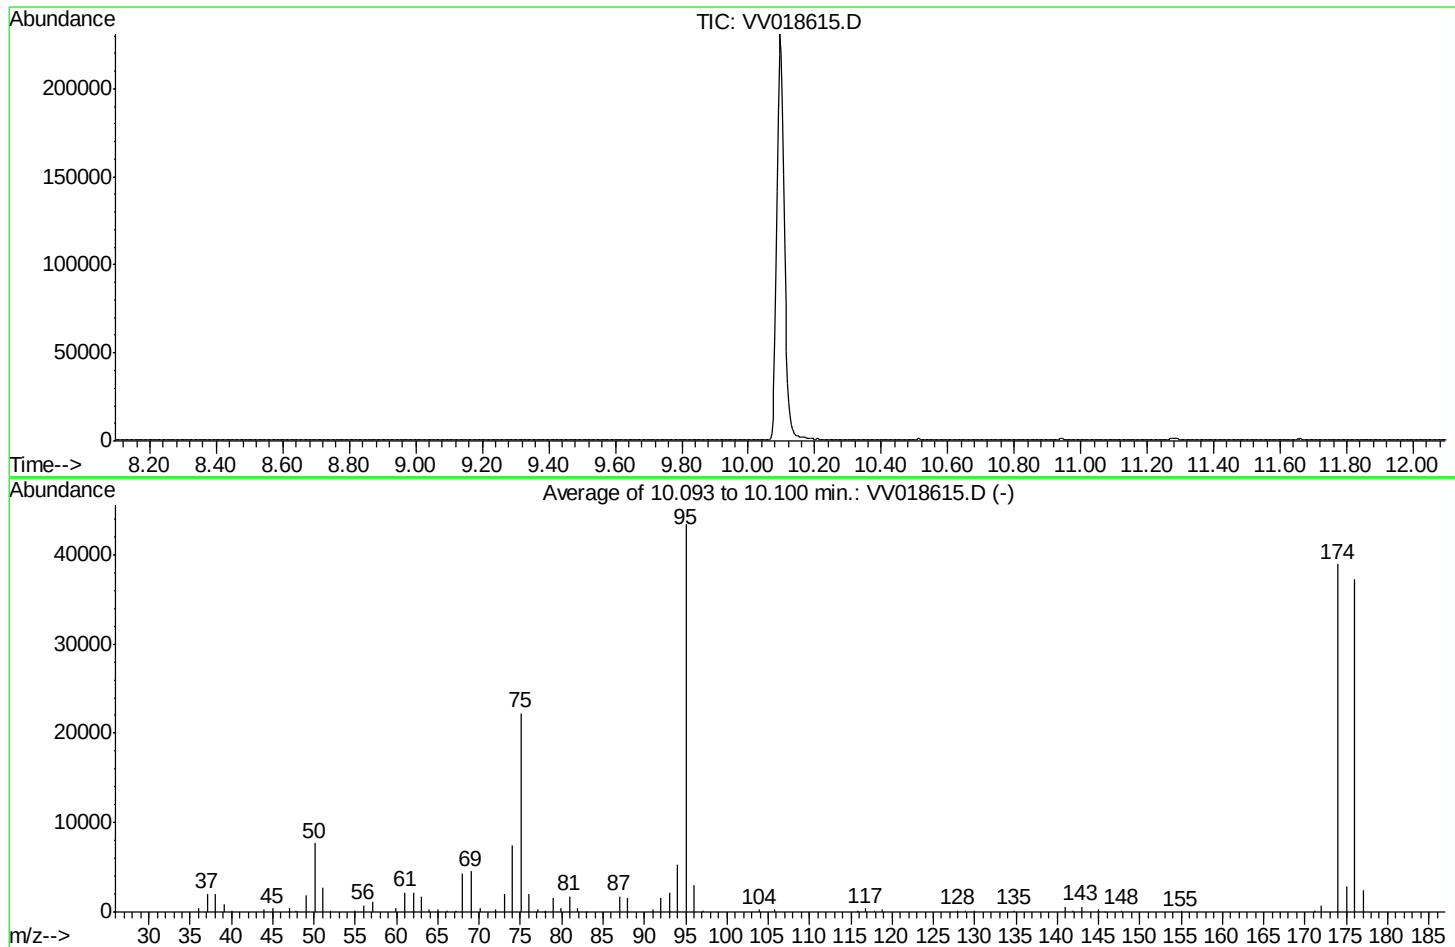

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	7710	PASS
75	95	30	80	51.3	22274	PASS
95	95	100	100	100.0	43397	PASS
96	95	5	9	6.8	2953	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	89.8	38949	PASS
175	174	5	9	7.3	2855	PASS
176	174	95	101	95.7	37290	PASS
177	176	5	9	6.6	2461	PASS

m/z	Abundance
36.00	451.0
37.10	2082.0
38.10	2038.0
39.10	907.0
40.10	272.0
44.00	835.0
45.00	387.0
47.00	551.0
47.80	235.0
49.00	1862.0
50.10	7816.0
51.00	2654.0
52.00	169.0
55.00	180.0
56.00	715.0
57.10	1172.0
60.00	395.0
61.00	2204.0
62.00	2096.0
63.00	1779.0
63.90	328.0
65.00	308.0
67.10	227.0
68.00	4208.0
69.00	4587.0
70.10	384.0
71.90	338.0
73.00	2002.0
74.00	7231.0
75.10	22176.0
76.00	2136.0
77.10	267.0
77.90	178.0
78.90	1674.0
79.90	410.0
80.90	1771.0
81.90	427.0
87.00	1698.0
88.00	1715.0
91.00	207.0
92.00	1621.0
93.00	2169.0
94.00	5342.0
95.00	42640.0
96.00	2924.0
97.00	160.0
103.90	280.0
105.80	248.0
115.90	219.0
116.90	318.0
117.80	206.0
118.90	320.0
128.00	177.0
128.90	151.0
130.00	193.0
134.80	164.0
140.90	595.0
143.00	656.0
145.00	315.0
145.80	123.0
147.80	163.0
155.00	124.0
171.20	105.0
172.00	634.0
174.00	37168.0
175.00	2792.0
176.00	36016.0
177.00	2324.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

m/z	Abundance
36.00	469.0
37.10	2129.0
38.10	2030.0
39.00	880.0
40.10	314.0
44.00	796.0
45.00	402.0
46.90	477.0
47.80	206.0
49.00	1881.0
50.10	7881.0
51.00	2821.0
52.00	151.0
55.00	136.0
56.00	783.0
57.00	1163.0
60.00	426.0
61.00	2250.0
62.00	2219.0
63.00	1862.0
64.00	308.0
65.00	360.0
66.10	117.0
67.10	216.0
68.00	4406.0
69.00	4640.0
70.10	414.0
72.00	347.0
73.00	2140.0
74.10	7667.0
75.10	23064.0
76.00	2148.0
77.10	281.0
78.10	182.0
78.90	1685.0
79.90	433.0
80.90	1773.0
82.00	478.0
87.00	1808.0
88.00	1690.0
91.00	242.0
92.00	1710.0
93.00	2221.0
94.00	5540.0
95.00	45056.0
96.00	2986.0
97.00	149.0
104.00	281.0
105.80	289.0
115.90	215.0
116.80	381.0
117.80	232.0
118.90	313.0
127.90	210.0
128.80	159.0
130.00	212.0
134.80	172.0
140.90	598.0
141.90	122.0
143.00	662.0
145.00	361.0
145.80	103.0
147.80	214.0
155.10	131.0
171.10	123.0
172.00	696.0
174.00	40232.0
175.00	2911.0
176.00	38696.0
177.00	2523.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

m/z	Abundance
35.90	411.0
37.10	1965.0
38.00	1875.0
39.00	756.0
40.10	315.0
44.00	725.0
45.00	370.0
46.90	381.0
48.00	171.0
49.00	1766.0
50.00	7433.0
51.00	2679.0
52.10	105.0
55.00	114.0
56.00	770.0
57.00	1099.0
59.90	419.0
61.00	2125.0
62.00	2009.0
63.00	1723.0
64.00	302.0
65.00	390.0
66.10	128.0
67.10	144.0
68.00	4225.0
69.00	4338.0
70.10	390.0
72.00	296.0
73.00	2063.0
74.10	7432.0
75.00	21584.0
76.00	1912.0
77.10	282.0
78.10	185.0
79.00	1589.0
79.90	458.0
80.90	1676.0
82.00	478.0
83.00	106.0
87.00	1765.0
88.00	1491.0
91.00	260.0
92.00	1556.0
93.00	2003.0
94.00	5131.0
95.00	42496.0
96.00	2951.0
97.10	119.0
104.00	250.0
105.80	264.0
115.90	192.0
116.80	418.0
117.80	207.0
118.80	310.0
127.90	228.0
128.80	179.0
130.00	178.0
134.80	147.0
140.90	576.0
142.00	161.0
142.90	617.0
144.90	338.0
147.80	216.0
155.10	110.0
171.10	120.0
171.90	668.0
174.00	39448.0
175.00	2863.0
176.00	37160.0
177.00	2536.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

Scan 2790 (10.061 min): VV018615.D
BFB65

m/z	Abundance
40.00	196.0
44.00	515.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65