




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022423.D
 Acq On : 30 Sep 2021 11:42
 Operator : SY/MD
 Sample : M3978-12DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW8W9ME

Manual Integrations
 APPROVED

MMDadoda
 10/6/2021 2:27:30 PM

Quant Time: Oct 01 02:40:25 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 01 02:38:11 2021
 Response via : Initial Calibration

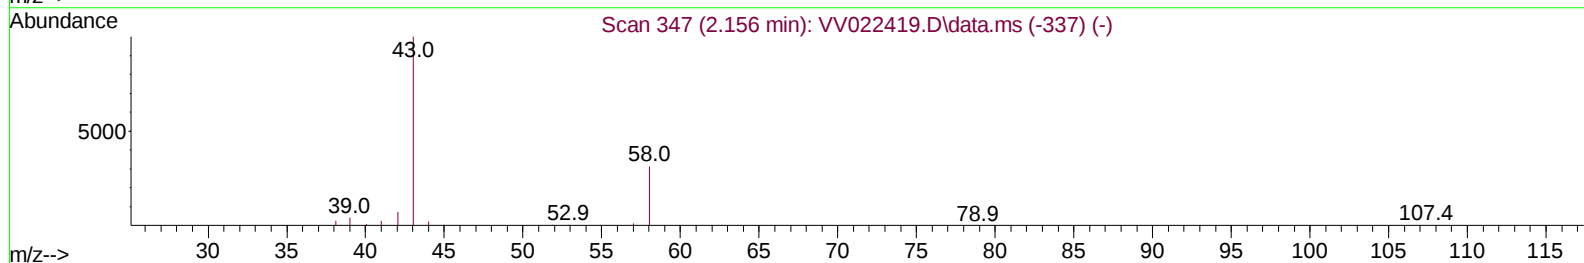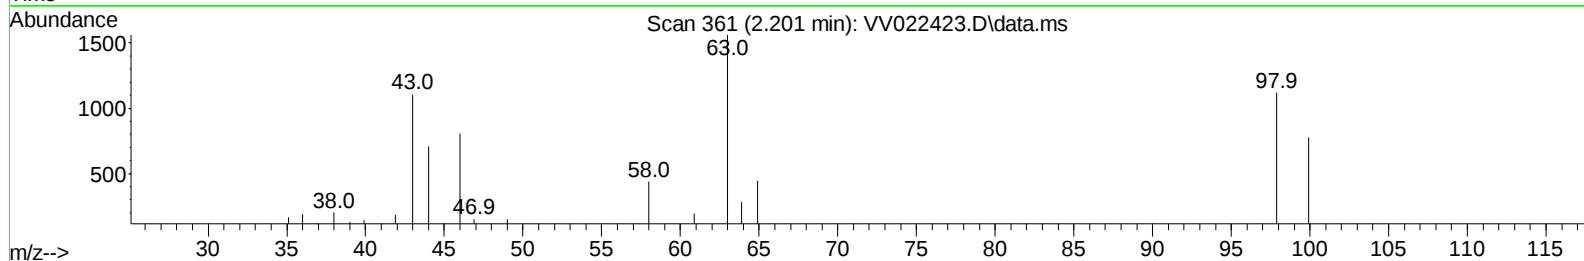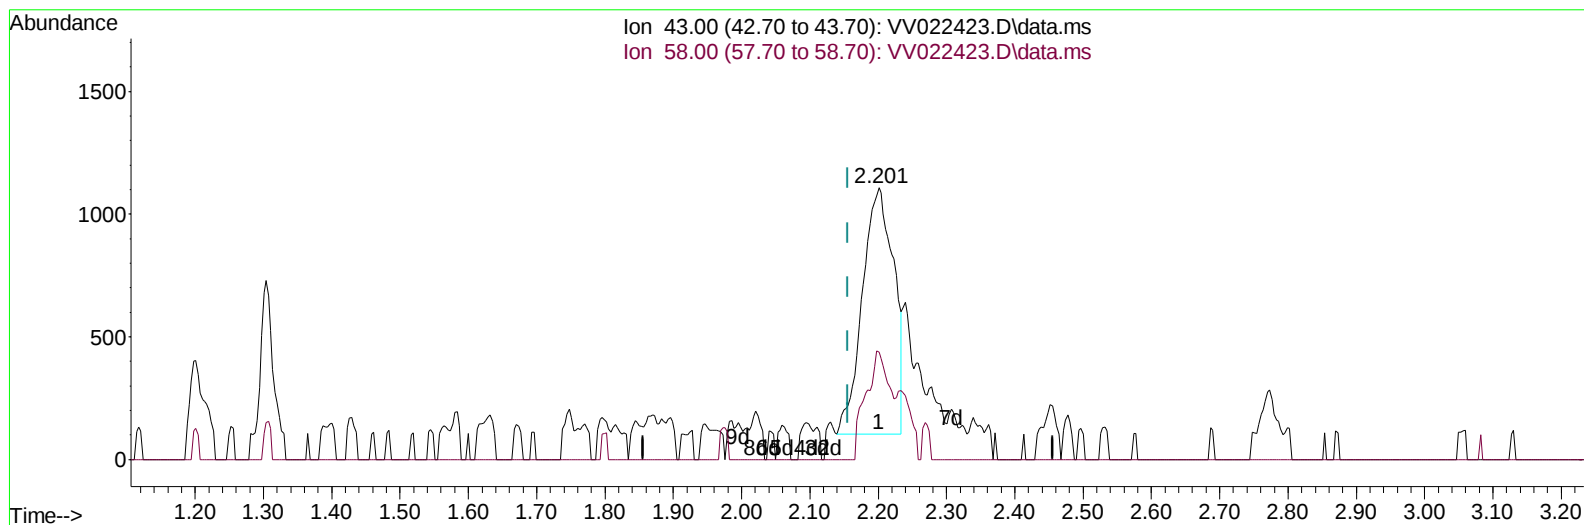

TIC: VV022423.D\data.ms

(13) Acetone (T)

2.201min (+ 0.045) 2.78 ug/L

response 3183

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	33.60	33.27
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV093021\
 Data File : VV022423.D
 Acq On : 30 Sep 2021 11:42
 Operator : SY/MD
 Sample : M3978-12DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW8W9ME

Manual Integrations
 APPROVED

MMDadoda
 10/6/2021 2:27:30 PM

Quant Time: Oct 01 02:40:25 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 01 02:38:11 2021
 Response via : Initial Calibration

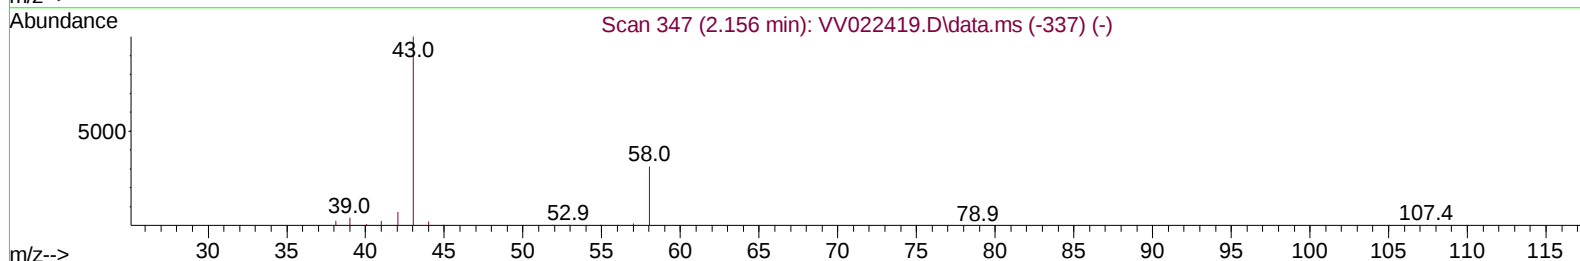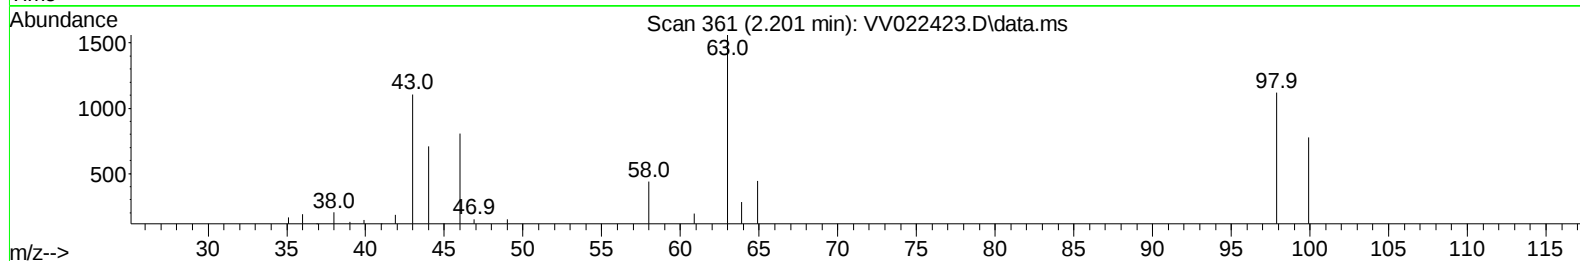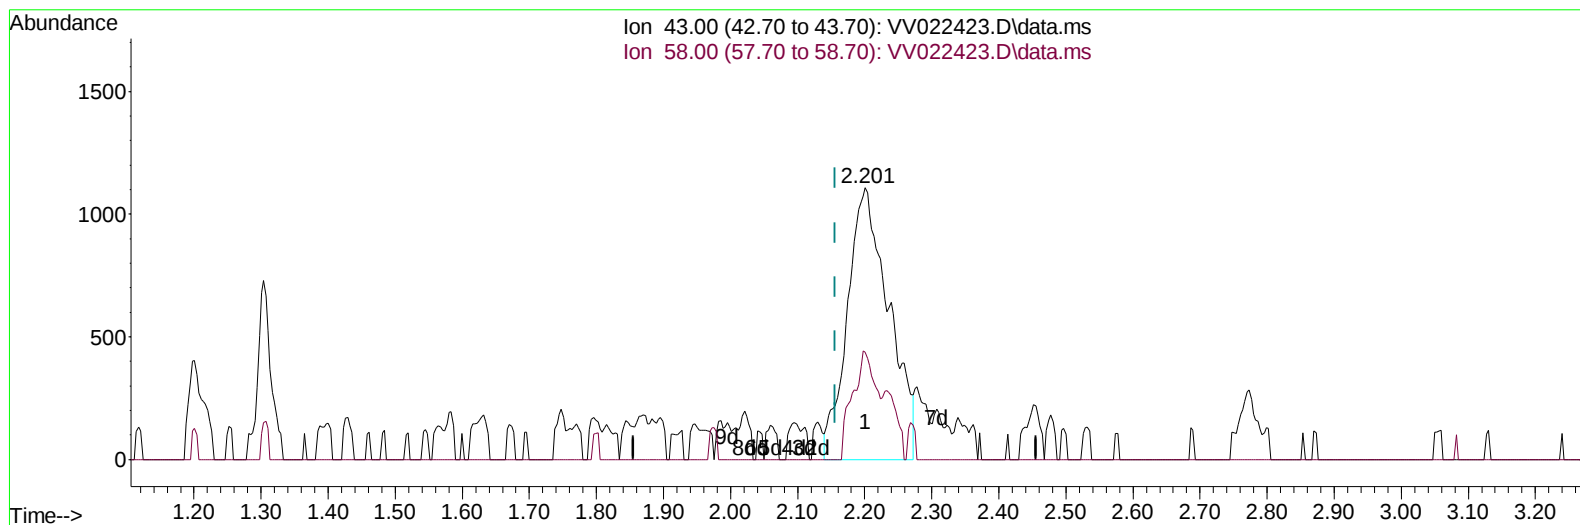

TIC: VV022423.D\data.ms

(13) Acetone (T)

2.201min (+ 0.045) 4.15 ug/L m

response 4742

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	33.60	22.33
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022508.D
 Acq On : 02 Oct 2021 14:08
 Operator : SY/MD
 Sample : M3973-03ME
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW8W9ME

Manual Integrations
 APPROVED

MMDadoda
 10/6/2021 2:27:30 PM

Quant Time: Oct 04 01:59:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Oct 04 01:01:56 2021
 Response via : Initial Calibration

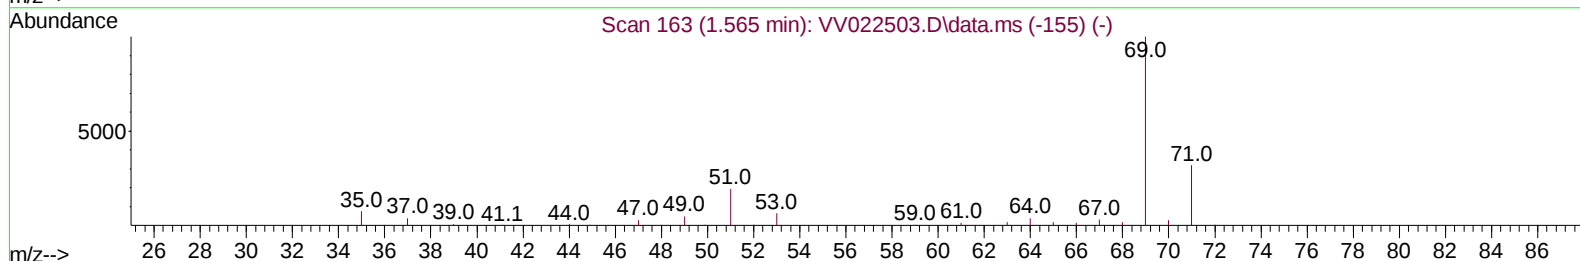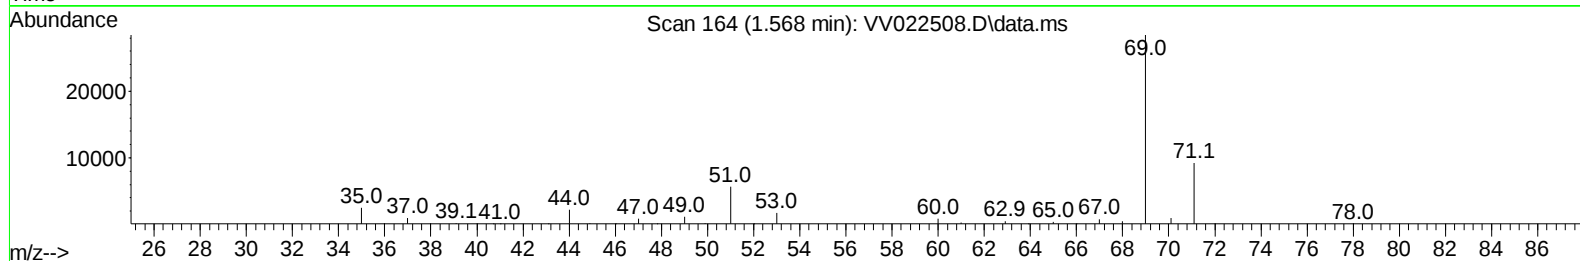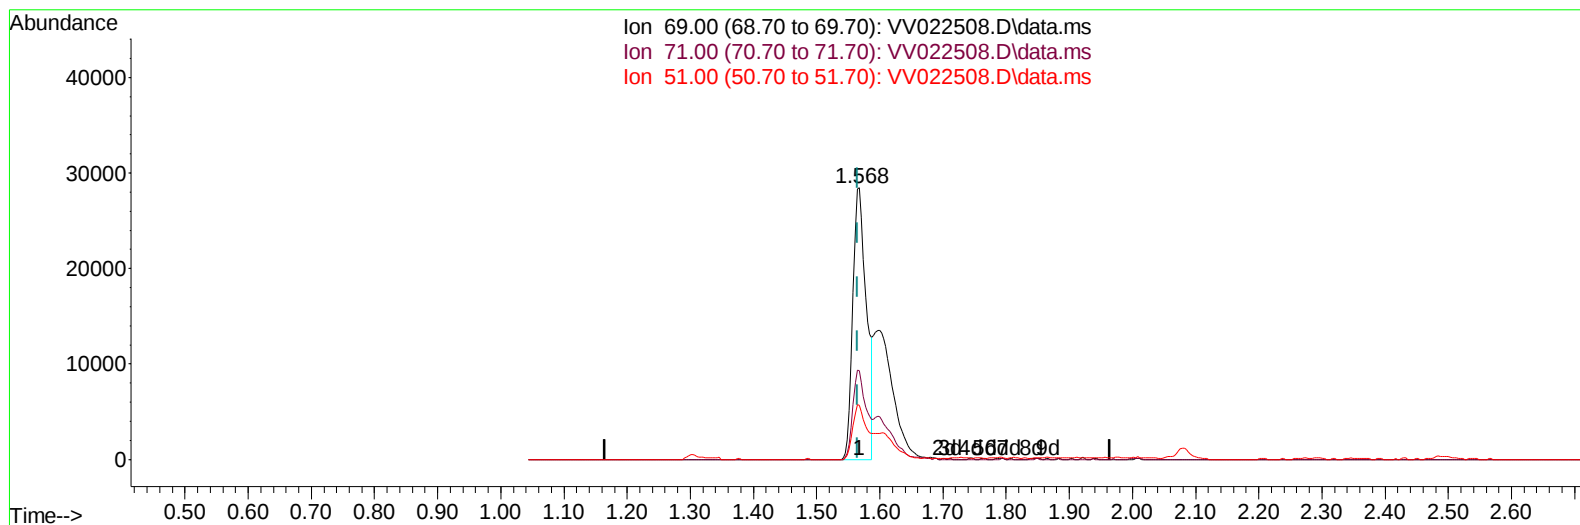

TIC: VV022508.D\data.ms

(7) Chloroethane-d5 (S)

1.568min (+ 0.003) 31.28 ug/L

response 42580

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.90	34.53
51.00	27.70	21.62
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022508.D
 Acq On : 02 Oct 2021 14:08
 Operator : SY/MD
 Sample : M3973-03ME
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW8W9ME

Manual Integrations
 APPROVED

MMDadoda
 10/6/2021 2:27:30 PM

Quant Time: Oct 04 01:59:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Oct 04 01:01:56 2021
 Response via : Initial Calibration

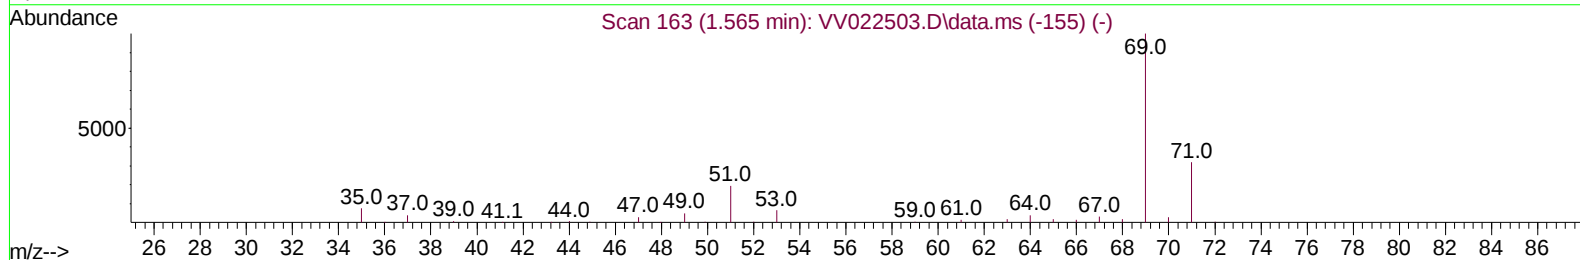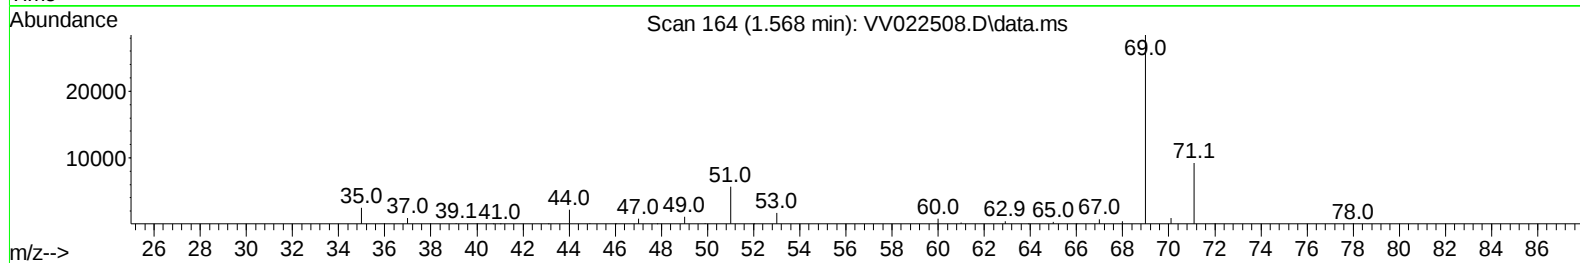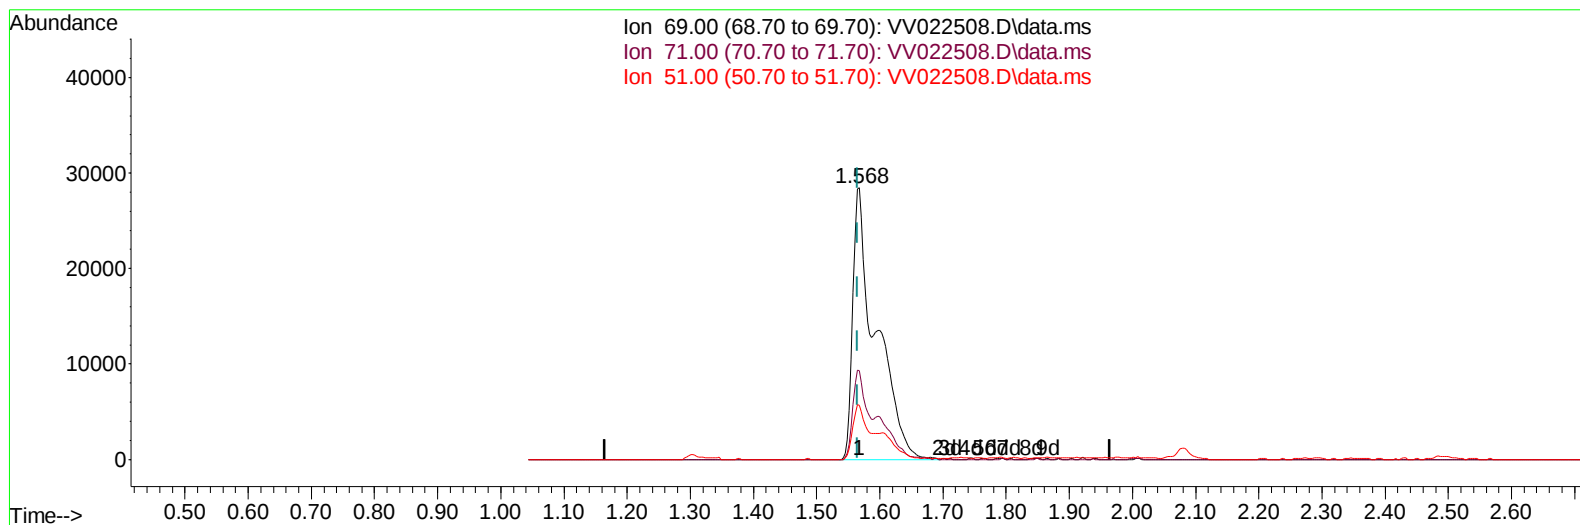

TIC: VV022508.D\data.ms

(7) Chloroethane-d5 (S)

1.568min (+ 0.003) 52.96 ug/L m

response 72087

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.90	20.40#
51.00	27.70	12.77#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022508.D
 Acq On : 02 Oct 2021 14:08
 Operator : SY/MD
 Sample : M3973-03ME
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW8W9ME

Manual Integrations
 APPROVED

MMDadoda
 10/6/2021 2:27:30 PM

Quant Time: Oct 04 01:59:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Oct 04 01:01:56 2021
 Response via : Initial Calibration

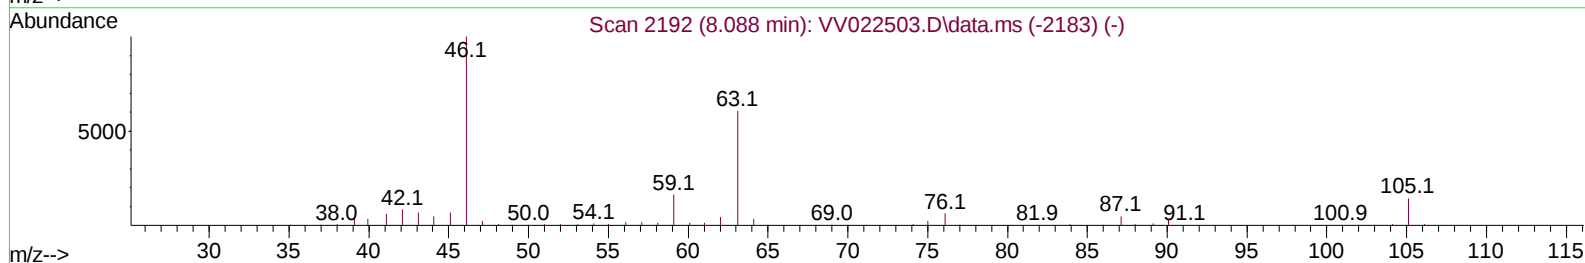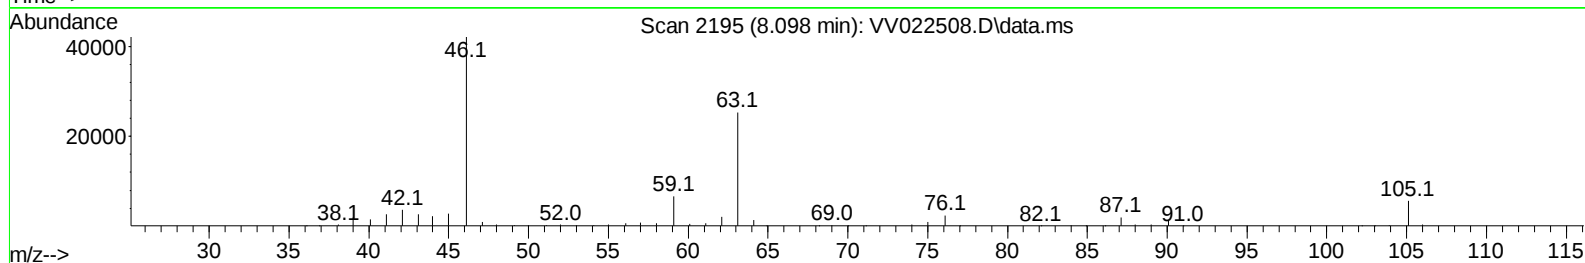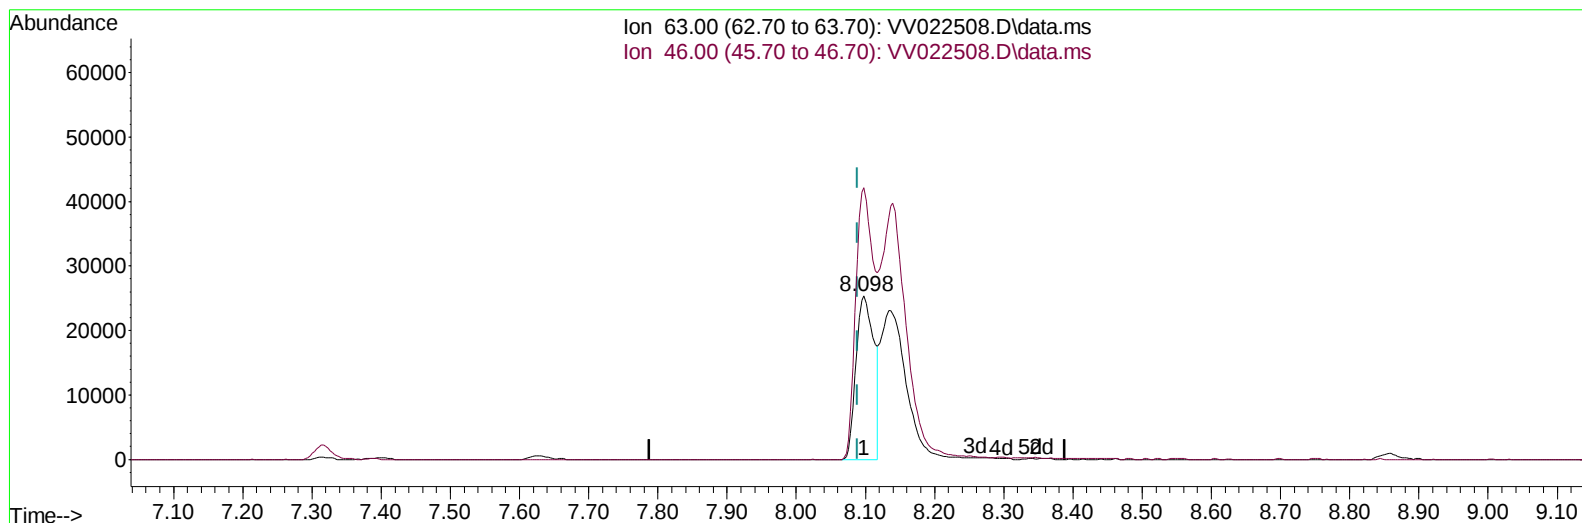

TIC: VV022508.D\data.ms

(47) 2-Hexanone-d5 (S)

8.098min (+ 0.010) 58.16 ug/L

response 45989

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	163.00	167.98
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022508.D
 Acq On : 02 Oct 2021 14:08
 Operator : SY/MD
 Sample : M3973-03ME
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW8W9ME

Manual Integrations
 APPROVED

MMDadoda
 10/6/2021 2:27:30 PM

Quant Time: Oct 04 01:59:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Oct 04 01:01:56 2021
 Response via : Initial Calibration

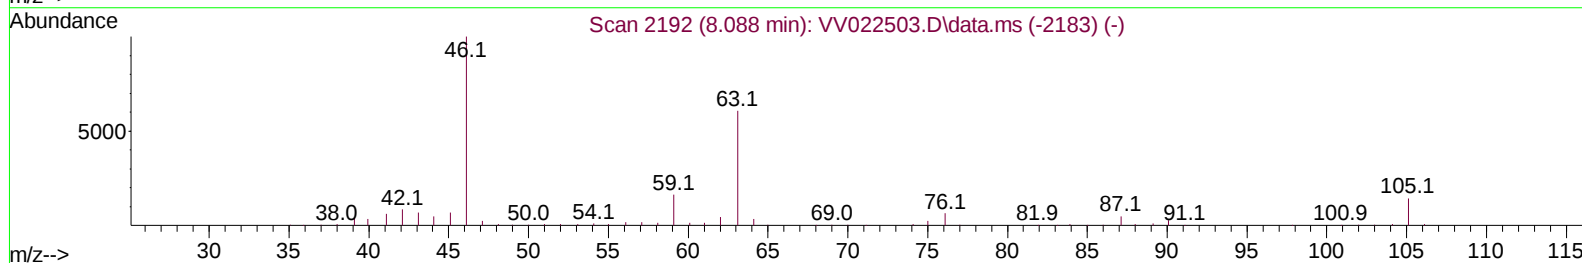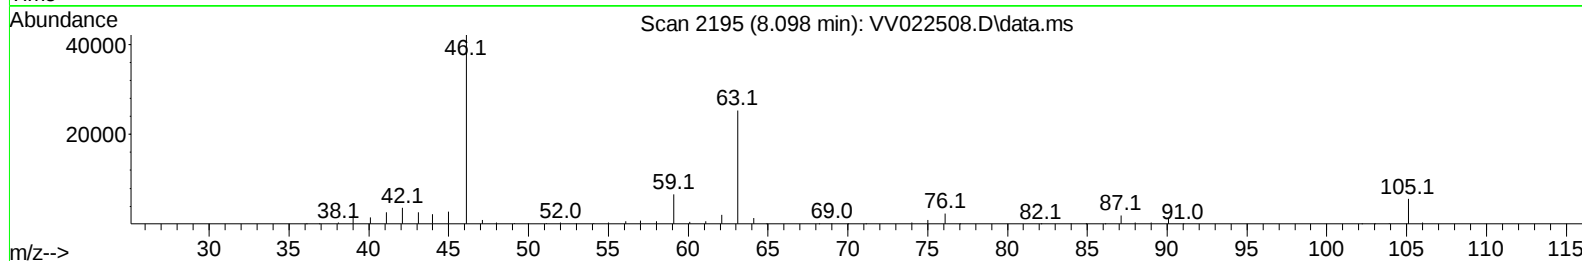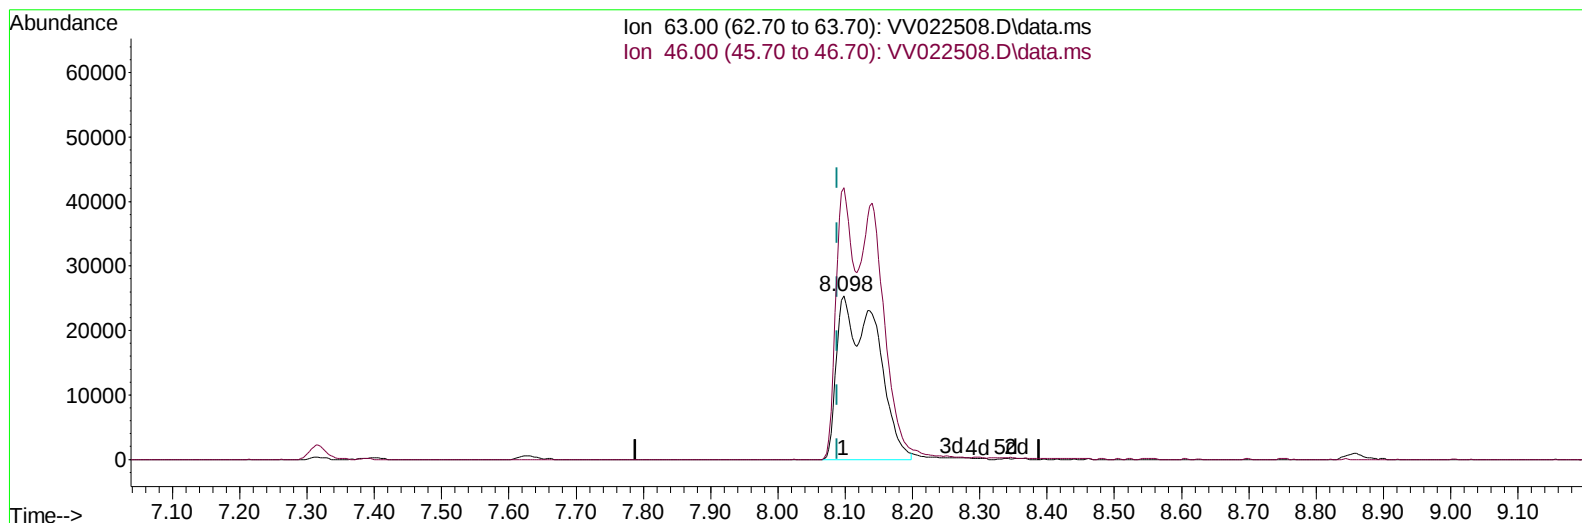

TIC: VV022508.D\data.ms

(47) 2-Hexanone-d5 (S)

8.098min (+ 0.010) 131.27 ug/L m

response 103799

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	163.00	74.42#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022508.D
 Acq On : 02 Oct 2021 14:08
 Operator : SY/MD
 Sample : M3973-03ME
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleID :
 EW8W9ME

Manual Integrations
 APPROVED

MMDadoda
 10/6/2021 2:27:30 PM

Quant Time: Oct 04 01:59:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Oct 04 01:01:56 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	279964	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	267652	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	125313	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	103866	59.987	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	119.980%	
7) Chloroethane-d5	1.568	69	72087m	52.965	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	105.920%	
11) 1,1-Dichloroethene-d2	2.082	63	158850	46.528	ug/L	-0.03
Spiked Amount 50.000	Range 60	- 125	Recovery	=	93.060%	
21) 2-Butanone-d5	3.905	46	149648	157.015	ug/L	0.02
Spiked Amount 100.000	Range 40	- 130	Recovery	=	157.010%#	
24) Chloroform-d	4.346	84	186979	59.106	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	118.220%	
26) 1,2-Dichloroethane-d4	5.030	65	130897	71.330	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	142.660%#	
32) Benzene-d6	5.043	84	419197	67.606	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	135.220%#	
36) 1,2-Dichloropropane-d6	6.069	67	131272	68.770	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	137.540%#	
41) Toluene-d8	7.317	98	384873	67.667	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	135.340%#	
43) trans-1,3-Dichloroprop...	7.625	79	59494	65.875	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	131.740%#	
47) 2-Hexanone-d5	8.098	63	103799m	131.266	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	131.270%#	
56) 1,1,2,2-Tetrachloroeth...	10.226	84	167019	62.923	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	125.840%#	
66) 1,2-Dichlorobenzene-d4	11.631	152	151603	74.186	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	148.380%#	
Target Compounds						
						Qvalue
25) Chloroform	4.375	83	21884	5.725	ug/L	93
34) Trichloroethene	5.915	95	6444	2.986	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022508.D
Acq On : 02 Oct 2021 14:08
Operator : SY/MD
Sample : M3973-03ME
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW8W9ME

Manual Integrations
APPROVED

MMDadoda
10/6/2021 2:27:30 PM

Quant Time: Oct 04 01:59:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Oct 04 01:01:56 2021
Response via : Initial Calibration

