




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV100221\  
 Data File : VV022542.D  
 Acq On : 03 Oct 2021 04:22  
 Operator : SY/MD  
 Sample : M3974-05MEMSD  
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA\_V/MEOH  
 ALS Vial : 44 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 EW8Y9MEMSD

Manual Integrations  
 APPROVED

MMDadoda  
 10/6/2021 2:30:22 PM

Quant Time: Oct 04 04:32:31 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM100121WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Mon Oct 04 04:27:20 2021  
 Response via : Initial Calibration

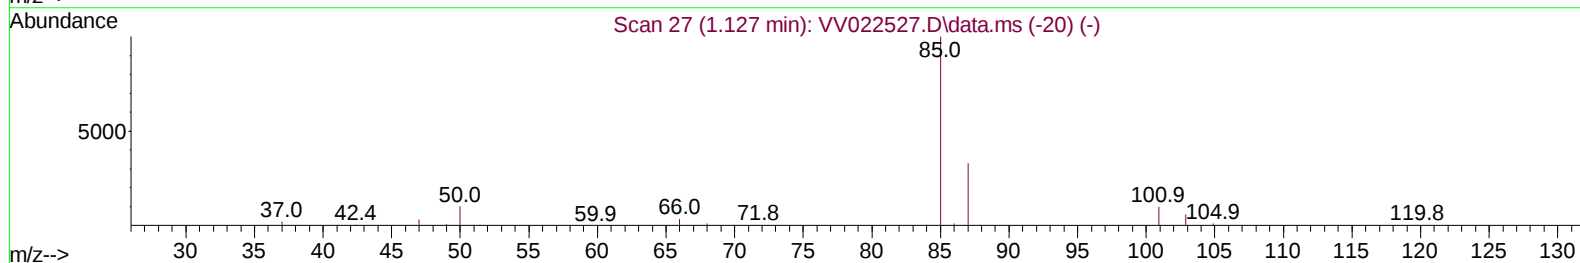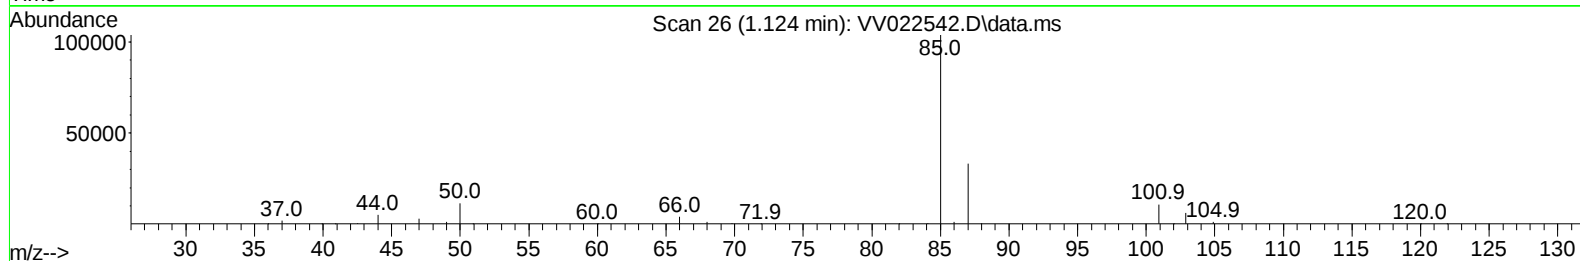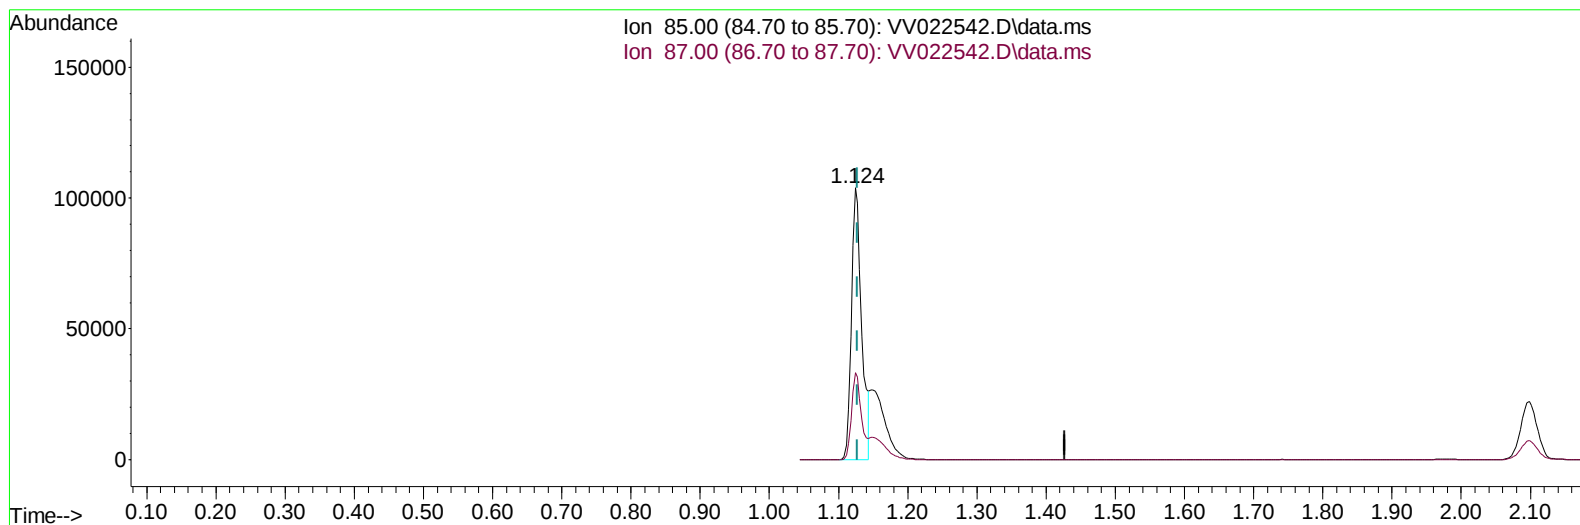

TIC: VV022542.D\data.ms

(2) Dichlorodifluoromethane (T)

1.124min (-0.003) 32.96 ug/L

response 108318

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 85.00 | 100.00 | 100.00 |
| 87.00 | 32.20  | 31.79  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV100221\  
Data File : VV022542.D  
Acq On : 03 Oct 2021 04:22  
Operator : SY/MD  
Sample : M3974-05MEMSD  
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA\_V/MEOH  
ALS Vial : 44 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
EW8Y9MEMSD

Manual Integrations  
APPROVED

MMDadoda  
10/6/2021 2:30:22 PM

Quant Time: Oct 04 04:32:31 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM100121WMA.M  
Quant Title : VOC Analysis  
QLast Update : Mon Oct 04 04:27:20 2021  
Response via : Initial Calibration

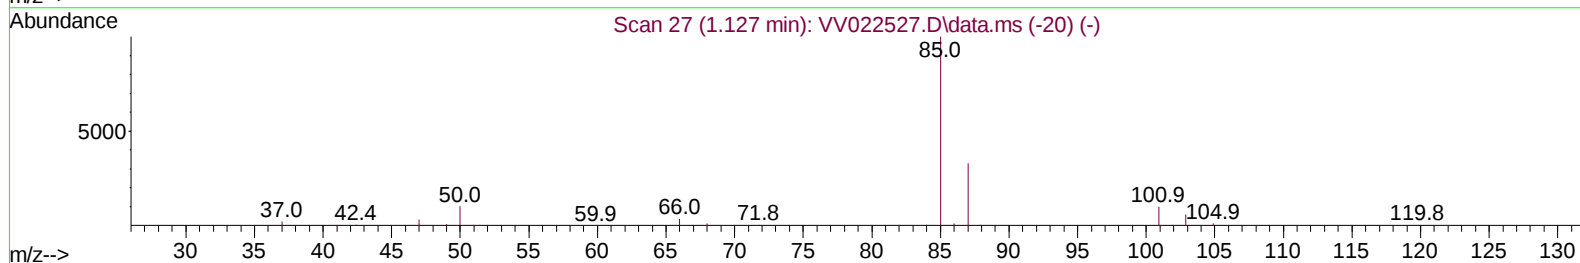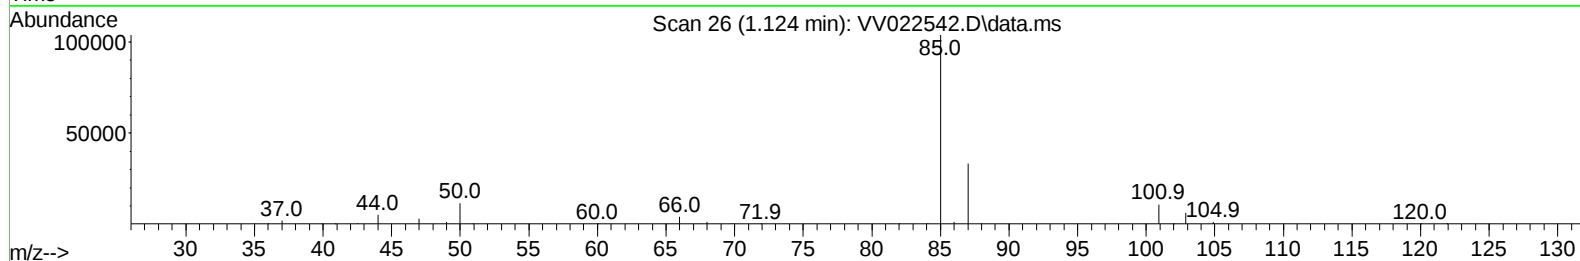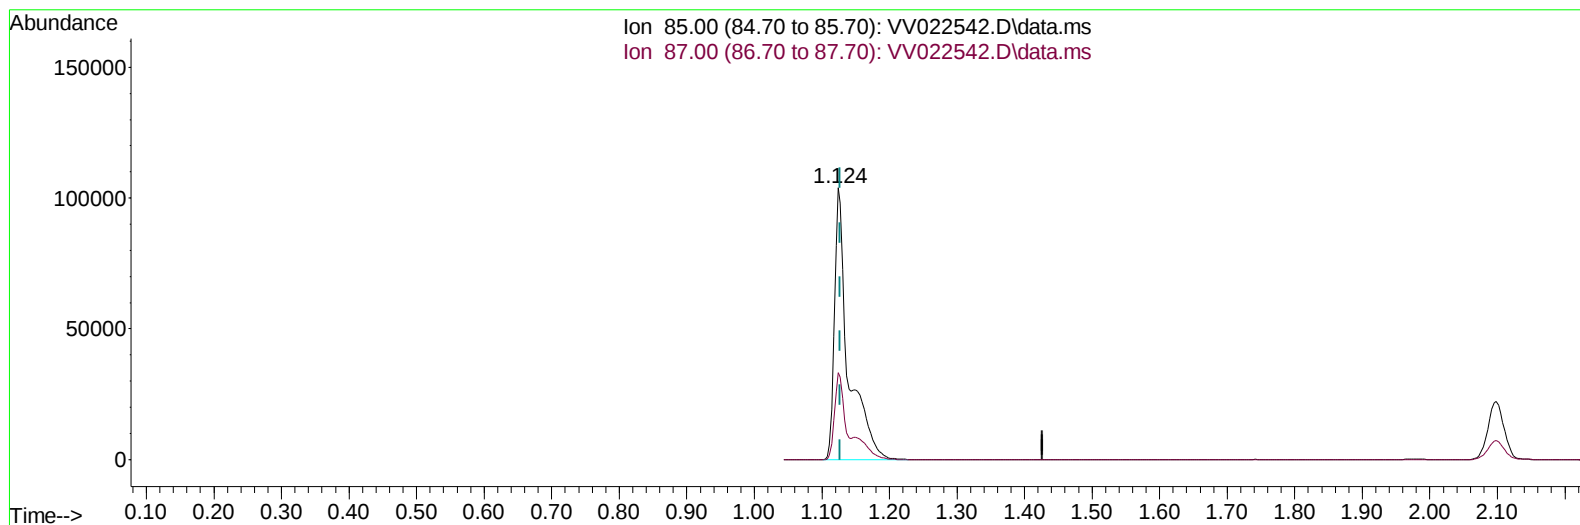

TIC: VV022542.D\data.ms

(2) Dichlorodifluoromethane (T)

1.124min (-0.003) 45.36 ug/L m

response 149083

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 85.00 | 100.00 | 100.00 |
| 87.00 | 32.20  | 23.10# |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV100221\  
Data File : VV022542.D  
Acq On : 03 Oct 2021 04:22  
Operator : SY/MD  
Sample : M3974-05MEMSD  
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA\_V/MEOH  
ALS Vial : 44 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
EW8Y9MEMSD

Manual Integrations  
APPROVED

MMDadoda  
10/6/2021 2:30:22 PM

Quant Time: Oct 04 04:32:31 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM100121WMA.M  
Quant Title : VOC Analysis  
QLast Update : Mon Oct 04 04:27:20 2021  
Response via : Initial Calibration

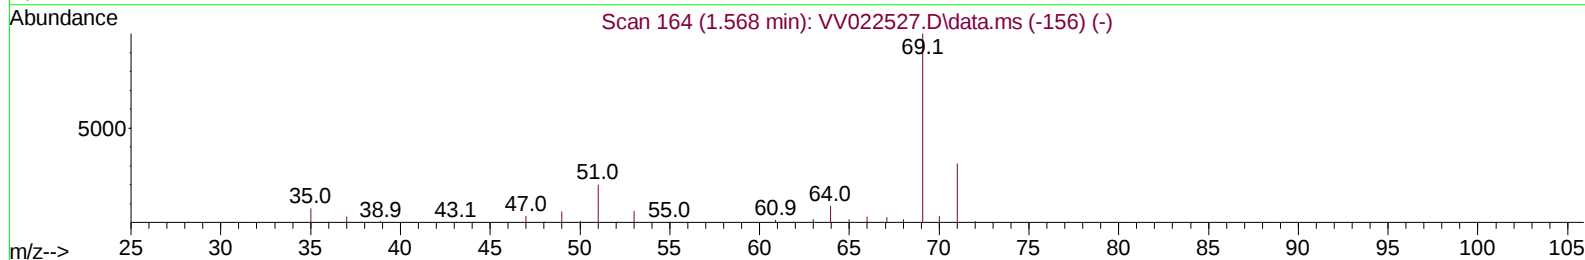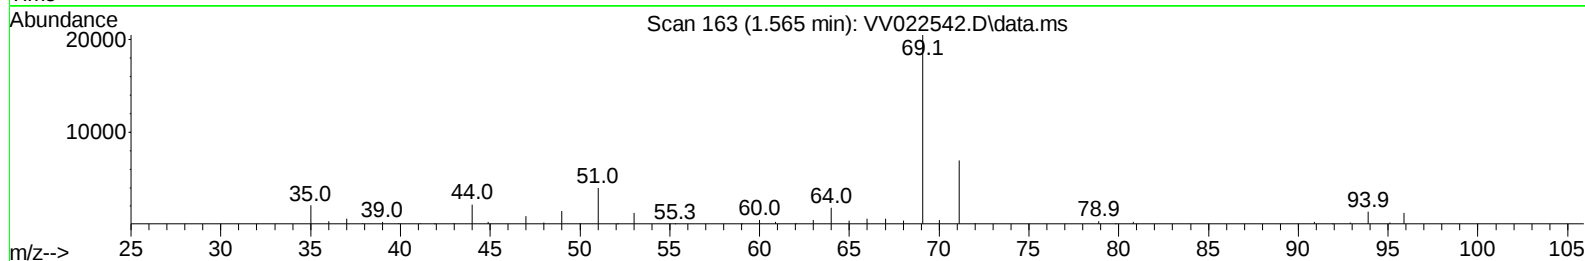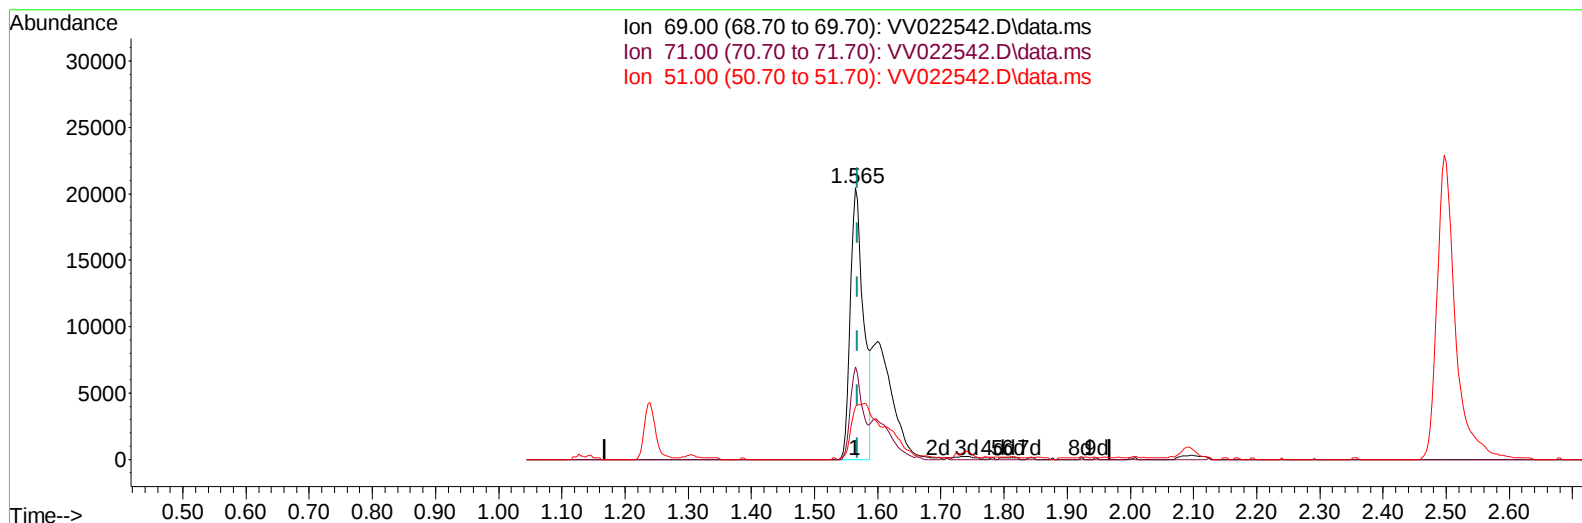

TIC: VV022542.D\data.ms

(7) Chloroethane-d5 (S)

1.565min (-0.003) 18.47 ug/L

response 29511

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 69.00 | 100.00 | 100.00 |
| 71.00 | 32.90  | 31.44  |
| 51.00 | 27.70  | 13.78# |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV100221\  
 Data File : VV022542.D  
 Acq On : 03 Oct 2021 04:22  
 Operator : SY/MD  
 Sample : M3974-05MEMSD  
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA\_V/MEOH  
 ALS Vial : 44 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 EW8Y9MEMSD

Manual Integrations  
 APPROVED

MMDadoda  
 10/6/2021 2:30:22 PM

Quant Time: Oct 04 04:32:31 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM100121WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Mon Oct 04 04:27:20 2021  
 Response via : Initial Calibration

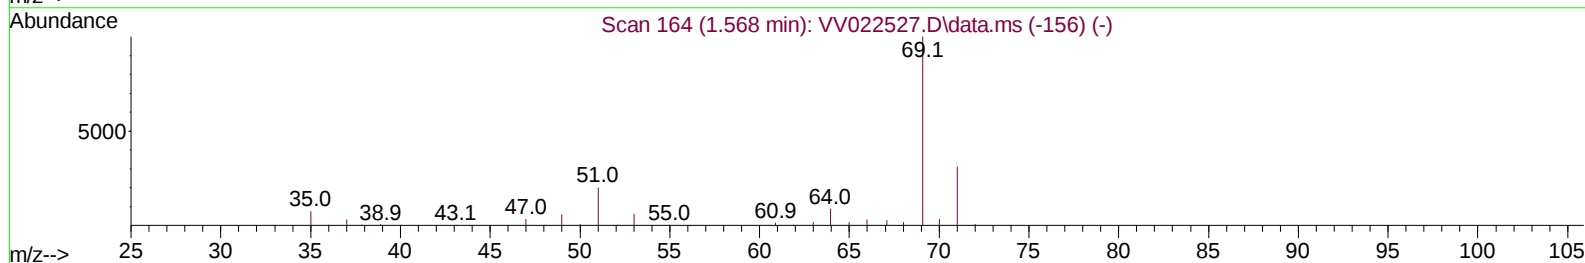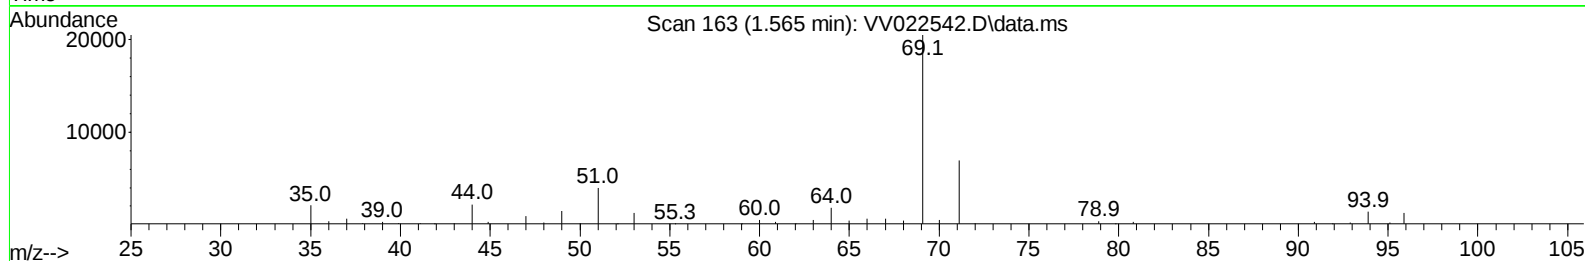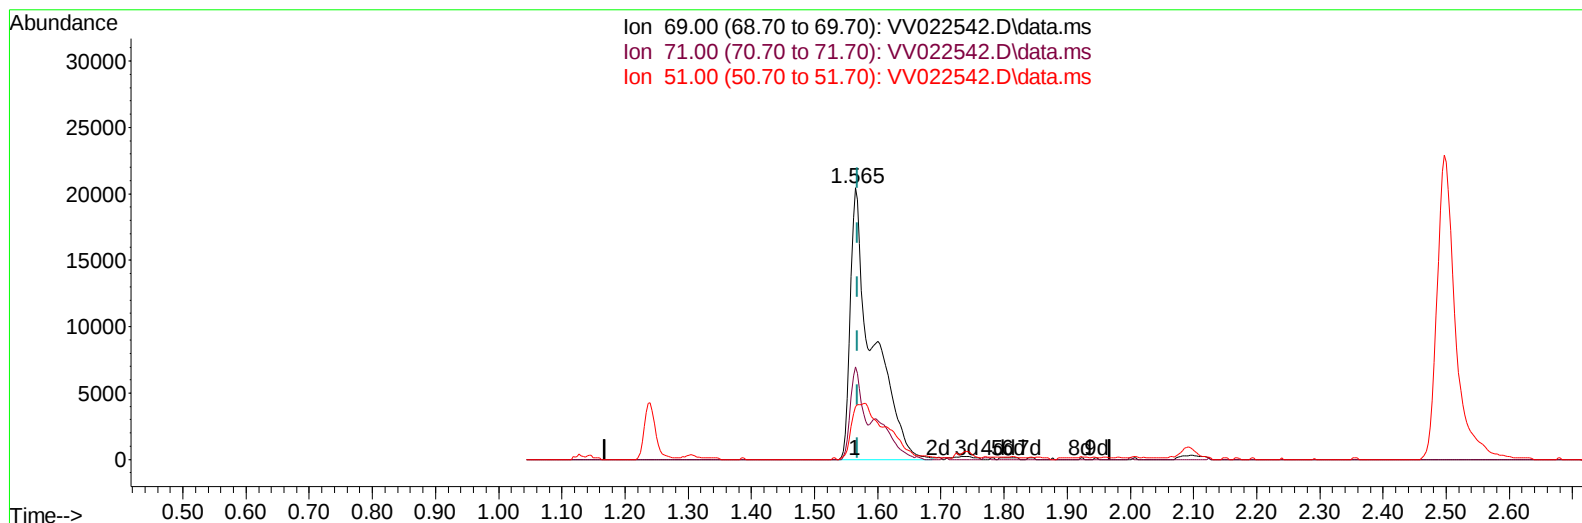

TIC: VV022542.D\data.ms

(7) Chloroethane-d5 (S)

1.565min (-0.003) 31.30 ug/L m

response 50007

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 69.00 | 100.00 | 100.00 |
| 71.00 | 32.90  | 18.55# |
| 51.00 | 27.70  | 8.13#  |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV100221\  
 Data File : VV022542.D  
 Acq On : 03 Oct 2021 04:22  
 Operator : SY/MD  
 Sample : M3974-05MEMSD  
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA\_V/MEOH  
 ALS Vial : 44 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 EW8Y9MEMSD

Manual Integrations  
 APPROVED

MMDadoda  
 10/6/2021 2:30:22 PM

Quant Time: Oct 04 04:32:31 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM100121WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Mon Oct 04 04:27:20 2021  
 Response via : Initial Calibration

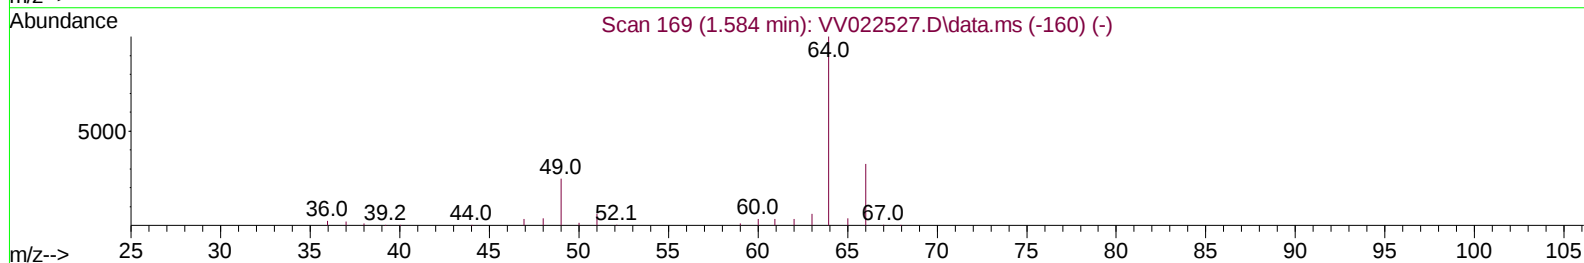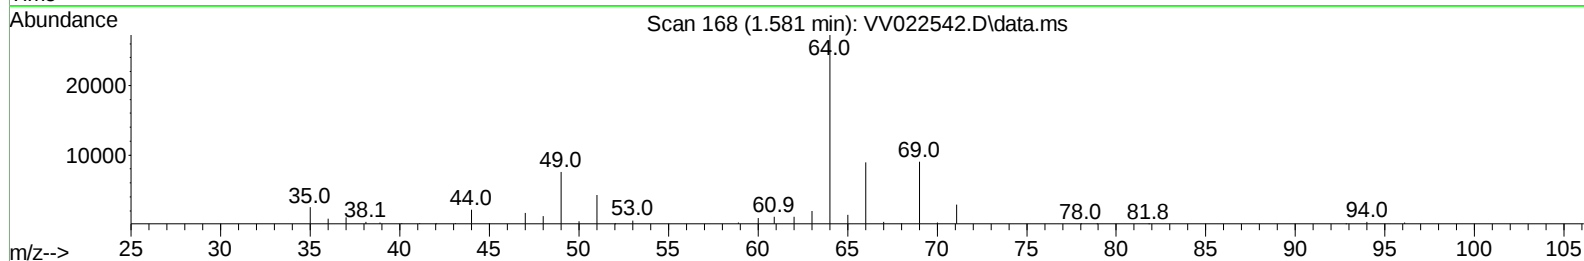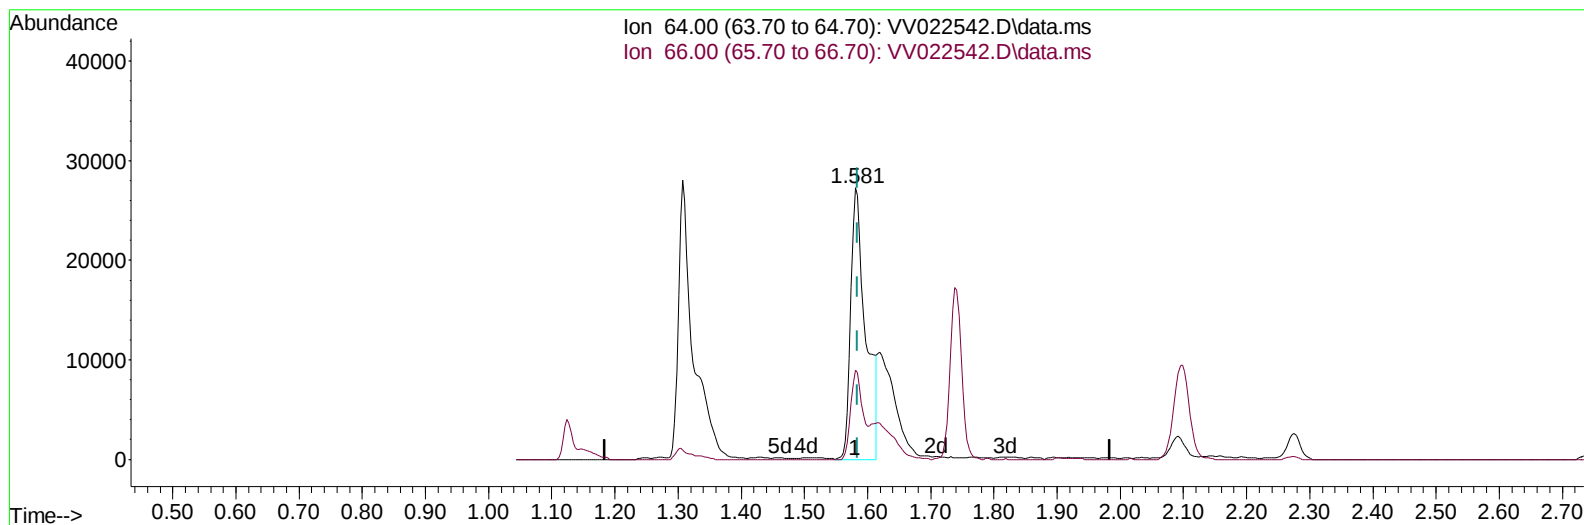

TIC: VV022542.D\data.ms

**(8) Chloroethane (T)**

**1.581min (-0.003) 23.65 ug/L**

**response 44676**

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 64.00 | 100.00 | 100.00 |
| 66.00 | 32.50  | 32.98  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV100221\  
 Data File : VV022542.D  
 Acq On : 03 Oct 2021 04:22  
 Operator : SY/MD  
 Sample : M3974-05MEMSD  
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA\_V/MEOH  
 ALS Vial : 44 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 EW8Y9MEMSD

Manual Integrations  
 APPROVED

MMDadoda  
 10/6/2021 2:30:22 PM

Quant Time: Oct 04 04:32:31 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM100121WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Mon Oct 04 04:27:20 2021  
 Response via : Initial Calibration

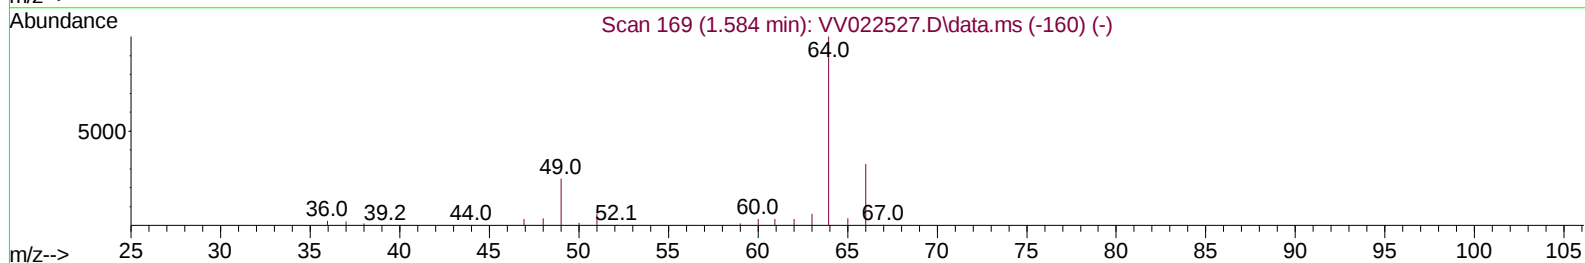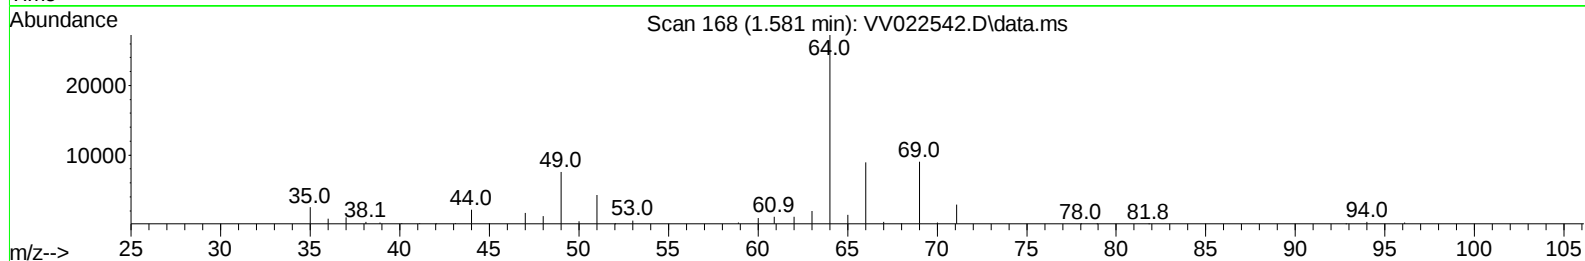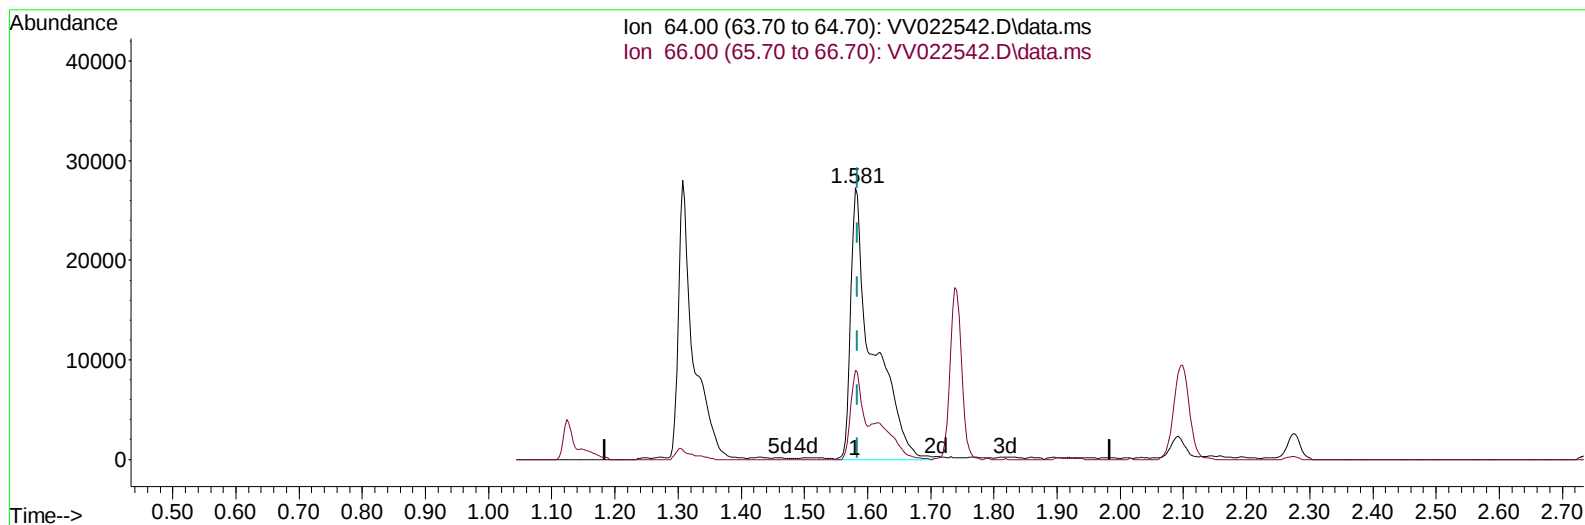

TIC: VV022542.D\data.ms

# (8) Chloroethane (T)

1.581min (-0.003) 35.01 ug/L m

response 66153

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 64.00 | 100.00 | 100.00 |
| 66.00 | 32.50  | 32.98  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV100221\  
 Data File : VV022542.D  
 Acq On : 03 Oct 2021 04:22  
 Operator : SY/MD  
 Sample : M3974-05MEMSD  
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA\_V/MEOH  
 ALS Vial : 44 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 EW8Y9MEMSD

Manual Integrations  
 APPROVED

MMDadoda  
 10/6/2021 2:30:22 PM

Quant Time: Oct 04 04:32:31 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM100121WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Mon Oct 04 04:27:20 2021  
 Response via : Initial Calibration

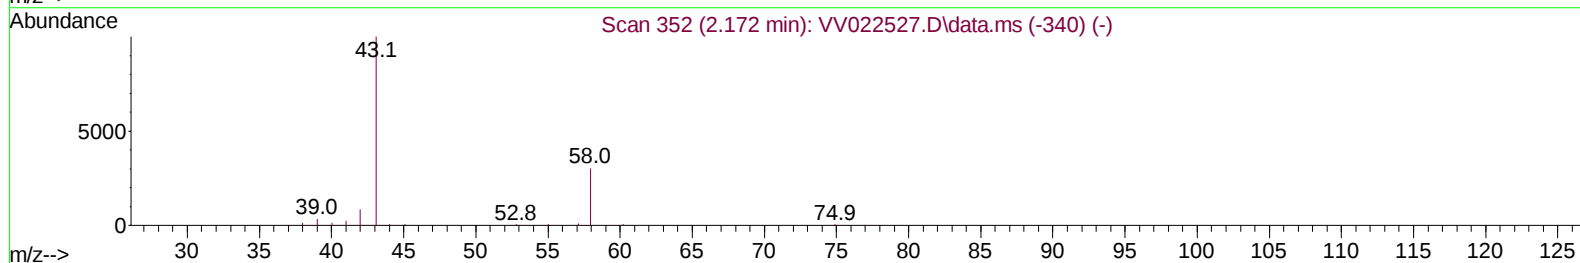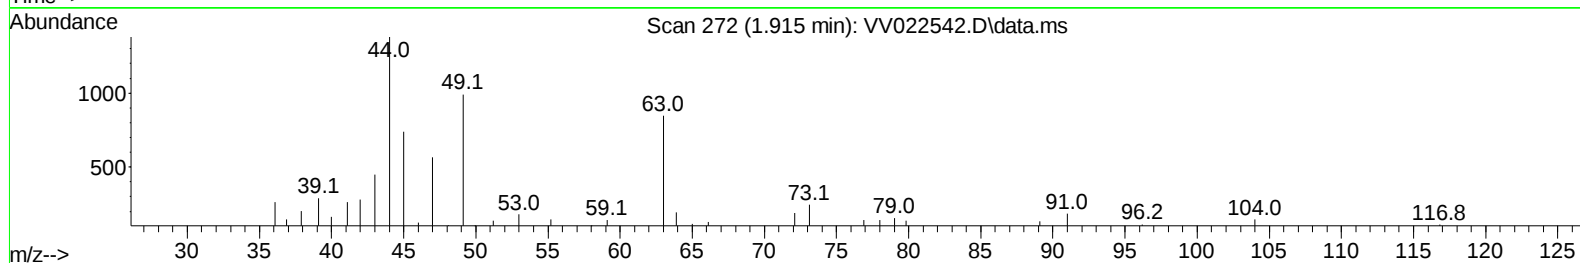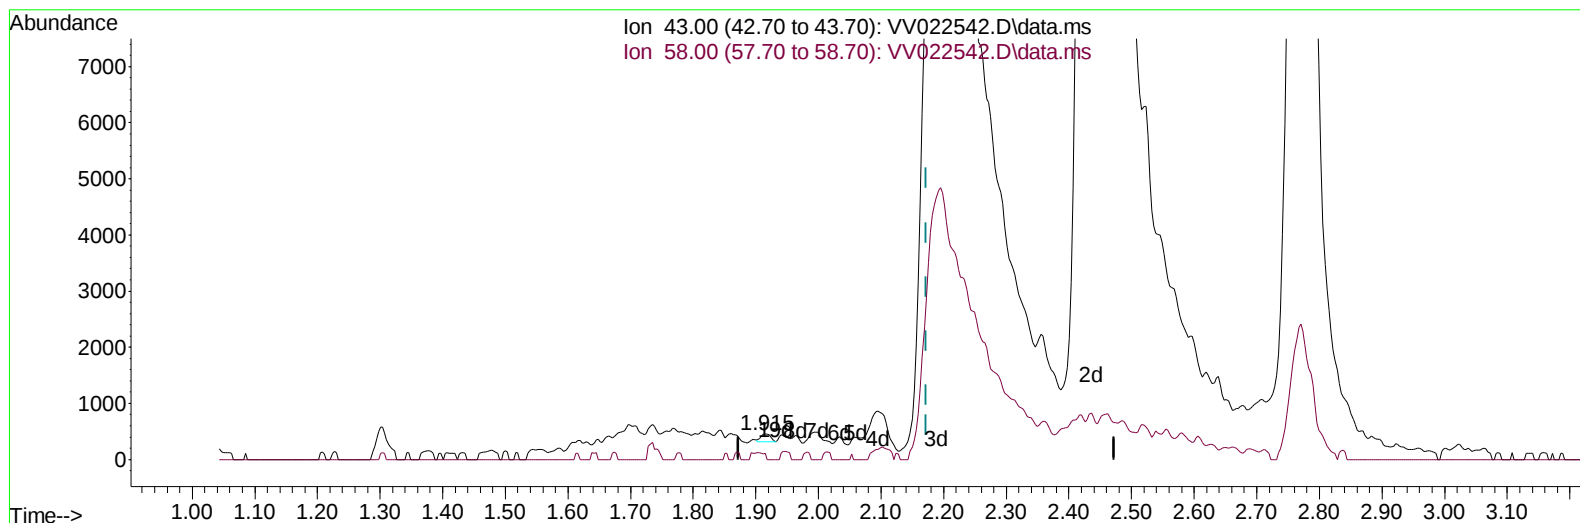

TIC: VV022542.D\data.ms

(13) Acetone (T)

1.915min (-0.257) 0.11 ug/L

response 160

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.00 | 100.00 | 100.00 |
| 58.00 | 10.60  | 12.50  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV100221\  
 Data File : VV022542.D  
 Acq On : 03 Oct 2021 04:22  
 Operator : SY/MD  
 Sample : M3974-05MEMSD  
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA\_V/MEOH  
 ALS Vial : 44 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 EW8Y9MEMSD

Manual Integrations  
 APPROVED

MMDadoda  
 10/6/2021 2:30:22 PM

Quant Time: Oct 04 04:32:31 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM100121WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Mon Oct 04 04:27:20 2021  
 Response via : Initial Calibration

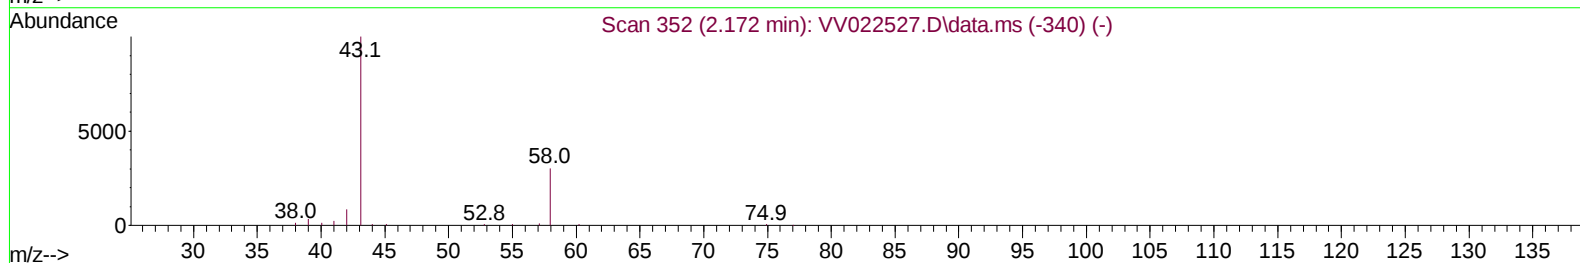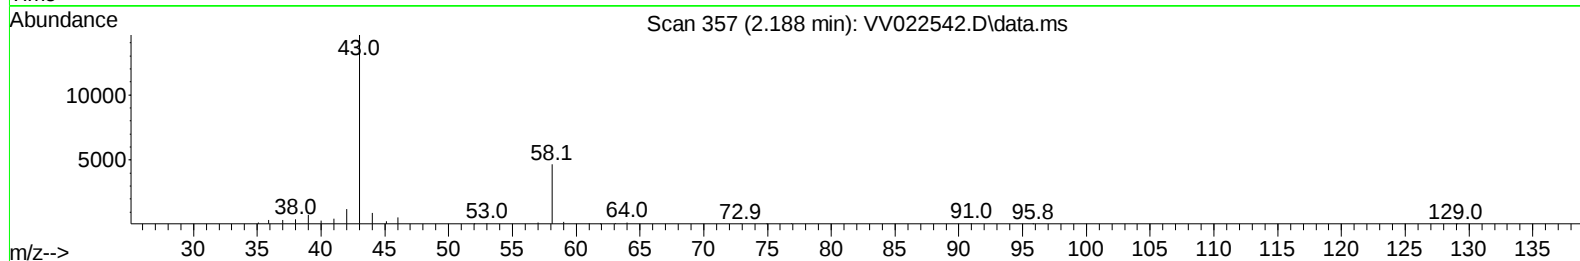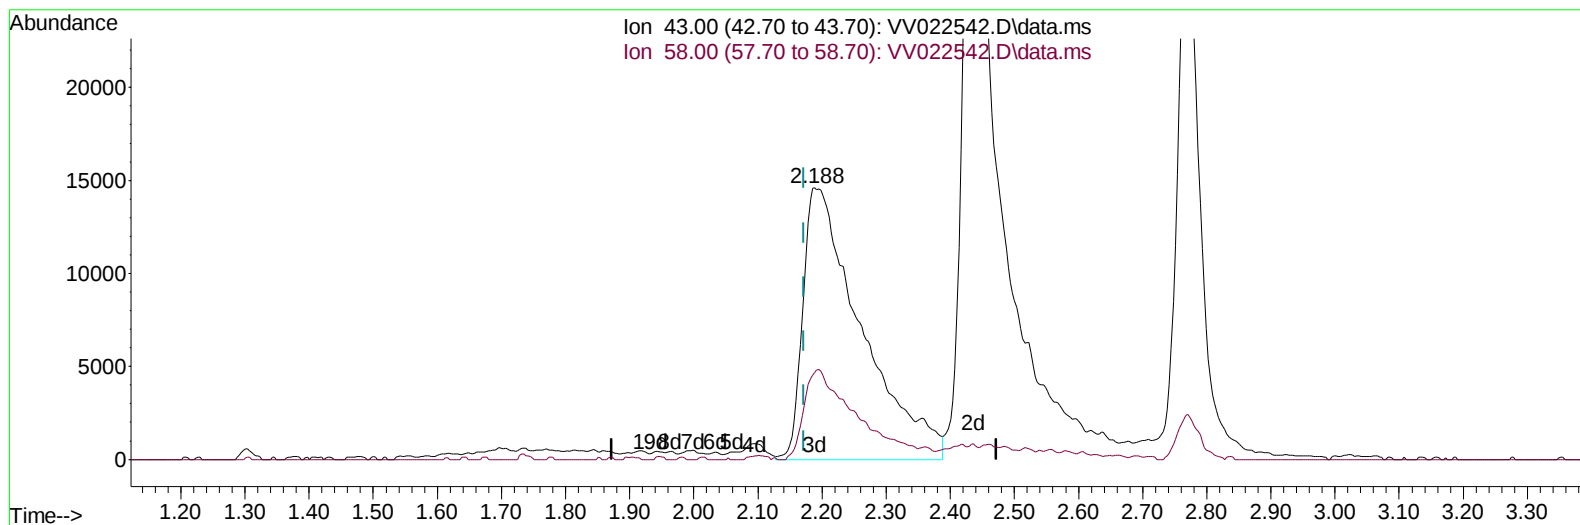

TIC: VV022542.D\data.ms

(13) Acetone (T)

2.188min (+ 0.016) 65.17 ug/L m

response 92097

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.00 | 100.00 | 100.00 |
| 58.00 | 10.60  | 0.02   |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV100221\  
 Data File : VV022542.D  
 Acq On : 03 Oct 2021 04:22  
 Operator : SY/MD  
 Sample : M3974-05MEMSD  
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA\_V/MEOH  
 ALS Vial : 44 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 EW8Y9MEMSD

Manual Integrations  
 APPROVED

MMDadoda  
 10/6/2021 2:30:22 PM

Quant Time: Oct 04 04:32:31 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM100121wMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Mon Oct 04 04:27:20 2021  
 Response via : Initial Calibration

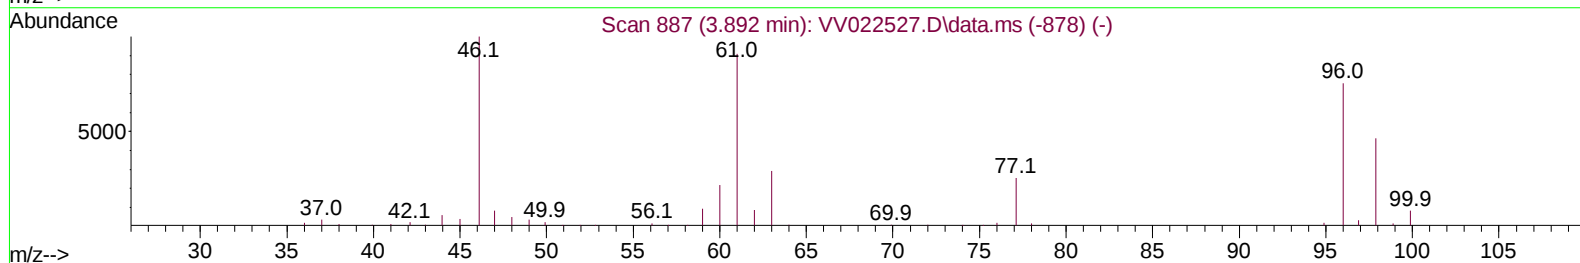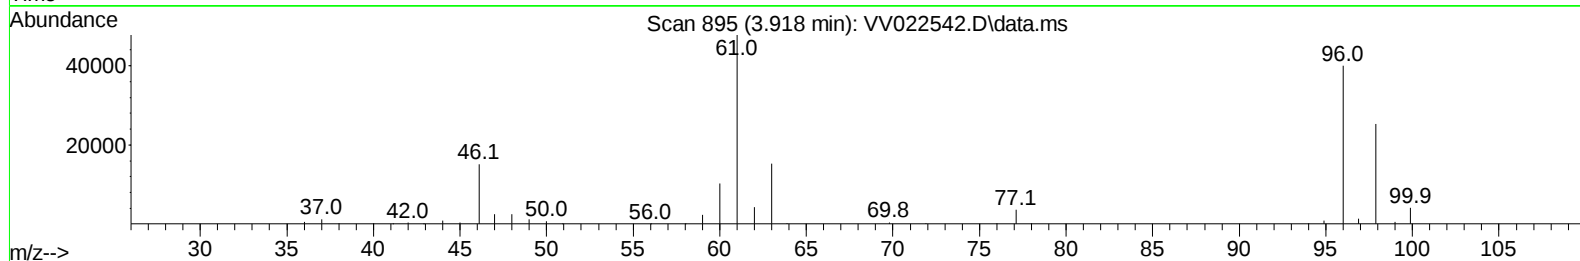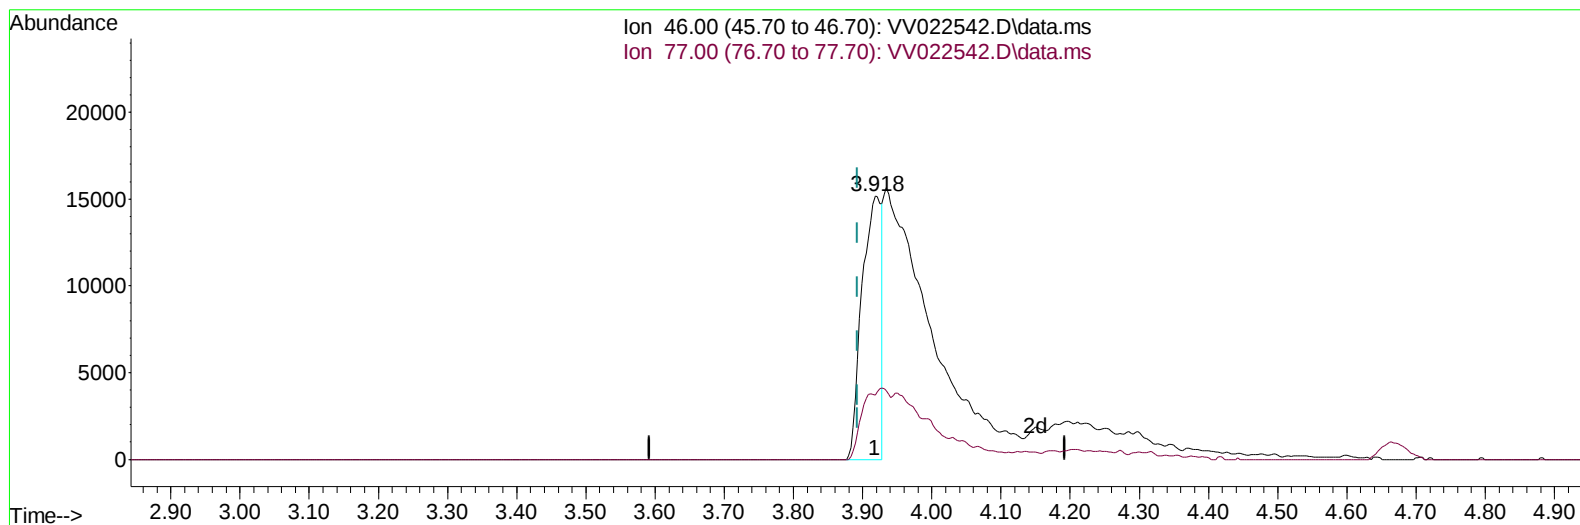

TIC: VV022542.D\data.ms

**(21) 2-Butanone-d5 (S)**

**3.918min (+ 0.026) 26.64 ug/L**

**response 29801**

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 46.00 | 100.00 | 100.00 |
| 77.00 | 26.40  | 19.15  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV100221\  
Data File : VV022542.D  
Acq On : 03 Oct 2021 04:22  
Operator : SY/MD  
Sample : M3974-05MEMSD  
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA\_V/MEOH  
ALS Vial : 44 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
EW8Y9MEMSD

Manual Integrations  
APPROVED

MMDadoda  
10/6/2021 2:30:22 PM

Quant Time: Oct 04 04:32:31 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM100121WMA.M  
Quant Title : VOC Analysis  
QLast Update : Mon Oct 04 04:27:20 2021  
Response via : Initial Calibration

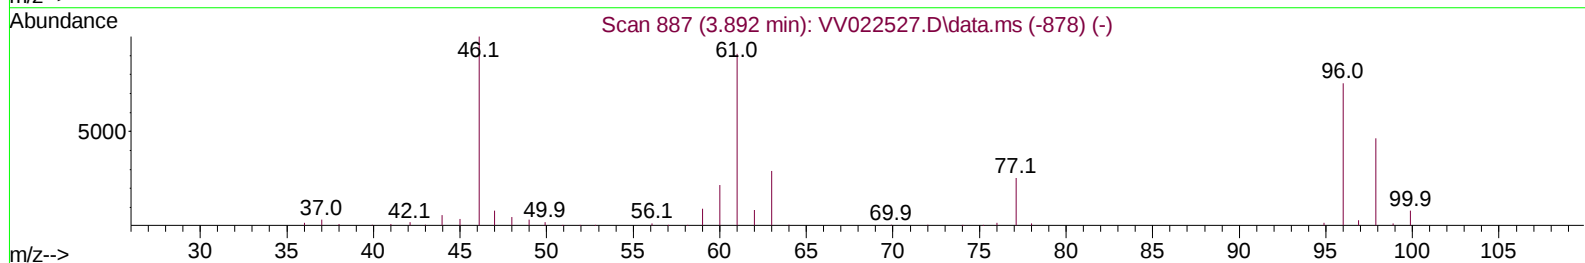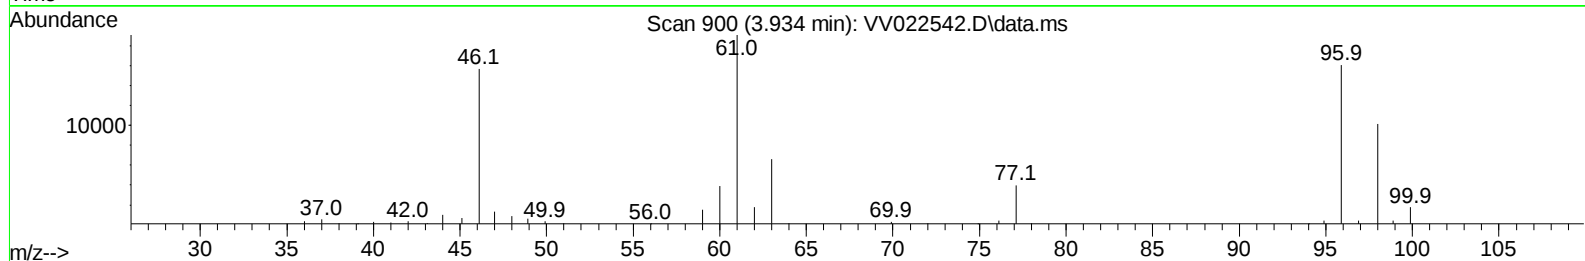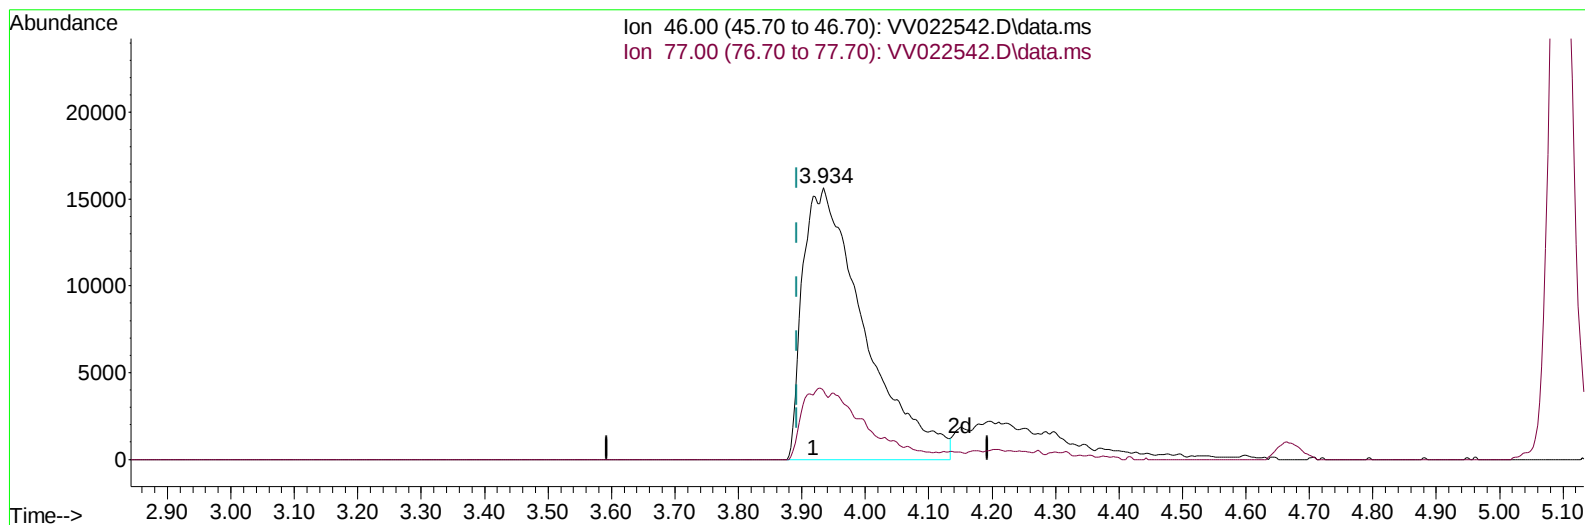

TIC: VV022542.D\data.ms

(21) 2-Butanone-d5 (S)

3.934min (+ 0.042) 93.98 ug/L m

response 105148

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 46.00 | 100.00 | 100.00 |
| 77.00 | 26.40  | 5.43#  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV100221\  
 Data File : VV022542.D  
 Acq On : 03 Oct 2021 04:22  
 Operator : SY/MD  
 Sample : M3974-05MEMSD  
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA\_V/MEOH  
 ALS Vial : 44 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 EW8Y9MEMSD

Manual Integrations  
 APPROVED

MMDadoda  
 10/6/2021 2:30:22 PM

Quant Time: Oct 04 04:32:31 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM100121WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Mon Oct 04 04:27:20 2021  
 Response via : Initial Calibration

| Compound                      | R.T.     | QIon  | Response   | Conc     | Units  | Dev(Min) |
|-------------------------------|----------|-------|------------|----------|--------|----------|
| -----                         |          |       |            |          |        |          |
| Internal Standards            |          |       |            |          |        |          |
| 1) 1,4-Difluorobenzene        | 5.616    | 114   | 328644     | 50.000   | ug/L   | 0.00     |
| 28) Chlorobenzene-d5          | 8.857    | 117   | 310904     | 50.000   | ug/L   | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.256   | 152   | 162595     | 50.000   | ug/L   | 0.00     |
| System Monitoring Compounds   |          |       |            |          |        |          |
| 4) Vinyl Chloride-d3          | 1.304    | 65    | 73650      | 36.236   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 60 | - 135 | Recovery = | 72.480%  |        |          |
| 7) Chloroethane-d5            | 1.565    | 69    | 50007m     | 31.299   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 | - 130 | Recovery = | 62.600%# |        |          |
| 11) 1,1-Dichloroethene-d2     | 2.092    | 63    | 141239     | 35.242   | ug/L   | -0.02    |
| Spiked Amount 50.000          | Range 60 | - 125 | Recovery = | 70.480%  |        |          |
| 21) 2-Butanone-d5             | 3.934    | 46    | 105148m    | 93.983   | ug/L   | 0.04     |
| Spiked Amount 100.000         | Range 40 | - 130 | Recovery = | 93.980%  |        |          |
| 24) Chloroform-d              | 4.349    | 84    | 157647     | 42.452   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 | - 125 | Recovery = | 84.900%  |        |          |
| 26) 1,2-Dichloroethane-d4     | 5.034    | 65    | 94154      | 43.708   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 | - 125 | Recovery = | 87.420%  |        |          |
| 32) Benzene-d6                | 5.047    | 84    | 314547     | 43.671   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 | - 125 | Recovery = | 87.340%  |        |          |
| 36) 1,2-Dichloropropane-d6    | 6.069    | 67    | 95511      | 43.075   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 | - 120 | Recovery = | 86.160%  |        |          |
| 41) Toluene-d8                | 7.317    | 98    | 293252     | 44.386   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 80 | - 120 | Recovery = | 88.780%  |        |          |
| 43) trans-1,3-Dichloroprop... | 7.625    | 79    | 46326      | 44.159   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 60 | - 125 | Recovery = | 88.320%  |        |          |
| 47) 2-Hexanone-d5             | 8.111    | 63    | 84459      | 91.950   | ug/L   | 0.02     |
| Spiked Amount 100.000         | Range 45 | - 130 | Recovery = | 91.950%  |        |          |
| 56) 1,1,2,2-Tetrachloroeth... | 10.223   | 84    | 130746     | 42.405   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 65 | - 120 | Recovery = | 84.800%  |        |          |
| 66) 1,2-Dichlorobenzene-d4    | 11.628   | 152   | 117834     | 44.440   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 80 | - 120 | Recovery = | 88.880%  |        |          |
| Target Compounds              |          |       |            |          |        |          |
|                               |          |       |            |          | Qvalue |          |
| 2) Dichlorodifluoromethane    | 1.124    | 85    | 149083m    | 45.359   | ug/L   |          |
| 3) Chloromethane              | 1.237    | 50    | 141418     | 43.269   | ug/L   | 100      |
| 5) Vinyl chloride             | 1.307    | 62    | 138599     | 44.738   | ug/L   | 99       |
| 6) Bromomethane               | 1.520    | 94    | 72415      | 33.478   | ug/L   | 99       |
| 8) Chloroethane               | 1.581    | 64    | 66153m     | 35.012   | ug/L   |          |
| 9) Trichlorofluoromethane     | 1.741    | 101   | 168544     | 39.610   | ug/L   | 100      |
| 10) 1,1,2-Trichloro-1,2,2-... | 2.098    | 101   | 80761      | 33.529   | ug/L   | 97       |
| 12) 1,1-Dichloroethene        | 2.098    | 96    | 82889      | 36.106   | ug/L   | 94       |
| 13) Acetone                   | 2.188    | 43    | 92097m     | 65.165   | ug/L   |          |
| 14) Carbon disulfide          | 2.275    | 76    | 264569     | 38.151   | ug/L   | 99       |
| 15) Methyl Acetate            | 2.436    | 43    | 125915     | 48.839   | ug/L   | 97       |
| 16) Methylene chloride        | 2.497    | 84    | 127966     | 44.366   | ug/L   | 97       |
| 17) trans-1,2-Dichloroethene  | 2.748    | 96    | 118370     | 46.971   | ug/L   | 98       |
| 18) Methyl tert-butyl Ether   | 2.770    | 73    | 382918     | 49.216   | ug/L   | 98       |
| 19) 1,1-Dichloroethane        | 3.182    | 63    | 204379     | 45.835   | ug/L   | 98       |
| 20) cis-1,2-Dichloroethene    | 3.905    | 96    | 125853     | 46.877   | ug/L   | 97       |
| 22) 2-Butanone                | 3.999    | 43    | 143591     | 77.163   | ug/L # | 57       |
| 23) Bromochloromethane        | 4.246    | 128   | 67965      | 46.079   | ug/L   | 93       |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV100221\  
 Data File : VV022542.D  
 Acq On : 03 Oct 2021 04:22  
 Operator : SY/MD  
 Sample : M3974-05MEMSD  
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA\_V/MEOH  
 ALS Vial : 44 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 EW8Y9MEMSD

Manual Integrations  
 APPROVED

MMDadoda  
 10/6/2021 2:30:22 PM

Quant Time: Oct 04 04:32:31 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM100121WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Mon Oct 04 04:27:20 2021  
 Response via : Initial Calibration

| Compound                      | R.T.   | QIon | Response | Conc   | Units  | Dev(Min) |
|-------------------------------|--------|------|----------|--------|--------|----------|
| 25) Chloroform                | 4.375  | 83   | 209639   | 46.721 | ug/L   | 99       |
| 27) 1,2-Dichloroethane        | 5.130  | 62   | 152859   | 47.046 | ug/L   | 98       |
| 29) Cyclohexane               | 4.671  | 56   | 181191   | 49.999 | ug/L   | 99       |
| 30) 1,1,1-Trichloroethane     | 4.603  | 97   | 186747   | 48.084 | ug/L   | 99       |
| 31) Carbon tetrachloride      | 4.822  | 117  | 162475   | 47.620 | ug/L   | 98       |
| 33) Benzene                   | 5.095  | 78   | 456338   | 47.537 | ug/L   | 100      |
| 34) Trichloroethene           | 5.912  | 95   | 222083   | 88.604 | ug/L   | 99       |
| 35) Methylcyclohexane         | 6.127  | 83   | 183294   | 48.228 | ug/L   | 98       |
| 37) 1,2-Dichloropropane       | 6.175  | 63   | 114193   | 46.461 | ug/L   | 100      |
| 38) Bromodichloromethane      | 6.513  | 83   | 148124   | 46.396 | ug/L   | 97       |
| 39) cis-1,3-Dichloropropene   | 7.027  | 75   | 175139   | 47.381 | ug/L   | 99       |
| 40) 4-Methyl-2-pentanone      | 7.236  | 43   | 328821   | 95.214 | ug/L   | 96       |
| 42) Toluene                   | 7.387  | 91   | 487479   | 48.207 | ug/L   | 100      |
| 44) trans-1,3-Dichloropropene | 7.654  | 75   | 164071   | 46.102 | ug/L   | 99       |
| 45) 1,1,2-Trichloroethane     | 7.844  | 97   | 118102   | 46.419 | ug/L   | 98       |
| 46) Tetrachloroethene         | 7.976  | 164  | 97902    | 46.657 | ug/L   | 98       |
| 48) 2-Hexanone                | 8.156  | 43   | 243151   | 92.056 | ug/L # | 94       |
| 49) Dibromochloromethane      | 8.249  | 129  | 130536   | 47.411 | ug/L   | 99       |
| 50) 1,2-Dibromoethane         | 8.355  | 107  | 127728   | 46.628 | ug/L   | 97       |
| 51) Chlorobenzene             | 8.886  | 112  | 321120   | 47.742 | ug/L   | 99       |
| 52) Ethylbenzene              | 9.014  | 91   | 524266   | 49.814 | ug/L   | 100      |
| 53) m,p-Xylene                | 9.140  | 106  | 206069   | 49.420 | ug/L   | 100      |
| 54) o-Xylene                  | 9.548  | 106  | 203223   | 50.024 | ug/L   | 99       |
| 55) Styrene                   | 9.567  | 104  | 347640   | 49.865 | ug/L   | 98       |
| 57) 1,1,2,2-Tetrachloroethane | 10.249 | 83   | 176743   | 44.946 | ug/L   | 98       |
| 59) Bromoform                 | 9.738  | 173  | 94885    | 47.195 | ug/L   | 99       |
| 60) Isopropylbenzene          | 9.934  | 105  | 533197   | 51.542 | ug/L   | 100      |
| 61) 1,2,3-Trichloropropane    | 10.281 | 75   | 142028   | 45.931 | ug/L   | 99       |
| 62) 1,3,5-Trimethylbenzene    | 10.542 | 105  | 459486   | 52.753 | ug/L   | 100      |
| 63) 1,2,4-Trimethylbenzene    | 10.918 | 105  | 456410   | 52.710 | ug/L   | 100      |
| 64) 1,3-Dichlorobenzene       | 11.185 | 146  | 255857   | 48.750 | ug/L   | 99       |
| 65) 1,4-Dichlorobenzene       | 11.278 | 146  | 254131   | 46.624 | ug/L   | 98       |
| 67) 1,2-Dichlorobenzene       | 11.648 | 146  | 256898   | 47.897 | ug/L   | 99       |
| 68) 1,2-Dibromo-3-chloropr... | 12.432 | 75   | 38233    | 45.128 | ug/L   | 99       |
| 69) 1,3,5-Trichlorobenzene    | 12.648 | 180  | 185724   | 47.626 | ug/L   | 100      |
| 70) 1,2,4-trichlorobenzene    | 13.265 | 180  | 166997   | 47.622 | ug/L   | 98       |
| 71) Naphthalene               | 13.503 | 128  | 565677   | 48.989 | ug/L   | 100      |
| 72) 1,2,3-Trichlorobenzene    | 13.747 | 180  | 170544   | 47.054 | ug/L   | 99       |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

MMDadoda  
10/6/2021 2:30:22 PM

[illegible]