




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022545.D
 Acq On : 03 Oct 2021 05:33
 Operator : SY/MD
 Sample : M3974-09ME 10X
 Misc : 5.08g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW8Z3ME

Manual Integrations
 APPROVED

MMDadoda
 10/6/2021 2:30:33 PM

Quant Time: Oct 04 04:33:15 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Oct 04 04:27:20 2021
 Response via : Initial Calibration

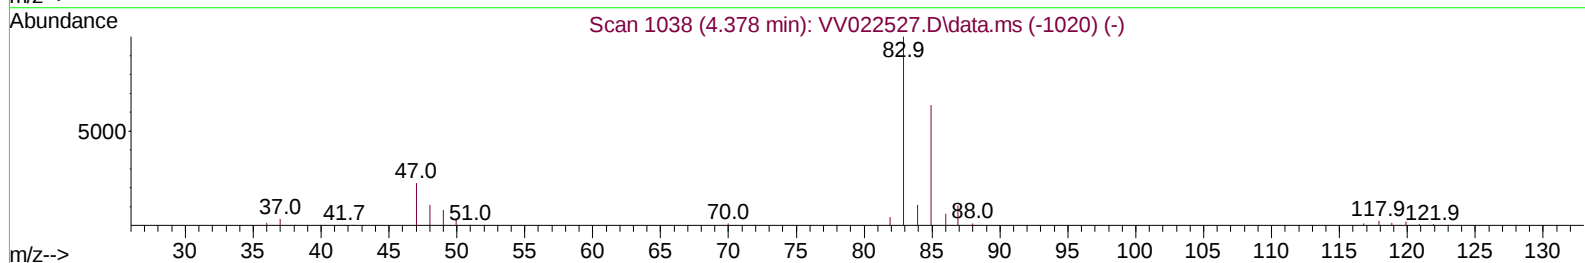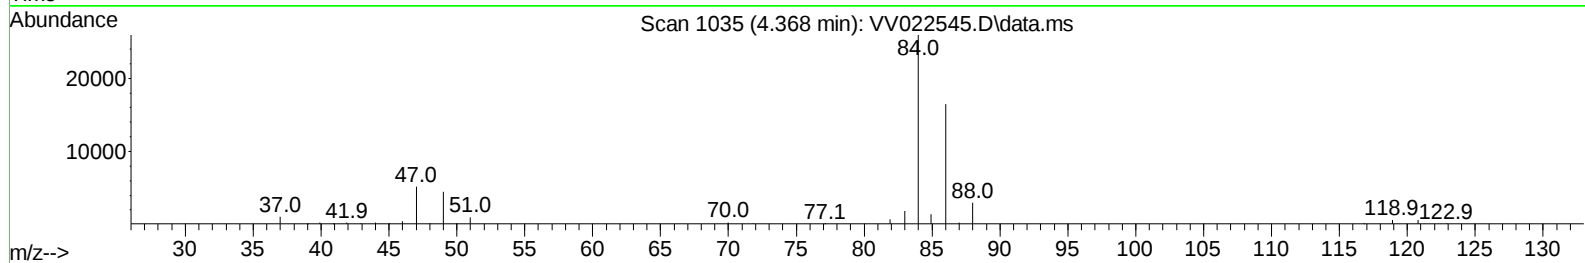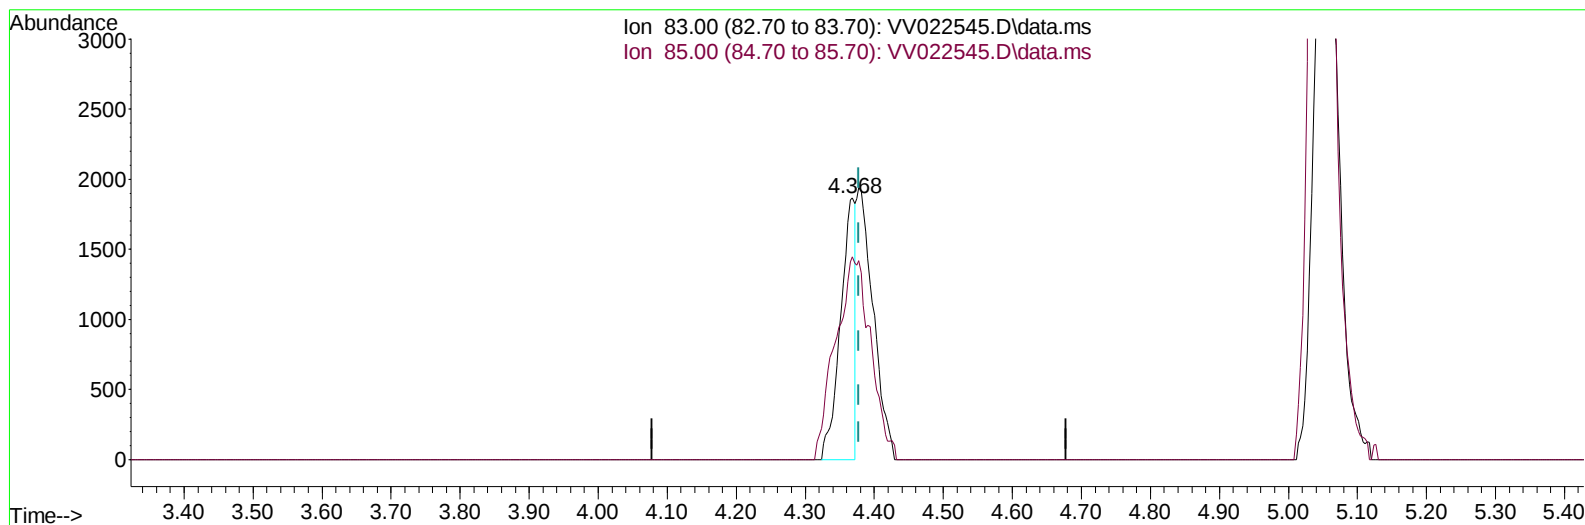

TIC: VV022545.D\data.ms

(25) Chloroform (T)

4.368min (-0.010) 0.67 ug/L

response 2713

Ion	Exp%	Act%
83.00	100.00	100.00
85.00	65.40	77.64
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022545.D
Acq On : 03 Oct 2021 05:33
Operator : SY/MD
Sample : M3974-09ME 10X
Misc : 5.08g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW8Z3ME

Manual Integrations
APPROVED

MMDadoda
10/6/2021 2:30:33 PM

Quant Time: Oct 04 04:33:15 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Oct 04 04:27:20 2021
Response via : Initial Calibration

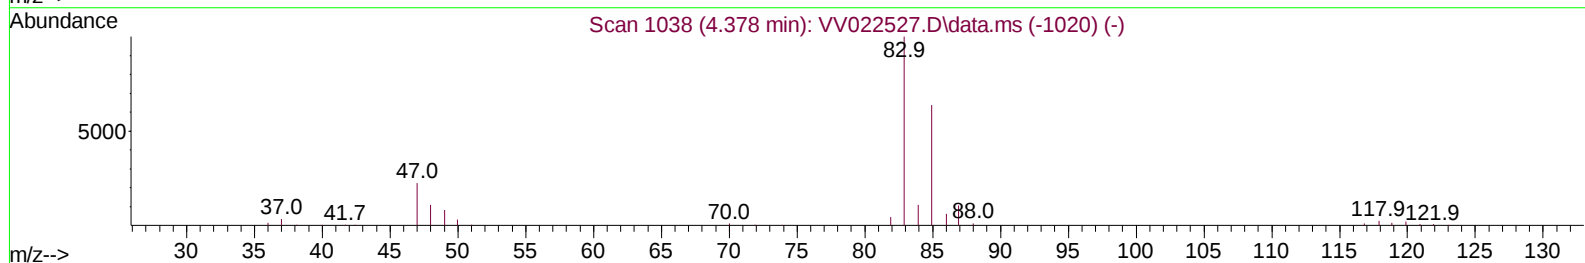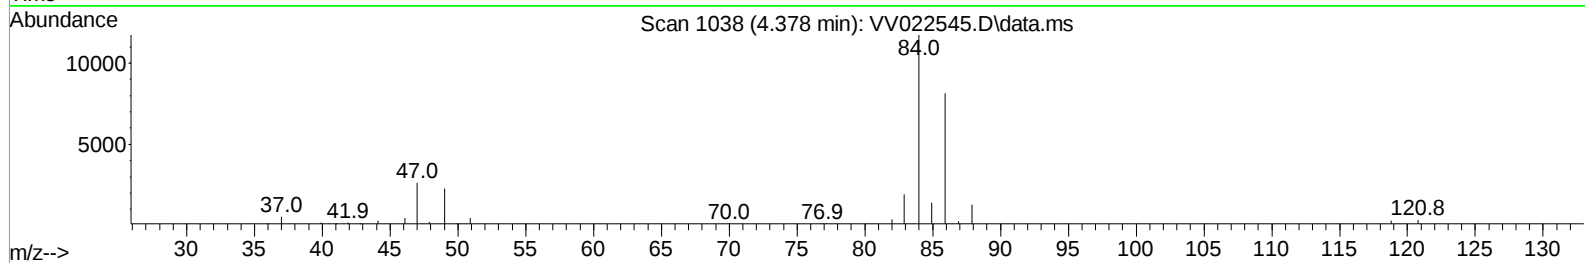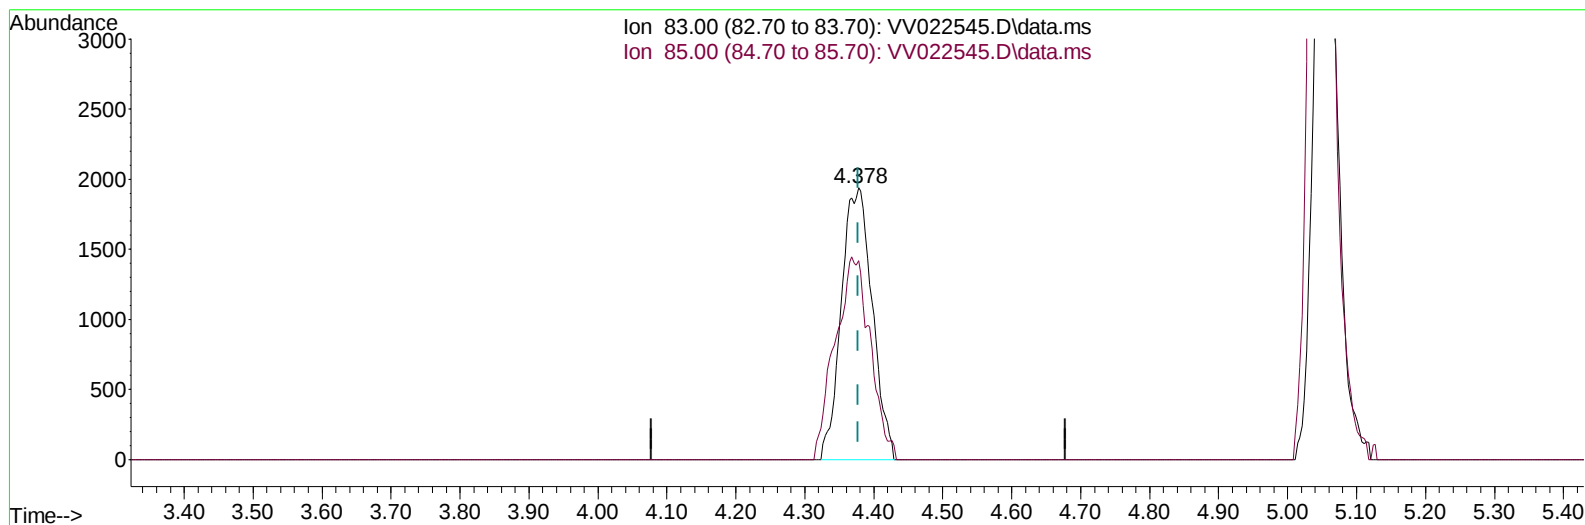

TIC: VV022545.D\data.ms

(25) Chloroform (T)

4.378min (-0.000) 1.48 ug/L m

response 6023

Ion	Exp%	Act%
83.00	100.00	100.00
85.00	65.40	73.12
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022545.D
 Acq On : 03 Oct 2021 05:33
 Operator : SY/MD
 Sample : M3974-09ME 10X
 Misc : 5.08g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW8Z3ME

Manual Integrations
 APPROVED

MMDadoda
 10/6/2021 2:30:33 PM

Quant Time: Oct 04 04:33:15 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Oct 04 04:27:20 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	297211	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	278877	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	136401	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	69504	37.812	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	75.620%	
7) Chloroethane-d5	1.564	69	53045	36.712	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	73.420%	
11) 1,1-Dichloroethene-d2	2.101	63	97815	26.988	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	53.980%#	
21) 2-Butanone-d5	3.895	46	80994	80.050	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	80.050%	
24) Chloroform-d	4.349	84	136971	40.785	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	81.580%	
26) 1,2-Dichloroethane-d4	5.034	65	85403	43.838	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	87.680%	
32) Benzene-d6	5.050	84	290803	45.011	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	90.020%	
36) 1,2-Dichloropropane-d6	6.072	67	89430	44.964	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	89.920%	
41) Toluene-d8	7.317	98	265245	44.758	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	89.520%	
43) trans-1,3-Dichloroprop...	7.625	79	35874	38.123	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	76.240%	
47) 2-Hexanone-d5	8.095	63	73265	88.923	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	88.920%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	116701	42.196	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	84.400%	
66) 1,2-Dichlorobenzene-d4	11.625	152	104080	46.791	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	93.580%	
Target Compounds						Qvalue
20) cis-1,2-Dichloroethene	3.912	96	5857	2.412	ug/L	99
25) Chloroform	4.378	83	6023m	1.484	ug/L	
34) Trichloroethene	5.915	95	32937	14.650	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022545.D
Acq On : 03 Oct 2021 05:33
Operator : SY/MD
Sample : M3974-09ME 10X
Misc : 5.08g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW8Z3ME

Manual Integrations
APPROVED

MMDadoda
10/6/2021 2:30:33 PM

Quant Time: Oct 04 04:33:15 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Oct 04 04:27:20 2021
Response via : Initial Calibration

