

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022505.D
 Acq On : 02 Oct 2021 12:24
 Operator : SY/MD
 Sample : VV1002WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK273

Quant Time: Oct 04 04:15:08 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Oct 04 04:08:39 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	236467	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	222778	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	103383	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	72811	49.787	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	99.580%		
7) Chloroethane-d5	1.565	69	58473	50.865	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	101.720%		
11) 1,1-Dichloroethene-d2	2.101	63	109047	37.816	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	75.640%		
21) 2-Butanone-d5	3.889	46	91902	114.163	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	114.160%		
24) Chloroform-d	4.343	84	122480	45.839	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.680%		
26) 1,2-Dichloroethane-d4	5.027	65	76731	49.504	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.000%		
32) Benzene-d6	5.043	84	255483	49.502	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.000%		
36) 1,2-Dichloropropane-d6	6.066	67	77844	48.995	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	97.980%		
41) Toluene-d8	7.314	98	228987	48.369	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.740%		
43) trans-1,3-Dichloroprop...	7.619	79	33818	44.988	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	89.980%		
47) 2-Hexanone-d5	8.088	63	56438	85.749	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	85.750%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	98010	44.362	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	88.720%		
66) 1,2-Dichlorobenzene-d4	11.625	152	88651	52.583	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	105.160%		
Target Compounds					Qvalue	
25) Chloroform	4.372	83	3434	1.064	ug/L	99
34) Trichloroethene	5.915	95	4918	2.738	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022505.D
Acq On : 02 Oct 2021 12:24
Operator : SY/MD
Sample : VV1002WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK273

Quant Time: Oct 04 04:15:08 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Oct 04 04:08:39 2021
Response via : Initial Calibration

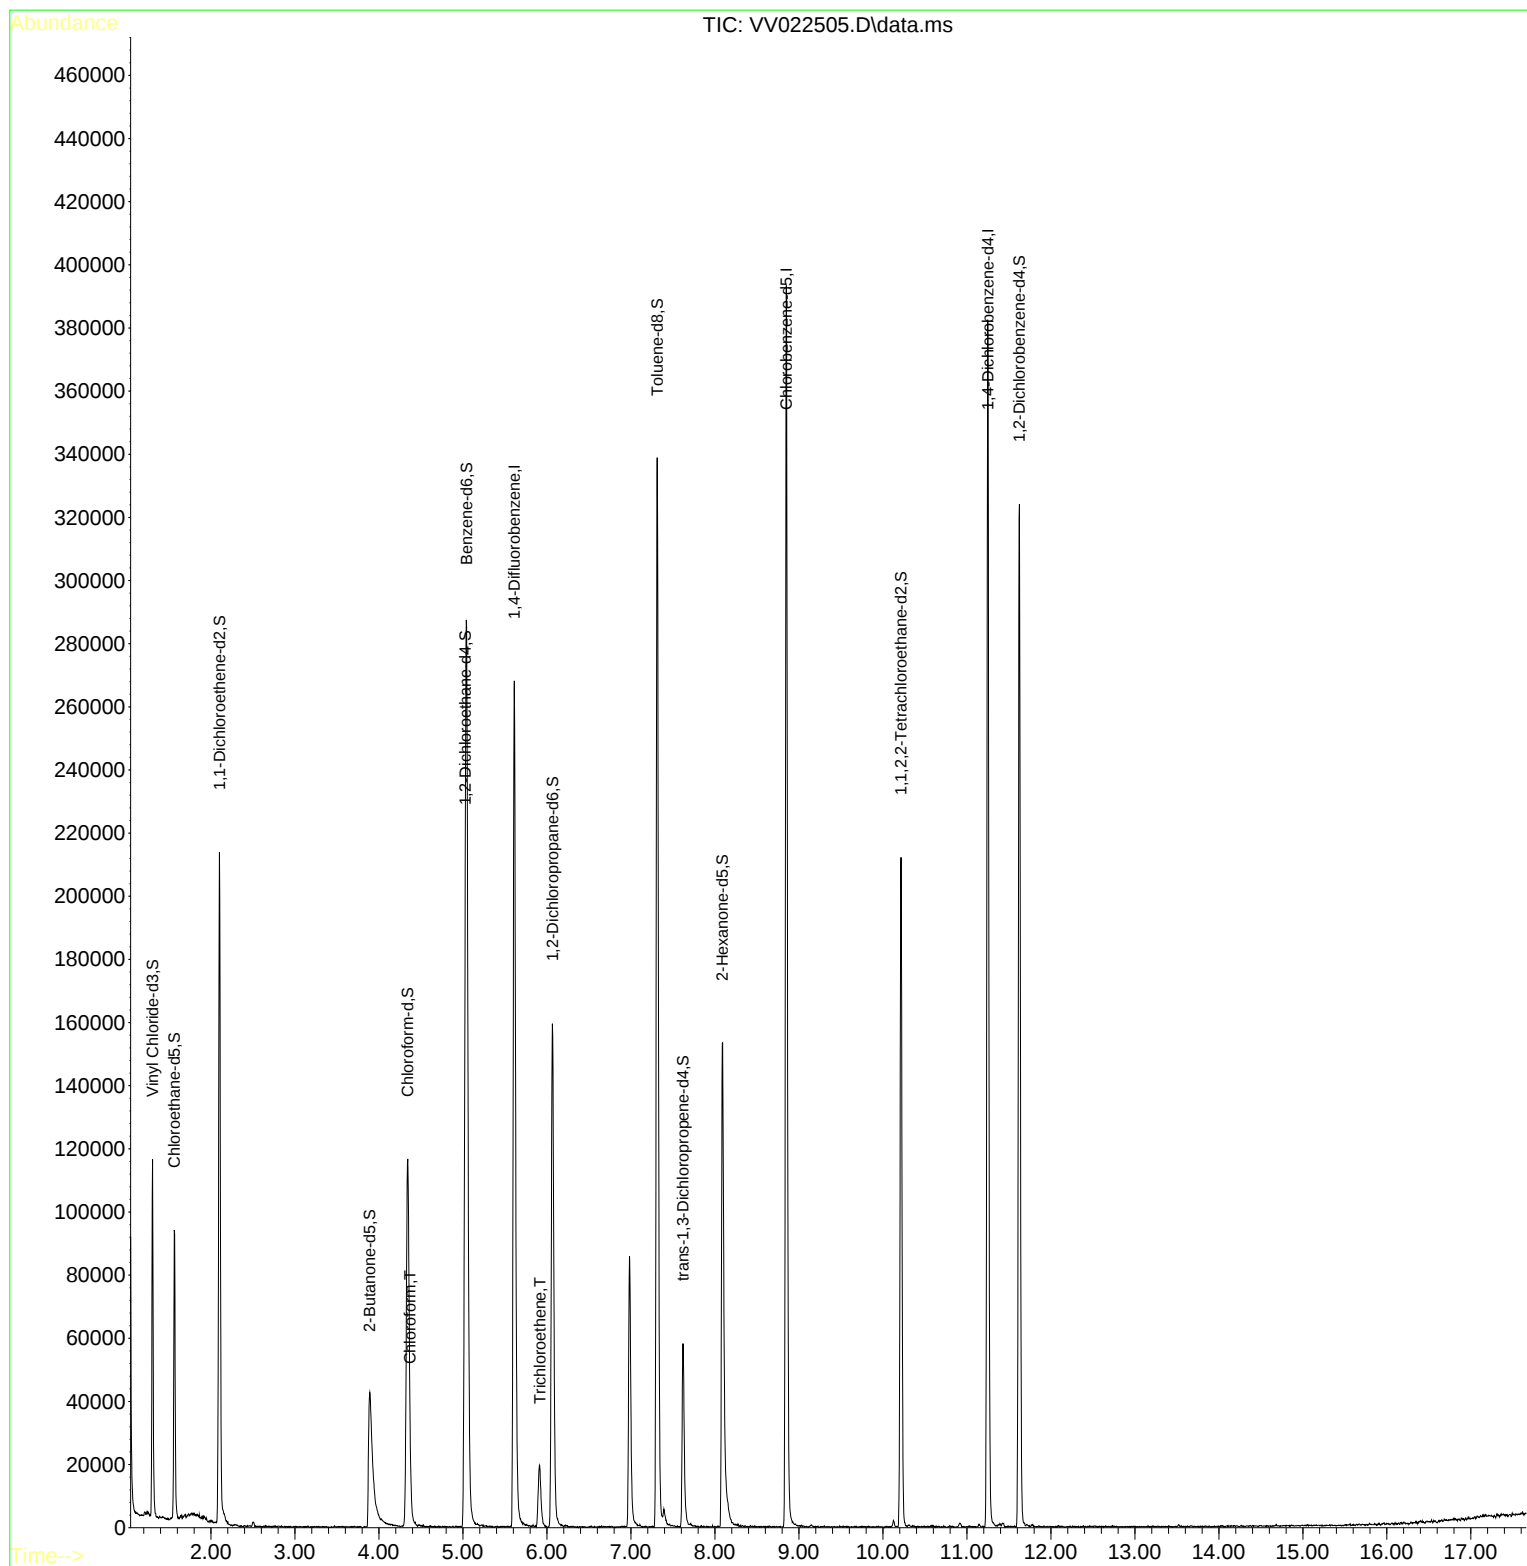




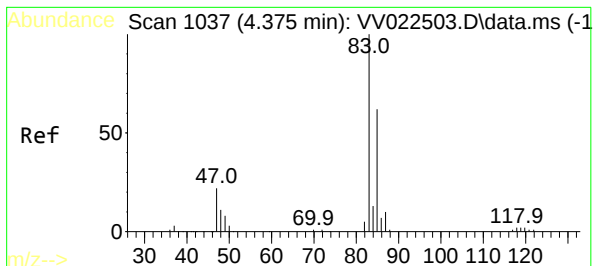


#25

Chloroform
Concen: 1.064 ug/L
RT: 4.372 min Scan# 1036
Delta R.T. -0.006 min
Lab File: VV022505.D
Acq: 02 Oct 2021 12:24

Instrument :
MSVOA_V
ClientSampleId :
VBLK273

Tgt Ion: 83 Resp: 3434
Ion Ratio Lower Upper
83 100
85 66.4 45.8 85.0

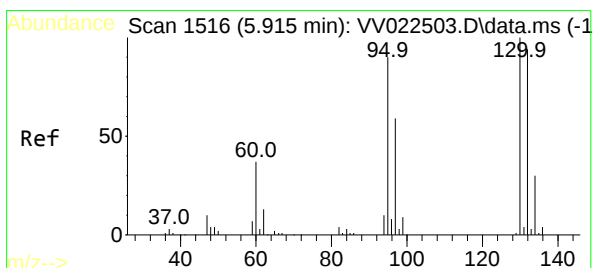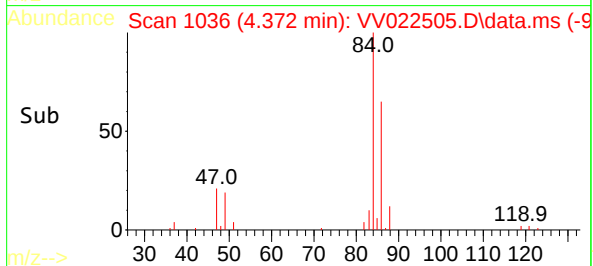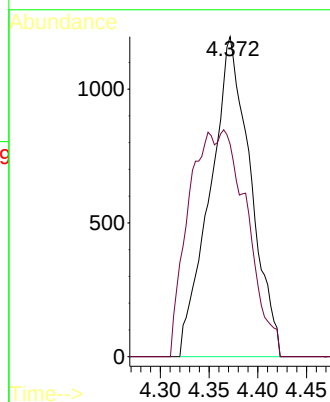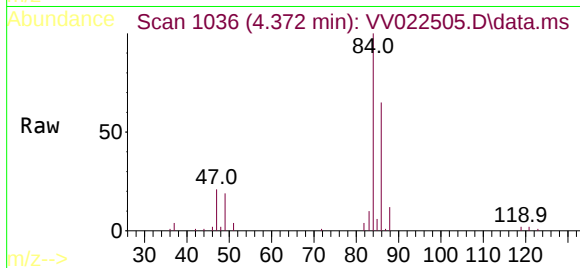

#34

Trichloroethene
Concen: 2.738 ug/L
RT: 5.915 min Scan# 1516
Delta R.T. -0.000 min
Lab File: VV022505.D
Acq: 02 Oct 2021 12:24

Tgt Ion: 95 Resp: 4918
Ion Ratio Lower Upper
95 100
97 61.0 45.4 84.4
132 108.6 71.5 132.9
130 92.5 75.2 139.6

