

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022547.D
 Acq On : 03 Oct 2021 06:21
 Operator : SY/MD
 Sample : M4000-08 500X
 Misc : 5.04g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW903

Quant Time: Oct 04 04:33:34 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Oct 04 04:27:20 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	282364	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	261803	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	128623	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	66853	38.283	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	76.560%		
7) Chloroethane-d5	1.568	69	55171	40.191	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	80.380%		
11) 1,1-Dichloroethene-d2	2.101	63	94328	27.394	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	54.780%#		
21) 2-Butanone-d5	3.895	46	78475	81.638	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	81.640%		
24) Chloroform-d	4.349	84	128150	40.165	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	80.340%		
26) 1,2-Dichloroethane-d4	5.034	65	80150	43.305	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.620%		
32) Benzene-d6	5.047	84	272547	44.937	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.880%		
36) 1,2-Dichloropropane-d6	6.069	67	82893	44.396	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	88.800%		
41) Toluene-d8	7.317	98	245305	44.092	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.180%		
43) trans-1,3-Dichloroprop...	7.625	79	34466	39.015	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	78.040%		
47) 2-Hexanone-d5	8.091	63	66811	86.378	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	86.380%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	110102	42.407	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	84.820%		
66) 1,2-Dichlorobenzene-d4	11.625	152	98275	46.853	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.700%		
Target Compounds					Qvalue	
25) Chloroform	4.381	83	3980	1.032	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022547.D
Acq On : 03 Oct 2021 06:21
Operator : SY/MD
Sample : M4000-08 500X
Misc : 5.04g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW903

Quant Time: Oct 04 04:33:34 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Oct 04 04:27:20 2021
Response via : Initial Calibration

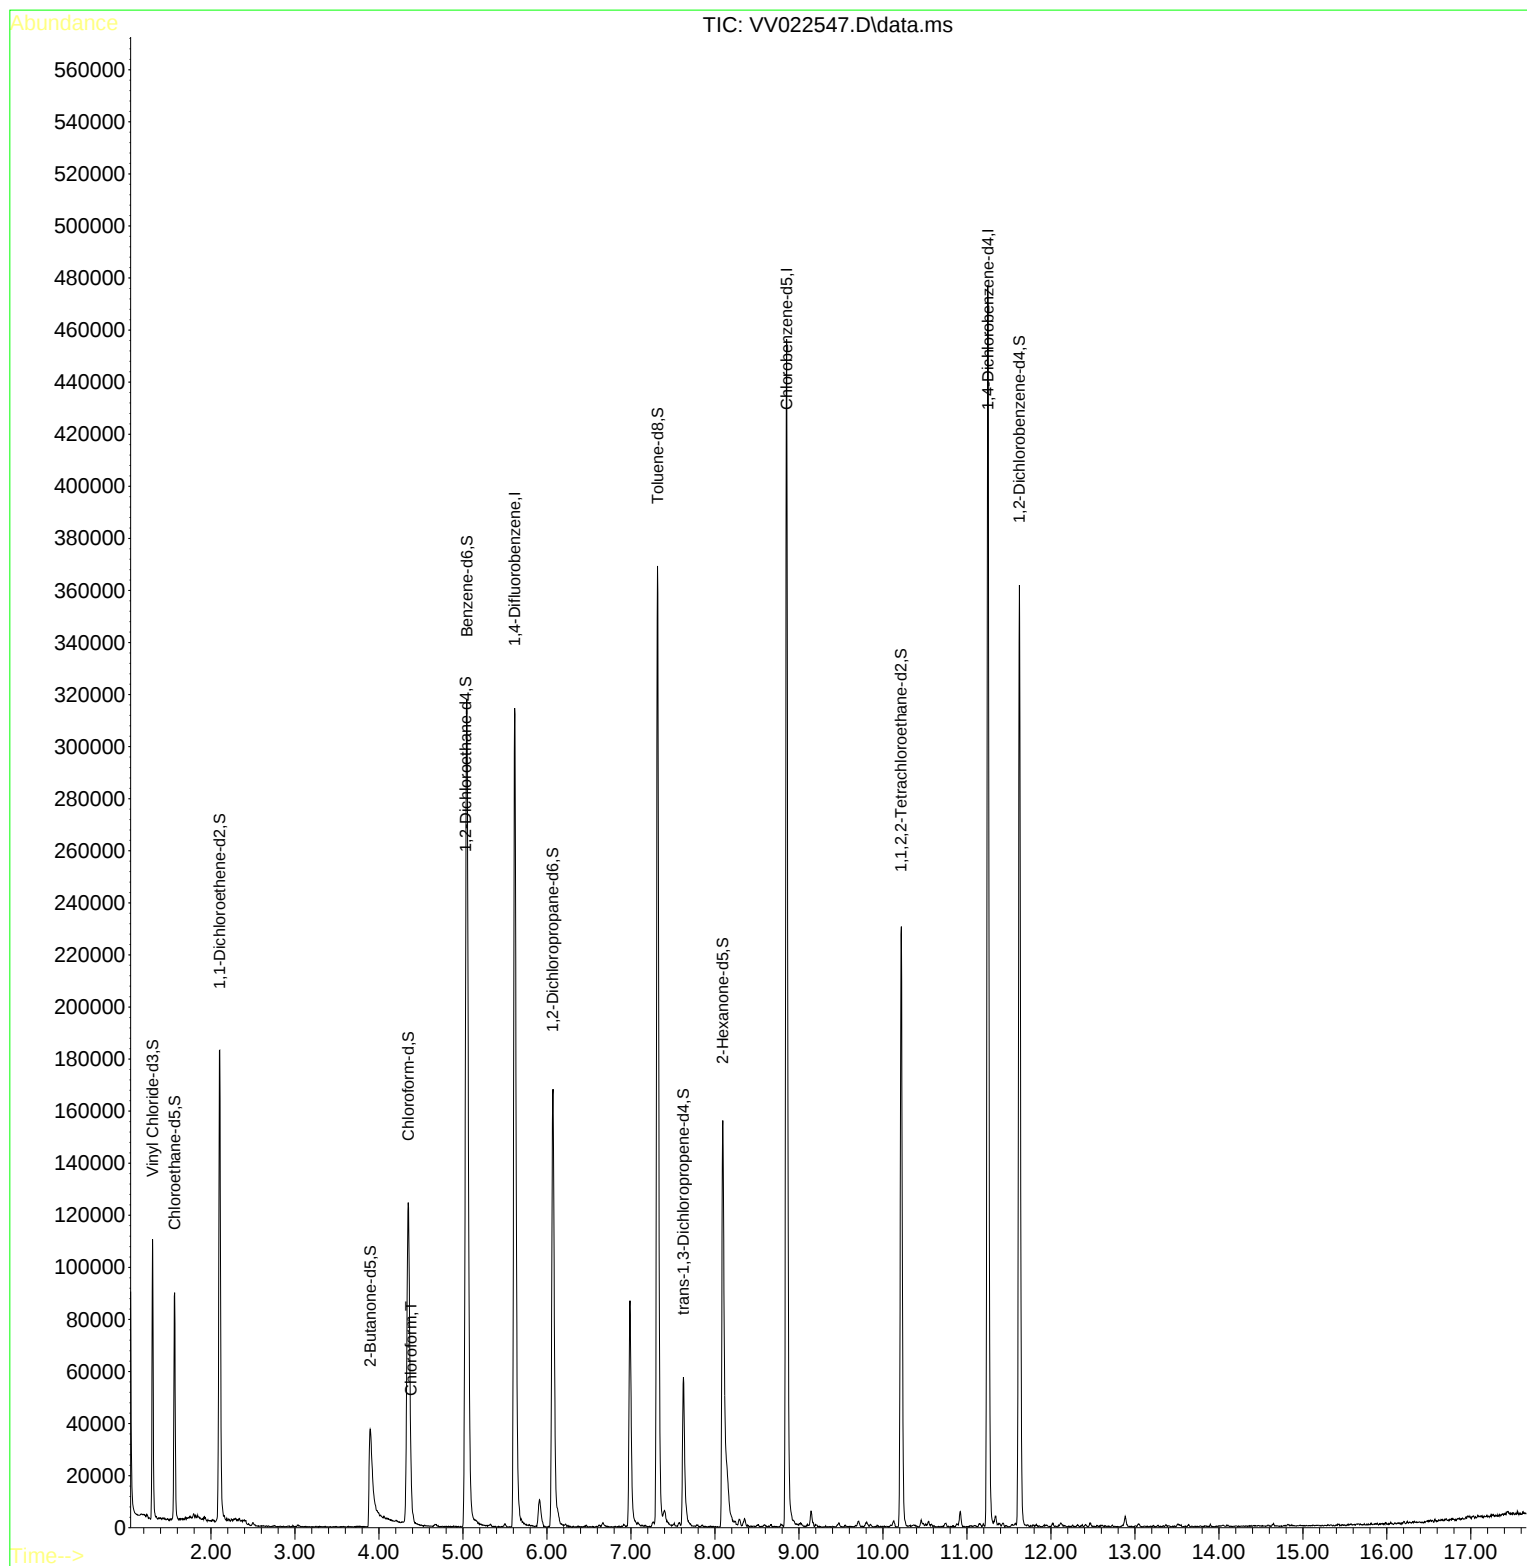

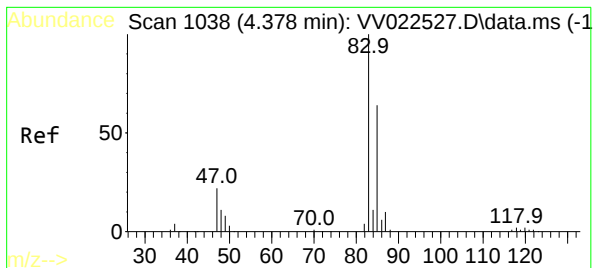

#25
Chloroform
Concen: 1.032 ug/L
RT: 4.381 min Scan# 1039
Delta R.T. 0.003 min
Lab File: VV022547.D
Acq: 03 Oct 2021 06:21

Instrument :
MSVOA_V
ClientSampleId :
EW903

Tgt Ion: 83 Resp: 3980
Ion Ratio Lower Upper
83 100
85 65.8 45.8 85.0

