

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022504.D
 Acq On : 02 Oct 2021 11:46
 Operator : SY/MD
 Sample : VV1002MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK272

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

Signal : TIC: VV022504.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	101	rVB	99048	98831	15.16%	1.926%
2	1.564	156	163	174	rBV	82494	93388	14.33%	1.820%
3	2.105	321	331	358	rVB	163407	243750	37.40%	4.749%
4	2.510	448	457	465	rVB5	3047	5399	0.83%	0.105%
5	2.761	532	535	536	rBV	323	165	0.03%	0.003%
6	2.857	561	565	570	rVB3	359	356	0.05%	0.007%
7	2.979	600	603	606	rBV3	426	245	0.04%	0.005%
8	3.085	631	636	645	rBV2	376	555	0.09%	0.011%
9	3.217	674	677	681	rBV2	254	223	0.03%	0.004%
10	3.253	684	688	691	rBV3	469	427	0.07%	0.008%
11	3.384	726	729	732	rBV2	361	308	0.05%	0.006%
12	3.420	735	740	742	rBV	381	262	0.04%	0.005%
13	3.503	761	766	769	rBV2	175	192	0.03%	0.004%
14	3.555	778	782	786	rBV	329	309	0.05%	0.006%
15	3.658	808	814	815	rBV	292	229	0.04%	0.004%
16	3.719	827	833	834	rBV2	327	260	0.04%	0.005%
17	3.886	876	885	929	rBV	42969	151752	23.29%	2.957%
18	4.346	1011	1028	1058	rBV2	104830	263540	40.44%	5.135%
19	4.606	1104	1109	1111	rBV	419	376	0.06%	0.007%
20	4.683	1131	1133	1142	rVB4	583	566	0.09%	0.011%
21	4.732	1142	1148	1149	rBV2	303	230	0.04%	0.004%
22	4.806	1169	1171	1175	rVB2	322	206	0.03%	0.004%
23	4.896	1195	1199	1203	rVB2	246	221	0.03%	0.004%
24	4.937	1209	1212	1218	rVB2	195	236	0.04%	0.005%
25	4.973	1218	1223	1228	rBV2	337	370	0.06%	0.007%
26	5.043	1228	1245	1269	rBV2	256179	651706	100.00%	12.698%
27	5.359	1340	1343	1345	rVV	321	177	0.03%	0.003%
28	5.561	1397	1406	1408	rBV2	194	297	0.05%	0.006%
29	5.616	1409	1423	1448	rBV	226886	460241	70.62%	8.968%
30	5.915	1502	1516	1540	rVB7	25723	59520	9.13%	1.160%
31	6.066	1551	1563	1584	rBV	144247	297143	45.59%	5.790%
32	6.204	1605	1606	1610	rBV3	328	206	0.03%	0.004%
33	6.391	1660	1664	1668	rBV3	209	217	0.03%	0.004%
34	6.603	1727	1730	1733	rVV2	314	170	0.03%	0.003%
35	6.725	1764	1768	1773	rBV2	274	331	0.05%	0.006%
36	6.985	1839	1849	1865	rBV	71585	129499	19.87%	2.523%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022504.D
 Acq On : 02 Oct 2021 11:46
 Operator : SY/MD
 Sample : VV1002MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK272

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

37	7.159	1901	1903	1908	rVB2	459	274	0.04%	0.005%
38	7.317	1940	1952	1969	rBV	276040	489305	75.08%	9.534%
39	7.622	2037	2047	2067	rBV2	48937	85892	13.18%	1.674%
40	7.767	2088	2092	2094	rVB	342	207	0.03%	0.004%
41	7.892	2128	2131	2133	rBV	295	223	0.03%	0.004%
42	8.014	2165	2169	2173	rBV2	214	253	0.04%	0.005%
43	8.088	2182	2192	2227	rBV	152492	292072	44.82%	5.691%
44	8.538	2325	2332	2335	rBV2	496	355	0.05%	0.007%
45	8.661	2366	2370	2374	rVB	322	277	0.04%	0.005%
46	8.686	2374	2378	2380	rBV	200	182	0.03%	0.004%
47	8.850	2418	2429	2451	rBV	339602	546395	83.84%	10.646%
48	9.001	2473	2476	2481	rBV3	525	389	0.06%	0.008%
49	9.104	2505	2508	2515	rVB2	393	443	0.07%	0.009%
50	9.153	2515	2523	2530	rBV5	619	1242	0.19%	0.024%
51	9.194	2534	2536	2539	rVV	274	165	0.03%	0.003%
52	9.439	2608	2612	2615	rBV2	251	209	0.03%	0.004%
53	9.555	2641	2648	2651	rBV3	638	623	0.10%	0.012%
54	9.673	2683	2685	2688	rVB2	441	191	0.03%	0.004%
55	9.725	2697	2701	2705	rBV2	273	285	0.04%	0.006%
56	9.911	2755	2759	2761	rBV	187	176	0.03%	0.003%
57	9.924	2761	2763	2766	rVV3	378	272	0.04%	0.005%
58	9.985	2780	2782	2784	rVV	412	208	0.03%	0.004%
59	10.008	2787	2789	2792	rBV	489	252	0.04%	0.005%
60	10.056	2799	2804	2808	rBV	368	417	0.06%	0.008%
61	10.111	2818	2821	2822	rVV	488	239	0.04%	0.005%
62	10.127	2823	2826	2837	rVB4	1402	1635	0.25%	0.032%
63	10.175	2837	2841	2843	rBV	350	292	0.04%	0.006%
64	10.217	2843	2854	2876	rVV	192262	305788	46.92%	5.958%
65	10.365	2894	2900	2902	rBV3	436	312	0.05%	0.006%
66	10.625	2975	2981	2982	rBV	238	213	0.03%	0.004%
67	10.760	3020	3023	3026	rBV2	189	168	0.03%	0.003%
68	10.889	3059	3063	3065	rBV2	196	184	0.03%	0.004%
69	10.918	3068	3072	3079	rVV2	1289	1367	0.21%	0.027%
70	11.079	3114	3122	3124	rBV2	257	377	0.06%	0.007%
71	11.188	3152	3156	3159	rBV2	714	475	0.07%	0.009%
72	11.249	3164	3175	3195	rBV	318254	491056	75.35%	9.568%
73	11.426	3228	3230	3232	rBV3	517	246	0.04%	0.005%
74	11.545	3264	3267	3269	rBV2	419	284	0.04%	0.006%
75	11.625	3280	3292	3312	rBV	272524	430998	66.13%	8.398%
76	11.818	3349	3352	3357	rVB3	322	280	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022504.D
 Acq On : 02 Oct 2021 11:46
 Operator : SY/MD
 Sample : VV1002MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK272

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

77	11.847	3357	3361	3363	rBV2	317	223	0.03%	0.004%
78	11.882	3369	3372	3376	rBV3	248	210	0.03%	0.004%
79	12.085	3432	3435	3439	rVB3	441	326	0.05%	0.006%
80	12.107	3439	3442	3446	rBV	269	267	0.04%	0.005%
81	12.368	3519	3523	3526	rVB2	270	197	0.03%	0.004%
82	12.384	3526	3528	3533	rVB	284	206	0.03%	0.004%
83	12.407	3533	3535	3539	rBV	399	310	0.05%	0.006%
84	12.519	3567	3570	3574	rBV2	258	270	0.04%	0.005%
85	12.596	3591	3594	3597	rBV2	300	181	0.03%	0.004%
86	12.651	3608	3611	3617	rVB3	968	926	0.14%	0.018%
87	12.744	3636	3640	3644	rBV2	228	221	0.03%	0.004%
88	12.953	3701	3705	3707	rBV2	207	168	0.03%	0.003%
89	13.101	3748	3751	3756	rBV3	286	260	0.04%	0.005%
90	13.268	3797	3803	3810	rVV5	1374	1933	0.30%	0.038%
91	13.400	3840	3844	3846	rBV2	386	336	0.05%	0.007%
92	13.513	3869	3879	3889	rBV3	3492	5399	0.83%	0.105%
93	13.651	3919	3922	3925	rBV	236	183	0.03%	0.004%
94	13.689	3931	3934	3936	rBV2	406	209	0.03%	0.004%
95	13.747	3947	3952	3958	rBV5	2159	2729	0.42%	0.053%
96	14.111	4062	4065	4071	rBV2	436	362	0.06%	0.007%
97	14.175	4082	4085	4089	rVB	349	261	0.04%	0.005%
98	14.214	4093	4097	4100	rVV3	369	312	0.05%	0.006%
99	14.268	4109	4114	4115	rBV2	430	305	0.05%	0.006%
100	14.313	4123	4128	4129	rBV2	395	310	0.05%	0.006%


Sum of corrected areas: 5132228

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022504.D
Acq On : 02 Oct 2021 11:46
Operator : SY/MD
Sample : VV1002MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK272

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

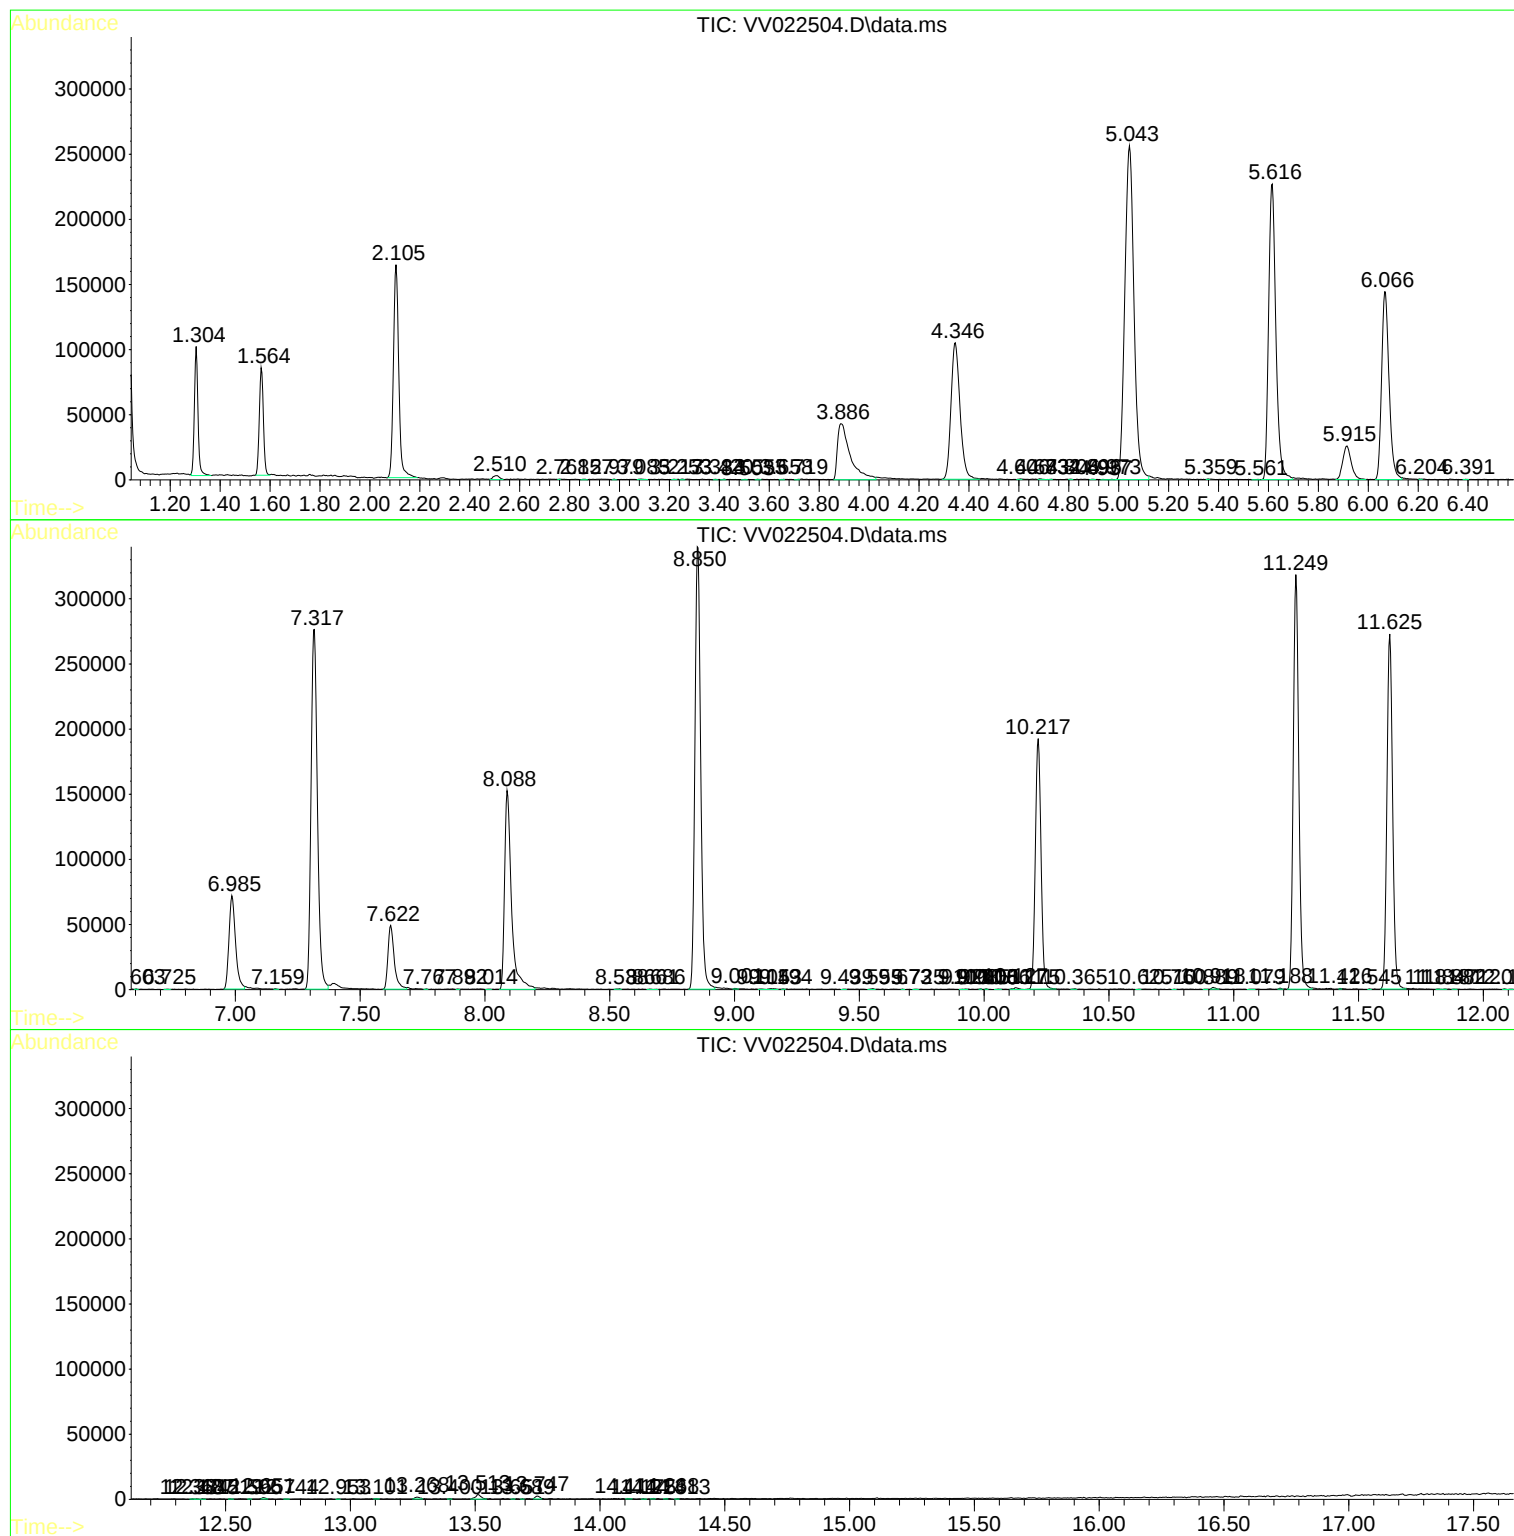

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022504.D
Acq On : 02 Oct 2021 11:46
Operator : SY/MD
Sample : VV1002MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK272

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022504.D
Acq On : 02 Oct 2021 11:46
Operator : SY/MD
Sample : VV1002MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK272

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
