

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022516.D
 Acq On : 02 Oct 2021 17:18
 Operator : SY/MD
 Sample : M3997-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

Signal : TIC: VV022516.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	104697	110291	16.19%	1.756%
2	1.568	157	164	178	rVB	87162	99396	14.59%	1.582%
3	2.108	322	332	357	rVB	187031	278348	40.85%	4.431%
4	2.330	399	401	402	rBV	449	157	0.02%	0.002%
5	2.764	525	536	558	rVB2	52367	102329	15.02%	1.629%
6	2.880	570	572	573	rBV2	361	170	0.02%	0.003%
7	3.053	624	626	629	rBV2	455	353	0.05%	0.006%
8	3.095	637	639	640	rBB	82	47	0.01%	0.001%
9	3.147	654	655	658	rVB	327	118	0.02%	0.002%
10	3.166	658	661	662	rBV	423	249	0.04%	0.004%
11	3.253	686	688	690	rBV	208	95	0.01%	0.002%
12	3.317	706	708	710	rBV	246	107	0.02%	0.002%
13	3.391	728	731	732	rBV	343	212	0.03%	0.003%
14	3.468	752	755	758	rBV3	383	227	0.03%	0.004%
15	3.520	768	771	774	rBV	183	138	0.02%	0.002%
16	3.587	790	792	794	rBV	223	92	0.01%	0.001%
17	3.632	802	806	809	rBV2	238	181	0.03%	0.003%
18	3.725	832	835	838	rVB	206	145	0.02%	0.002%
19	3.741	838	840	841	rVV	124	34	0.00%	0.001%
20	3.770	845	849	854	rBV	336	333	0.05%	0.005%
21	3.822	863	865	867	rVB	187	73	0.01%	0.001%
22	3.847	871	873	874	rBV	139	41	0.01%	0.001%
23	3.889	874	886	921	rBV2	60351	223227	32.76%	3.554%
24	4.349	1014	1029	1055	rBV2	105657	272615	40.01%	4.340%
25	4.587	1098	1103	1104	rBV2	312	294	0.04%	0.005%
26	4.783	1158	1164	1167	rBV2	472	514	0.08%	0.008%
27	4.815	1172	1174	1177	rVB2	352	163	0.02%	0.003%
28	4.905	1199	1202	1204	rBV2	276	217	0.03%	0.003%
29	4.947	1212	1215	1216	rBV2	223	146	0.02%	0.002%
30	4.979	1222	1225	1227	rBV	171	85	0.01%	0.001%
31	5.047	1227	1246	1276	rBV2	263832	681359	100.00%	10.847%
32	5.269	1312	1315	1319	rBV3	423	352	0.05%	0.006%
33	5.449	1369	1371	1373	rBV	140	81	0.01%	0.001%
34	5.516	1390	1392	1393	rBV	219	86	0.01%	0.001%
35	5.619	1412	1424	1452	rBV	246584	498218	73.12%	7.932%
36	5.918	1506	1517	1539	rVB7	14324	33562	4.93%	0.534%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022516.D
 Acq On : 02 Oct 2021 17:18
 Operator : SY/MD
 Sample : M3997-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

37	6.072	1550	1565	1586	rBV	148794	303842	44.59%	4.837%
38	6.323	1638	1643	1645	rBV2	329	296	0.04%	0.005%
39	6.468	1682	1688	1696	rVB2	332	375	0.06%	0.006%
40	6.503	1696	1699	1705	rBV2	232	302	0.04%	0.005%
41	6.584	1721	1724	1726	rBV	309	215	0.03%	0.003%
42	6.616	1732	1734	1735	rBV	289	117	0.02%	0.002%
43	6.661	1743	1748	1752	rBV3	310	328	0.05%	0.005%
44	6.786	1785	1787	1788	rVB	274	105	0.02%	0.002%
45	6.806	1789	1793	1795	rBV2	231	182	0.03%	0.003%
46	6.844	1802	1805	1811	rBV2	210	294	0.04%	0.005%
47	6.915	1825	1827	1828	rBV2	116	64	0.01%	0.001%
48	6.989	1839	1850	1876	rBV	76579	142528	20.92%	2.269%
49	7.227	1922	1924	1925	rBV	137	74	0.01%	0.001%
50	7.317	1940	1952	1973	rBV	314884	550472	80.79%	8.764%
51	7.622	2037	2047	2067	rBV	51425	91573	13.44%	1.458%
52	7.857	2118	2120	2121	rBV	179	51	0.01%	0.001%
53	7.902	2132	2134	2136	rBV	121	69	0.01%	0.001%
54	7.976	2145	2157	2183	rBV	374903	622340	91.34%	9.908%
55	8.092	2183	2193	2222	rBV	150290	280626	41.19%	4.468%
56	8.481	2312	2314	2316	rBV2	193	67	0.01%	0.001%
57	8.513	2322	2324	2326	rBV	171	88	0.01%	0.001%
58	8.677	2371	2375	2377	rBV2	345	300	0.04%	0.005%
59	8.751	2395	2398	2399	rBV	145	77	0.01%	0.001%
60	8.854	2419	2430	2453	rBV	375714	602215	88.38%	9.587%
61	9.079	2499	2500	2512	rBV	226	281	0.04%	0.004%
62	9.143	2518	2520	2522	rBV2	406	205	0.03%	0.003%
63	9.207	2532	2540	2546	rVB4	982	1282	0.19%	0.020%
64	9.397	2595	2599	2601	rBV2	190	161	0.02%	0.003%
65	9.410	2601	2603	2604	rVB2	422	165	0.02%	0.003%
66	9.545	2643	2645	2648	rVB2	252	105	0.02%	0.002%
67	9.635	2671	2673	2675	rBV	175	104	0.02%	0.002%
68	9.908	2757	2758	2764	rBV	411	340	0.05%	0.005%
69	10.011	2781	2790	2801	rBV	2342	4220	0.62%	0.067%
70	10.127	2820	2826	2835	rBV4	1410	2316	0.34%	0.037%
71	10.217	2841	2854	2871	rBV	199124	312966	45.93%	4.983%
72	10.481	2934	2936	2938	rVB2	238	92	0.01%	0.001%
73	10.506	2941	2944	2946	rBV2	124	81	0.01%	0.001%
74	10.625	2978	2981	2984	rBV2	369	235	0.03%	0.004%
75	10.764	3022	3024	3027	rVB2	211	94	0.01%	0.001%
76	10.780	3027	3029	3030	rBV	169	91	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022516.D
 Acq On : 02 Oct 2021 17:18
 Operator : SY/MD
 Sample : M3997-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

77	10.828	3043	3044	3047	rBV	426	179	0.03%	0.003%
78	11.011	3099	3101	3105	rBV	242	160	0.02%	0.003%
79	11.143	3140	3142	3143	rBV	525	276	0.04%	0.004%
80	11.191	3155	3157	3159	rBV	120	56	0.01%	0.001%
81	11.249	3164	3175	3198	rVV	365053	562893	82.61%	8.961%
82	11.625	3280	3292	3312	rBV	305889	484957	71.17%	7.721%
83	11.757	3331	3333	3336	rVB2	355	186	0.03%	0.003%
84	11.773	3336	3338	3340	rVV	360	173	0.03%	0.003%
85	11.786	3340	3342	3343	rVB	314	99	0.01%	0.002%
86	11.834	3356	3357	3358	rBV	214	63	0.01%	0.001%
87	11.998	3403	3408	3410	rBV	297	304	0.04%	0.005%
88	12.468	3552	3554	3557	rBV	300	205	0.03%	0.003%
89	12.796	3654	3656	3657	rBV	276	130	0.02%	0.002%
90	13.027	3725	3728	3731	rBV	394	246	0.04%	0.004%
91	13.278	3801	3806	3807	rBV2	483	238	0.03%	0.004%
92	13.304	3811	3814	3817	rBV3	425	260	0.04%	0.004%
93	13.583	3897	3901	3904	rBV2	357	335	0.05%	0.005%
94	13.780	3960	3962	3964	rBV	324	172	0.03%	0.003%
95	13.866	3987	3989	3990	rBV2	277	91	0.01%	0.001%
96	14.117	4065	4067	4069	rBV	397	239	0.04%	0.004%
97	14.326	4130	4132	4135	rBV2	394	245	0.04%	0.004%
98	14.712	4248	4252	4257	rVB2	471	475	0.07%	0.008%
99	14.738	4257	4260	4262	rBV2	441	327	0.05%	0.005%
100	16.181	4704	4709	4717	rVB5	4382	5555	0.82%	0.088%




Sum of corrected areas: 6281257

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022516.D
Acq On : 02 Oct 2021 17:18
Operator : SY/MD
Sample : M3997-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

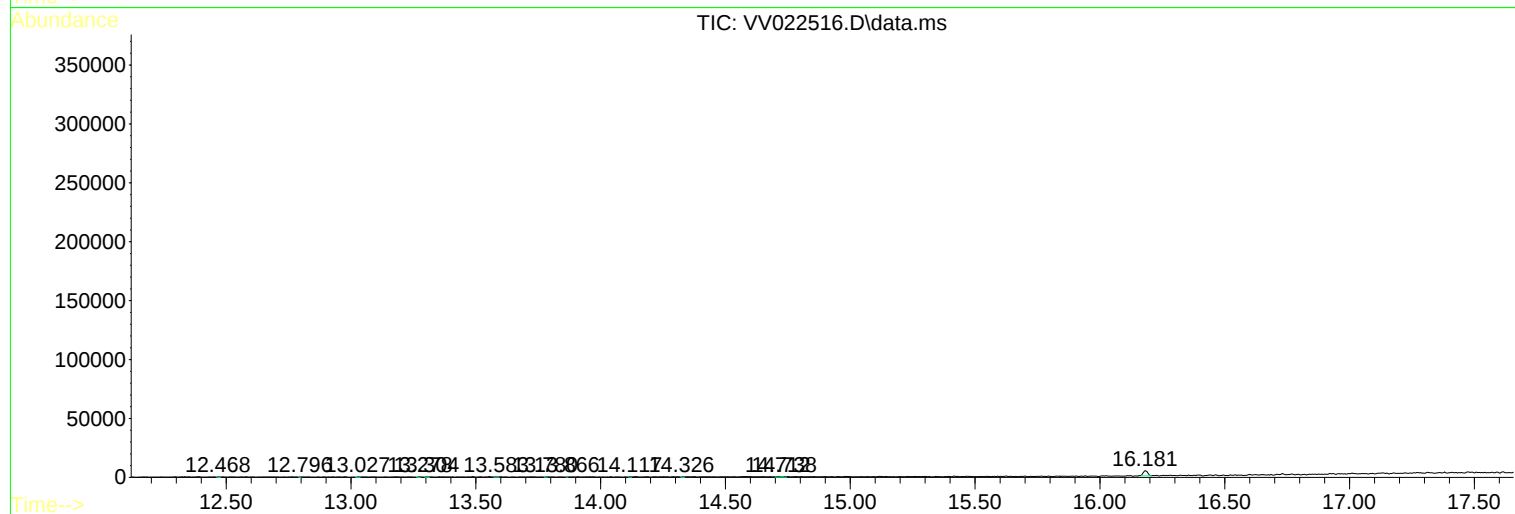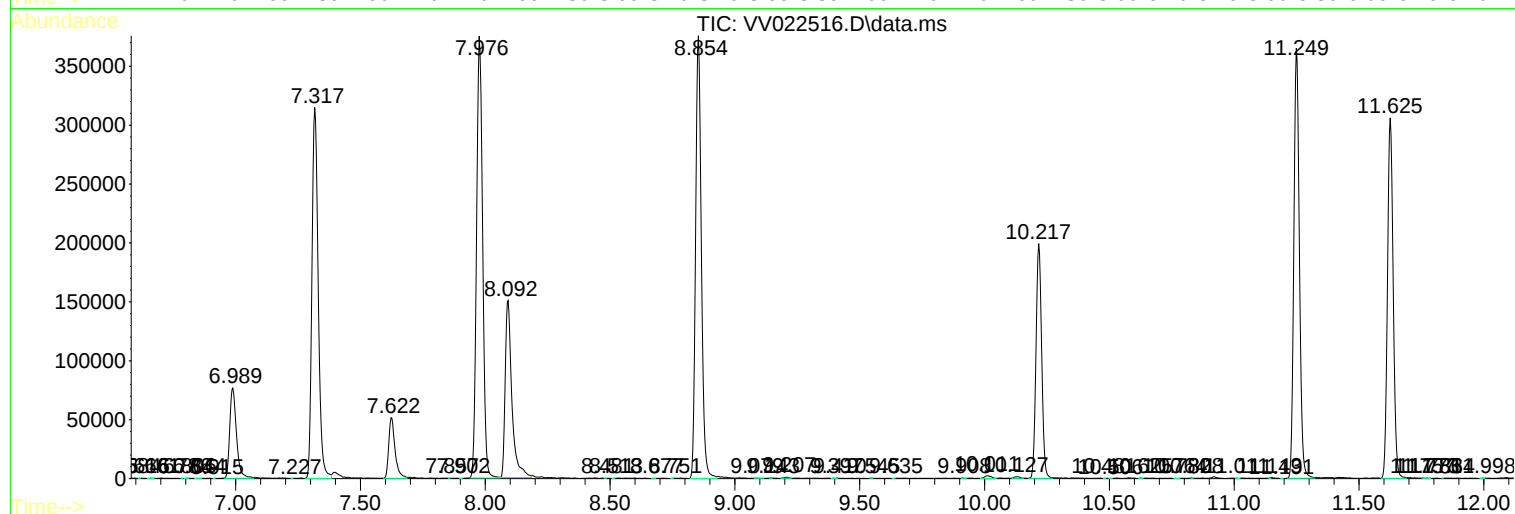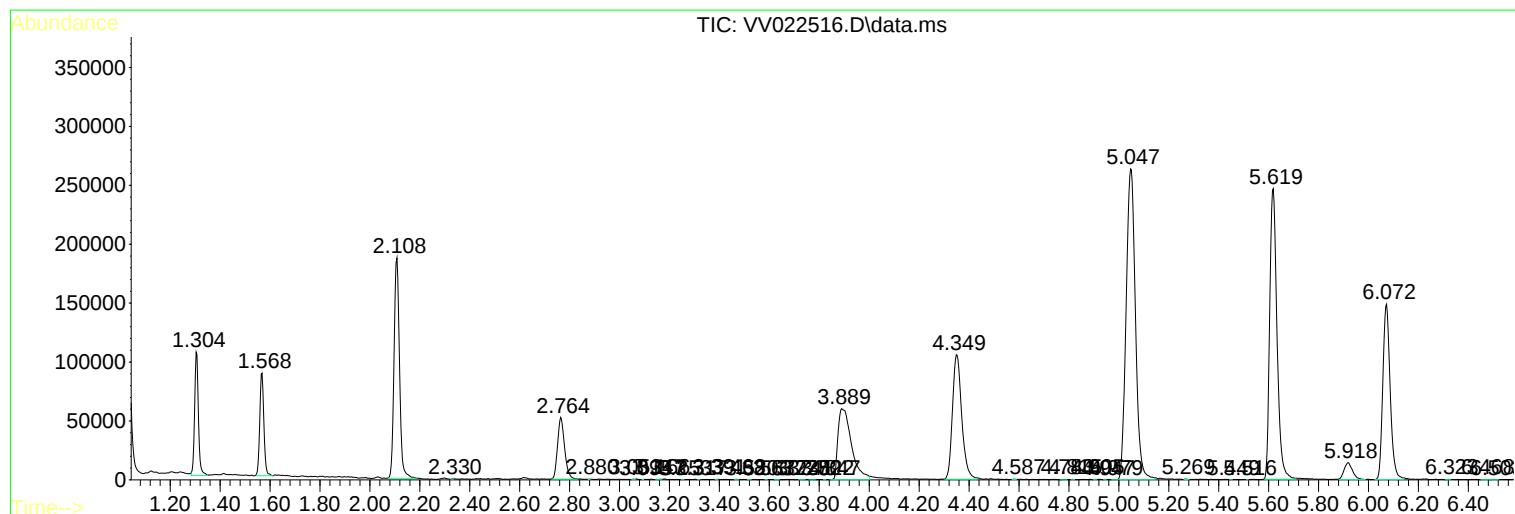

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022516.D
Acq On : 02 Oct 2021 17:18
Operator : SY/MD
Sample : M3997-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022516.D
Acq On : 02 Oct 2021 17:18
Operator : SY/MD
Sample : M3997-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
