

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022519.D
 Acq On : 02 Oct 2021 18:29
 Operator : SY/MD
 Sample : M3997-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

Signal : TIC: VV022519.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	102290	105395	15.33%	1.695%
2	1.565	157	163	180	rVB	87343	96106	13.98%	1.546%
3	2.105	321	331	351	rBV	184666	277182	40.31%	4.458%
4	2.510	452	457	461	rBV3	554	585	0.09%	0.009%
5	2.561	471	473	478	rBV	386	299	0.04%	0.005%
6	2.622	482	492	495	rBV3	1422	2303	0.33%	0.037%
7	2.773	530	539	549	rVB4	3345	6126	0.89%	0.099%
8	2.847	560	562	564	rBV3	220	141	0.02%	0.002%
9	2.918	580	584	586	rBV	269	180	0.03%	0.003%
10	2.934	586	589	590	rBV	215	103	0.01%	0.002%
11	2.992	603	607	610	rVB2	302	241	0.04%	0.004%
12	3.018	612	615	616	rBV	172	103	0.01%	0.002%
13	3.085	634	636	638	rBV	194	96	0.01%	0.002%
14	3.265	690	692	693	rBV	275	151	0.02%	0.002%
15	3.381	725	728	730	rBV2	301	155	0.02%	0.002%
16	3.449	744	749	751	rBV	324	273	0.04%	0.004%
17	3.545	774	779	781	rBV	297	235	0.03%	0.004%
18	3.574	786	788	790	rBV	208	100	0.01%	0.002%
19	3.828	865	867	869	rBV	231	127	0.02%	0.002%
20	3.892	876	887	920	rBV3	52683	180252	26.21%	2.899%
21	4.352	1013	1030	1062	rBV2	101976	274555	39.93%	4.416%
22	4.584	1100	1102	1103	rBV	243	114	0.02%	0.002%
23	4.593	1103	1105	1109	rVV2	293	190	0.03%	0.003%
24	4.645	1117	1121	1124	rBV	487	451	0.07%	0.007%
25	4.712	1136	1142	1143	rBV	399	386	0.06%	0.006%
26	4.789	1164	1166	1168	rVB2	319	147	0.02%	0.002%
27	4.831	1177	1179	1180	rBV2	439	178	0.03%	0.003%
28	4.986	1224	1227	1229	rBV	176	131	0.02%	0.002%
29	5.047	1229	1246	1284	rBV2	266068	687664	100.00%	11.059%
30	5.230	1301	1303	1305	rBV	319	165	0.02%	0.003%
31	5.314	1326	1329	1331	rBV2	437	322	0.05%	0.005%
32	5.355	1339	1342	1344	rBV	243	172	0.03%	0.003%
33	5.413	1358	1360	1363	rBV2	220	118	0.02%	0.002%
34	5.433	1364	1366	1368	rBV	411	200	0.03%	0.003%
35	5.616	1412	1423	1451	rBV	247131	503915	73.28%	8.104%
36	5.754	1464	1466	1473	rVB2	663	571	0.08%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022519.D
 Acq On : 02 Oct 2021 18:29
 Operator : SY/MD
 Sample : M3997-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

37	5.841	1492	1493	1496	rBV	324	186	0.03%	0.003%
38	5.918	1505	1517	1541	rVB4	31480	71138	10.34%	1.144%
39	6.069	1551	1564	1584	rBV	147438	303138	44.08%	4.875%
40	6.416	1669	1672	1677	rBV	436	425	0.06%	0.007%
41	6.490	1691	1695	1698	rBV2	344	259	0.04%	0.004%
42	6.741	1770	1773	1775	rBV2	425	276	0.04%	0.004%
43	6.786	1783	1787	1788	rBV	275	215	0.03%	0.003%
44	6.841	1801	1804	1807	rVV	194	152	0.02%	0.002%
45	6.905	1821	1824	1826	rBV	206	145	0.02%	0.002%
46	6.934	1830	1833	1834	rBV	281	145	0.02%	0.002%
47	6.989	1839	1850	1874	rBV	79088	147154	21.40%	2.367%
48	7.140	1895	1897	1899	rBV2	276	146	0.02%	0.002%
49	7.317	1941	1952	1972	rBV	318584	553627	80.51%	8.904%
50	7.622	2037	2047	2066	rBV	53851	94920	13.80%	1.527%
51	7.767	2089	2092	2096	rVB2	496	441	0.06%	0.007%
52	7.789	2096	2099	2100	rBV2	246	124	0.02%	0.002%
53	7.976	2145	2157	2174	rBV	387833	643555	93.59%	10.350%
54	8.092	2183	2193	2230	rVB	159404	288718	41.99%	4.643%
55	8.368	2276	2279	2280	rBV	255	135	0.02%	0.002%
56	8.484	2312	2315	2317	rVB	392	174	0.03%	0.003%
57	8.635	2361	2362	2365	rBV	239	163	0.02%	0.003%
58	8.760	2399	2401	2407	rBV2	277	234	0.03%	0.004%
59	8.854	2418	2430	2454	rBV	374643	604217	87.87%	9.717%
60	9.149	2520	2522	2525	rVB	708	268	0.04%	0.004%
61	9.352	2583	2585	2588	rBV	290	182	0.03%	0.003%
62	9.403	2599	2601	2603	rVV	409	144	0.02%	0.002%
63	9.432	2607	2610	2612	rBV	288	109	0.02%	0.002%
64	9.728	2700	2702	2704	rBV	225	114	0.02%	0.002%
65	9.744	2704	2707	2709	rBV2	203	135	0.02%	0.002%
66	9.793	2717	2722	2725	rBV	165	182	0.03%	0.003%
67	9.918	2759	2761	2763	rVB2	348	141	0.02%	0.002%
68	9.976	2777	2779	2780	rBV2	257	128	0.02%	0.002%
69	10.059	2802	2805	2810	rBV2	168	207	0.03%	0.003%
70	10.101	2816	2818	2820	rVB	273	131	0.02%	0.002%
71	10.130	2820	2827	2835	rBV3	1754	2969	0.43%	0.048%
72	10.217	2841	2854	2869	rBV	205119	317029	46.10%	5.099%
73	10.571	2962	2964	2965	rBV2	308	114	0.02%	0.002%
74	10.796	3032	3034	3036	rVB2	311	115	0.02%	0.002%
75	10.918	3065	3072	3080	rVB5	1381	1904	0.28%	0.031%
76	10.950	3080	3082	3086	rBV	240	176	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022519.D
 Acq On : 02 Oct 2021 18:29
 Operator : SY/MD
 Sample : M3997-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

77	10.985	3090	3093	3096	rBV2	296	201	0.03%	0.003%
78	11.034	3106	3108	3111	rBV2	349	219	0.03%	0.004%
79	11.201	3156	3160	3162	rBV2	218	151	0.02%	0.002%
80	11.249	3164	3175	3197	rBV	364872	556002	80.85%	8.942%
81	11.423	3226	3229	3230	rBV2	747	387	0.06%	0.006%
82	11.503	3247	3254	3255	rBV	363	339	0.05%	0.005%
83	11.625	3280	3292	3310	rBV	308760	484123	70.40%	7.786%
84	11.889	3370	3374	3378	rBV2	368	297	0.04%	0.005%
85	11.934	3386	3388	3392	rVB	224	111	0.02%	0.002%
86	11.953	3392	3394	3396	rBV2	277	151	0.02%	0.002%
87	12.217	3473	3476	3477	rBV2	262	133	0.02%	0.002%
88	12.410	3534	3536	3538	rBV2	220	129	0.02%	0.002%
89	12.442	3543	3546	3548	rBV	273	159	0.02%	0.003%
90	12.529	3572	3573	3576	rBV	216	114	0.02%	0.002%
91	12.616	3598	3600	3602	rBV	276	130	0.02%	0.002%
92	12.683	3617	3621	3624	rBV	314	256	0.04%	0.004%
93	12.776	3648	3650	3653	rBV	286	165	0.02%	0.003%
94	13.062	3733	3739	3743	rBV2	357	385	0.06%	0.006%
95	13.136	3760	3762	3764	rBV	281	140	0.02%	0.002%
96	13.374	3834	3836	3841	rBV2	414	288	0.04%	0.005%
97	13.734	3946	3948	3952	rBV	349	224	0.03%	0.004%
98	13.931	4008	4009	4010	rBV	330	112	0.02%	0.002%
99	14.133	4068	4072	4076	rBV	374	412	0.06%	0.007%
100	14.201	4090	4093	4094	rBV2	298	161	0.02%	0.003%


Sum of corrected areas: 6217956

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022519.D
Acq On : 02 Oct 2021 18:29
Operator : SY/MD
Sample : M3997-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

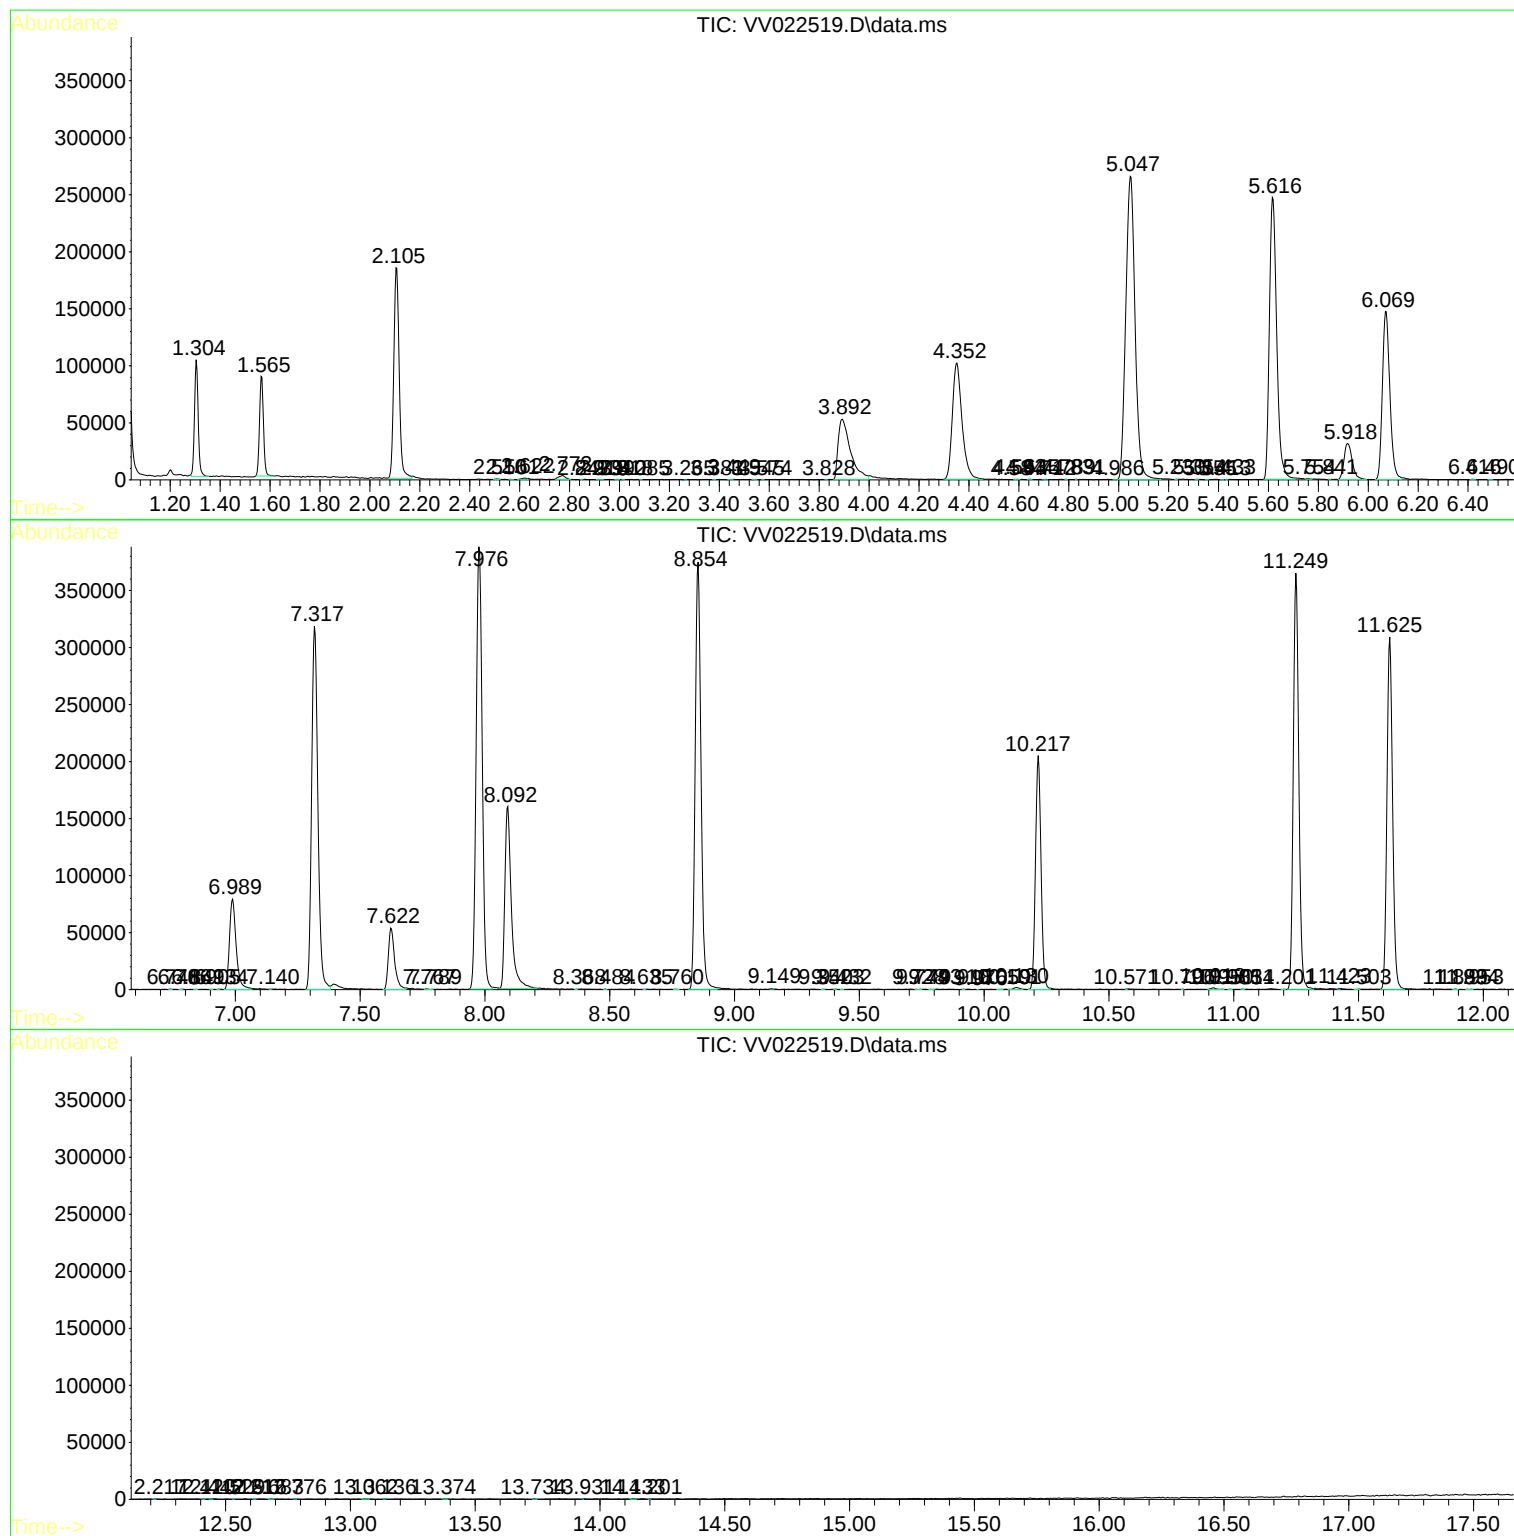

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022519.D
Acq On : 02 Oct 2021 18:29
Operator : SY/MD
Sample : M3997-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022519.D
Acq On : 02 Oct 2021 18:29
Operator : SY/MD
Sample : M3997-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
