

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022520.D
 Acq On : 02 Oct 2021 18:53
 Operator : SY/MD
 Sample : M3997-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A68

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M

Title : VOC Analysis

Signal : TIC: VV022520.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	104542	107906	15.58%	1.931%
2	1.568	156	164	174	rBV	89071	100820	14.56%	1.805%
3	2.108	322	332	344	rBV	185302	269306	38.89%	4.820%
4	2.439	428	435	451	rBV2	4336	8721	1.26%	0.156%
5	2.568	471	475	479	rBV2	450	376	0.05%	0.007%
6	2.590	479	482	488	rVB	562	463	0.07%	0.008%
7	2.667	502	506	507	rBV2	521	301	0.04%	0.005%
8	2.947	590	593	596	rBV3	280	268	0.04%	0.005%
9	3.159	655	659	662	rVB2	311	214	0.03%	0.004%
10	3.179	662	665	667	rBV2	295	191	0.03%	0.003%
11	3.220	675	678	681	rBV2	319	238	0.03%	0.004%
12	3.249	685	687	691	rVB	347	182	0.03%	0.003%
13	3.272	691	694	698	rVB2	239	186	0.03%	0.003%
14	3.294	698	701	705	rBV2	323	288	0.04%	0.005%
15	3.333	711	713	717	rVB2	435	203	0.03%	0.004%
16	3.378	724	727	731	rVB	258	216	0.03%	0.004%
17	3.667	813	817	820	rBV2	292	205	0.03%	0.004%
18	3.690	820	824	827	rBV2	275	249	0.04%	0.004%
19	3.764	842	847	850	rBV	211	204	0.03%	0.004%
20	3.796	854	857	862	rBV3	296	317	0.05%	0.006%
21	3.844	869	872	877	rBV2	221	190	0.03%	0.003%
22	3.892	877	887	929	rBV2	42665	153044	22.10%	2.739%
23	4.349	1015	1029	1060	rBV2	104155	282384	40.78%	5.054%
24	4.529	1082	1085	1088	rBV2	348	201	0.03%	0.004%
25	4.577	1096	1100	1103	rBV3	333	223	0.03%	0.004%
26	4.597	1103	1106	1109	rBV	256	204	0.03%	0.004%
27	4.645	1118	1121	1122	rBV2	291	193	0.03%	0.003%
28	4.687	1130	1134	1138	rBV2	425	320	0.05%	0.006%
29	4.835	1177	1180	1186	rVB	245	273	0.04%	0.005%
30	4.880	1191	1194	1196	rBV	289	180	0.03%	0.003%
31	5.047	1229	1246	1278	rBV2	271873	692433	100.00%	12.394%
32	5.323	1330	1332	1336	rVB2	405	209	0.03%	0.004%
33	5.339	1336	1337	1340	rBV2	326	203	0.03%	0.004%
34	5.436	1364	1367	1373	rBV2	322	336	0.05%	0.006%
35	5.523	1390	1394	1396	rBV2	311	260	0.04%	0.005%
36	5.619	1411	1424	1454	rBV	254413	515436	74.44%	9.226%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022520.D
 Acq On : 02 Oct 2021 18:53
 Operator : SY/MD
 Sample : M3997-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A68

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

37	5.912	1504	1515	1534	rVB6	15213	36827	5.32%	0.659%
38	5.986	1534	1538	1541	rVB2	332	185	0.03%	0.003%
39	6.072	1552	1565	1590	rBV	147992	304967	44.04%	5.458%
40	6.185	1598	1600	1604	rVB2	583	350	0.05%	0.006%
41	6.217	1604	1610	1612	rBV2	415	427	0.06%	0.008%
42	6.256	1617	1622	1624	rBV3	376	306	0.04%	0.005%
43	6.294	1631	1634	1637	rVB2	319	181	0.03%	0.003%
44	6.375	1655	1659	1664	rVB	290	251	0.04%	0.004%
45	6.407	1664	1669	1671	rBV2	222	236	0.03%	0.004%
46	6.577	1715	1722	1728	rVV3	487	645	0.09%	0.012%
47	6.706	1760	1762	1766	rBV2	168	177	0.03%	0.003%
48	6.786	1784	1787	1794	rBV2	324	265	0.04%	0.005%
49	6.989	1839	1850	1878	rBV	78607	147721	21.33%	2.644%
50	7.191	1909	1913	1916	rBV2	314	231	0.03%	0.004%
51	7.249	1924	1931	1934	rBV4	566	721	0.10%	0.013%
52	7.317	1940	1952	1970	rBV	319844	553363	79.92%	9.904%
53	7.625	2037	2048	2071	rBV	53339	95380	13.77%	1.707%
54	7.931	2138	2143	2145	rBV2	380	372	0.05%	0.007%
55	7.982	2152	2159	2167	rVV4	1832	2683	0.39%	0.048%
56	8.031	2169	2174	2178	rBV	286	307	0.04%	0.005%
57	8.092	2183	2193	2232	rBV	156680	294006	42.46%	5.262%
58	8.368	2277	2279	2284	rBV3	490	443	0.06%	0.008%
59	8.471	2306	2311	2315	rBV3	549	601	0.09%	0.011%
60	8.638	2359	2363	2369	rVV2	279	328	0.05%	0.006%
61	8.854	2418	2430	2467	rBV	379261	619644	89.49%	11.091%
62	9.140	2517	2519	2521	rBV	436	242	0.03%	0.004%
63	9.240	2545	2550	2552	rBV2	268	241	0.03%	0.004%
64	9.294	2564	2567	2572	rVB	333	263	0.04%	0.005%
65	9.449	2610	2615	2618	rBV2	270	275	0.04%	0.005%
66	9.686	2684	2689	2692	rBV2	301	314	0.05%	0.006%
67	10.133	2818	2828	2838	rVB4	1698	2727	0.39%	0.049%
68	10.217	2843	2854	2874	rBV	194149	303492	43.83%	5.432%
69	10.313	2881	2884	2888	rBV3	637	553	0.08%	0.010%
70	10.574	2962	2965	2972	rVB2	589	591	0.09%	0.011%
71	10.622	2975	2980	2983	rBV2	217	231	0.03%	0.004%
72	10.657	2988	2991	2995	rVB3	287	208	0.03%	0.004%
73	10.812	3034	3039	3042	rBV2	266	322	0.05%	0.006%
74	10.918	3065	3072	3079	rVB5	1729	2226	0.32%	0.040%
75	10.989	3090	3094	3096	rBV2	252	238	0.03%	0.004%
76	11.027	3104	3106	3108	rBV	342	189	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022520.D
 Acq On : 02 Oct 2021 18:53
 Operator : SY/MD
 Sample : M3997-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4A68

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

77	11.143	3136	3142	3150	rBV4	902	1377	0.20%	0.025%
78	11.249	3164	3175	3193	rBV	375987	565751	81.70%	10.126%
79	11.384	3212	3217	3218	rBV2	777	627	0.09%	0.011%
80	11.532	3255	3263	3275	rVV3	7777	13690	1.98%	0.245%
81	11.625	3280	3292	3308	rBV	312804	488471	70.54%	8.743%
82	11.776	3336	3339	3340	rBV	448	301	0.04%	0.005%
83	11.995	3404	3407	3410	rVB2	508	380	0.05%	0.007%
84	12.014	3410	3413	3417	rBV2	426	375	0.05%	0.007%
85	12.098	3437	3439	3443	rVB2	524	224	0.03%	0.004%
86	12.223	3475	3478	3479	rBV2	371	207	0.03%	0.004%
87	12.265	3489	3491	3494	rVB	557	265	0.04%	0.005%
88	12.284	3494	3497	3499	rBV2	396	247	0.04%	0.004%
89	12.349	3513	3517	3519	rBV2	1174	946	0.14%	0.017%
90	12.477	3554	3557	3560	rBV	313	196	0.03%	0.004%
91	12.603	3594	3596	3600	rVB3	633	335	0.05%	0.006%
92	12.728	3632	3635	3636	rBV2	298	201	0.03%	0.004%
93	12.792	3648	3655	3656	rBV	291	284	0.04%	0.005%
94	13.291	3804	3810	3816	rBV5	1058	1139	0.16%	0.020%
95	13.825	3973	3976	3979	rBV2	385	296	0.04%	0.005%
96	13.905	3995	4001	4007	rBV2	410	578	0.08%	0.010%
97	14.046	4042	4045	4048	rBV2	574	371	0.05%	0.007%
98	14.175	4081	4085	4090	rBV2	402	445	0.06%	0.008%
99	14.339	4133	4136	4138	rBV2	421	302	0.04%	0.005%
100	14.484	4177	4181	4184	rBV2	341	337	0.05%	0.006%


Sum of corrected areas: 5587017

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022520.D
Acq On : 02 Oct 2021 18:53
Operator : SY/MD
Sample : M3997-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F4A68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

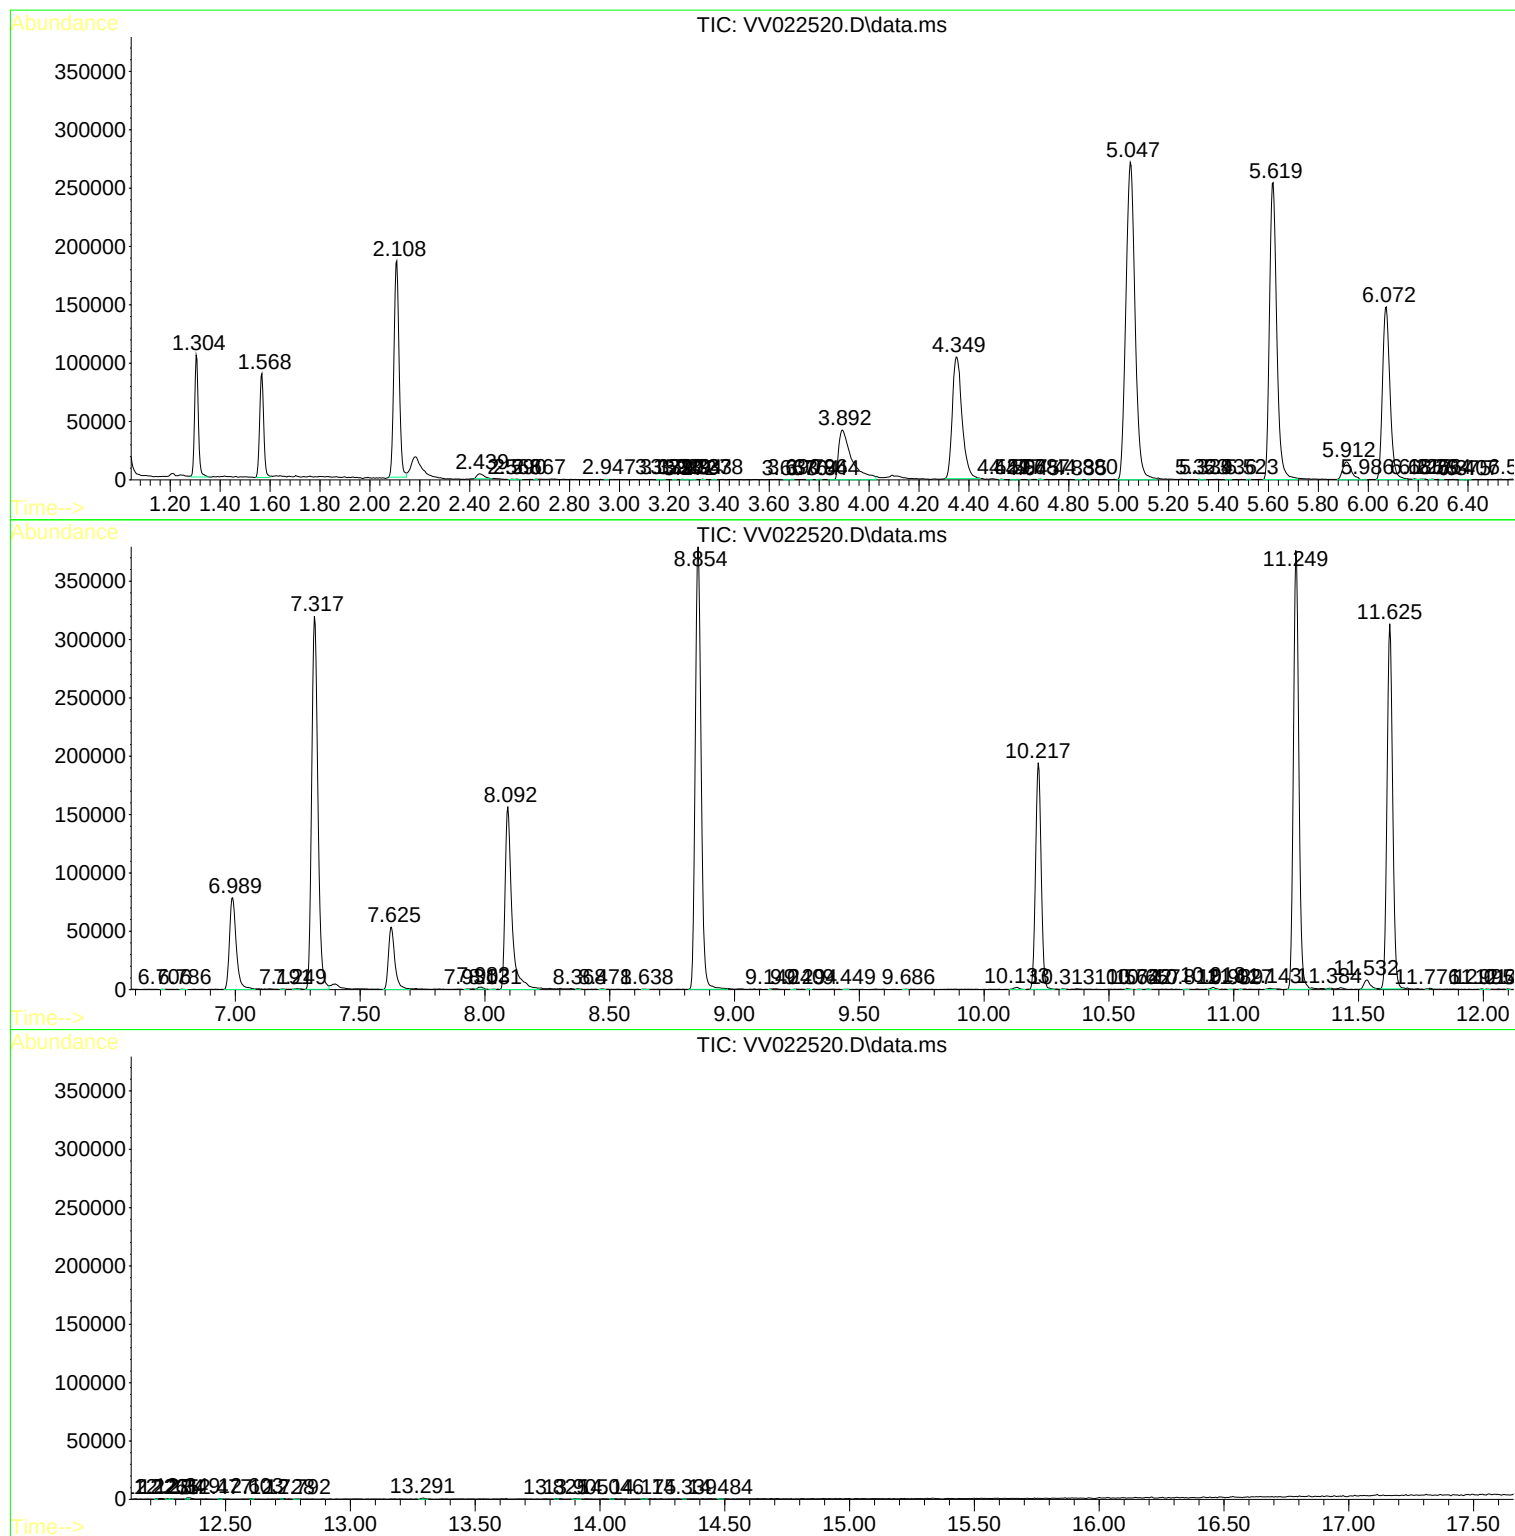

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022520.D
Acq On : 02 Oct 2021 18:53
Operator : SY/MD
Sample : M3997-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022520.D
Acq On : 02 Oct 2021 18:53
Operator : SY/MD
Sample : M3997-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4A68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
