

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022521.D
 Acq On : 02 Oct 2021 19:17
 Operator : SY/MD
 Sample : M4023-01DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M

Title : VOC Analysis

Signal : TIC: VV022521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	103	rVB2	294187	321215	43.98%	4.912%
2	1.568	157	164	178	rVB	88508	97970	13.41%	1.498%
3	2.108	322	332	356	rVB2	205752	324770	44.46%	4.967%
4	2.506	448	456	466	rBV6	2321	4141	0.57%	0.063%
5	2.683	507	511	513	rBV2	265	227	0.03%	0.003%
6	2.764	531	536	544	rVB3	2102	3073	0.42%	0.047%
7	2.825	552	555	557	rBV	316	216	0.03%	0.003%
8	3.191	657	669	687	rBV2	14692	31393	4.30%	0.480%
9	3.288	696	699	700	rBV2	198	132	0.02%	0.002%
10	3.387	727	730	734	rBV2	219	209	0.03%	0.003%
11	3.436	743	745	748	rBV	247	147	0.02%	0.002%
12	3.555	778	782	786	rVB	182	169	0.02%	0.003%
13	3.580	787	790	792	rBV2	316	183	0.03%	0.003%
14	3.912	876	893	925	rBV2	271804	730422	100.00%	11.170%
15	4.352	1013	1030	1060	rBV4	98762	278929	38.19%	4.266%
16	4.609	1097	1110	1131	rVB	24957	60977	8.35%	0.932%
17	4.850	1182	1185	1187	rBV2	252	153	0.02%	0.002%
18	5.047	1230	1246	1271	rBV2	270444	687988	94.19%	10.521%
19	5.439	1364	1368	1370	rBV2	290	218	0.03%	0.003%
20	5.500	1382	1387	1388	rBV	214	158	0.02%	0.002%
21	5.619	1411	1424	1448	rBV	255146	506145	69.29%	7.740%
22	5.918	1504	1517	1544	rVB6	23247	57321	7.85%	0.877%
23	6.072	1551	1565	1582	rBV	147470	305292	41.80%	4.669%
24	6.281	1625	1630	1631	rBV	354	243	0.03%	0.004%
25	6.362	1649	1655	1659	rVB2	356	346	0.05%	0.005%
26	6.526	1703	1706	1709	rVV2	431	346	0.05%	0.005%
27	6.635	1736	1740	1742	rBV	189	161	0.02%	0.002%
28	6.661	1745	1748	1749	rBV	226	147	0.02%	0.002%
29	6.815	1793	1796	1798	rBV2	204	151	0.02%	0.002%
30	6.866	1808	1812	1817	rBV2	223	272	0.04%	0.004%
31	6.940	1831	1835	1838	rBB2	293	240	0.03%	0.004%
32	6.989	1838	1850	1873	rBV	78221	146118	20.00%	2.235%
33	7.111	1886	1888	1893	rBV4	357	223	0.03%	0.003%
34	7.133	1893	1895	1899	rVB2	472	278	0.04%	0.004%
35	7.230	1923	1925	1928	rBV2	266	179	0.02%	0.003%
36	7.317	1940	1952	1970	rBV	317787	549217	75.19%	8.399%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022521.D
 Acq On : 02 Oct 2021 19:17
 Operator : SY/MD
 Sample : M4023-01DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

37	7.545	2021	2023	2025	rBV2	415	175	0.02%	0.003%
38	7.625	2038	2048	2069	rBV	53364	95600	13.09%	1.462%
39	7.799	2100	2102	2104	rVB2	313	143	0.02%	0.002%
40	7.812	2104	2106	2110	rVB	354	228	0.03%	0.003%
41	7.834	2110	2113	2116	rBV2	387	268	0.04%	0.004%
42	7.879	2125	2127	2131	rVB2	439	203	0.03%	0.003%
43	7.931	2141	2143	2146	rBV	172	143	0.02%	0.002%
44	7.953	2147	2150	2154	rVB	514	240	0.03%	0.004%
45	7.976	2154	2157	2161	rBV4	883	830	0.11%	0.013%
46	8.037	2171	2176	2177	rVB	324	210	0.03%	0.003%
47	8.053	2177	2181	2183	rBV	226	201	0.03%	0.003%
48	8.091	2183	2193	2225	rBV	156940	290313	39.75%	4.440%
49	8.304	2257	2259	2260	rBV	390	160	0.02%	0.002%
50	8.419	2293	2295	2299	rVB	317	173	0.02%	0.003%
51	8.452	2299	2305	2308	rBV3	517	504	0.07%	0.008%
52	8.471	2308	2311	2314	rBV3	380	254	0.03%	0.004%
53	8.603	2349	2352	2353	rBV3	255	133	0.02%	0.002%
54	8.853	2418	2430	2449	rBV	377424	601644	82.37%	9.201%
55	9.024	2474	2483	2497	rVB2	5082	9004	1.23%	0.138%
56	9.107	2505	2509	2510	rBV2	322	238	0.03%	0.004%
57	9.143	2510	2520	2537	rVV2	20985	35006	4.79%	0.535%
58	9.548	2637	2646	2657	rBV2	9863	15704	2.15%	0.240%
59	9.725	2697	2701	2706	rBV2	262	236	0.03%	0.004%
60	9.773	2712	2716	2719	rBV	183	168	0.02%	0.003%
61	9.956	2771	2773	2774	rBV	262	126	0.02%	0.002%
62	10.024	2790	2794	2800	rVB2	722	766	0.10%	0.012%
63	10.130	2819	2827	2836	rVB4	1483	2380	0.33%	0.036%
64	10.217	2843	2854	2872	rBV	201329	314240	43.02%	4.806%
65	10.316	2882	2885	2891	rBV2	495	519	0.07%	0.008%
66	10.390	2905	2908	2909	rBV2	383	231	0.03%	0.004%
67	10.606	2973	2975	2979	rBV	242	144	0.02%	0.002%
68	10.667	2990	2994	2998	rBV2	265	296	0.04%	0.005%
69	10.738	3013	3016	3018	rBV	280	202	0.03%	0.003%
70	10.767	3022	3025	3028	rBV2	407	292	0.04%	0.004%
71	10.853	3049	3052	3054	rBV2	425	244	0.03%	0.004%
72	10.882	3057	3061	3064	rVB	283	202	0.03%	0.003%
73	10.915	3068	3071	3081	rVV4	1512	2012	0.28%	0.031%
74	10.956	3081	3084	3090	rVB3	347	296	0.04%	0.005%
75	11.107	3128	3131	3133	rBV2	186	166	0.02%	0.003%
76	11.117	3133	3134	3138	rVB2	363	161	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100221\
 Data File : VW022521.D
 Acq On : 02 Oct 2021 19:17
 Operator : SY/MD
 Sample : M4023-01DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

77	11.146	3140	3143	3149	rVB2	1091	961	0.13%	0.015%
78	11.249	3164	3175	3196	rBV	365778	560888	76.79%	8.577%
79	11.513	3253	3257	3261	rBV2	349	305	0.04%	0.005%
80	11.625	3281	3292	3312	rBV	316246	487745	66.78%	7.459%
81	11.757	3330	3333	3337	rVB2	472	356	0.05%	0.005%
82	11.783	3337	3341	3343	rBV2	405	321	0.04%	0.005%
83	11.911	3377	3381	3386	rVB	371	282	0.04%	0.004%
84	11.950	3391	3393	3399	rBV2	222	166	0.02%	0.003%
85	12.152	3451	3456	3459	rBV2	292	308	0.04%	0.005%
86	12.181	3463	3465	3469	rBV	285	217	0.03%	0.003%
87	12.564	3582	3584	3586	rBV	199	129	0.02%	0.002%
88	12.596	3589	3594	3596	rBV	280	237	0.03%	0.004%
89	12.763	3644	3646	3647	rBV	325	168	0.02%	0.003%
90	13.114	3751	3755	3763	rBV	288	445	0.06%	0.007%
91	13.204	3781	3783	3785	rBV2	398	216	0.03%	0.003%
92	13.236	3789	3793	3797	rBV2	261	271	0.04%	0.004%
93	13.368	3827	3834	3835	rBV2	316	349	0.05%	0.005%
94	13.422	3848	3851	3852	rBV2	313	158	0.02%	0.002%
95	13.670	3922	3928	3931	rBV2	439	437	0.06%	0.007%
96	13.898	3996	3999	4004	rBV3	239	176	0.02%	0.003%
97	14.033	4037	4041	4043	rBV3	834	713	0.10%	0.011%
98	14.268	4113	4114	4119	rVB3	419	260	0.04%	0.004%
99	14.609	4217	4220	4225	rBV2	369	394	0.05%	0.006%
100	14.635	4226	4228	4231	rBV3	282	230	0.03%	0.004%




Sum of corrected areas: 6539156

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022521.D
Acq On : 02 Oct 2021 19:17
Operator : SY/MD
Sample : M4023-01DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

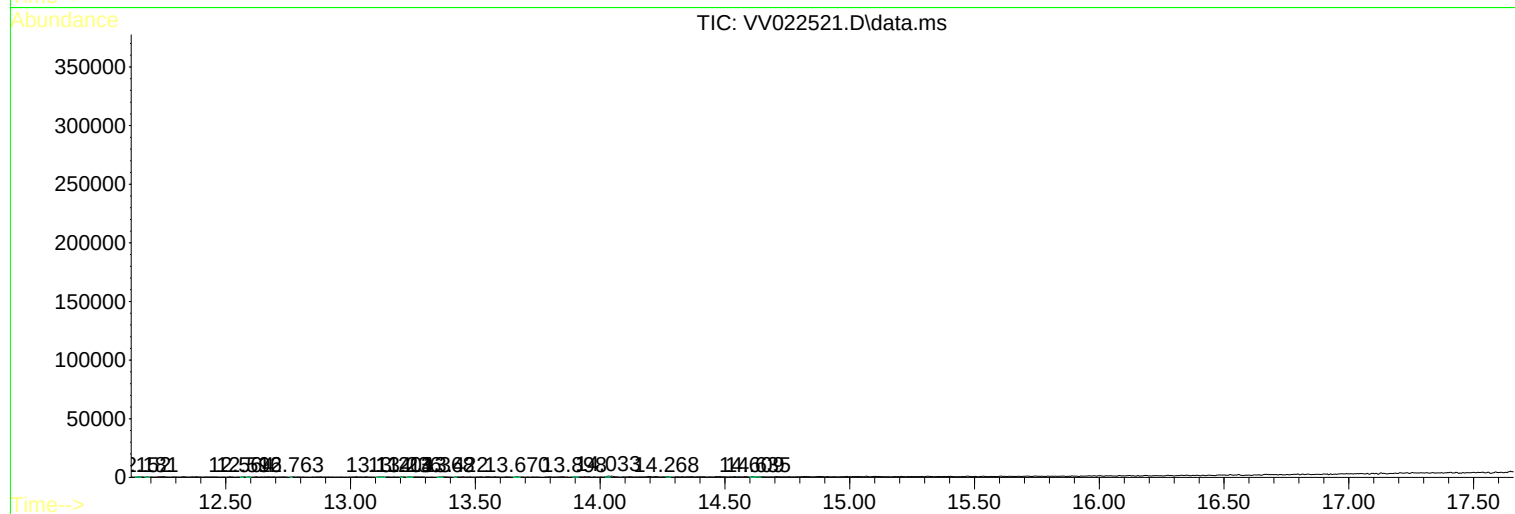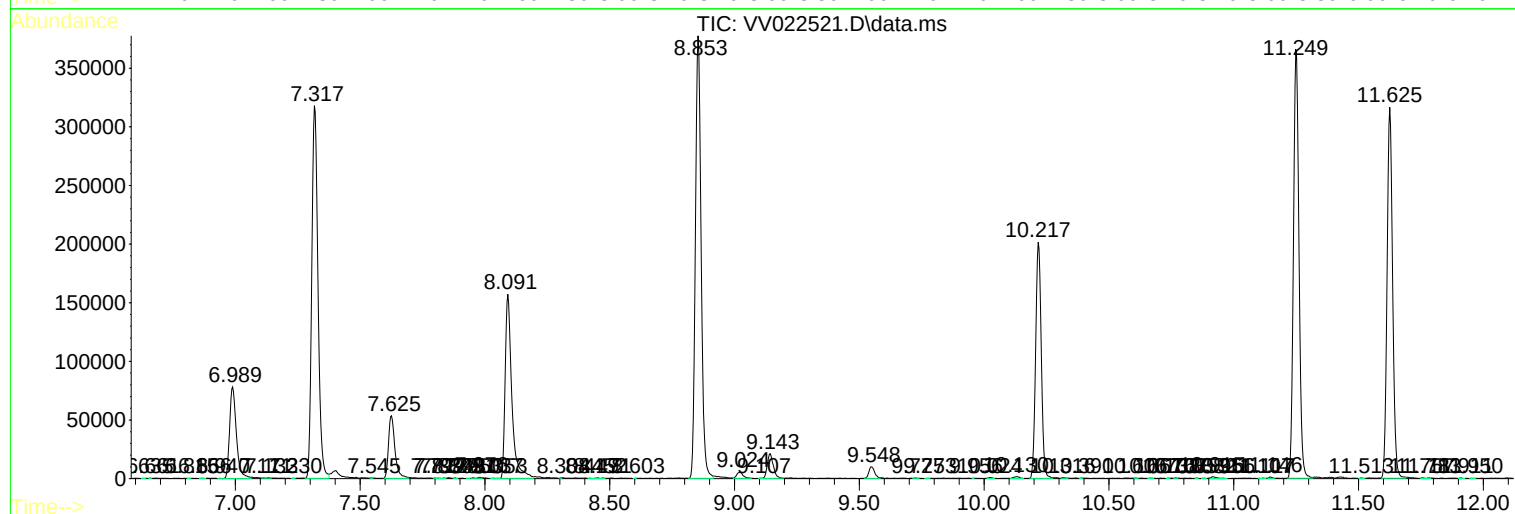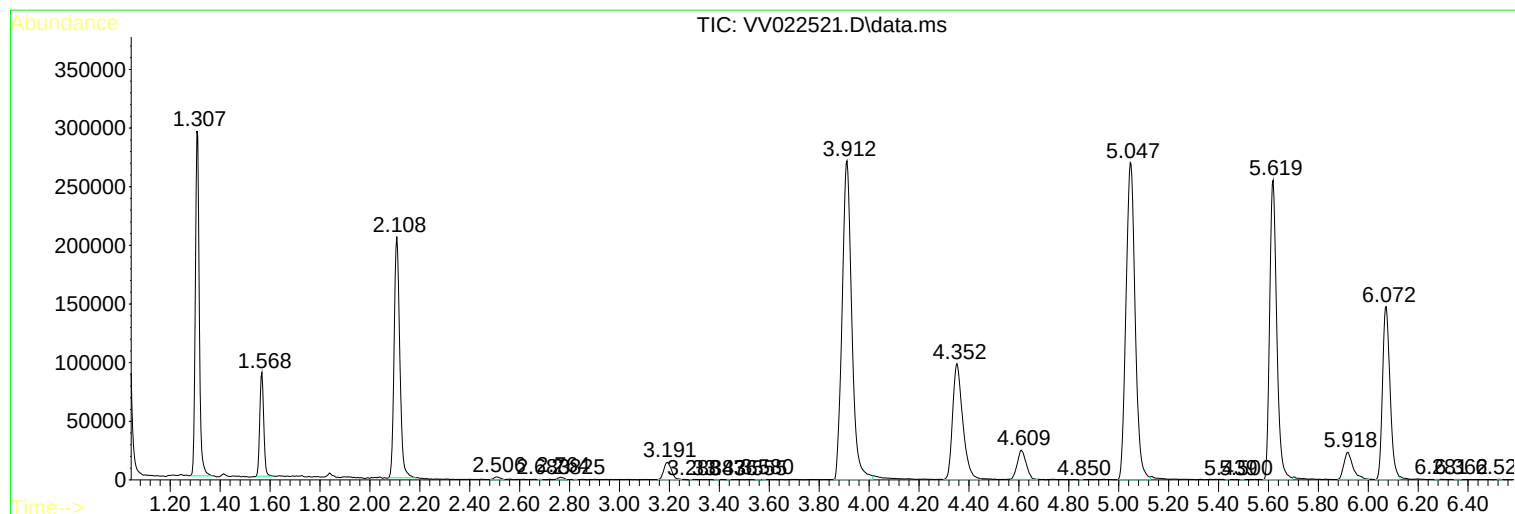

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022521.D
Acq On : 02 Oct 2021 19:17
Operator : SY/MD
Sample : M4023-01DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022521.D
Acq On : 02 Oct 2021 19:17
Operator : SY/MD
Sample : M4023-01DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
