

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022522.D
 Acq On : 02 Oct 2021 19:41
 Operator : SY/MD
 Sample : M4023-03DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M

Title : VOC Analysis

Signal : TIC: VV022522.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	104761	106411	15.30%	1.616%
2	1.564	157	163	174	rVB	86712	95029	13.67%	1.443%
3	2.108	322	332	354	rVB3	209632	333202	47.92%	5.059%
4	2.507	449	456	466	rVB4	3667	5305	0.76%	0.081%
5	2.580	475	479	481	rBV2	317	250	0.04%	0.004%
6	2.716	519	521	524	rVB	266	117	0.02%	0.002%
7	2.767	530	537	545	rVB5	1218	1917	0.28%	0.029%
8	3.034	613	620	623	rBV2	243	355	0.05%	0.005%
9	3.101	637	641	644	rBV2	211	228	0.03%	0.003%
10	3.243	683	685	688	rVB2	282	116	0.02%	0.002%
11	3.336	711	714	719	rBV2	244	187	0.03%	0.003%
12	3.384	724	729	731	rBV2	230	206	0.03%	0.003%
13	3.474	755	757	760	rBV2	173	131	0.02%	0.002%
14	3.613	794	800	804	rBV2	232	349	0.05%	0.005%
15	3.667	812	817	822	rBV2	269	270	0.04%	0.004%
16	3.725	832	835	838	rVB	315	214	0.03%	0.003%
17	3.831	867	868	870	rBV	212	122	0.02%	0.002%
18	3.912	877	893	918	rBV3	138516	395449	56.87%	6.005%
19	4.349	1016	1029	1058	rVB2	96710	266145	38.27%	4.041%
20	4.609	1094	1110	1127	rBV2	46393	115565	16.62%	1.755%
21	4.735	1147	1149	1150	rBV2	367	153	0.02%	0.002%
22	4.760	1155	1157	1159	rBV	213	138	0.02%	0.002%
23	4.828	1176	1178	1182	rBV2	295	206	0.03%	0.003%
24	4.899	1198	1200	1201	rBV	381	152	0.02%	0.002%
25	5.047	1229	1246	1273	rBV2	265337	680033	97.79%	10.326%
26	5.506	1387	1389	1394	rBV2	250	175	0.03%	0.003%
27	5.529	1394	1396	1398	rBV2	188	125	0.02%	0.002%
28	5.561	1400	1406	1408	rBV2	431	316	0.05%	0.005%
29	5.616	1411	1423	1454	rBV	255713	514005	73.92%	7.805%
30	5.915	1502	1516	1548	rBV2	347919	695373	100.00%	10.559%
31	6.072	1553	1565	1587	rVV	145516	295859	42.55%	4.492%
32	6.272	1625	1627	1632	rVB2	388	281	0.04%	0.004%
33	6.362	1651	1655	1656	rBV	380	253	0.04%	0.004%
34	6.407	1667	1669	1672	rBV2	205	152	0.02%	0.002%
35	6.506	1699	1700	1703	rBV2	248	119	0.02%	0.002%
36	6.603	1727	1730	1734	rVB2	285	190	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022522.D
 Acq On : 02 Oct 2021 19:41
 Operator : SY/MD
 Sample : M4023-03DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

37	6.683	1751	1755	1760	rBV2	305	371	0.05%	0.006%
38	6.780	1782	1785	1787	rBV	366	233	0.03%	0.004%
39	6.828	1796	1800	1803	rBV	139	148	0.02%	0.002%
40	6.934	1831	1833	1835	rBV2	248	119	0.02%	0.002%
41	6.989	1839	1850	1876	rBV	77448	145458	20.92%	2.209%
42	7.137	1894	1896	1900	rVB2	523	389	0.06%	0.006%
43	7.153	1900	1901	1903	rBV2	430	180	0.03%	0.003%
44	7.201	1913	1916	1917	rBV2	328	207	0.03%	0.003%
45	7.317	1937	1952	1971	rBV	318185	550459	79.16%	8.358%
46	7.561	2024	2028	2029	rBV3	358	284	0.04%	0.004%
47	7.625	2038	2048	2065	rBV	53013	93541	13.45%	1.420%
48	7.792	2097	2100	2101	rBV	285	152	0.02%	0.002%
49	7.809	2101	2105	2107	rVB2	340	257	0.04%	0.004%
50	7.854	2115	2119	2120	rBV2	506	311	0.04%	0.005%
51	7.985	2157	2160	2164	rVB3	768	623	0.09%	0.009%
52	8.091	2183	2193	2223	rBV	137907	288149	41.44%	4.375%
53	8.442	2298	2302	2305	rVV2	254	176	0.03%	0.003%
54	8.481	2312	2314	2315	rBV2	251	124	0.02%	0.002%
55	8.532	2328	2330	2335	rBV2	297	248	0.04%	0.004%
56	8.651	2363	2367	2370	rBV2	316	232	0.03%	0.004%
57	8.667	2370	2372	2374	rBV	260	140	0.02%	0.002%
58	8.722	2387	2389	2390	rBV	279	111	0.02%	0.002%
59	8.802	2412	2414	2415	rBV	278	139	0.02%	0.002%
60	8.854	2419	2430	2451	rBV	378927	612156	88.03%	9.295%
61	9.069	2494	2497	2499	rVB	272	116	0.02%	0.002%
62	9.149	2513	2522	2531	rBV3	2927	5107	0.73%	0.078%
63	9.358	2583	2587	2589	rVB	447	269	0.04%	0.004%
64	9.374	2589	2592	2594	rBV	161	124	0.02%	0.002%
65	9.429	2605	2609	2611	rBV2	226	163	0.02%	0.002%
66	9.477	2620	2624	2625	rBV2	369	314	0.05%	0.005%
67	9.548	2640	2646	2656	rVB4	2429	3530	0.51%	0.054%
68	9.661	2678	2681	2685	rBV	170	136	0.02%	0.002%
69	9.728	2699	2702	2704	rBV	183	126	0.02%	0.002%
70	9.818	2724	2730	2733	rBV2	279	300	0.04%	0.005%
71	9.956	2769	2773	2775	rBV	457	225	0.03%	0.003%
72	10.050	2800	2802	2807	rBV2	177	204	0.03%	0.003%
73	10.130	2818	2827	2835	rVB4	1529	2675	0.38%	0.041%
74	10.169	2835	2839	2842	rBV	163	147	0.02%	0.002%
75	10.217	2842	2854	2871	rBV	201659	311812	44.84%	4.735%
76	10.374	2897	2903	2908	rBV3	516	567	0.08%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022522.D
 Acq On : 02 Oct 2021 19:41
 Operator : SY/MD
 Sample : M4023-03DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH8DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

77	10.503	2941	2943	2951	rVB2	325	256	0.04%	0.004%
78	10.837	3043	3047	3053	rBV2	368	401	0.06%	0.006%
79	10.918	3066	3072	3075	rBV3	784	950	0.14%	0.014%
80	11.005	3097	3099	3101	rBV	272	142	0.02%	0.002%
81	11.066	3115	3118	3121	rBV2	318	212	0.03%	0.003%
82	11.149	3138	3144	3148	rVB3	693	777	0.11%	0.012%
83	11.249	3164	3175	3200	rBV	370412	568159	81.71%	8.627%
84	11.625	3280	3292	3313	rBV	304855	482321	69.36%	7.324%
85	11.779	3339	3340	3342	rBV	445	177	0.03%	0.003%
86	11.837	3355	3358	3360	rVB3	258	128	0.02%	0.002%
87	11.905	3376	3379	3382	rBV	326	240	0.03%	0.004%
88	12.239	3480	3483	3484	rBV	327	192	0.03%	0.003%
89	12.336	3511	3513	3516	rBV	311	203	0.03%	0.003%
90	12.651	3608	3611	3616	rVB2	279	245	0.04%	0.004%
91	12.947	3697	3703	3706	rBV	267	305	0.04%	0.005%
92	13.098	3746	3750	3755	rBV	283	285	0.04%	0.004%
93	13.332	3819	3823	3825	rBV2	170	124	0.02%	0.002%
94	13.422	3849	3851	3855	rVB2	485	186	0.03%	0.003%
95	13.628	3913	3915	3919	rBV2	288	134	0.02%	0.002%
96	13.660	3923	3925	3928	rVB2	209	115	0.02%	0.002%
97	13.776	3957	3961	3963	rBV2	300	273	0.04%	0.004%
98	14.114	4062	4066	4067	rBV2	372	235	0.03%	0.004%
99	14.596	4213	4216	4220	rBV3	328	303	0.04%	0.005%
100	15.570	4516	4519	4520	rBV	501	318	0.05%	0.005%




Sum of corrected areas: 6585801

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022522.D
Acq On : 02 Oct 2021 19:41
Operator : SY/MD
Sample : M4023-03DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

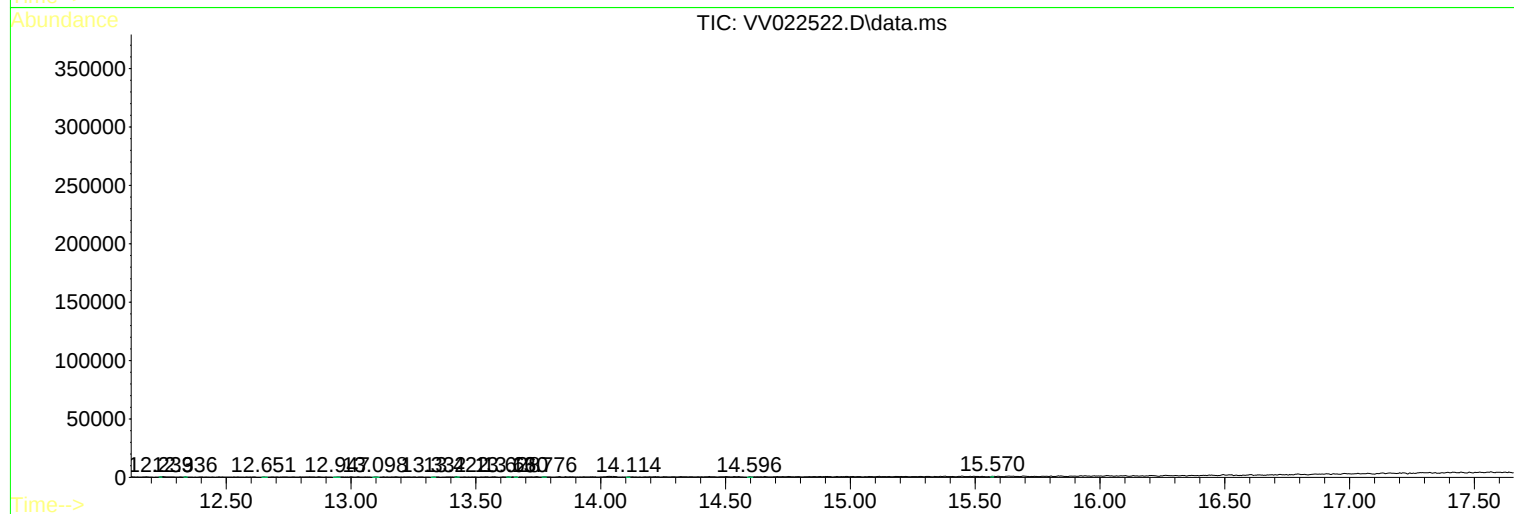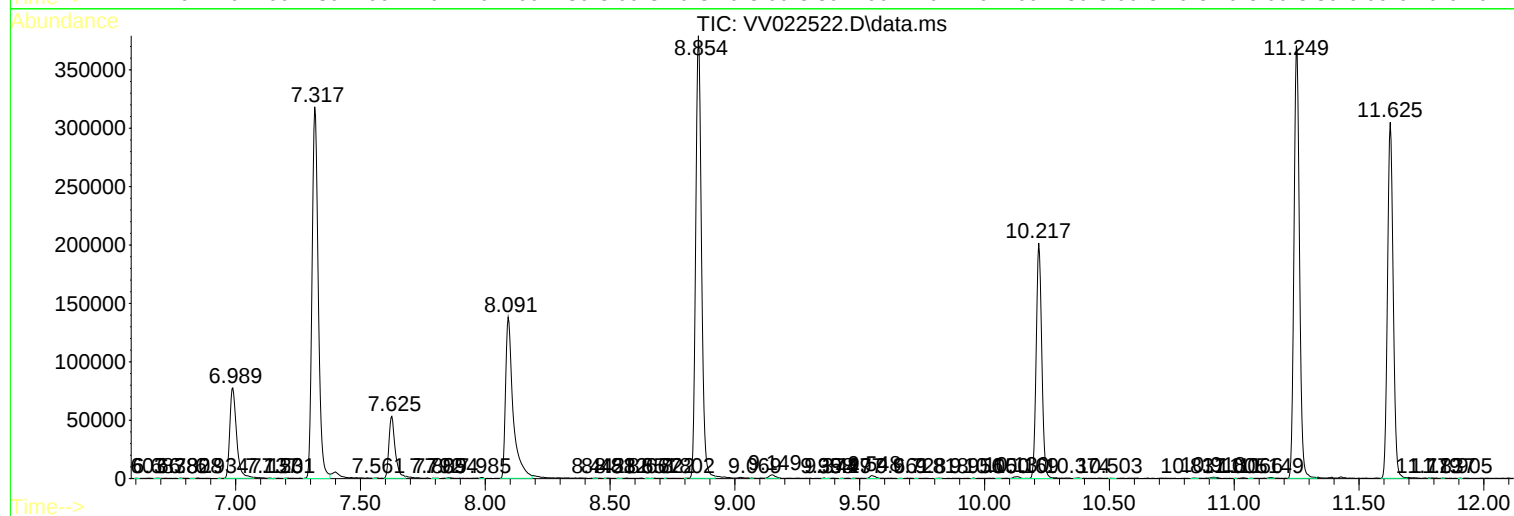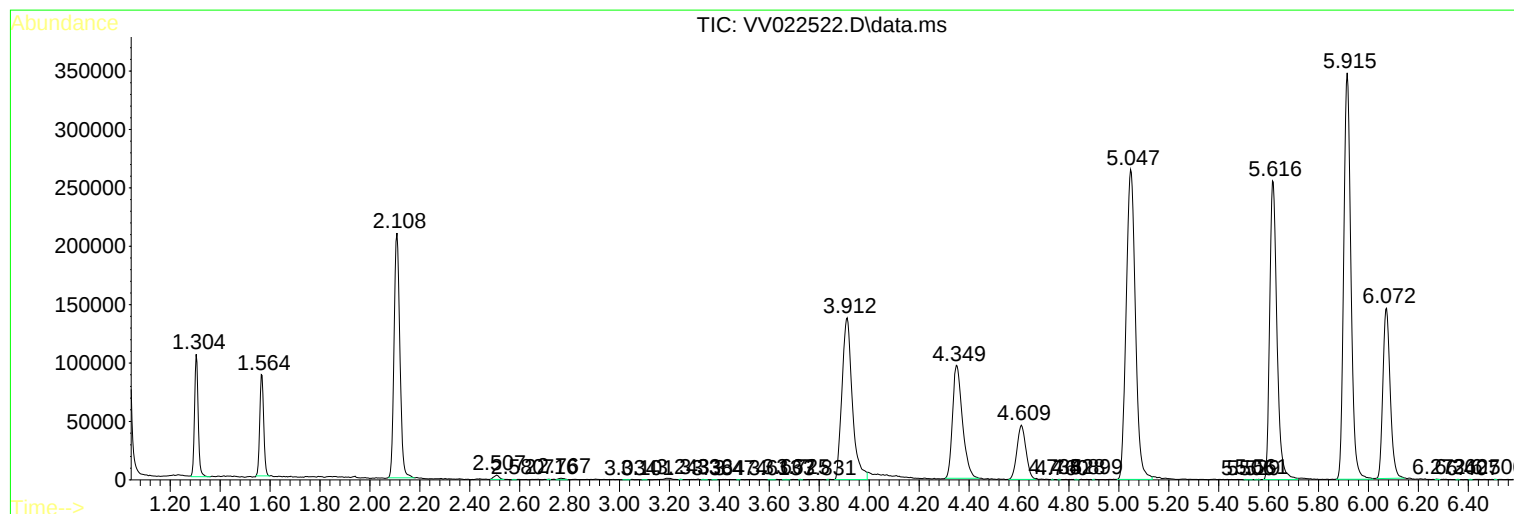

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022522.D
Acq On : 02 Oct 2021 19:41
Operator : SY/MD
Sample : M4023-03DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022522.D
Acq On : 02 Oct 2021 19:41
Operator : SY/MD
Sample : M4023-03DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
