

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022524.D
 Acq On : 02 Oct 2021 20:28
 Operator : SY/MD
 Sample : M4023-08DL 1000X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

Signal : TIC: VV022524.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	105019	108777	15.81%	1.751%
2	1.568	157	164	176	rVB	89767	100401	14.59%	1.616%
3	2.108	321	332	353	rBV2	203841	313915	45.62%	5.052%
4	2.507	447	456	470	rVB2	10295	16190	2.35%	0.261%
5	2.574	474	477	480	rBV	281	180	0.03%	0.003%
6	2.883	570	573	574	rBV	265	154	0.02%	0.002%
7	2.963	592	598	599	rBV2	278	287	0.04%	0.005%
8	2.986	602	605	607	rBV	228	173	0.03%	0.003%
9	3.240	681	684	687	rBV2	264	195	0.03%	0.003%
10	3.330	708	712	715	rBV	455	423	0.06%	0.007%
11	3.426	740	742	746	rBV2	350	203	0.03%	0.003%
12	3.497	760	764	767	rBV2	190	124	0.02%	0.002%
13	3.552	778	781	784	rBV2	187	158	0.02%	0.003%
14	3.590	791	793	794	rBV2	277	132	0.02%	0.002%
15	3.645	808	810	812	rVB	272	122	0.02%	0.002%
16	3.674	817	819	820	rVB	344	121	0.02%	0.002%
17	3.687	820	823	824	rBV	310	209	0.03%	0.003%
18	3.751	839	843	846	rBV	225	176	0.03%	0.003%
19	3.770	847	849	852	rBV2	151	88	0.01%	0.001%
20	3.905	879	891	919	rBV2	31796	119641	17.39%	1.925%
21	4.349	1015	1029	1059	rVB2	100193	273945	39.81%	4.409%
22	4.484	1069	1071	1073	rBV2	613	369	0.05%	0.006%
23	4.613	1099	1111	1129	rVB3	13053	32164	4.67%	0.518%
24	4.690	1133	1135	1138	rBV2	366	276	0.04%	0.004%
25	4.835	1175	1180	1185	rBV2	358	386	0.06%	0.006%
26	4.867	1188	1190	1194	rVV3	414	210	0.03%	0.003%
27	4.957	1216	1218	1222	rVB	205	82	0.01%	0.001%
28	5.047	1230	1246	1271	rBV2	273594	688089	100.00%	11.074%
29	5.368	1344	1346	1349	rBV	263	177	0.03%	0.003%
30	5.384	1349	1351	1355	rVV2	246	166	0.02%	0.003%
31	5.471	1374	1378	1380	rBV	372	260	0.04%	0.004%
32	5.484	1380	1382	1383	rBV	182	91	0.01%	0.001%
33	5.510	1388	1390	1392	rVV	385	166	0.02%	0.003%
34	5.523	1392	1394	1396	rVB2	355	125	0.02%	0.002%
35	5.616	1412	1423	1443	rBV	245289	495939	72.07%	7.981%
36	5.793	1476	1478	1482	rBV	486	248	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022524.D
 Acq On : 02 Oct 2021 20:28
 Operator : SY/MD
 Sample : M4023-08DL 1000X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

37	5.915	1502	1516	1547	rBV	327597	648827	94.29%	10.442%
38	6.072	1552	1565	1585	rBV2	148513	306407	44.53%	4.931%
39	6.272	1625	1627	1628	rBV2	292	138	0.02%	0.002%
40	6.342	1648	1649	1652	rVB2	267	107	0.02%	0.002%
41	6.420	1669	1673	1676	rBV2	467	350	0.05%	0.006%
42	6.452	1681	1683	1684	rVB	312	101	0.01%	0.002%
43	6.484	1691	1693	1697	rBV	402	223	0.03%	0.004%
44	6.764	1777	1780	1782	rBV3	269	156	0.02%	0.003%
45	6.870	1810	1813	1815	rBV	157	108	0.02%	0.002%
46	6.892	1818	1820	1821	rBV	242	99	0.01%	0.002%
47	6.924	1827	1830	1835	rVB3	281	248	0.04%	0.004%
48	6.989	1839	1850	1867	rBV	77817	144077	20.94%	2.319%
49	7.146	1897	1899	1901	rBV2	274	189	0.03%	0.003%
50	7.217	1918	1921	1924	rBV2	159	118	0.02%	0.002%
51	7.262	1932	1935	1936	rBV2	221	93	0.01%	0.001%
52	7.317	1941	1952	1972	rBV	326193	564349	82.02%	9.082%
53	7.625	2038	2048	2073	rBV	53879	97277	14.14%	1.565%
54	7.770	2090	2093	2095	rBV	361	204	0.03%	0.003%
55	7.802	2100	2103	2105	rBV2	280	152	0.02%	0.002%
56	7.857	2118	2120	2125	rBV2	258	211	0.03%	0.003%
57	7.928	2138	2142	2145	rBV	251	254	0.04%	0.004%
58	7.963	2149	2153	2154	rBV	220	167	0.02%	0.003%
59	8.092	2183	2193	2229	rBV	130446	303363	44.09%	4.882%
60	8.455	2301	2306	2311	rBV3	342	452	0.07%	0.007%
61	8.600	2349	2351	2356	rBV2	282	181	0.03%	0.003%
62	8.625	2356	2359	2361	rVV3	352	228	0.03%	0.004%
63	8.658	2365	2369	2373	rBV2	262	275	0.04%	0.004%
64	8.748	2393	2397	2398	rBV2	251	206	0.03%	0.003%
65	8.809	2414	2416	2418	rBV	159	109	0.02%	0.002%
66	8.854	2418	2430	2451	rBV	364584	599103	87.07%	9.641%
67	9.124	2511	2514	2515	rBV	313	163	0.02%	0.003%
68	9.146	2515	2521	2528	rVV4	1833	2575	0.37%	0.041%
69	9.227	2544	2546	2552	rBV	190	190	0.03%	0.003%
70	9.272	2557	2560	2562	rBV2	173	132	0.02%	0.002%
71	9.429	2604	2609	2612	rBV2	240	246	0.04%	0.004%
72	9.519	2633	2637	2638	rBV	275	239	0.03%	0.004%
73	9.555	2642	2648	2655	rVV3	1028	1523	0.22%	0.025%
74	9.693	2687	2691	2697	rBV2	358	366	0.05%	0.006%
75	9.937	2764	2767	2772	rVB2	271	245	0.04%	0.004%
76	9.985	2779	2782	2784	rBV	304	196	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
 Data File : VV022524.D
 Acq On : 02 Oct 2021 20:28
 Operator : SY/MD
 Sample : M4023-08DL 1000X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

77	10.217	2842	2854	2874	rBV	203711	320066	46.52%	5.151%
78	10.352	2893	2896	2897	rBV	270	120	0.02%	0.002%
79	10.715	3006	3009	3012	rBV2	194	159	0.02%	0.003%
80	10.792	3030	3033	3038	rVB2	360	238	0.03%	0.004%
81	10.818	3038	3041	3043	rBV	164	141	0.02%	0.002%
82	10.870	3055	3057	3061	rVB	258	129	0.02%	0.002%
83	10.908	3065	3069	3070	rBV3	729	479	0.07%	0.008%
84	10.953	3080	3083	3085	rBV	196	142	0.02%	0.002%
85	11.034	3103	3108	3110	rBV2	375	392	0.06%	0.006%
86	11.153	3138	3145	3150	rBV4	658	852	0.12%	0.014%
87	11.249	3165	3175	3195	rBV	365143	557000	80.95%	8.964%
88	11.625	3280	3292	3319	rBV	323616	503255	73.14%	8.099%
89	11.882	3368	3372	3375	rVB3	409	308	0.04%	0.005%
90	11.905	3375	3379	3381	rBV	163	129	0.02%	0.002%
91	11.956	3392	3395	3398	rBV2	248	185	0.03%	0.003%
92	12.082	3432	3434	3441	rBV3	322	340	0.05%	0.005%
93	12.342	3512	3515	3519	rBV	349	320	0.05%	0.005%
94	12.426	3538	3541	3543	rBV	303	207	0.03%	0.003%
95	12.873	3678	3680	3681	rBV	275	130	0.02%	0.002%
96	13.082	3743	3745	3751	rBV	281	223	0.03%	0.004%
97	13.291	3807	3810	3811	rBV	243	126	0.02%	0.002%
98	13.599	3902	3906	3909	rBV4	411	291	0.04%	0.005%
99	14.239	4102	4105	4109	rBV2	318	338	0.05%	0.005%
100	14.738	4258	4260	4262	rBV	460	248	0.04%	0.004%




Sum of corrected areas: 6213827

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022524.D
Acq On : 02 Oct 2021 20:28
Operator : SY/MD
Sample : M4023-08DL 1000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

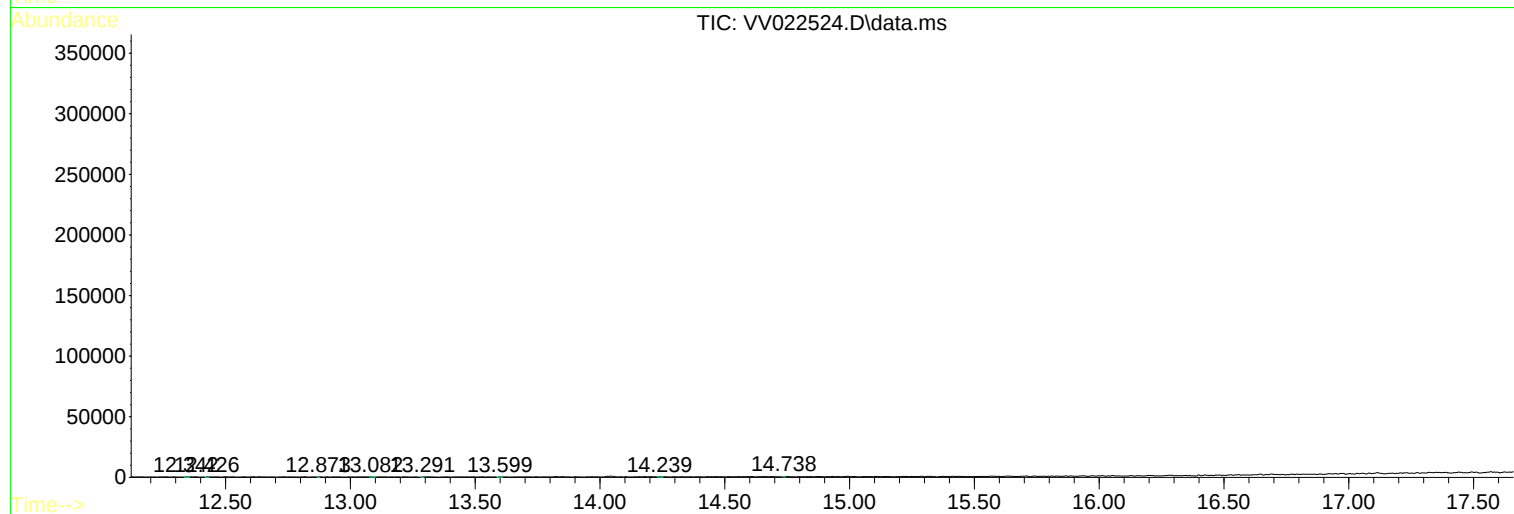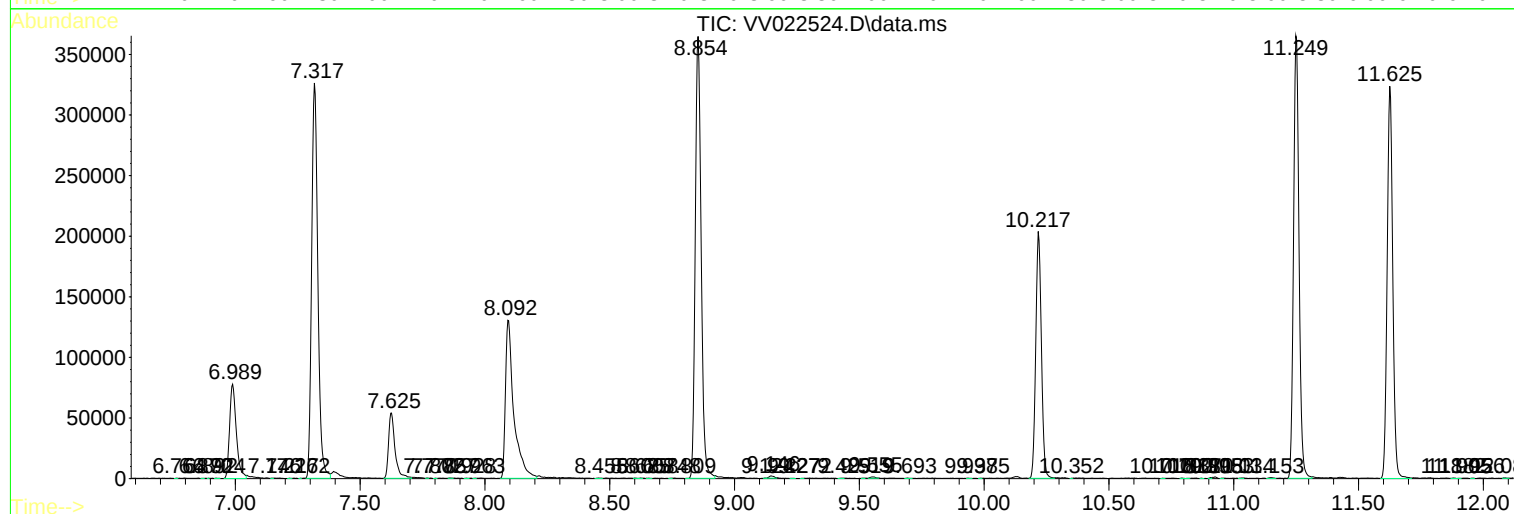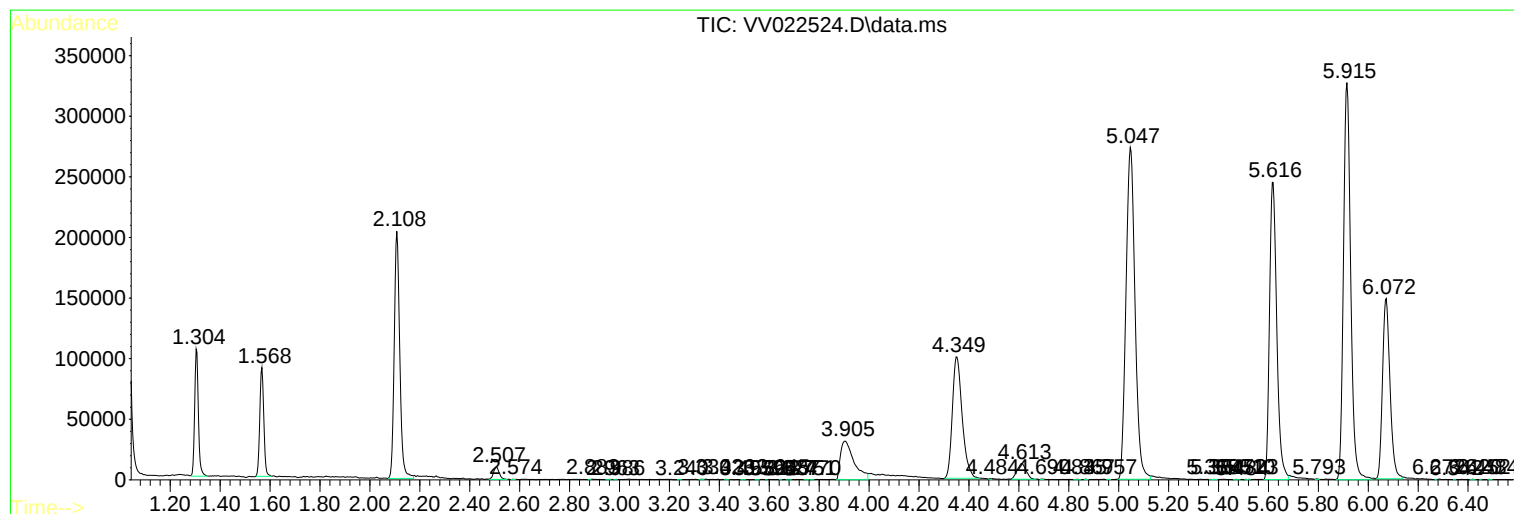

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022524.D
Acq On : 02 Oct 2021 20:28
Operator : SY/MD
Sample : M4023-08DL 1000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100221\
Data File : VV022524.D
Acq On : 02 Oct 2021 20:28
Operator : SY/MD
Sample : M4023-08DL 1000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
